I.V./O, Cylinder Holder Accessory Kit

Assembly, Installation and Operating Instructions

Model Nos. 1487,1496 and T1496



Yes, you can:

NOTE: Check all parts for shipping damage. If shipping damage is noted, DO NOT use. Contact Dealer/Invacare for further instructions.

SAFETY SUMMARY

The following recommendations are made for the safe installation of the IV/O2 Cylinder Holder Accessory Kit:

WARNING

DO NOT assemble or use this equipment without first reading and understanding this instruction sheet. If you are unable to understand the Warnings, Cautions or Instructions, contact a healthcare professional, dealer or technical personnel if applicable before attempting to install this equipment - otherwise, injury or damage may occur.

After ANY adjustments, repair or service and BEFORE use, make sure all attaching hardware is tightened securely.

Follow the Oxygen Cylinder manufacturers guidelines for proper usage of the oxygen cylinder.

INSTALLING IV/O2 CYLINDER HOLDER (FIGURE 1)

NOTE: IF rear step tube is 7/8-inch diameter tubing, install the long tube guide insert into the rear step tube before installing the IV/O2 cylinder holder.

1. Place the IV/O2 cylinder holder and slide it onto the rear step tube of the wheelchair.

NOTE: IF rear upright tubing is 7/8-inch diameter tubing, install the short tube guide insert over the rear upright before installing and securing the IV/O2 cylinder holder bracket.

- Push the bracket of the IV/O2 cylinder holder over the rear upright of the wheelchair and secure in place with the hex screw, spacer and locknut.
- Secure IV/O2 cylinder holder to push handle using a ty-wrap.
- 4. Loosen the short adjustment knob to move IV/O2 cylinder holder to desired height and then retighten.
- Use the long adjustment knob on the IV/O2 cylinder holder bracket to secure the oxygen cylinder in place.

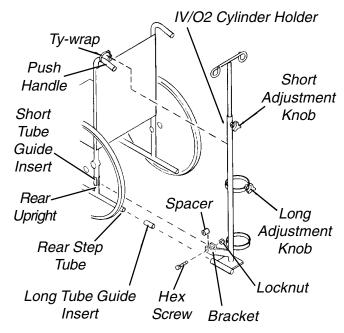


FIGURE 1 - INSTALLING IV/O2 CYLINDER HOLDER

