

# TELEDYNE HASTINGS INSTRUMENTS

INSTRUCTION MANUAL



## HFM-I-401 AND HFM-I-405 INDUSTRIAL FLOW METERS



# Manual Print History




The print history shown below lists the printing dates of all revisions and addenda created for this manual. The revision level letter increases alphabetically as the manual undergoes subsequent updates. Addenda, which are released between revisions, contain important change information that the user should incorporate immediately into the manual. Addenda are numbered sequentially. When a new revision is created, all addenda associated with the previous revision of the manual are incorporated into the new revision of the manual. Each new revision includes a revised copy of this print history page.

Revision A (Document Number 171-042008)	March 2008
Revision B (Document Number 171-102008)	October 2008
Revision C (Document Number 171-112008)	November 2008
Revision D (Document Number 171-032009)	March 2009
Revision E (Document Number 171-082010)	August 2010




**Visit [www.teledyne-hi.com](http://www.teledyne-hi.com) for WEEE disposal guidance.**

## Description of Symbols and Messages used in this manual


<b>WARNING</b> 	<p>This indicates a potential personnel hazard. It calls attention to a procedure, practice, condition or the like, which, if not correctly performed or adhered to, could result in injury to personnel.</p>
<b>CAUTION</b> 	<p>This indicates a potential equipment hazard. It calls attention to an operating procedure, practice, or the like, which, if not correctly performed or adhered to, could result in damage to or destruction of all or part of the product.</p>
<b>NOTE</b> 	<p>This indicates important information. It calls attention to a procedure, practice, condition or the like, which is worthy of special mention.</p>

Teledyne Hastings Instruments reserves the right to change or modify the design of its equipment without any obligation to provide notification of change or intent to change.


# Quick Start Instructions

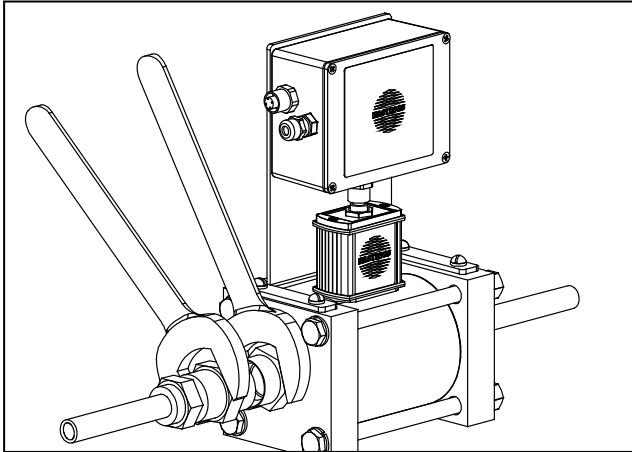


Connect dry, clean gas and ensure connections are leak free.

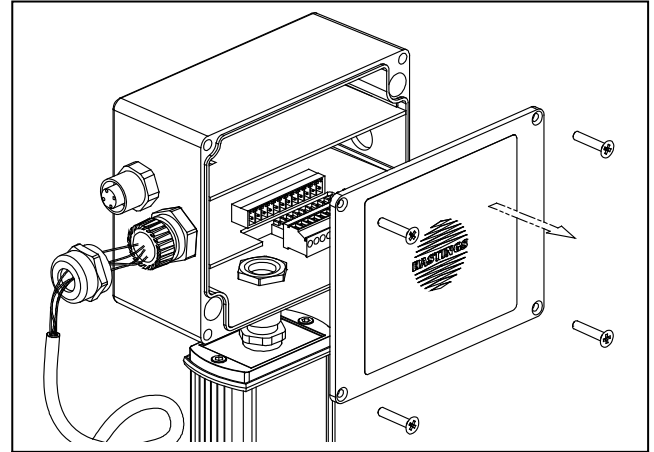

Connect Cable for power and analog signal output.

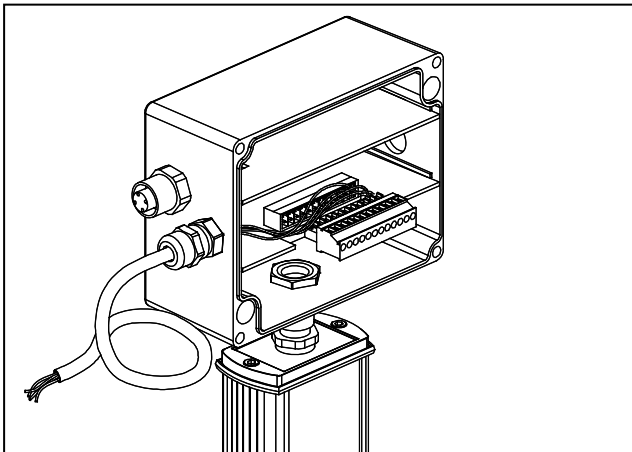


Check that electrical connections are correct.  
(See diagrams below)

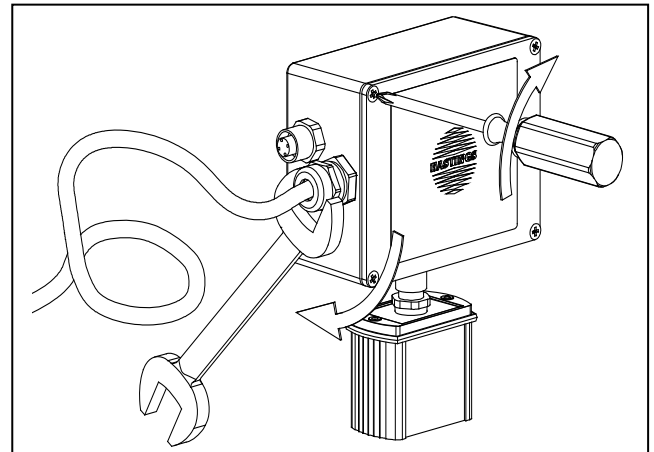


Replace front cover and cable feed-through ensuring gasket is seated and fasteners are secure.

Terminal Strip

Digital Connector

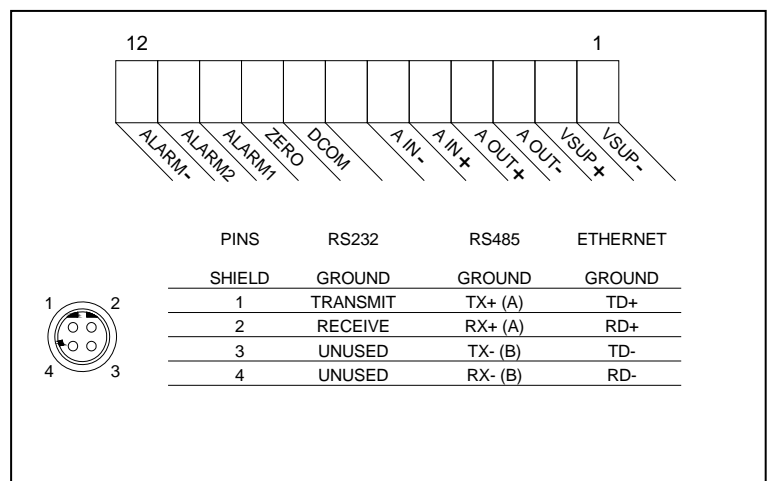


COPYRIGHT 2009 TELEDYNE HASTINGS INSTRUMENTS ALL RIGHT RESERVED	REVISIONS			
	REV	DESCRIPTION	DATE	APPROVED
	A	INITIAL RELEASE	03/10/09	W. J. A.

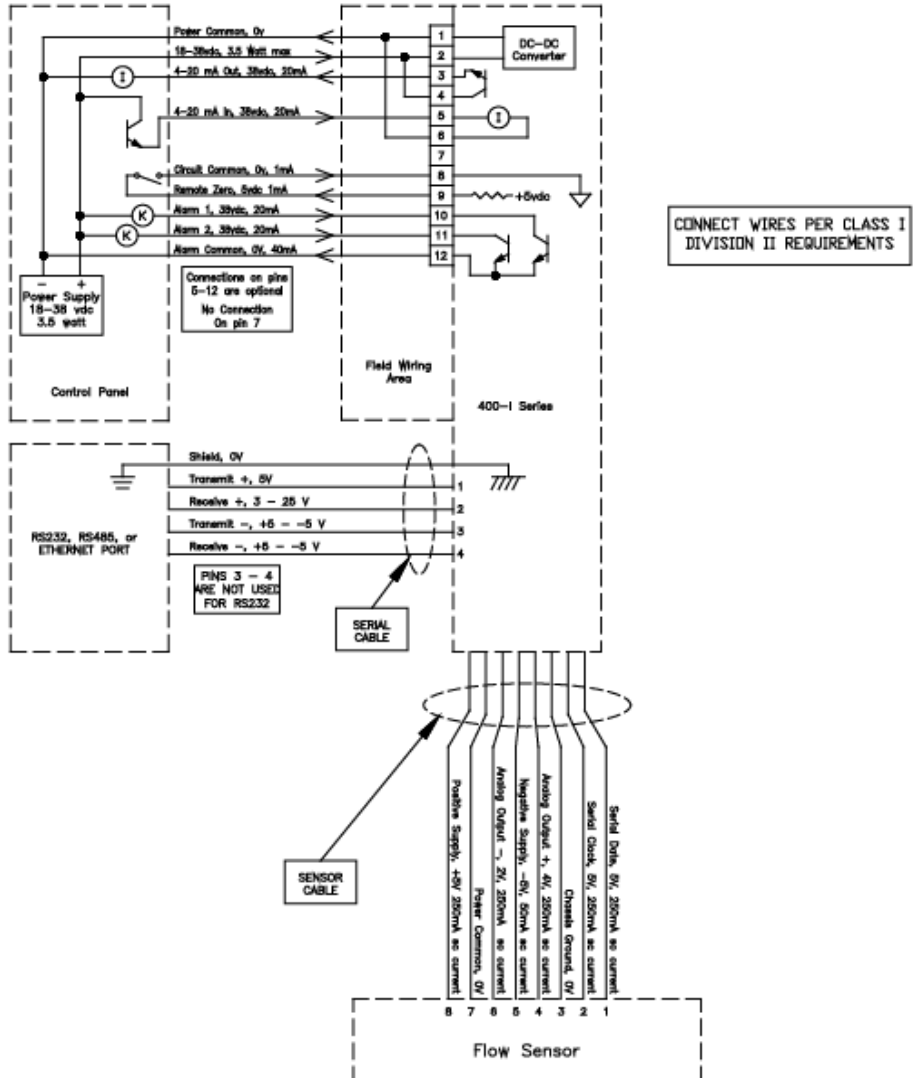

THE INFORMATION CONTAINED IN OR DISCLOSED BY THIS DOCUMENT IS PROPRIETARY PROPERTY OF TELEDYNE TECHNOLOGIES INCORPORATED (TDY). THIS DOCUMENT AND THE ITEMS AND INFORMATION CONTAINED OR DISCLOSED HEREIN SHALL NOT BE USED, COPIED, OR REPRODUCED IN WHOLE OR IN PART, NOR SHALL THE CONTENTS BE DISCLOSED IN ANY FORM, IN WHOLE OR IN PART, TO ANY PERSON EXCEPT AS SPECIFICALLY AUTHORIZED BY TDY, OR ITS AUTHORIZED REPRESENTATIVE. NO RIGHT OR LICENSE TO ANY PROPRIETARY INFORMATION OWNED OR CONTROLLED BY TDY IS GRANTED OR IMPLIED BY THE DISCLOSURE OF THIS DOCUMENT. THIS DOCUMENT AND THE ITEMS AND INFORMATION CONTAINED OR DISCLOSED HERE MAY BE SUBJECT TO THE INTERNATIONAL TRAFFIC IN ARMS REGULATIONS (ITAR) OR THE EXPORT ADMINISTRATION REGULATIONS (EAR)


UNLESS OTHERWISE SPECIFIED DIMENSIONS ARE IN INCHES TOLERANCES ARE: FRACTIONS DECIMALS ANGLES ± .XX ± .01 1/64 .XXX ± .005 ± 2°	STOCK NO. N/A	<b>TELEDYNE HASTINGS INSTRUMENTS</b>			
	DRAWN A. ARAIZA		03/04/09		
MATERIAL ---	ENG. MGR. W. ALVESTEFFER	03/10/09			
FINISH ---	NEXT ASSY	USED ON 400 SERIES	SIZE A	DWG NO. 32076	REV A
			SCALE N/A	SHEET 1 of 2	

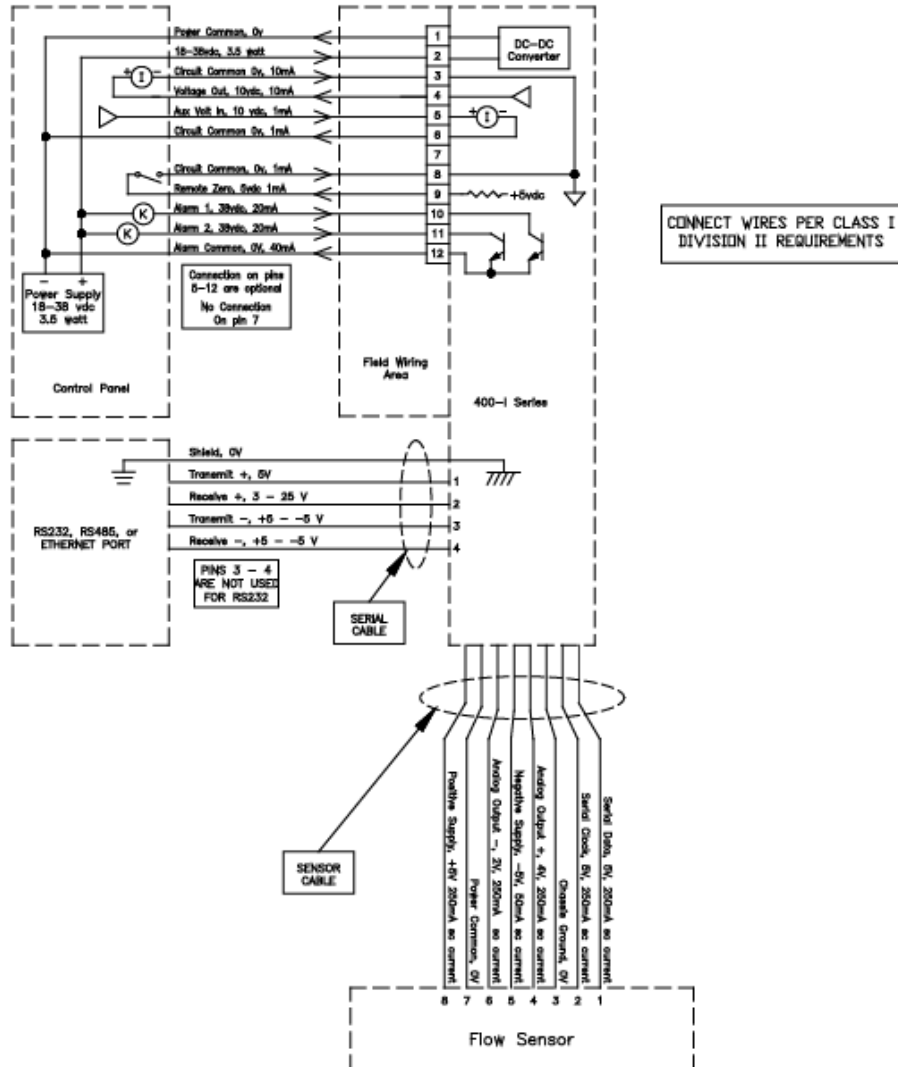



**TELEDYNE HASTINGS INSTRUMENTS**


**I/O WIRING DIAGRAM  
0-5, 0-10 VOLTS**


DRAWN A. ARAIZA	03/04/09	USED ON 400 SERIES	SIZE A	DWG NO. 32076	REV A
ISSUED W. ALVESTEFFER	03/10/09		SCALE N/A	SHEET 2 of 2	

<p><b>CAUTION</b></p> 	<p>This instrument is available with multiple pin-outs. Ensure electrical connections are correct.</p>
---	--

<p><b>CAUTION</b></p> 	<p>The 400-I series flow meters are designed for IEC Installation/Over voltage Category II – single phase receptacle connected loads.</p>
---	---

<p><b>NOTE</b></p> 	<p>The Hastings 400 Series flow meters are designed for INDOOR and OUTDOOR operation.</p>
--	---

<p><b>CAUTION</b></p> 	<p>In order to maintain the integrity of the Electrostatic Discharge immunity both parts of the remote mounted version of the HFM-I-400 instrument must be screwed to a well grounded structure.</p>
---	--

<p><b>CAUTION</b></p> 	<p>In order to maintain the environmental integrity of the enclosure the power/signal cable jacket must have a diameter of 0.12 - 0.35" (3 - 9 mm) for the cable gland or 0.25 - 0.275" (6.5 - 7 mm) for the circular connector. The nut on the cable gland must be tightened down sufficiently to secure the cable. This cable must be rated for at least 85°C.</p>
---	--

# Table of Contents

<b>GENERAL INFORMATION.....</b>	<b>1</b>
1. GENERAL INFORMATION .....	1
1.1. OVERVIEW.....	1
1.1.1. 400 Series Family .....	1
1.1.2. 400 Series Meters .....	1
1.1.3. Measurement Approach.....	1
1.1.4. Additional Functions.....	1
1.2. SPECIFICATIONS .....	2
<b>INSTALLATION.....</b>	<b>4</b>
2. INSTALLATION.....	4
2.1. RECEIVING INSPECTION .....	4
2.2. ENVIRONMENTAL AND GAS REQUIREMENTS .....	4
2.3. MECHANICAL CONNECTIONS .....	4
2.4. MOUNTING THE ELECTRONICS REMOTELY.....	5
2.5. ELECTRICAL CONNECTION .....	5
2.5.1. Power Supply.....	6
2.5.2. Analog Output.....	6
2.5.2.1. Current Loop Output .....	6
2.5.2.2. Voltage output.....	9
2.6. DIGITAL CONNECTION.....	9
2.7. DIGITAL CONFIGURATION .....	9
2.7.1. RS-232 .....	9
2.7.2. RS-485 .....	10
2.7.3. Ethernet .....	10
2.8. ALARM OUTPUT CONNECTION .....	10
2.9. AUXILIARY INPUT CONNECTION .....	11
2.10. ROTARY GAS SELECTOR.....	12
2.11. ELECTRICAL REMOTE ZERO CONNECTION .....	13
2.12. CHECK INSTALLATION PRIOR TO OPERATION.....	13
<b>OPERATION.....</b>	<b>15</b>
3. OPERATION .....	15
3.1. ENVIRONMENTAL AND GAS CONDITIONS .....	15
3.2. INTERPRETING THE ANALOG OUTPUT .....	15
3.3. DIGITAL COMMUNICATIONS .....	15
3.3.1. Digitally Reported Flow Output .....	16
3.3.2. Digitally Reported Analog Input.....	16
3.4. ZEROING THE INSTRUMENT .....	16
3.4.1. Preparing for a Zero Check.....	16
3.4.2. Adjusting Zero .....	17
3.5. OVER-RANGE.....	17
3.6. REVERSE FLOW .....	18
3.7. HIGH PRESSURE OPERATION .....	18
3.7.1. Zero Shift .....	19
3.7.2. Span Shift.....	19
3.8. WARNINGS/ALARMS .....	19
3.9. MULTI-GAS CALIBRATIONS .....	19
3.10. FLOW TOTALIZATION .....	20
3.11. ADDITIONAL DIGITAL CAPABILITIES .....	20
<b>PARTS AND ACCESSORIES .....</b>	<b>21</b>
4. PARTS & ACCESSORIES .....	21
4.1. POWER POD – POWER & DISPLAY UNITS .....	21
4.2. FITTINGS.....	22
4.3. CABLES .....	22
<b>WARRANTY .....</b>	<b>23</b>

5.	WARRANTY .....	23
5.1.	WARRANTY REPAIR POLICY .....	23
5.2.	NON-WARRANTY REPAIR POLICY .....	23
<b>APPENDICES.....</b>		<b>24</b>
6.	APPENDICES .....	24
6.1.	APPENDIX 1- VOLUMETRIC VERSUS MASS FLOW .....	24
6.2.	APPENDIX 2 - GAS CONVERSION FACTORS.....	25



# 1. General Information

## 1. General Information

### 1.1. Overview

#### 1.1.1. 400 Series Family

The Hastings 400 Series is a family of flow instruments which is specifically designed to meet the needs of the industrial gas flow market. The “I” family in the 400 Series features an IP-65 enclosure which allows the use of the instrument in a wide variety of environments. The 400 I products consist of four configurations: a flow meter, HFM-I-401, which has a nominal nitrogen full scale between 10 SLM and 300 SLM and a corresponding flow controller, the HFC-I-403; a larger flow meter, HFM-I-405, which ranges from 100 SLM to 2500 SLM, and a corresponding flow controller, the HFC-I-407. These instruments are configured in a convenient in-line flow-through design with standard fittings. Each instrument in the series can be driven by either a +24 VDC power supply or a bipolar  $\pm 15$  volt supply. The electrical connection can be made via either a terminal strip located inside the enclosure or optionally through an IP-65 compatible electrical connector. Also, these instruments include both analog and digital communications capabilities.

#### 1.1.2. 400 Series Meters

The Hastings HFM-I-401 and HFM-I-405 thermal mass flow meters are designed to provide very accurate measurements over a wide range of flow rates and environmental conditions. The design is such that no damage will occur from moderate overpressure or overflows and no maintenance is required under normal operating conditions when using clean gases.

#### 1.1.3. Measurement Approach

The instrument is based on mass flow sensing. This is accomplished by combining a high-speed thermal transfer sensor with a parallel laminar flow shunt (see Figure 1-1). The flow through the meter is split between the sensor and shunt in a constant ratio set by the full scale range. The thermal sensor consists of a stainless steel tube with a heater at its center and two thermocouples symmetrically located upstream and downstream of the heater. The ends of the sensor tube pass through an aluminum block and into the stainless steel sensor base. With no flow in the tube the thermocouples report the same elevated temperature; however a forward flow cools the upstream thermocouple relative to the downstream. This temperature difference generates a voltage signal in the sensor which is digitized and transferred to the main processor in the electronics enclosure. The processor uses this real-time information and the sensor/shunt characteristics stored in non-volatile memory to calculate and report the flow.

To ensure an inherently linear response to flow, both the thermal sensor and the shunt have been engineered to overcome problems common to other flow meter designs. For example, nonlinearities and performance variations often arise in typical flow meters due to pressure-related effects at the entrance and exit areas of the laminar flow shunt. Hastings has designed the 400 Series meters such that the flow-critical splitting occurs at locations safely downstream from the entrance effects and well upstream from the exit effects. This vastly improves the stability of the flow ratio between the sensor and shunt. The result of this design feature is a better measurement when the specific gravity of the flowing medium varies, for instance due to changes in pressure or gas type. Also, a common problem in typical flow meters is a slow response to flow changes. To improve response time, some flow meter designs introduce impurities such as silica gel. Alternatively, Hastings has designed the 400 Series sensor with reduced thermal mass to improve the response time without exposing additional materials to the gas stream.


#### 1.1.4. Additional Functions

These instruments contain a number of functions in addition to reporting flow which include:

- Settable alarms and warnings with semiconductor switch outputs

- A digitally reported status of alarms and warnings such as overflow/underflow
- A flow totalizer to track the amount of gas added to a system
- A digitizing channel for an auxiliary analog signal
- An internal curve fitting routine for “fine tuning” the base calibration
- An alternate calibration set of 8 different ranges/gases

## 1.2. Specifications

<p><b>WARNING</b></p> 	<p>Do not operate this instrument in excess of the specifications listed below. Failure to heed this warning can result in serious personal injury and/or damage to the equipment.</p>
---	--

<i>Performance</i>	<i>HFM-I-401</i>	<i>HFM-I-405</i>
Full Scale Flow Ranges (in N <sub>2</sub> ) Accuracy <sup>1</sup> Repeatability Operating Temperature Warm up time Settling Time/Reponse Time Temperature Coefficient of Zero Temperature Coefficient of Span Operating Pressure - Maximum Pressure Coefficient of Span Pressure Drop(N <sub>2</sub> @14.7 psia) Attitude Sensitivity of Zero	0-10 slm up to 0-350 slm <b>Standard:</b> ± 1% full scale Optional: ± (0.5% reading + 0.2%FS) ± 0.1% of F.S. -20 to 70°C 30 min for optimum accuracy 2 min for ± 2% of full scale < 2.5 seconds (to within ± 2% of full scale) < ±0.05% of Full Scale /°C < ±0.16% of reading/°C <b>Standard:</b> 500 psig Optional: 1500 psig < 0.01%of reading /psi (N <sub>2</sub> , 0-1000 psig) < 1.1 psi at full scale flow < 2% of F.S.	0-100 slm up to 0-2500 slm <b>Standard:</b> ± 1% full scale Optional: ± (0.5% reading + 0.2%FS) ± 0.1% of F.S. -20 to 70°C 30 min for optimum accuracy 2 min for ± 2% of full scale < 2.5 seconds (to within ± 2% of full scale) < ±0.05% of Full Scale /°C < ±0.16% of reading/°C <b>Standard:</b> 500 psig Optional: 1000 psig < 0.01%of reading /psi (N <sub>2</sub> , 0-1000 psig) < 5.1 psi at full scale flow < 2% of F.S.
<b><i>Electrical</i></b> Power Requirements Analog Output Digital Output Analog Connector Digital Connector	18-38 VDC, 3.5 watts(Ethernet) 2.5 watts(RS232/485) <b>Standard:</b> 4 – 20 mA Optional: 0-10 VDC, 0-20 mA, 0-5 VDC, 1-5 VDC <b>Standard:</b> RS 232 Optional: RS 485 Optional: Ethernet <b>Std:</b> Terminal Block – M16 Cable Gland Optional: 12 pin Circular Connector 4 pin, D-coded M12	18-38 VDC, 3.5 watts(Ethernet) 2.5 watts(RS232/485) <b>Standard:</b> 4 – 20 mA Optional: 0-10 VDC, 0-20 mA, 0-5 VDC, 1-5 VDC <b>Standard:</b> RS 232 Optional: RS 485 Optional: Ethernet <b>Std:</b> Terminal Block – M16 Cable Gland Optional: 12 pin Circular Connector 4 pin, D-coded M12


<b>Mechanical</b>		
Fittings	<b>Standard:</b> 1/2" Swagelok Optional: 1/2" VCO®, 1/2" VCR®, 3/4" Swagelok, 10mm Swagelok, 3/8" male NPT, 1/2" male NPT 12mm Swagelok, 3/4"-16 SAE/MS straight thread	<b>Standard:</b> 1" Swagelok Optional: 1" VCO®, 1" VCR®, 3/4" Swagelok, 1" male NPT, 3/4" male NPT, 1 5/16"-12 straight thread
Leak Integrity	< 1x10 <sup>-8</sup> sccs He	< 1x10 <sup>-8</sup> sccs He
Wetted Materials	316L SS, Nickel 200, 302 SS, Viton®	316L SS, Nickel 200, 302 SS, Viton®
Weight (approx.)	12 lb (5.5 kg)	18 lb (8 kg)

Viton® is a trademark of DuPont Dow Elastomers, LLC.

Swagelok®, VCO® and VCR® are trademarks of the Swagelok Company.

# 2. Installation

## 2. Installation

<p><b>CAUTION</b></p> 	<p>Many of the functions described in this section require removing the enclosure front plate. Care must be taken when reinstalling this plate to ensure that the sealing gasket is properly positioned and the fasteners are secure to maintain an IP65 compliant seal.</p>
---	--

### 2.1. Receiving Inspection

Your instrument has been manufactured, calibrated, and carefully packed so it is ready for operation. However, please inspect all items for any obvious signs of damage due to shipment. Immediately advise Teledyne Hastings and the carrier if any damage is suspected.

Use the packing slip as a check list to ensure all parts are present (e.g. flow meter, power supply, cables etc.) and that the options are correctly configured (output, range, gas, connector).

If a return is necessary, obtain an RMA (Return Material Authorization) number from Teledyne Hastings' Customer Service Department at 1-800-950-2468 or [hastings\\_instruments@teledyne.com](mailto:hastings_instruments@teledyne.com).

### 2.2. Environmental and Gas Requirements

- Use the following guidelines prior to installing the flow meter:
- Ensure that the temperature of all components and gas supply are between -20° and 70° C
- Ensure that the gas line is free of debris and contamination
- Ensure that the gas is dry and filtered (water and debris may clog the meter and/or affect its performance)
- If corrosive gases are used, purge ambient (moist) air from the gas lines

### 2.3. Mechanical Connections

The meter can be mounted in any orientation unless using dense gases or pressures higher than 250 psig in which case a “flow horizontal” orientation is required. The meter’s measured flow direction is indicated by the arrow on the electronics enclosure.


A straight run of tubing upstream or downstream is *not* necessary for proper operation of the meter. The flow meter incorporates elements that pre-condition the flow profile before the measurement region. So for example, an elbow may be installed upstream from the flow meter entrance port without affecting the flow performance.

Compression fittings should be connected and secured according to recommended procedures for that fitting. Two wrenches should be used when tightening fittings (as shown in the Quick Start Guide on page iii) to avoid subjecting the flow meter body to undue torque and related stress.

The fittings are not intended to support the weight of the meter. For mechanical structural support, four mounting holes (#1/4-20 thread, 3/8” depth) are located in the bottom of the meter. The position of these holes is documented on the outline drawing in Appendix 3 (Section 6.3).

Leak-check all fittings according to an established procedure appropriate for the facility.

## 2.4. Mounting the Electronics Remotely

<p><b>CAUTION</b></p> 	<p>In order to maintain the integrity of the Electrostatic Discharge immunity both parts of the remote mounted version of the HFM-I-400 instrument must be screwed to a well grounded structure. The ferrite that is shipped with the instrument must be installed on the cable next to the electronics enclosure.</p>
---	--

The electronics enclosure can be separated and relocated up to 30 feet away from the flow meter base. This requires a cable which is supplied with the instrument if ordered as a cable mounted unit. Alternatively, a 2, 5, or 10 meter cable can be purchased separately. See section 4.2 for ordering information and part numbers.

When remote mounting the electronics enclosure, the support bracket can remain attached to either the flow meter base or the electronics. To separate the electronics enclosure from the support bracket, remove the two screws located on the back of the support bracket. To separate the flow meter base from the support bracket, remove the four screws that mount the bracket to the top of the flow meter base. Unscrew the electrical connector between electronics enclosure and the flow meter base. Remove the electronics enclosure from the flow meter base. Connect the female end of the remote electronics cable to the flow meter base and the male end to the electronics enclosure. The electronics enclosure can be mounted remotely by using the two threaded holes in the enclosure. The size and spacing of these two holes are specified on the outline drawing in Appendix 3 (Section 6.3). These holes may be used by inserting fasteners from behind through a new mounting bracket or they may be accessed from the front side by temporarily removing the enclosure panel. This enables mounting the enclosure to a wall or other solid structure. Alternatively, if the instrument was originally configured as a bracket mounted unit the bracket may be directly mounted to a support structure. The bracket mounting holes locations are the same as those for the flow meter base mounting. (See the outline drawing in Appendix 3, Section 6.3.)

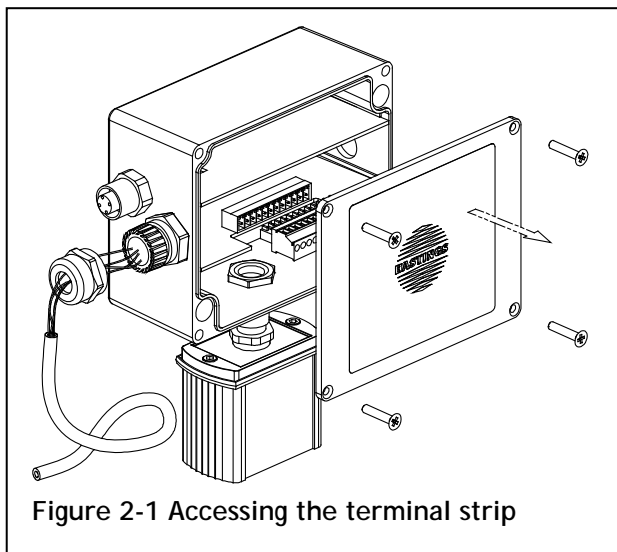


Figure 2-1 Accessing the terminal strip

## 2.5. Electrical Connection


There are two electrical connectors on the Hastings 400-I Series flow meters—an analog terminal strip (located within the electronics enclosure) and a digital connector. The analog connector provides for the power supply to the meter along with analog signals and functions. As such, its use is required for operation. The digital connector is used for communications in either of RS232, RS485, or Ethernet mode depending on the instrument's configuration. The digital connector does not have to be used if the meter is operated as an analog-only instrument.

Terminal Strip Pin-out	
(Pins numbered right to left as viewed from the front)	
1	- Power Supply
2	+ Power Supply
3	- Flow Output
4	+ Flow Output
5	+ Auxiliary Input
6	- Auxiliary Input
7	No Connection
8	Digital Common
9	Remote Zero
10	Alarm 1
11	Alarm 2
12	Alarm Common


Figure 2-2 Electrical connections for analog inputs/outputs and power

There are two possible connection methods to the analog terminal strip. The standard method is by inserting a cable through the supplied cable gland with an external jacket that meets the specifications of the following caution note and tightening down the cable gland nut securely to seal against the cable jacket.

There is also an optional sealed circular connector that may be ordered with the instrument. If this connector is ordered the internal terminal board will be connected to pins on the circular connector. This option will be supplied with the mating connector (*if a power cable was not ordered with the instrument*). This mating connector has pins that must be soldered to wires (24 - 28 AWG) in a customer supplied cable that meets the specifications in the caution note below. Other sealing collets for cable diameters other than specified below can be ordered from Bulgin PX0482 (3 - 5 mm) or PX0483 (5 - 7 mm). Ensure that the parts are installed on the cable assembly correctly before assembling. Installation and removal of the outer housing may damage the latches and prevent the connector from making a leak-free seal.



OPTIONAL CIRCULAR CONNECTOR

<p><b>CAUTION</b></p> 	<p>In order to maintain the environmental integrity of the enclosure the power/signal cable jacket must have a diameter of 0.12 - 0.35" (3 - 9 mm) for the cable gland or 0.25 - 0.275" (6.5 - 7 mm) for the circular connector. The nut on the cable gland must be tightened down sufficiently to secure the cable. This cable must be rated for at least 85°C.</p>
---	--


### 2.5.1. Power Supply

Ensure that the power source meets the requirements detailed in the specifications section. Hastings offers several power supply and readout products that meet these standards and are CE marked. If multiple flow meters or other devices are sharing the same power supply, it must have sufficient capability to provide the combined maximum current.

Power is delivered to the instrument through pins 1 and 2 of the analog terminal strip located within the electronics enclosure (see Figure 2-1). As shown in the pin-out diagram Figure 2-2, the positive polarity of the power supply is connected to pin 2 and the negative is connected to pin 1. (For a unipolar power supply, pin 1 is power common and pin 2 is +24V. For a bipolar  $\pm 15V$  power supply, pin 1 is -15V and pin 2 is + 15V.) To allow for inadvertent reversal of the power polarity, an internal diode bridge will ensure that the proper polarity is applied to the internal circuitry. A green LED located next to the terminal strip will illuminate when the meter is properly powered. The power supply inputs are galvanically isolated from all other analog and digital circuitry.

### 2.5.2. Analog Output

The indicated flow output signal is found on pins 3 and 4 of the terminal strip as shown in Figure 2-2. The negative output pin 3 is galvanically isolated from chassis ground and from the power supply input common. The 400 Series meters can be configured to provide one of many available current and voltage outputs; the standard 4 -20 mA or the optional 0 -20 mA, 0-5 Vdc, 1-5 Vdc, or 0-10 Vdc.

<p><b>NOTE</b></p> 	<p>When the meter is configured with milliamp output it cannot generate a signal that is below the zero current value; therefore the 0-20 mA unit is limited in its ability to indicate a negative flow with the analog signal.</p>
--	---

#### 2.1.1.1. Current Loop Output

The standard instrument output is a 4 - 20 mA signal proportional to the measured flow (i.e. 4 mA = zero flow and 20 mA = 100% FS). An optional current output of 0 - 20 mA (where 0 mA = zero flow and 20 mA = 100% FS) may be selected at the time of ordering.

If either current loop output has been selected, the flow meter acts as a passive transmitter. It neither sources nor sinks the current signal. The polarity of the loop must be such that pin 4 is at a higher potential than pin 3 on the flow meter terminal strip. Loop power must be supplied with a potential in

the range of 5-28 Vdc from a source external to the flow meter. The loop supply can be the same supply as that for the instrument power or it can be an isolated loop supply.

Figure 2-3 shows a typical setup using the same supply. This method requires a jumper from pin 2 to pin 4 on the terminal strip while connecting pin 3 to a wire that carries this signal to the indicator (for example, a process ammeter, data acquisition system, or PLC board). To complete the current loop, another wire carries the return signal from the flow indicator back to the negative end of the input supply. (Alternatively, the loop current can be measured on the “high potential side” by connecting the indicator between the pins 2 and 4 while connecting pin 3 to pin 1.)

Figure 2-4 shows an arrangement using a separate loop supply which is isolated from the instrument power supply.

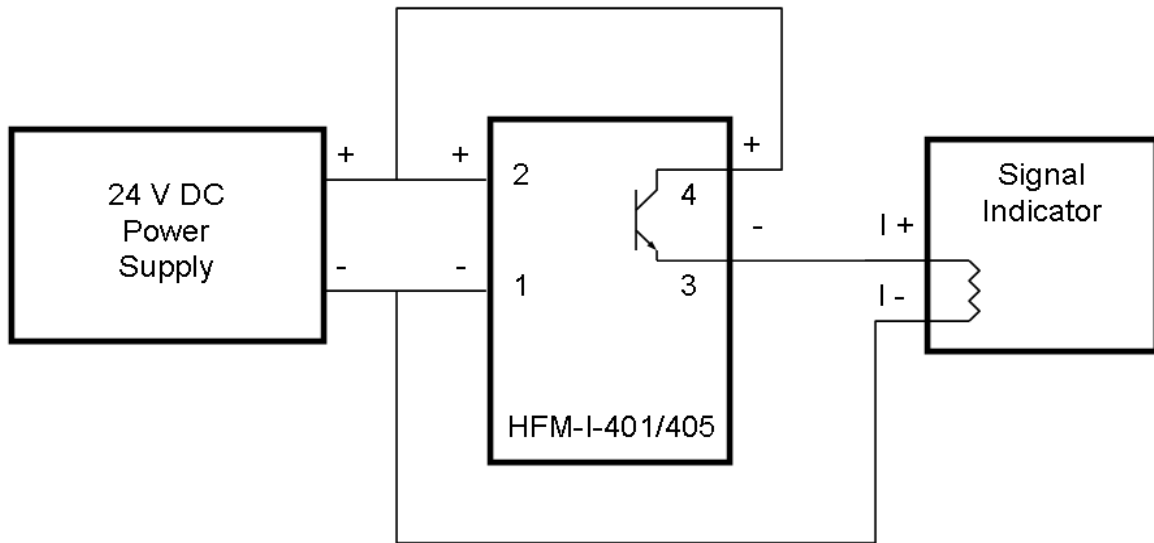


Figure 2-3 Wiring diagram showing the current loop supply powered by the instrument supply

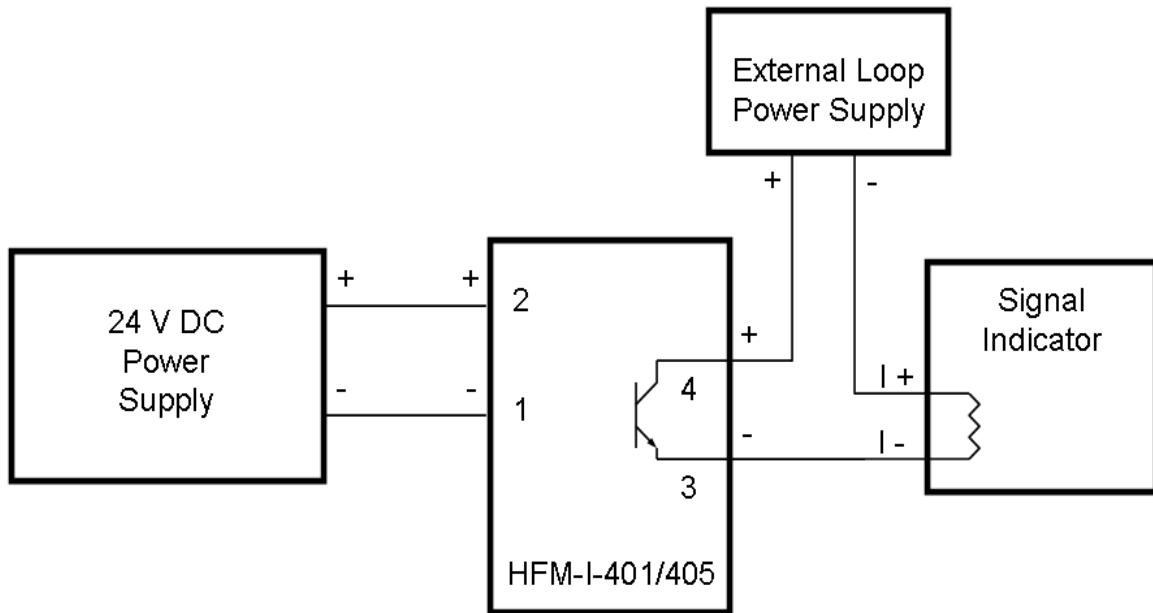


Figure 2-4 Wiring diagram showing the current loop powered by an external supply



### 2.1.1.2. Voltage output

If the flow meter is configured for a voltage output, the signal will be available as a positive potential on pin 4 relative to pin 3 of the terminal strip. Since these pins are galvanically isolated, the signal cannot be read by an indicator between pin 4 and pin 1 of the terminal strip. Pin 3 must be used as the return to properly read the output on pin 4. If an output that is referenced to power supply common is desired then pins 3 and 1 must be connected. It is recommended that these signals be transmitted through shielded cable, especially for installations where long cable runs are required or if the cable is located near equipment that emits RF energy or uses large currents.

Note: When the meter is configured with a voltage output it cannot generate a signal that is more than a few mV below the zero volt value; therefore the 0-5 volt and 0-10 volt units are limited in their ability to indicate a negative flow with the analog signal.

## 2.6. Digital Connection

The digital signals are available on a sealed female D-coded M12 connector that is designed for use on industrial Ethernet connections. There are many options for connecting to the M12. Hastings offers an 8 foot cable (stock# CB-RS232-M12) with a compatible male M12 connector to a 9-pin D connector suitable for connecting the 400 I series instrument directly to the RS232 port on a PC. A cable to convert USB to RS232 9-pin is available from Hastings (stock# CB-USB-RS232). Also, a 5 meter M12 male-male cable suitable for digital communications can be purchased from Hastings (stock# CB-ETHERNET-M12). Other length cables are available from Lumberg (#0985 342 100/5 M) or Phoenix. Converters from the M12 connector to a standard modular Ethernet connector are available from Hastings or from Lumberg (#0981 ENC 100). A compatible M12 connector suitable for field wiring can be acquired from Harting (21 03 281 1405) or Mouser (617-21-03-281-1405).

The pin-out for the digital connector is shown in Figure 2-5.

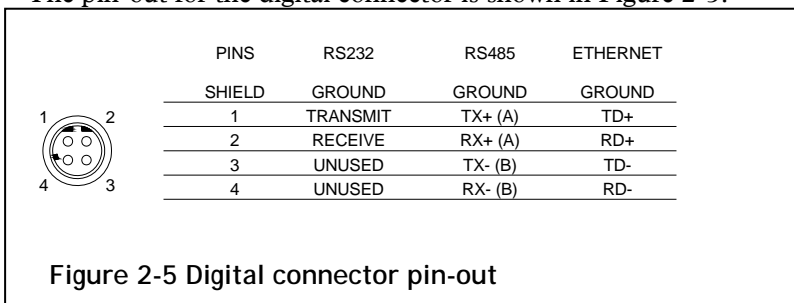


Figure 2-5 Digital connector pin-out

## 2.7. Digital Configuration

A Hastings 400-I Series flow meter is available with one of three digital communications interfaces, RS232, RS485, or Ethernet. Unless specified differently at the time of ordering, the flow meter is configured for RS232 operation. For each interface, there are changes that can be made to the configuration, either via software or hardware settings. A brief overview of these is included here. For more detailed information, consult the Hastings 400 Series Software Manual.

### 2.7.1. RS-232

The default configuration for the RS-232 interface is 19200 baud, 8 data bits, no-parity, one stop bit. The baud rate is software selectable and can be overridden by a hardware setting. Hardware settings for RS-232 and RS-485 are enacted on 12 pin jumper field located on the left end of the top circuit board in the electronics enclosure. Only the state of jumpers 1, 2, and 5 affect the RS-232 operation. These jumpers are installed vertically over two pins when enabled and are numbered from left to right. Jumper 1 must be disabled for RS-232; jumper 2 is used to select

Jumper	Enabled	Disabled
1	RS485	RS232
2	Half Duplex	Full Duplex
3	TX Terminated	Unterminated
4	RX Terminated	Unterminated
5	9600 Baud	Software Selected
6	Addr = 99	Software Selected

Figure 2-6 Functions for digital jumper field

half or full duplex; and jumper 5 is enabled when a hardware override of the baud rate (forcing it to 9600) is desired. These functions are summarized in Figure 2-6.

### 2.7.2. RS-485

If RS485 is specified on the order, the flow meter is set to the default values: address 61, unterminated Tx and Rx lines. While the default address is 61, all instruments will respond to an address of FF. Hardware settings for RS-232 and RS-485 are enacted on 12 pin jumper field located on the left end of the top circuit board in the electronics enclosure. Only the state of jumpers 1, 3, 4, and 6 affect the RS-485 operation (see Figure 2-6). These jumpers are installed vertically over two pins when enabled and are numbered from left to right. Jumper 1 must be enabled for RS-485. Enabling jumpers 3 and 4 effect a 120 ohm resistance across the transmit and receive signal pairs respectively. These should only be enabled in the last instrument on a long buss. Enabling jumper 6 forces the address to 99; this is sometimes used when initiating communications.

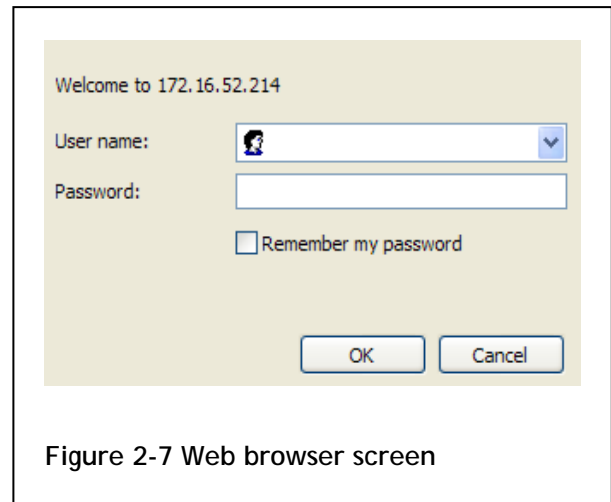


Figure 2-7 Web browser screen

### 2.7.3. Ethernet

If Ethernet is specified on the order, the flow meter has IP address 172.16.52.250 and communication port number 10001. There are no hardware settings required or available to modify the configuration. This IP address can be changed using a web browser to access the configuration of the instrument by typing the IP address into the URL section of the browser. Press OK to ignore the username/password screen as shown in Figure 2-7. Select the new IP address under the network section of the web page configuration utility. If this address cannot be reached, the instrument can be reconfigured by downloading and installing the Lantronix Device Installer routine from: <http://www.lantronix.com/device-networking/utilities-tools/device-installer.html>.

A standard web browser cannot be used to send and receive messages (such as flow readings) from the main processor of the flow meter. An Ethernet capable software program is required to communicate with the meter's processor. Suitable examples of such programs are "Hyperterminal" (typically installed as standard on PCs and shown in Figure 2-8) or custom Ethernet capable software such as LabView®. For more information see the Software Manual.

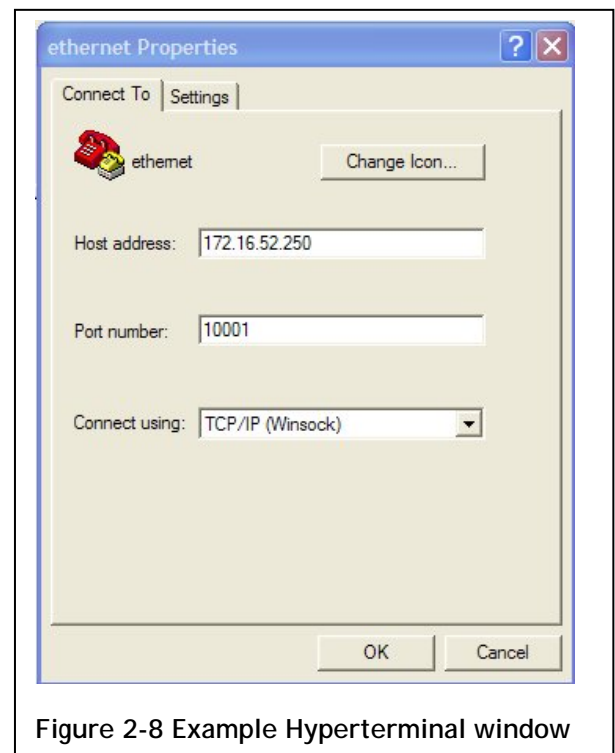


Figure 2-8 Example Hyperterminal window

## 2.8. Alarm Output Connection

The Hastings 400 Series flow meters include two software settable hardware alarms. Each is an open-collector transistor functioning as a semiconductor switch designed to conduct DC current when activated. (See Figure 2-9.) These sink sufficient current to illuminate an external LED or to activate a remote relay and can tolerate up to 70Vdc across the transistor. The alarm lines and the alarm common are galvanically isolated from all other circuit components. The connections for Alarm 1, Alarm 2 and Alarm Common are available as pins 10, 11, and 12 respectively on the analog terminal strip (see Quick Start Guide on page iii).

Since the alarms act as switches they do not produce a voltage or current signal. However, they can be used to generate a voltage signal on an Alarm Out line. This is done by connecting a suitable pull-up resistor between an external voltage supply and the desired alarm line while connecting Alarm Common to the common of the power supply. When activated, the alarm line voltage will be pulled toward the alarm common line generating a sudden drop in the signal line voltage.

To use the alarm to illuminate an LED connect the positive terminal of the LED to a suitable power supply and connect the other end to a current limiting resistor. This resistor should be sized such that the current is less than 20 mA when the entire supply voltage is applied. Connect the other end of the resistor to Alarm 1 or Alarm 2. Connect Alarm Common to the circuit common of the power supply. When activated, the alarm line is pulled toward the alarm common generating sufficient current through the LED to cause it to illuminate.

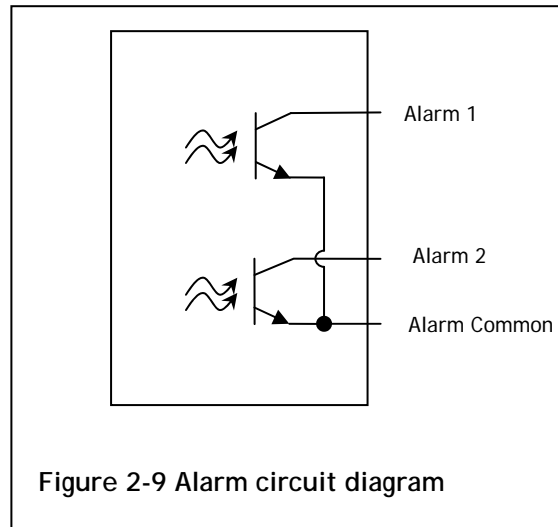


Figure 2-9 Alarm circuit diagram

Figure 2-10 shows an example of the LED circuit arrangement applied to Alarm 1 while Alarm 2 is configured with a suitable pull-up resistor to provide a voltage output on an Alarm Out line.

Since the Alarm Common is a shared contact, if both alarms are being used independently they must each be wired such that the current passes through the external signaling device before reaching the alarm line.

The alarm settings and activation status are available via software commands and queries. The software interprets an activated Alarm 1 as an “Alarm” condition, while an activated Alarm 2 is interpreted as a “Warning” condition. The software manual includes the detailed descriptions for configuring and interpreting the activation of these alarms.

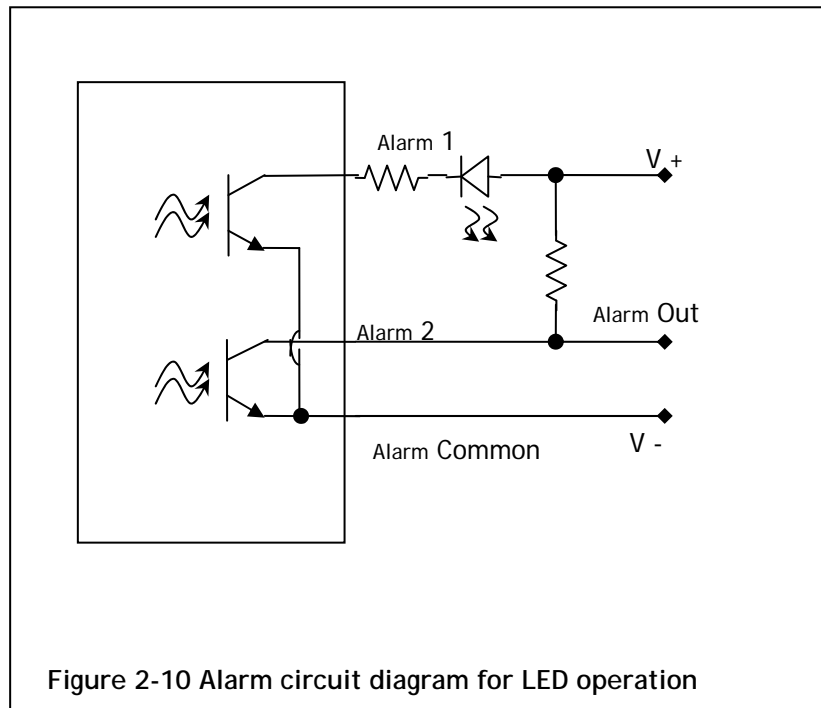


Figure 2-10 Alarm circuit diagram for LED operation

## 2.9. Auxiliary Input Connection

The Hastings 400 Series flow meters provide an auxiliary analog input function. The flow meter can read the analog value present between pins 5 and 6 on the terminal strip (as shown in Figure 2-2) and make its value available via the digital interface. The accepted electrical input signal is the same as that configured for the analog output signal (4 – 20 mA, 0 -20 mA, 0-5 Vdc, 1-5 Vdc, or 0-10 Vdc). Unlike the analog output signal, which is isolated and capable operating at common mode offsets of over 1000V, the analog input signal cannot be galvanically isolated from ground potential.

## 2.2. Rotary Gas Selector

The Hastings 400 Series flow meters can have up to eight different calibrations stored internally. These are referred to as gas records. These records are used to select different gases, but they can also be useful in other ways; for instance reporting the flow in an alternate range, flow unit or reference temperature. The records are referred to by their number label from #0 – #7.

The first six records will, by default, be setup for most common six gases as shown in Figure 2-11. If a gas other than one of these six is specified on the customer order it will be placed in record #6. If a second different gas is selected, it will be placed in record #7. If multiple different gases or ranges are specified they will replace some of the standard six gases.

Record#	Gas
0	Nitrogen
1	Air
2	Helium
3	Hydrogen
4	Argon
5	Oxygen
6	Custom
7	Custom

Figure 2-11 Gas record table

The purchased calibration certificate is provided for the gas (or gases) specified by the customer when ordering. This gas will be indicated with an “X” on the Gas Label (diagram below) that is located on the top of the 400 Series Mass flow meter’s electronics enclosure. The remaining gas records will have a different full scale value and an unverified calibration. The full scale range can be calculated by using the Gas conversion factor or GCF. A comprehensive list is found in Appendix 2 in this manual.

<input checked="" type="checkbox"/> 0 N <sub>2</sub>	<input type="checkbox"/> 4 Ar	X= cal report generated (others use GCF)
<input type="checkbox"/> 1 Air	<input type="checkbox"/> 5 O <sub>2</sub>	
<input type="checkbox"/> 2 He	<input type="checkbox"/> 6	
<input type="checkbox"/> 3 H <sub>2</sub>	<input type="checkbox"/> 7	
	S/N	

Record#	Gas	Full Scale Range
0	Nitrogen	100 slm
1	Air	100.15 slm
2	Helium	140 slm
3	Hydrogen	100.38 slm
4	Argon	140.37 slm
5	Oxygen	97.95 slm
6	Custom	Not included if not specified
7	Custom	Not included if not specified

### Example 1

To convert the calibration of a full scale range of 100 slm of Nitrogen to the other full scale ranges:

$$FS_2 = FS_1 \frac{GCF_2}{GCF_1}$$

#### 1. Calculate full scale value of Helium

Calibrated gas = Nitrogen ( $GCF_1 = 1.000$ )

Full scale range ( $FS_1$ ) = 100 slm

Secondary gas ( $FS_2$ ) = Helium ( $GCF_2 = 1.40$ )

$1.40/1 = 1.40$ ,  $1.40 \times 100 = 140$  slm of Helium

#### 2. Calculate full scale value of Hydrogen

Calibrated gas = Nitrogen ( $GCF_1 = 1.000$ )

Full scale range ( $FS_1$ ) = 100 slm

Secondary gas ( $FS_2$ ) = Hydrogen ( $GCF_2 = 1.0038$ )

$1.0038/1 = 1.0038$ ,  $1.0038 \times 100 = 100.38$  slm of Hydrogen

## **Example 2- Changing the active gas record**

Selecting the active gas record is accomplished in one of two ways:

1. Hardware setting
2. Software setting

### **Hardware:**

The hardware setting is selected by accessing a rotary encoder on the upper PC board in the electronics enclosure. When set to a number position from 0 to 7 it activates the corresponding gas record. If a number greater than 7 is selected, then gas record control is passed to software.

### **Software:**

See Section 3.9 Multi-Gas Calibrations and the software manual for more information about the software control capabilities.


The software setting will override the hardware settings. If gas records are changed through the software setting and the rotary encoder is not changed, the software setting will be active. However, when the meter is powered down and subsequently powered up, the active setting will be based on the rotary encoder setting.

## **2.10. Electrical Remote Zero Connection**

The Hastings 400 Series allows the flow meter zeroing operation to be activated remotely using pins 8 and 9 of the analog terminal strip. (See Drawing in Quick Start Guide.) If these pins are connected together, the meter initiates an internal routine that measures the current reading, stores it in nonvolatile memory as a zero offset, and removes this value from all subsequent readings. When the pin 9 is electrically isolated the flow meter operates normally. The typical implementation of this type of remote zeroing operation involves connecting a remote switch or relay to pins 8 and 9 of the terminal strip. (For more about the zeroing operation, see Section 3.4)

## **2.11. Check Installation Prior to Operation**

Before applying gas to the meter it is advisable to ensure that the mechanical and electrical connections and digital communications (if applicable) are established and operating properly. This can be done by following the guideline procedure below:

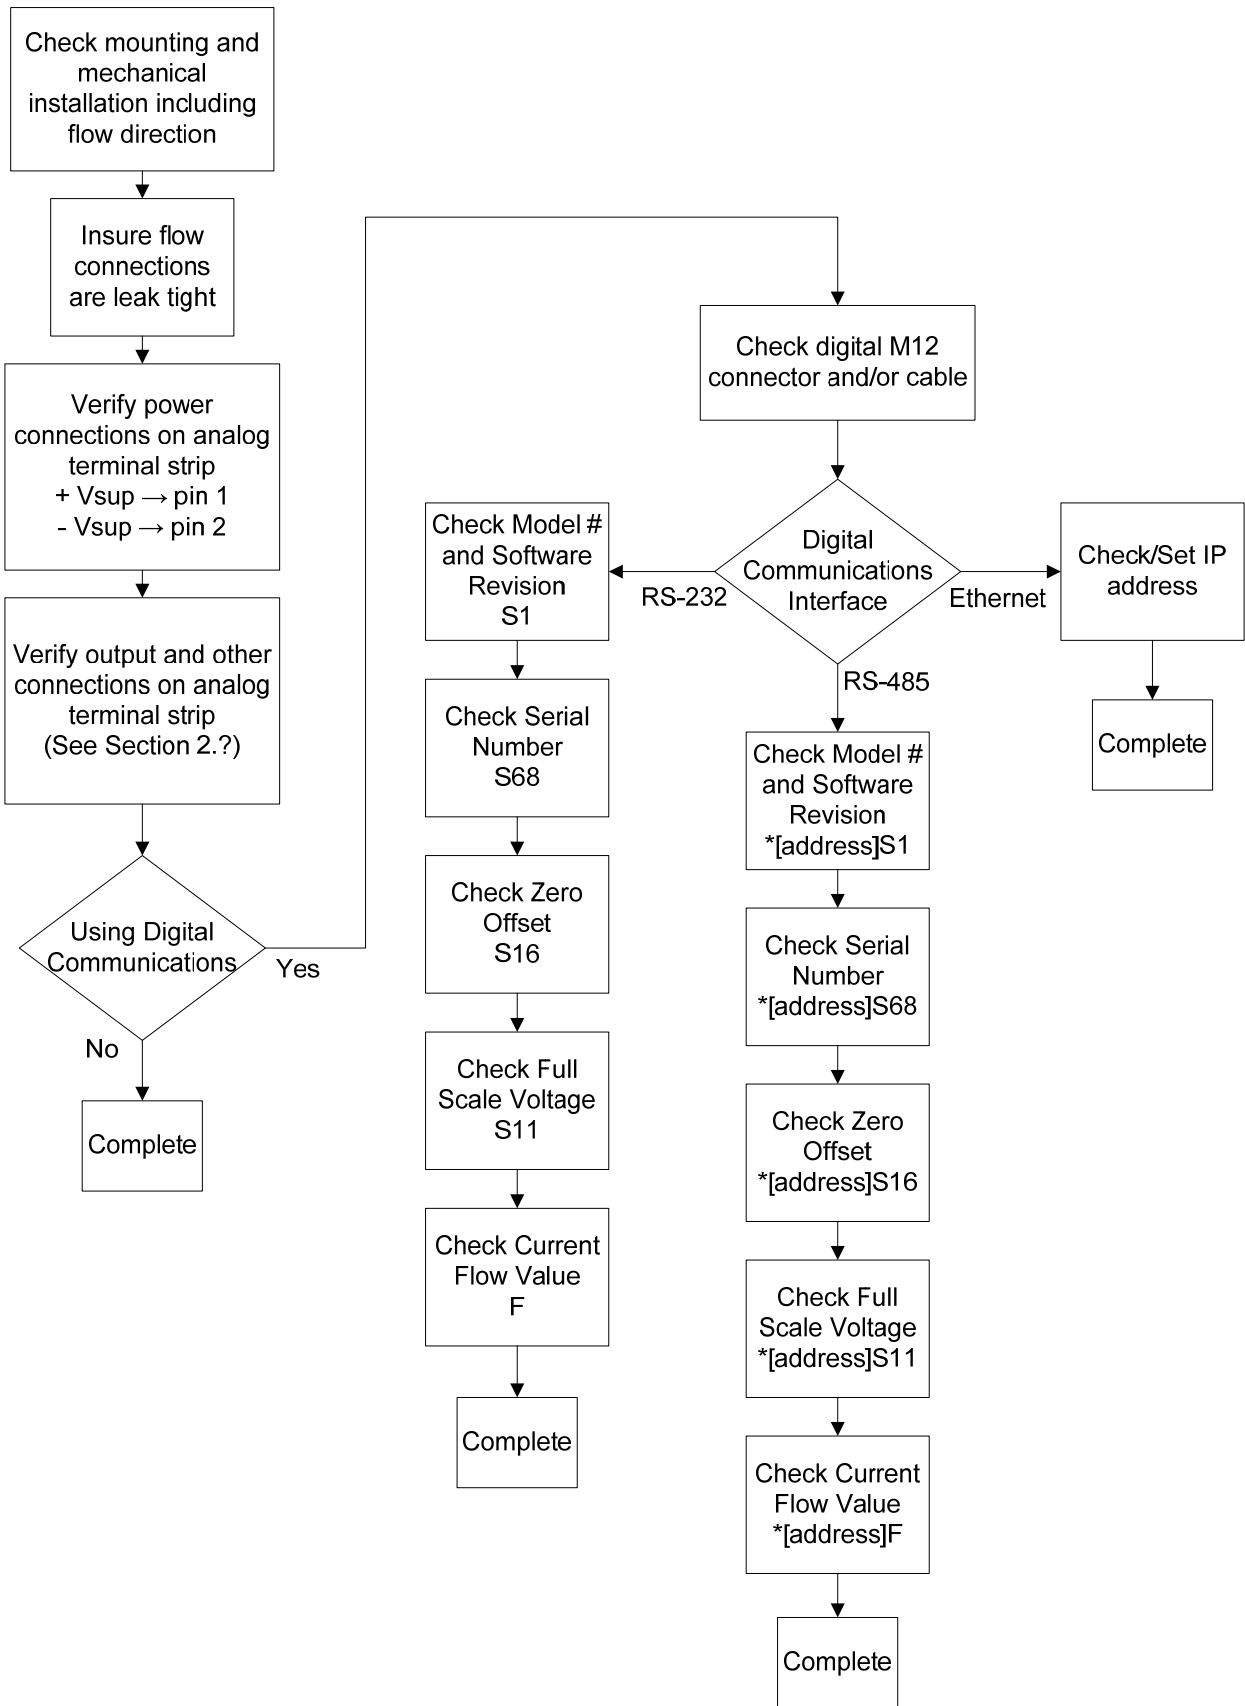

# 3. Operation

## 3. Operation

The Hastings 400 Series flow meters are designed for operation with clean dry gas and in specified environmental conditions (See Section 1.2). The properly installed meter measures and reports the mass flow as an analog signal and, depending on the configuration and set up, as a digital response. Other features can assist in the measurement operation and provide additional functions. The following sections serve as a guide for correctly interpreting the analog and digital flow output, optimizing the performance, and using the additional features of the instrument.

### 3.1. Environmental and Gas Conditions

For proper operation, the ambient and gas temperatures must be such that the flow meter remains between -20 and 70°C. Optimal performance is achieved when the environment and gas temperatures are equilibrated and stable. The 400 I series is intended for use with clean, non-condensing gases only. Particles, contamination, condensate, or any other liquids which enter the flow meter body may obstruct critical flow paths in the sensor or shunt, thus causing erroneous readings.

### 3.2. Interpreting the Analog Output

The analog output signal is proportional to mass flow rate. Each instrument is configured to provide one of the available forms of analog output as described in Section 2.2. The signal read by an indicator (for example, a process ammeter, data acquisition system, or PLC board) can be mapped to the measured flow rate by applying the proper conversion equation selected from the table below.

Table 3-1 The Signal → Flow mapping equations

Analog Output Configuration	Mapping Equation
4 -20 mA	$\text{Flow} = \text{FS flow} * (\text{I}_{\text{out}} - 4) / 16$
0 -20 mA	$\text{Flow} = \text{FS flow} * \text{I}_{\text{out}} / 20$
0 - 5 Vdc	$\text{Flow} = \text{FS flow} * \text{V}_{\text{out}} / 5$
0 - 10 Vdc	$\text{Flow} = \text{FS flow} * \text{V}_{\text{out}} / 10$
1 - 5 Vdc	$\text{Flow} = \text{FS flow} * (\text{V}_{\text{out}} - 1) / 4$

Alternatively an analog display meter can indicate the flow rate directly in the desired flow units by setting the offset and scaling factors properly.

The flow meter is typically able to measure and report flow which slightly exceeds the full scale value. Reverse or “negative” flows are indicated (to values up to 25% of full scale) by meters with 4-20 mA or 1-5 volt output. However, meters with 0-5 Volt, 0-10 volt or 0-20 mA output are limited in their ability to indicate a negative flow with the analog signal since negative currents or voltages cannot be generated by the meter’s circuitry.

### 3.3. Digital Communications

Many of the Hastings 400 Series flow meter’s operating parameters such as the flow measurement, alarm settings, status, or gas type can be read or changed by digital communications. The digital communications commands and protocols for each particular interface (RS-232, RS-485, and Ethernet) are treated in detail in the Software Manual. However, the function and interpretation of flow output and auxiliary input are also briefly presented here.

### 3.3.1. Digitally Reported Flow Output

The flow rate can be read digitally by sending an ascii “F” command (preceded by the address for RS-485). The instrument will respond with an ascii representation of the numerical value of the flow rate in the units of flow specified on the nameplate label.

*Example: A meter with RS-232 communications, calibrated for 500 slm FS N<sub>2</sub>*

Computer transmits: {F}

HFM flow meter replies: {137.5}

*This is interpreted as 137.5 slm of nitrogen equivalent flow.*

In most situations, the flow meter can measure beyond its range (i.e. a flow that exceeds the full scale or a reverse flow) and report the value via the digital output. While the meter can perform beyond its stated range, the accuracy of these values has not been verified during the calibration process. Flows that exceed 160% of the nominal shunt range (S46 response) should not be relied upon. See the software manual for further information.

### 3.3.2. Digitally Reported Analog Input

The flow meter can read the analog value present on pins 5 & 6 of the terminal strip (See Section 2.9). This function is typically used to read the analog output from a nearby sensor such as a pressure sensor or vacuum gauge. This value is spanned for the same range as the analog output signal; it reads volts for flow meter configured for 0-5, 0-10 or 1-5 volt output and milliamps for a flow meter configured for 0-20 or 4-20 milliamp output. The value is accessed via the “S26” software query as shown below.

*Example: A meter calibrated for 0-5 volt output and RS-232 communications.*

Computer transmits: {S26}

HFM flow meter replies: {2.532}

*This is interpreted as 2.532 volts.*

## 3.4. Zeroing the Instrument

A proper zeroing of the flow meter is recommended after initial installation and warm-up. It is also advisable to check the zero flow indication periodically during operation. Any uncertainty at zero flow is an offset value which affects all subsequent flow readings. The frequency of these routine checks depends on factors such as: the environmental conditions, the desired level of accuracy, and the desire to measure low flow rates (relative to the meter full scale). To achieve the most precise flow readings, the zeroing procedure is done while the meter is at the expected operating conditions including temperature, line pressure, and gas type. This is especially true for cases where the flow meter is operating at high pressure or with very dense gas.

### 3.4.1. Preparing for a Zero Check

Before checking or adjusting the meter’s zero, the following three requirements must be satisfied:

**Warm-up** – The instrument must be powered and in the operating environment for at least 30 minutes. Even though the meter will operate within a few minutes after power is applied, the entire warm-up period is needed to establish a suitable zero reading.


**No Flow** – There must be an independent method to ensure that all flow through the instrument has completely ceased before checking or adjusting the zero. Typically this is achieved by closing valve downstream from the flow meter and waiting a sufficient time for any transient flow to decay. This is especially critical for low flow units that have long piping lengths before or after the flow meter. In such situations, it can require a significant settling time for the flow cease and enable a precise zero.

**Stability** – The flow meter must stabilize for at least 3 minutes at zero flow, especially following a high flow or overflow condition. This will allow all parts of the sensor to come to thermal equilibrium resulting in the best possible zero value.



### 3.4.2. Adjusting Zero


The pre-conditions required for a zero check must also be followed when making a zero adjustment. The zero adjustment is a digitally controlled “reset” type operation. When commanded, the meter initiates an internal routine that performs the following sequence: measure the current flow reading, store it in nonvolatile memory as a zero offset, and remove this value from all subsequent readings.

<b>NOTE</b> 	If the instrument is inadvertently or improperly zeroed, for example while flow is passing through the instrument, the flow reading is subtracted from all future flow readings. This will produce large flow indication errors.
--	--

This offset value can be accessed via the “S40” software query. The reported value is relative to an internal, un-spanned sensor voltage. As an interpretation guideline, an offset that exceeds 0.15 volts typically indicates that a faulty zero value is present.

There are three different methods to activate the zero reset function--manually, digitally, and electrically.

Manually – With the electronics enclosure cover plate removed, a pushbutton switch on the upper board is pressed.

<b>CAUTION</b> 	Accessing the manual zero pushbutton requires removing the enclosure front plate. Care must be taken when reinstalling this plate to ensure that the sealing gasket is properly positioned and the fasteners are secure to maintain an IP65 compliant seal.
---	---


Digitally – A “ZRO” (“\*[address]ZRO” for RS485) command is received properly by the flow meter’s main processor.

Electrically – An external contact closure generates continuity between pins 8 and 9 of the terminal strip.

#### 3.4.2.3.5. Over-range

The thermal mass flow sensor heats a portion of the gas in order to measure the flow rate. As the flow increases the heated tube is cooled and the slope of the sensor output versus the flow rate decreases. The sensor linearization function corrects for this effect while the flow rate is within the normal operating region. If the flow exceeds the normal operating region the digital flow indication will continue to track this increase with a reduced accuracy. The analog flow will also indicate this overflow condition until the circuitry reaches its limits (approximately 10 -25% over-range).

As the flow continues to increase above the normal operating region the sensor will be cooled sufficiently that the output of the sensor will reach a peak value around 2 – 4 times the full scale flow rate. If the flow continues to increase the sensor output will begin decreasing and the digital flow will indicate a decreasing flow rate even though the flow is actually getting increasing. At approximately 3 – 7 times the full scale flow rate the sensor output will drop within range of the normal output and even the analog output will record an on-scale flow rate when there is a very large over range flow rate.

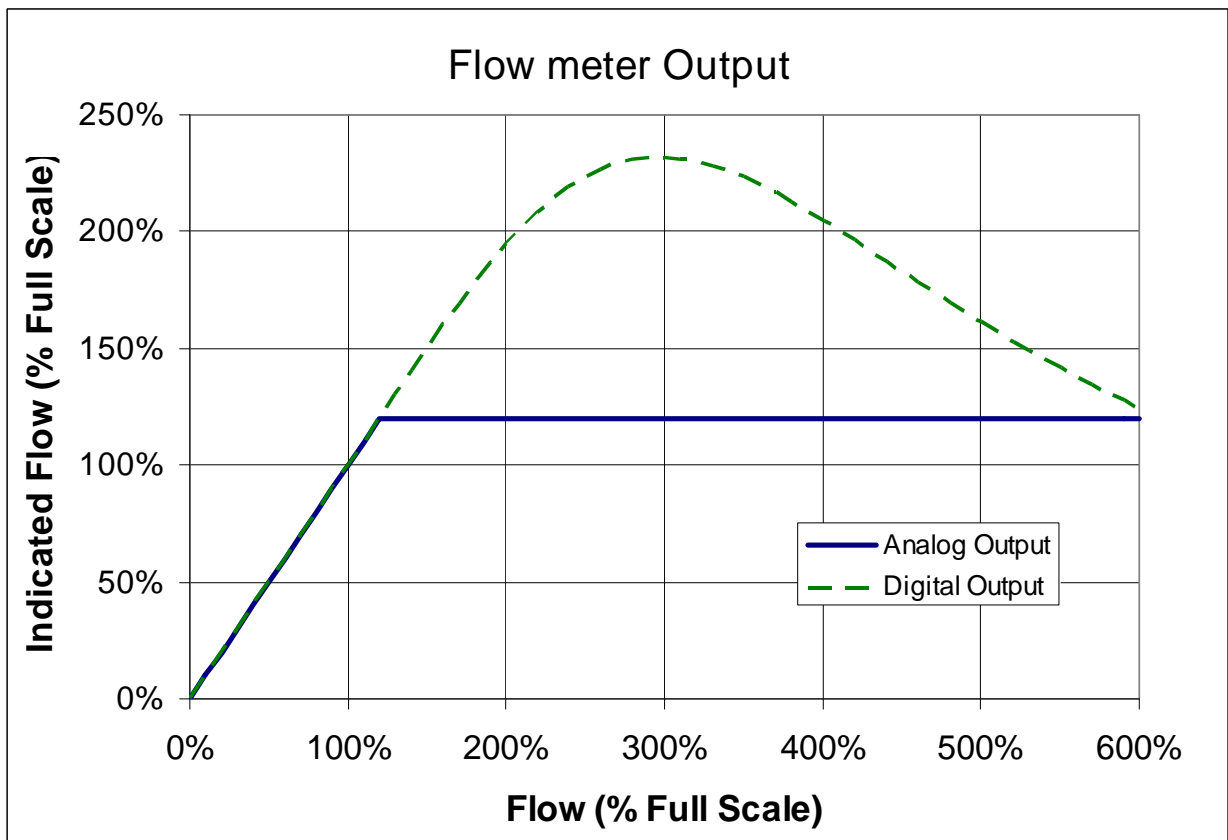

### 3.4.2.3.6. Reverse Flow

If the flow through the flow meter reverses and flow begins to enter the exit of the flow meter and leave through the entrance of the flow meter the flow meter will measure this flow and report it digitally with reduced accuracy. The analog output will also indicate this by either generating a negative output voltage or decreases the current output below 4 mA, depending on whether a voltage or current output has been selected.

### 3.7. High Pressure Operation

When operating at high pressure, the meter's performance can be affected in two distinct and separate ways—a zero shift and a span (calibration) shift.

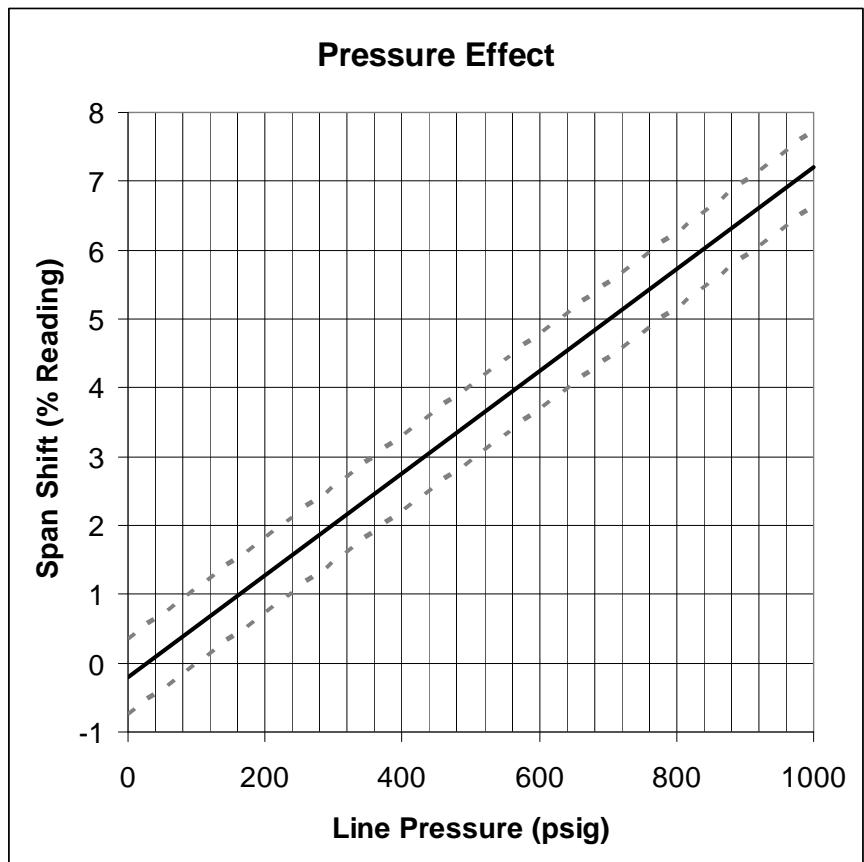


Figure 3-1 The pressure effect on flow calibration (for nitrogen)

### 3.7.1. Zero Shift

The zero offset can occur as the result of natural convection flow through the sensor tube if the instrument is not mounted in a level orientation with flow horizontal. This natural convection effect causes a zero shift proportional to the system pressure. The overall effect is more pronounced for gases with higher density. Normally the shift is within the allowable zero offset range and can be removed by activating the zero reset at the operating pressure.

### 3.7.2. Span Shift

The gas properties which form the basis for the flow measurement, such as viscosity and specific heat, exhibit a slight dependence on the gas pressure. Fortunately, this pressure dependence is predictable and can be corrected for in cases where it has an impact on accuracy (typically only significant for pressures in excess of 100 psig). The graph shown in Figure 3-1 shows the expected span shift as a function of pressure for nitrogen. This behavior is similar for most diatomic gases (O<sub>2</sub>, H<sub>2</sub>, etc), whereas this effect is insignificant for the monatomic gases (He, Ar, etc). This span shift must be considered and accounted for as appropriate for accurate flow measurements at high pressure conditions.

## 3.8. Warnings/Alarms

There are two alarm contacts on the terminal strip connector within the electronics enclosure (See Section 2.8). These function as isolated semiconductor switches sharing a single, isolated common line. In its normal state each switch is “open”; when an alarm is activated the switch is “closed”.

The meter’s processor can be configured via the digital interface to establish the internal condition for activating each alarm. There are many choices for internal alarms and warnings including overflow, underflow, or various instrument error conditions. Each alarm can also be given a selectable “wait time”—a period for which it must remain in the alarm condition before the physical alarm is activated. See the Software Manual for detailed alarm setting and configuration information.

## 3.9. Multi-gas Calibrations

The Hastings 400 Series flow meters can have up to eight different calibrations stored internally. These are referred to as gas records. These records are typically used to represent different gases, but they can also be useful in other ways; for instance reporting the flow in an alternate range, flow unit or reference temperature. The records are referred to by their number label from #0 – #7. The first six records are, by default, setup for the same range in the most common six gases as shown in Figure 2-11. If a gas other than one of these six is specified on the customer order it will be placed in record #6. If a second different gas is selected, it will be placed in record #7. If multiple different gases or ranges are specified they will replace some of the standard six gases. Only the gas(es) specified on the order will be verified. The other records will use nominal gas factors to approximate the gas sensitivity until an actual calibration is performed to correct for individual instrument variations. Selecting the active gas record can be done in one of two ways—a hardware setting or a software setting. The hardware setting is done by accessing a rotary encoder on the upper PC board in the electronics enclosure. When set to a number position from 0 to 7 it activates the corresponding gas record. When set to a number greater than 7, the gas record control is passed to software. If the software setting mode is enabled, then the “S6” digital command can be used to set the active gas record as shown in the example below.

*Example: To first determine and then change the active gas record using RS-232,*

Computer transmits: {S6}


HFM flow meter replies: {0}


*This indicates that gas record #0 is currently active.*

Computer transmits: {S6=4}

*This changes the active gas record to #4.*

See the Software Manual for further information including how to setup a new gas record and how to reconfigure an existing gas record.

<p><b>CAUTION</b></p> 	<p>Accessing the rotary encoder requires removing the enclosure front plate. Care must be taken when reinstalling this plate to ensure that the sealing gasket is properly positioned and the fasteners are secure to maintain an IP65 compliant seal.</p>
---	--

<p><b>NOTE</b></p> 	<p>The software command to change the active gas record will not be executed unless the rotary encoder is set to a number greater than 7. However, the software query will return the current active gas record number even when it has been set by the hardware.</p>
--	---

### 3.10. Flow Totalization

The Hastings 400 Series flow meters are capable of providing a value for the “total amount of gas” that has passed through the flow meter since the last time the totalization function was reset. This value can be used to determine for example, the amount of gas used to fill a chamber or drawn from a supply vessel. To initialize the totalization function, reset the totalized flow value to zero using the S36 digital command as shown in the example below. All subsequent flow readings are added over time and stored as the totalized flow value. The totalized flow value can be read by querying the flow meter digitally as in the example below. The totalized flow is reported in the flow units chosen for the active gas without the time unit. For example, if the flow units are standard liters per minute, the totalized flow is reported in standard liters; if flow units are standard cubic feet per hour, the totalized flow is reported in standard cubic feet.

*Example: For a 100 slm FS flow meter, to first reset/start the flow totalization function and then later read the value using RS-232,*

Computer transmits: {S36=0}

*This resets the totalized value to zero and starts the totalization function. At some point later in time:*

Computer transmits: {S36}

HFM flow meter replies: {45.7}

*This is interpreted as a total gas amount of 45.7 standard liters has passed through the meter since the flow totalizer was started.*

### 3.11. Additional Digital Capabilities

The Hastings 400 series flow meters have a wide selection of other functions, operating parameters, and values that can be reported and configured via digital communications such as the calibration date, the instrument temperature, the number of hours that gas has been flowing, etc. See the Software Manual for detailed information on these additional digital features.

## 4. Parts and Accessories

### 4. Parts & accessories

These are parts and accessories that are available by separate order from Teledyne Hastings Instruments.

#### 4.1. Power Pod – Power & Display units

##### THPS-100 Singel Channel Power Supply



The Teledyne Hastings Instruments microprocessor based Power<sup>Pod</sup>-100 Thermal Mass Flow Power Supply is a self-contained power supply and display for gas thermal mass flow meters, pressure transducers or any device with a voltage output. The unit features an automatically generated set point (0-5V or 0-10V), making it ideal for use with thermal mass flow controllers and pressure controllers. Features include 4.5display,  $\pm 15$  volt, 250mA transducer supply and an integrated  $\pm 15$ vdc @ 250ma power supply is available providing a well regulated, short circuit and thermal overload protected output, and CE compliance.

See the Teledyne Hastings Instruments Product Bulletin for the complete specification on this product.

##### THPS-400 Four Channel Power Supply



The Teledyne Hastings Instruments Digital 4-Channel Power<sup>Pod</sup> is featured in a half-rack profile for simple drop-in replacement of the existing Model 200 and 400 units, or be used as a bench top unit.

The Power<sup>Pod</sup>-400 is equipped with a four line by twenty-character, vacuum fluorescent display (VFD). The display emulates a liquid crystal display in its command structure but the VFD gives the unit a greater viewing angle than available with most conventional LED or LCD displays.

The Power<sup>Pod</sup> incorporates many features including an integrated totalizer with a count-up or count-down option; user selected filtering of readings; serial or Ethernet communications.

The unit also offers a simultaneous display of all four channels or selective blanking of unused channels, ratio control with analog outputs for stacking multiple power supplies, and easy to follow menu driven calibration and setup.

The digital design of the Power<sup>Pod</sup> allows the user to set both the minimum and maximum display values corresponding to specific voltage or current inputs. One advantage of this approach is that it negates the need to access hard to reach transducers to re-zero them. Should the analog signal from the transducer change due to a zero shift, the digital counts seen by the Power<sup>Pod</sup> can be changed to display zero either manually from the front panel or via serial communication with the unit.

## 4.1. Fittings

<b>Fittings</b>	<b>Hastings#</b>
HFM-I-401	
1/2" Swagelok Fittings	41-03-086
1/2" VCO Fittings	41-03-119
1/2" VCR Fittings	41-03-090
3/4" Swagelok Fitting	41-03-152
10 mm Swagelok	41-03-153
3/8" Male NPT	41-03-154
1/2" Male NPT	41-03-155
12 mm Swagelok	41-03-160
3/4-16 SAE/MS Straight Female (no fitting)	N/A
HFM-I-405	
1" Swagelok fitting	41-03-142
3/4" Swagelok	41-03-149
1" VCO Fitting	41-03-147
1" VCR fitting	41-03-148
1" Male NPT	41-03-150
3/4" Male NPT	41-03-151
1 5/16-12 Female SAE/MS straight thread (no fitting)	N/A

## 4.2. Cables

<b>Description</b>	<b>Hastings Stock#</b>
<b>Remote Electronics Cables</b>	
2 meter cable remote mounting cable	CB-8P-M12-2MRA
5 meter remote mounting cable	CB-8P-M12-5MRA
10 meter remote mounting cable	CB-8P-M12-10MRA
401 Local Bracket - mount direct to sensor	14-03-002
405 Local Bracket - mount direct to sensor	14-03-001
<b>Digital Communications</b>	
9 pin RS232 to 400 series M12 connector	CB-RS232-M12
Digital M12 connector to M12 connector	CB-ETHERNET-M12
USB to 9 pin RS232 connector	CB-USB-RS232
RJ45 Ethernet to M12 Ethernet connector	CB-RJ45-M12
<b>Analog I/O</b>	
8 foot D connector to 8 bare leads	CB-D15-Lead-8
25 foot D connector to 8 bare leads	CB-D15-Lead-25
100 foot D connector to 8 bare leads	CB-D15-Lead-100

# 5. WARRANTY

## 5. Warranty

### 5.1. Warranty Repair Policy

Hastings Instruments warrants this product for a period of one year from the date of shipment to be free from defects in material and workmanship. This warranty does not apply to defects or failures resulting from unauthorized modification, misuse or mishandling of the product. This warranty does not apply to batteries or other expendable parts, nor to damage caused by leaking batteries or any similar occurrence. This warranty does not apply to any instrument which has had a tamper seal removed or broken.

This warranty is in lieu of all other warranties, expressed or implied, including any implied warranty as to fitness for a particular use. Hastings Instruments shall not be liable for any indirect or consequential damages.

Hastings Instruments, will, at its option, repair, replace or refund the selling price of the product if Hastings Instruments determines, in good faith, that it is defective in materials or workmanship during the warranty period. Defective instruments should be returned to Hastings Instruments, **shipment prepaid**, together with a written statement of the problem and a Return Material Authorization (RMA) number.

Please consult the factory for your RMA number before returning any product for repair. Collect freight will not be accepted.

### 5.2. Non-Warranty Repair Policy

Any product returned for a non-warranty repair must be accompanied by a purchase order, RMA form and a written description of the problem with the instrument. If the repair cost is higher, you will be contacted for authorization before we proceed with any repairs. If you then choose not to have the product repaired, a minimum will be charged to cover the processing and inspection. Please consult the factory for your RMA number before returning any product repair.

TELEDYNE HASTINGS INSTRUMENTS  
804 NEWCOMBE AVENUE  
HAMPTON, VIRGINIA 23669 U.S.A.  
ATTENTION: REPAIR DEPARTMENT  
TELEPHONE (757) 723-6531  
1-800-950-2468  
FAX (757) 723-3925  
E MAIL [hastings\\_instruments@teledyne.com](mailto:hastings_instruments@teledyne.com)  
INTERNET ADDRESS <http://www.hastings-inst.com>

Repair Forms may be obtained from the "Information Request" section of the Hastings Instruments web site.

# 6. Appendices

## 6. Appendices

### 6.1. Appendix 1- Volumetric versus Mass Flow

Mass flow measures just what it says, the mass or weight of the gas flowing through the instrument. Mass flow (or weight per unit time) units are given in pounds per hour (lb/hour), kilograms per sec (kg/sec) etc. When your specifications state units of flow to be in mass units, there is no reason to reference a temperature or pressure. Mass does not change based on temperature or pressure.

However, if you need to see your results of gas flow in volumetric units, like liters per minute, cubic feet per hour, etc. you must consider the fact that volume DOES change with temperature and pressure.

A mass flow meter measures MASS (grams) and then converts mass to volume. To do this the density (grams/liter) of the gas must be known and this value changes with temperature and pressure.

When you heat a gas, the molecules have more energy and they move around faster, so when they bounce off each other, they become more spread out, therefore the volume is different for the same number of molecules.

Think about this:

The density of Air at 0° C is 1.29 g/liter

The density of Air at 25C is 1.19 g/liter


The difference is 0.1 g/liter. If you are measuring flows of 100 liters per minute, and you don't use the correct density factor then you will have an error of 10 g/minute!

Volume also changes with pressure. Think about a helium balloon with a volume of 1 liter. If you could scuba dive with this balloon and the pressure on it increases. What do you think happens to the weight of the helium? It stays the same. What would happen to the volume (1 liter)? It would shrink.

Why is the word standard included with the volume terms liters and cubic feet in mass flow applications?

A mass flow meter measures mass ...and we know we can convert to volume.

To use density we must pick one (or **standard**) temperature and pressure to use in our calculation. When this calculation is done, the units are called **standard** liters per minute (SLM) or **standard** cubic feet per minute (SCFM), etc because it is referenced to a standard temperature and pressure when the volume is calculated.

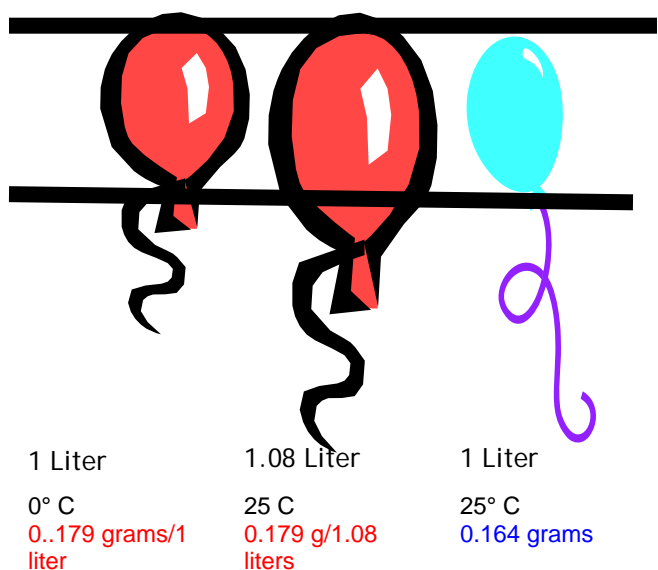

Using the example to the left, we can see a standard liter can be defined differently. The first balloon contains 0.179 grams of Helium at 0° C and 760 Torr (density of 0.179 grams/liter). Heat up that balloon to room temperature and the volume increases, but the mass has not changed - but the volume is not 1 liter anymore, it is 1.08 liters.

So to define a standard liter of Helium at 25 C, we must extract only one liter from the second balloon and that liter weighs only 0.175 grams.

If a mass flow meter is set up for STP at 0 C and 760 Torr, when it measures 0.179 grams of He, it will give you results of 1 SLM. If a second meter is set up for STP at 25 C and 760 Torr, when it measures 0.164 grams, it will give results of 1 SLM.



## 6.2. Appendix 2 - Gas Conversion Factors

The gas correction factors (GCF's) presented in this manual were obtained by one of four methods. The following table summarizes the different methods for determining GCF's and will help identify for which gases the highest degree of accuracy may be achieved when applying a correction factor.

1. Empirically determined
2. Calculated from virial coefficients of other investigator's empirical data
3. From NIST tables
4. Calculated from specific heat data at 0° C at 1 atmosphere

The most accurate method is by direct measurement. Gases that are easily handled with safety such as inert gases, gases common in the atmosphere or gases that are otherwise innocuous can be run through a standard flow meter and the GCF determined empirically.

Many gases that have been investigated sufficiently by other researchers, can have their molar specific heat ( $C_p$ ) calculated. The gas correction factor is then calculated using the following ratio:

$$\text{GCF} = \frac{C_{p,N_2}}{C_{p,GasX}}$$

GCF's calculated in this manner have been found to agree with the empirically determined GCF's within a few tenths of a percent.

The National Institute of Standards and Technology (NIST) maintains tables of thermodynamic properties of certain fluids. Using these tables, one may look up the necessary thermophysical property and calculate the GCF with the same degree of accuracy as going directly to the referenced investigator.

Lastly, for rare, expensive gases or gases requiring special handling due to safety concerns, one may look up specific heat properties in a variety of texts on the subject. Usually, data found in this manner applies only in the ideal gas case. This method yields GCF's for ideal gases but as the complexity of the gas increases, its behavior departs from that of an ideal gas. Hence the inaccuracy of the GCF increases.

Hastings Instruments will continue to search for better estimations of the GCF's of the difficult gases and will regularly update the list. Most Hastings flow meters and controllers are calibrated using nitrogen. The correction factors published by Hastings are meant to be applied to these instruments. To apply the GCF's, simply multiply the gas flow reading times the GCF for the process gas in use.

### Example:

Calculate the actual flow of argon passing through a nitrogen-calibrated meter that reads 20 sccm, multiply the reading times the GCF for argon.

$$20.000 \times 1.3978 = 27.956$$

Conversely, to determine what reading to set a nitrogen-calibrated meter in order to get a desired flow rate of a process gas other than nitrogen, you divide the desired rate by the GCF. For example, to get a desired flow of 20 sccm of argon flowing through the meter, divide 20 sccm by 1.3978

$$20.000 / 1.3978 = 14.308$$

That is, you (adjust the gas flow) to read 14.308 sccm.

Some meters, specifically the high flow meters, are calibrated in air. The flow readings must then be corrected twice. Convert once from air to nitrogen, then from nitrogen to the gas that will be measured with the meter. In this case, multiply the reading times the ratio of the process gas' GCF to the GCF of the calibration gas.

Example:

A meter calibrated in air is being used to flow propane. The reading from the meter is multiplied by the GCF for propane and then divided by the GCF of air.

$$20 \times (0.3499/1.0015) = 6.9875$$

To calculate a target setting (20 sccm) to achieve a desired flow rate of propane using a meter calibrated to air, invert the ratio above and multiply.

$$20 \times (1.0015/0.3499) = 57.2449$$

### Gas Conversion Table for Nitrogen





Rec #	Gas	Symbol	GCF	Derived	Density (g/L) 25° C / 1 atm	Z
1	Acetic Acid	C <sub>2</sub> H <sub>4</sub> F <sub>2</sub>	0.4155	4	2.700	2.0301
2	Acetic Acid, Anhydride	C <sub>4</sub> H <sub>6</sub> O <sub>3</sub>	0.2580	4	4.173	2.3384
3	Acetone	C <sub>3</sub> H <sub>6</sub> O	0.3556	4	2.374	1.7504
4	Acetonitril	C <sub>2</sub> H <sub>3</sub> N	0.5178	4	1.678	1.4462
5	Acetylene	C <sub>2</sub> H <sub>2</sub>	0.6255	4	1.064	0.9792
6	Air	Air	1.0015	1	1.185	1.0930
7	Allene	C <sub>3</sub> H <sub>4</sub>	0.4514	4	1.638	1.3876
8	Ammonia	NH <sub>3</sub>	0.7807	2	0.696	0.6409
9	Argon	Ar	1.4047	1	1.633	2.1243
10	Arsine	AsH <sub>3</sub>	0.7592	5	3.186	4.0839
11	Benzene	C <sub>6</sub> H <sub>6</sub>	0.3057	4	3.193	2.0636
12	Boron Trichloride	BCl <sub>3</sub>	0.4421	4	4.789	3.6531
13	Boron Trifluoride	BF <sub>3</sub>	0.5431	4	2.772	2.4109
14	Bromine	Br <sub>2</sub>	0.8007	4	6.532	1.0000
15	Bromochlorodifluoromethane	CBrClF <sub>2</sub>	0.3684	4	6.759	4.2789
16	Bromodifluoromethane	CHBrF <sub>2</sub>	0.4644	4	5.351	4.3990
17	Bromotrifluoromethane	CBrF <sub>3</sub>	0.3943	4	6.087	4.1546
18	Butane	C <sub>4</sub> H <sub>10</sub>	0.2622	2	2.376	1.6896
19	Butanol	C <sub>4</sub> H <sub>10</sub> O	0.2406	4	3.030	1.9233
20	Butene	C <sub>4</sub> H <sub>8</sub>	0.3056	4	2.293	1.6700
21	Carbon Dioxide	CO <sub>2</sub>	0.7526	1	1.799	1.7511
22	Carbon Disulfide	CS <sub>2</sub>	0.6160	4	3.112	3.0744
23	Carbon Monoxide	CO	1.0012	4	1.145	1.0433
24	Carbon Tetrachloride	CCl <sub>4</sub>	0.3333	4	6.287	3.6196
25	Carbonyl Sulfide	COS	0.6680	4	2.456	2.4230
26	Chlorine	Cl <sub>2</sub>	0.8451	4	2.898	3.9995
27	Chlorine Trifluoride	ClF <sub>3</sub>	0.4496	5	3.779	2.8970
28	Chlorobenzene	C <sub>6</sub> H <sub>5</sub> Cl	0.2614	4	4.601	2.4954
29	Chlorodifluoroethane	C <sub>2</sub> H <sub>3</sub> ClF <sub>2</sub>	0.3216	4	4.108	2.5119
30	Chloroform	CHCl <sub>3</sub>	0.4192	4	4.879	3.5284
31	Chloropentafluoroethane	C <sub>2</sub> ClF <sub>5</sub>	0.2437	4	6.314	2.9778
32	Chloropropane	C <sub>3</sub> H <sub>7</sub> Cl	0.3080	4	3.210	2.0756
33	Cisbutene	C <sub>4</sub> H <sub>8</sub>	0.3004	4	2.293	1.6672
34	Cyanogen	C <sub>2</sub> N <sub>2</sub>	0.4924	4	2.127	1.7626
35	Cyanogen Chloride	ClCN	0.6486	5	2.513	2.4405
36	Cyclobutane	C <sub>4</sub> H <sub>8</sub>	0.3562	4	2.293	1.7091

37	Cyclopropane	C <sub>3</sub> H <sub>6</sub>	0.4562	4	1.720	1.4440
38	Deuterium	H <sub>2</sub> <sup>2</sup>	1.0003	4	0.165	0.3102
39	Diborane	B <sub>2</sub> H <sub>6</sub>	0.5063	5	1.131	1.0486
40	Dibromodifluoromethane	CB <sub>2</sub> F <sub>2</sub>	0.3590	4	8.576	5.2998
41	Dichlorofluoromethane	CHCl <sub>2</sub> F	0.4481	4	4.207	3.2249
42	Dichloromethane	CH <sub>2</sub> Cl <sub>2</sub>	0.5322	4	3.472	3.0592
43	Dichloropropane	C <sub>3</sub> H <sub>6</sub> Cl <sub>2</sub>	0.2698	4	4.618	2.5291
44	Dichlorosilane	H <sub>2</sub> SiCl <sub>2</sub>	0.4716	5	4.129	3.3176
45	Diethyl Amine	C <sub>4</sub> H <sub>11</sub> N	0.2256	4	2.989	1.9080
46	Diethyl Ether	C <sub>4</sub> H <sub>10</sub> O	0.2235	4	3.030	1.9215
47	Diethyl Sulfide	C <sub>4</sub> H <sub>10</sub> S	0.2255	4	3.686	2.1300
48	Difluoroethylene	C <sub>2</sub> H <sub>2</sub> F <sub>2</sub>	0.4492	4	2.617	2.0457
49	Dimethylamine	C <sub>2</sub> H <sub>7</sub> N	0.3705	4	1.843	1.4793
50	Dimethyl Ether	C <sub>2</sub> H <sub>6</sub> O	0.4088	4	1.883	1.5211
51	Dimethyl Sulfide	C <sub>2</sub> H <sub>6</sub> S	0.3623	4	2.540	1.8455
52	Divinyl	C <sub>4</sub> H <sub>6</sub>	0.3248	4	2.211	1.6433
53	Ethane	C <sub>2</sub> H <sub>6</sub>	0.4998	2	1.229	1.1175
54	Ethane, 1-chloro-1,1,2,2-tetrafluoro-	C <sub>2</sub> HCIF <sub>4</sub>	0.2684	4	5.578	2.8629
55	Ethane, 1-chloro-1,2,2,2-tetrafluoro-	C <sub>2</sub> HCIF <sub>4</sub>	0.2719	4	5.578	2.8806
56	Ethanol	C <sub>2</sub> H <sub>6</sub> O	0.4046	4	1.883	1.5187
57	Ethylacetylene	C <sub>4</sub> H <sub>6</sub>	0.3256	4	2.211	1.6438
58	Ethyl Amine	C <sub>2</sub> H <sub>7</sub> N	0.3694	4	1.843	1.4789
59	Ethylbenzene	C <sub>8</sub> H <sub>10</sub>	0.2001	4	4.339	2.3099
60	Ethyl Bromide	C <sub>2</sub> H <sub>5</sub> Br	0.4124	4	4.454	3.1724
61	Ethyl Chloride	C <sub>2</sub> H <sub>5</sub> Cl	0.4212	4	2.637	2.0018
62	Ethyl Fluoride	C <sub>2</sub> H <sub>5</sub> F	0.4430	4	1.964	1.5967
63	Ethylene	C <sub>2</sub> H <sub>4</sub>	0.6062	1	1.147	1.0475
64	Ethylene Dibromide	C <sub>2</sub> H <sub>4</sub> Br <sub>2</sub>	0.3173	4	7.679	4.1196
65	Ethylene Dichloride	C <sub>2</sub> H <sub>4</sub> Cl <sub>2</sub>	0.3475	4	4.045	2.5846
66	Ethylene Oxide	C <sub>2</sub> H <sub>4</sub> O	0.5308	4	1.801	1.5495
67	Ethyleneimine	C <sub>2</sub> H <sub>4</sub> N	0.4790	4	1.719	1.4552
68	Ethylidene Dichloride	C <sub>2</sub> H <sub>4</sub> Cl <sub>2</sub>	0.3506	4	4.045	2.5976
69	Ethyl Mercaptan	C <sub>2</sub> H <sub>6</sub> S	0.3654	4	2.540	1.8499
70	Fluorine	F <sub>2</sub>	0.9115	4	1.553	1.5574
71	Formaldehyde	CH <sub>2</sub> O	0.7912	4	1.227	1.1232
72	Freon 11	CCl <sub>3</sub> F	0.3535	4	5.615	3.4473
73	Freon 12	CCl <sub>2</sub> F <sub>2</sub>	0.3712	4	4.942	3.2026
74	Freon 13	CClF <sub>3</sub>	0.3792	4	4.270	2.8572
75	Freon 14	CF <sub>4</sub>	0.4422	4	3.597	2.7242
76	Freon 22	CHClF <sub>2</sub>	0.4857	4	3.534	2.8794
77	Freon 23	CHF <sub>3</sub>	0.5282	4	2.862	2.4487
78	Freon 114	C <sub>2</sub> Cl <sub>2</sub> F <sub>4</sub>	0.2327	4	6.986	3.1174
79	Furan	C <sub>4</sub> H <sub>4</sub> O	0.3889	4	2.783	2.0253
80	Helium	He	1.4005	1	0.164	0.2304
81	Heptafluoropropane	C <sub>3</sub> HF <sub>7</sub>	0.1987	4	6.950	2.9681
82	Hexamethyldisilazane	C <sub>6</sub> H <sub>19</sub> NSi <sub>2</sub>	0.1224	4	6.597	3.2710
83	Hexamethyldisiloxane	C <sub>6</sub> H <sub>18</sub> OSi <sub>2</sub>	0.1224	4	6.637	3.2794
84	Hexane	C <sub>6</sub> H <sub>14</sub>	0.1828	4	3.522	2.1062
85	Hexafluorobenzene	C <sub>6</sub> F <sub>6</sub>	0.1733	4	7.605	3.0771
86	Hexene	C <sub>6</sub> H <sub>12</sub>	0.1918	4	3.440	2.0677
87	Hydrazine	N <sub>2</sub> H <sub>4</sub>	0.5506	4	1.310	1.1757
88	Hydrogen	H <sub>2</sub>	1.0038	1	0.082	0.3895
89	Hydrogen Bromide	HBr	1.0028	4	3.307	7.6975
90	Hydrogen Chloride	HCl	1.0034	4	1.490	1.5183
91	Hydrogen Cyanide	CHN	0.7772	4	1.105	1.0003
92	Hydrogen Fluoride	HF	1.0039	4	0.818	0.6845
93	Hydrogen Iodide	HI	0.9996	4	5.228	1.0000
94	Hydrogen Selenide	H <sub>2</sub> Se	0.8412	5	3.309	5.1920
95	Hydrogen Sulfide	H <sub>2</sub> S	0.8420	4	1.393	1.3174

96	Isobutane	C <sub>4</sub> H <sub>10</sub>	0.2725	2	2.376	1.6912
97	Isobutanol	C <sub>4</sub> H <sub>10</sub> O	0.2391	4	3.030	1.9228
98	Isobutene	C <sub>4</sub> H <sub>8</sub>	0.2984	4	2.293	1.6663
99	Isopentane	C <sub>5</sub> H <sub>12</sub>	0.2175	4	2.949	1.8975
100	Isopropyl Alcohol	C <sub>3</sub> H <sub>8</sub> O	0.2931	4	2.456	1.7335
101	Isoxazole	C <sub>3</sub> H <sub>3</sub> NO	0.4333	4	2.823	2.1501
102	Ketene	C <sub>2</sub> H <sub>2</sub> O	0.5732	4	1.718	1.5127
103	Krypton	Kr	1.4042	4	3.425	1.0000
104	Methane	CH <sub>4</sub>	0.7787	1	0.656	0.6105
105	Methanol	CH <sub>4</sub> O	0.6167	4	1.310	1.1818
106	Methyl Acetate	C <sub>3</sub> H <sub>6</sub> O <sub>2</sub>	0.3083	4	3.028	1.9967
107	Methyl Acetylene	C <sub>3</sub> H <sub>4</sub>	0.4430	4	1.638	1.3847
108	Methylamine	CH <sub>5</sub> N	0.5360	4	1.269	1.1449
109	Methyl Bromide	CH <sub>3</sub> Br	0.6358	4	3.881	4.3841
110	Methyl Chloride	CH <sub>3</sub> Cl	0.6639	4	2.064	1.9480
111	Methylcyclohexane	C <sub>7</sub> H <sub>14</sub>	0.1853	4	4.013	2.2334
112	Methyl Ethyl Amine	C <sub>3</sub> H <sub>9</sub> N	0.2692	4	2.416	1.7065
113	Methyl Ethyl Ether	C <sub>3</sub> H <sub>8</sub> O	0.2844	4	2.456	1.7285
114	Methyl Ethyl Sulfide	C <sub>3</sub> H <sub>8</sub> S	0.2743	4	3.113	1.9816
115	Methyl Fluoride	CH <sub>3</sub> F	0.7247	4	1.391	1.2790
116	Methyl Formate	C <sub>2</sub> H <sub>4</sub> O <sub>2</sub>	0.3975	4	2.455	1.8491
117	Methyl Iodide	CH <sub>3</sub> I	0.6514	4	5.802	10.2105
118	Methyl Mercaptan	CH <sub>4</sub> S	0.5409	4	1.966	1.6930
119	Methylpentene	C <sub>6</sub> H <sub>12</sub>	0.2037	4	3.440	2.0555
120	Methyl Vinyl Ether	C <sub>3</sub> H <sub>6</sub> O	0.3435	4	2.374	1.7377
121	Neon	Ne	1.4043	4	0.825	0.6173
122	Nitric Oxide	NO	0.9795	4	1.226	1.1430
123	Nitrogen	N <sub>2</sub>	1.0000	1	1.145	1.0434
124	Nitrogen Dioxide	NO <sub>2</sub>	0.7604	4	1.880	1.8624
125	Nitrogen Tetroxide	N <sub>2</sub> O <sub>4</sub>	0.3395	4	3.761	2.4128
126	Nitrogen Trifluoride	NF <sub>3</sub>	0.5406	5	2.902	2.5277
127	Nitromethane	CH <sub>3</sub> NO <sub>2</sub>	0.4653	4	2.495	1.9912
128	Nitrosyl Chloride	NOCl	0.6357	4	2.676	2.6013
129	Nitrous Oxide	N <sub>2</sub> O	0.7121	1	1.799	1.7098
130	n-Pentane	C <sub>5</sub> H <sub>12</sub>	0.2121	4	2.949	1.9008
131	Octane	C <sub>8</sub> H <sub>18</sub>	0.1386	4	4.669	2.6119
132	Oxygen	O <sub>2</sub>	0.9779	1	1.308	1.2483
133	Oxygen Difluoride	F <sub>2</sub> O	0.6454	4	2.207	2.0766
134	Ozone	O <sub>3</sub>	0.7022	4	1.962	1.8868
135	Pentaborane	B <sub>5</sub> H <sub>9</sub>	0.1499	5	2.580	1.9855
136	Pentane	C <sub>5</sub> H <sub>12</sub>	0.2175	4	2.949	1.8975
137	Perchloryl Fluoride	ClFO <sub>3</sub>	0.4155	4	4.188	3.0075
138	Perfluorocyclobutane	C <sub>4</sub> F <sub>8</sub>	0.1711	4	8.176	3.1946
139	Perfluoroethane	C <sub>2</sub> F <sub>6</sub>	0.2530	4	5.641	2.8112
140	Perfluoropropane	C <sub>3</sub> F <sub>8</sub>	0.1818	4	7.685	3.0998
141	Phenol	C <sub>6</sub> H <sub>6</sub> O	0.2489	4	3.847	2.2089
142	Phosgene	COCl <sub>2</sub>	0.4812	4	4.043	3.3063
143	Phosphine	PH <sub>3</sub>	0.7859	5	1.390	1.2956
144	Phosphorus Trifluoride	PF <sub>3</sub>	0.4973	5	3.596	2.9936
145	Propane	C <sub>3</sub> H <sub>8</sub>	0.3499	1	1.802	1.4516
146	Propyl Alcohol	C <sub>3</sub> H <sub>8</sub> O	0.3061	4	2.456	1.7427
147	Propyl Amine	C <sub>3</sub> H <sub>9</sub> N	0.2860	4	2.416	1.7126
148	Propylene	C <sub>3</sub> H <sub>6</sub>	0.4048	2	1.720	1.4223
149	Pyradine	C <sub>5</sub> H <sub>5</sub> N	0.3222	4	3.233	2.1151
150	R32	CH <sub>2</sub> F <sub>2</sub>	0.6197	2	2.126	1.9458
151	R123	C <sub>2</sub> HCl <sub>2</sub> F <sub>3</sub>	0.2583	2	6.251	3.0368
152	R123A	C <sub>2</sub> HCl <sub>2</sub> F <sub>3</sub>	0.2699	4	6.251	3.1065
153	R125	C <sub>2</sub> HF <sub>5</sub>	0.2826	2	4.906	2.6844
154	R134	C <sub>2</sub> H <sub>2</sub> F <sub>4</sub>	0.2996	4	4.170	2.4595
155	R134A	C <sub>2</sub> H <sub>2</sub> F <sub>4</sub>	0.3110	2	4.170	2.5001
156	R143	C <sub>2</sub> H <sub>3</sub> F <sub>3</sub>	0.3451	4	3.435	2.2693





157	R143A	$C_2H_3F_3$	0.3394	4	3.435	2.2533
158	R152A	$C_2H_4F_2$	0.3877	4	2.700	1.9753
159	R218	$C_3F_8$	0.1818	4	7.685	3.0998
160	R1416	$C_2H_3Cl_2F$	0.3047	4	4.780	2.7342
161	Radon	Rn	1.4043	4	9.074	1.0000
162	Sec-butanol	$C_4H_{10}O$	0.2327	4	3.030	1.9213
163	Silane	$SiH_4$	0.6809	5	1.313	1.1934
164	Silicone Tetrafluoride	$SiF_4$	0.3896	5	4.254	2.9041
165	Sulfur Dioxide	$SO_2$	0.6878	4	2.619	2.7013
166	Sulfur Hexafluoride	$SF_6$	0.2701	1	5.970	3.0092
167	Sulfur Tetrafluoride	$SF_4$	0.3752	4	4.417	2.9215
168	Sulfur Trifluoride	$SF_3$	0.4368	4	3.640	2.7312
169	Sulfur Trioxide	$SO_3$	0.5397	4	3.273	2.8922
170	Tetrachloroethylene	$C_2Cl_4$	0.2926	4	6.778	3.4711
171	Tetrafluoroethylene	$C_2F_4$	0.3395	4	4.088	2.5732
172	Tetrahydrofuran	$C_4H_8O$	0.3271	4	2.947	1.9924
173	Tert-butanol	$C_4H_{10}O$	0.2298	4	3.030	1.9210
174	Thiophene	$C_4H_4S$	0.3538	4	2.783	1.9586
175	Toluene	$C_7H_8$	0.2448	4	3.766	2.1756
176	Transbutene	$C_4H_8$	0.2053	4	2.293	1.6978
177	Trichloroethane	$C_2H_3Cl_3$	0.3133	4	5.453	3.0712
178	Trichloroethylene	$C_2HCl_3$	0.3423	4	6.820	3.9903
179	Trichlorotrifluoroethane	$C_2Cl_3F_3$	0.2253	4	7.659	3.2607
180	Triethylamine	$C_6H_{15}N$	0.1619	4	4.136	2.3280
181	Trimethyl Amine	$C_3H_9N$	0.2822	4	2.416	1.7109
182	Tungsten Hexafluoride	$WF_6$	0.2453	5	12.174	4.7379
183	Uranium Hexafluoride	$UF_6$	0.1859	4	14.389	4.4681
184	Vinyl Bromide	$C_2H_3Br$	0.4768	4	4.372	3.5770
185	Vinyl Chloride	$C_2H_3Cl$	0.4956	4	2.555	2.0988
186	Vinyl Fluoride	$C_2H_3F$	0.5716	5	1.882	1.6528
187	Water Vapor	$H_2O$	0.7992	5	0.742	0.6715
188	Xenon	Xe	1.4042	4	5.366	1.0000
189	Xylene, m-	$C_8H_{10}$	0.2036	4	4.339	2.3103
190	Xylene, o-	$C_8H_{10}$	0.1953	4	4.339	2.3108
191	Xylene, p-	$C_8H_{10}$	0.2028	4	4.339	2.3102

FITTINGS	
FITTING TYPE	DIM "A"
3/4" SWAGelok	8.02" [203.68]
1" SWAGelok	8.22" [208.79]
3/4" MALE NPT	8.52" [216.36]
1" MALE NPT	8.22" [208.79]
1" VCO	8.48" [215.39]
1" VCR	9.52" [241.81]

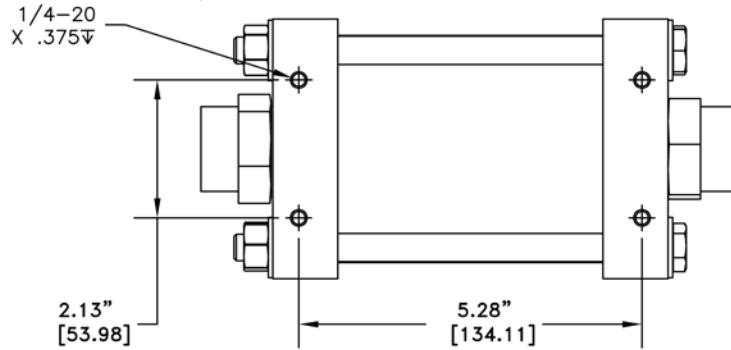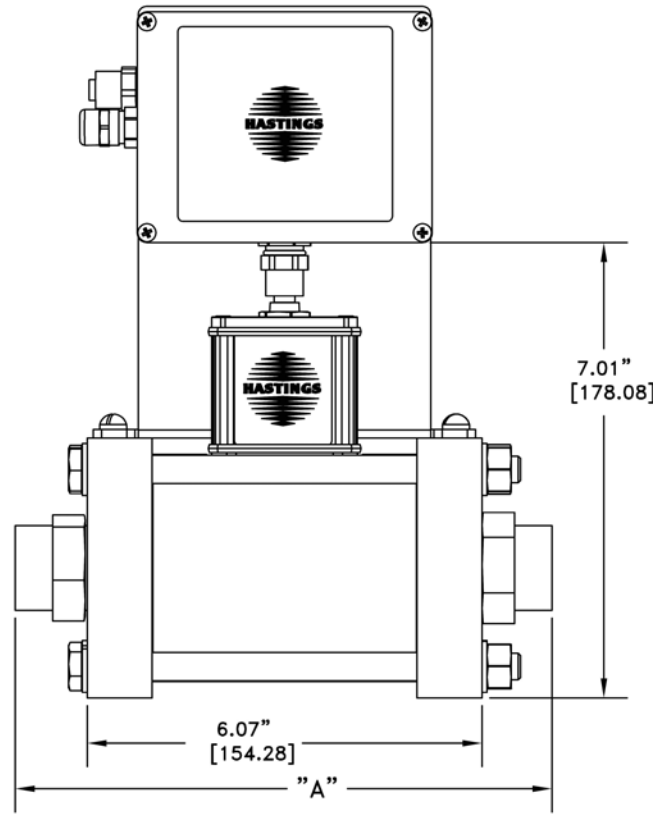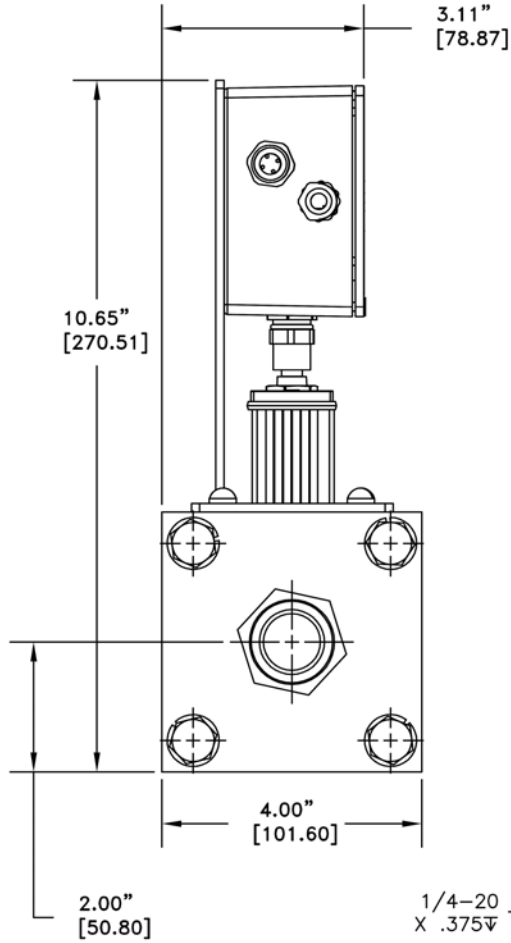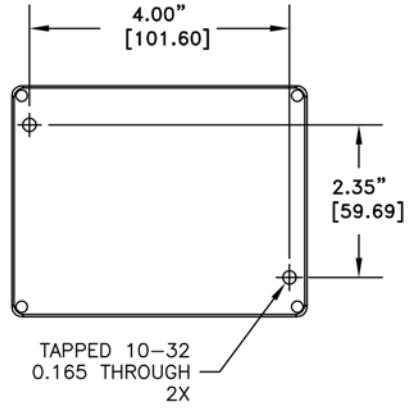

**HFM-I-405**  
Flow meter

FITTINGS	
FITTING TYPE	DIM "A"
10mm SWAG. 3/4"-16	7.72" [196.09]
12mm SWAG. 3/4"-16	7.72" [196.09]
1/2" SWAG. 3/4"-16	7.69" [195.28]
3/4" SWAG. 3/4"-16	8.01" [203.58]
1/2" VCO 3/4"-16	8.14" [206.76]
3/8" NPT 3/4"-16	8.25" [209.55]
1/2" NPT 1/2"-16	8.25" [209.55]
1/2" VCR	8.56" [217.50]

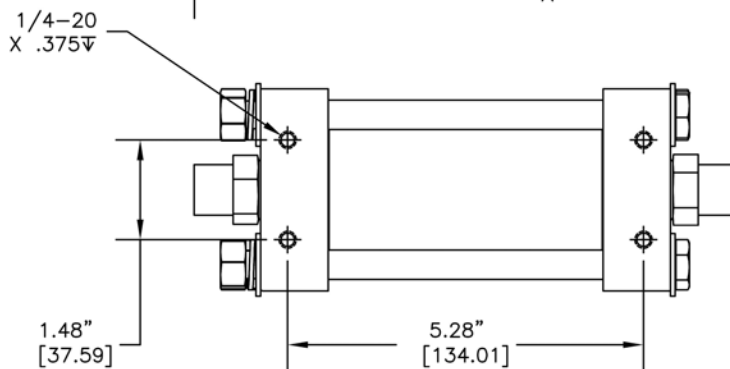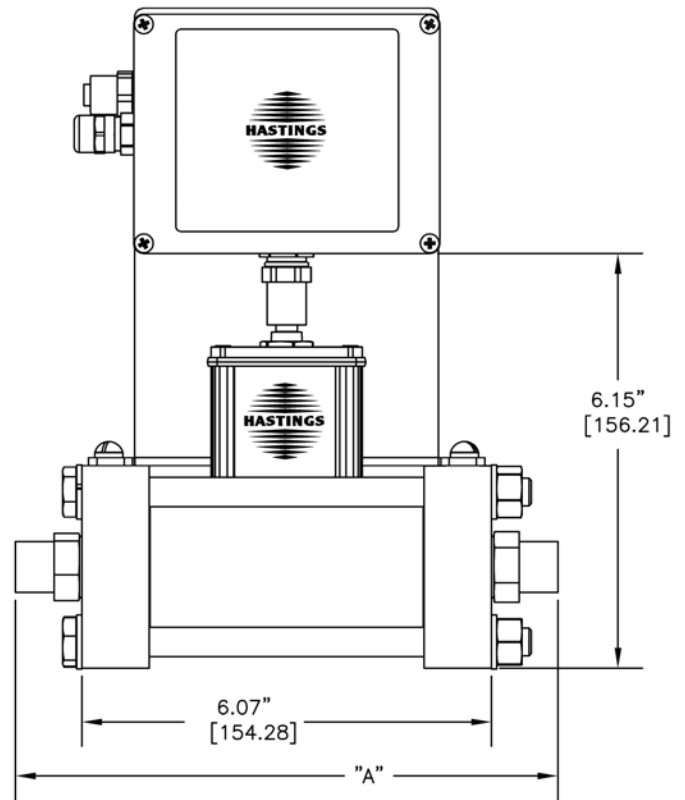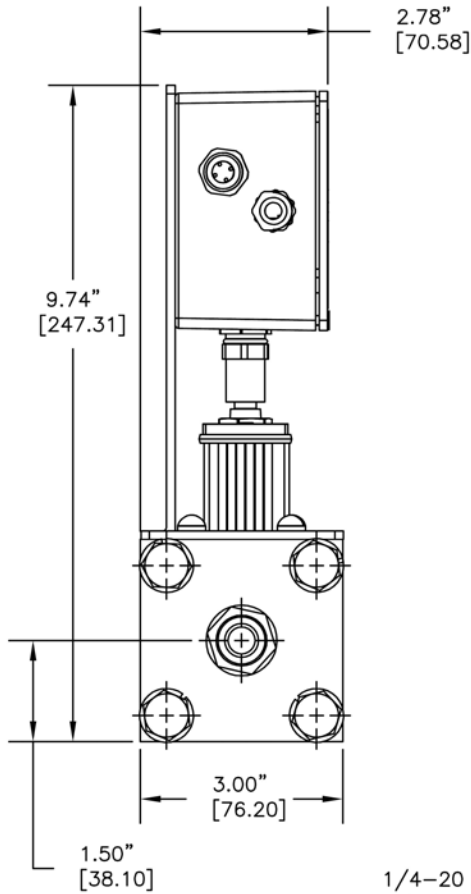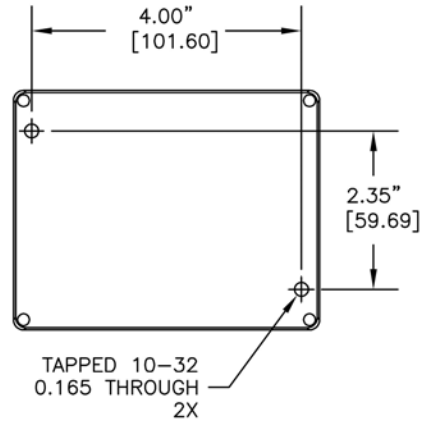

**HFM-I-401  
Flow Meter**