



BENCHTOP CO₂ INCUBATOR OPERATIONS MANUAL

FOR MODEL
7404-10



PO Box 715
Marietta, OH 45750
800-648-3042 • 740-373-6809
Fax 740-374-3760
www.caronproducts.com
service@caronproducts.com

Dear Valued Customer:

Thank you for purchasing CARON Products & Services equipment. We appreciate your business and look forward to being your preferred supplier of controlled environment equipment products in the future.

At CARON, we are committed to continuous quality improvement. Our goal is to supply our customers with highly reliable equipment at a fair price. In order to openly monitor our performance, we would appreciate your feedback on our products and services.

If you have questions, or any suggestions for improvement based on the installation or operation of the equipment you have purchased, please contact our service department at service@caronproducts.com or 740-373-6809.

Thanks again for your business!

TABLE OF CONTENTS

Section 1 – Warranty.....	5
Section 2 – Equipment Overview.....	10
Section 3 – Installation	12
Unpacking	
Choosing a Location	
Preliminary Cleaning	
Installing the Port Stopper	
Installing the Shelves	
Stacking two Units	
Leveling the Unit	
Connecting the Drain Line	
Connecting the Water Supply	
Connecting CO2 supply	
Connecting Electrical Power	
Section 4 – Optional Accessory Installation	19
Connecting Alarm Contacts (ALRM302)	
Installing the Carboy Water System (BOTL301)	
Connecting Alarm Contacts (OUTP302, OUTP303)	
Installing Drain Water Pump (PUMP301)	
Installing the Stacking Kit (STCK301)	
Section 5 – Operation	24
Using the Keypad	
Learning the Screen Saver	
Changing the Temperature Set-point	
Changing the Humidity Set-point	
Changing the CO2 Set-point	
Using the Decontamination Cycle	
Section 6 – Optional Accessory Operation	36
Carboy Water System (BOTL301)	
Operation of the Data Logging System (DLOG301)	
Built in Gas Guard System (GASG302)	
Ultraviolet Germicidal Lamp (LGHT602)	
Interior Electrical Outlet (OUTL305-OUTL309)	
Built in Temp or Temp/Rh 6” Pen Recorders (RCDR316/RCDR317)	
Built in Temp or Temp/Rh 10” Thermal Recorders (RCDR318/RCDR319)	

Section 7 – Calibration	53
Calibrating the Temperature	
Calibrating the Humidity	
Calibrating the CO2	
Section 8 – Alarms	57
Alarm System Overview	
Snoozing the Speaker	
Muting the Speaker	
Changing Alarm Set-points	
Section 9 – Alerts	63
Alert System Overview	
Maintenance	
Section 10 – Info	66
Info System Overview	
Section 11 – Advanced Features	67
Setting the time & day	
Locking the controls	
Changing the Passcode	
Factory menu & troubleshooting	
Section 12 – Preventative Maintenance	81
Section 13 – Specifications.....	82
Section 14 – Electrical Schematics	83
Section 15 – Troubleshooting.....	84
Section 16 – Spare Replacement Parts.....	85
Appendix A – Declaration of Conformity	87

SECTION 1- WARRANTY INFORMATION

CO² INCUBATOR LIMITED WARRANTY

Please review this section before requesting warranty service. At CARON, one of our primary goals is to provide customers with high levels of personal service and top quality products, delivered on time, backed by technical service and supported for the life of the product.

Before contacting us for warranty service, please be aware that there are repairs that are not covered under warranty.

WARRANTY DEFINED

Caron Products & Services, Inc. (herein after CARON) hereby warrants that equipment manufactured by CARON is free from defects in materials and workmanship when the equipment is used under normal operating conditions in accordance with the instructions provided by CARON.

COVERED:

- Parts and labor for a period of two (2) years from date of shipment.
- Any part found defective will be either repaired or replaced at CARON's discretion, free of charge, by CARON in Marietta, OH. Parts that are replaced will become the property of CARON.
- If CARON factory service personnel determine that the customer's unit requires further service, dependent of the model involved, CARON may, at its sole discretion, provide a service technician to correct the problem, or require the return of the equipment to the factory or authorized service depot.
- CARON will have the right to inspect the equipment and determine the repairs or replacement parts necessary. The customer will be notified, within a reasonable time after inspection, of any costs incurred that are not covered by this warranty prior to initiation of any such repairs.

NOT COVERED:

- Calibration of control parameters.
- Improper installation; including electrical service, gas and water supply tubing, gas supplies, room ventilation, unit leveling, facility structural inadequacies or ambient conditions that are out of specification.
- Cost of express shipment of equipment or parts.
- Any customer modifications of this equipment, or any repairs undertaken without the prior written consent of CARON, will render this limited warranty void.
- CARON is not responsible for consequential, incidental or special damages; whether shipping damage or damages that may occur during transfer to the customer's point of use. When the equipment is signed for at the customer's site, ownership is transferred to the customer. Any damage claims against the shipping company become the responsibility of the customer.
- Repairs necessary because of the equipment being used under other than normal operating conditions or for other than its intended use.
- Repair due to the customer's failure to follow normal maintenance instructions.
- Parts considered consumable; including: light bulbs, filters, gases, etc.
- Damage from use of improper water quality.
- Damage from chemicals or cleaning agents detrimental to equipment materials.
- Force Majeure or Acts of God.

This writing is a final and complete integration of the agreement between CARON and the customer. CARON makes no other warranties, express or implied, of merchantability, fitness for a particular purpose or otherwise, with respect to the goods sold under this agreement. This warranty cannot be altered unless CARON agrees to an alteration in writing and expressly stated herein shall be recognized to vary or modify this contract.

Ohio Law governs this warranty.

EQUIPMENT INTERNATIONAL LIMITED WARRANTY

Please review this section before requesting warranty service. At CARON, one of our primary goals is to provide customers with high levels of personal service and top quality products, delivered on time, backed by technical service and supported for the life of the product.

Before contacting your distributor for warranty service, please be aware that there are repairs that are not covered under warranty.

WARRANTY DEFINED

Caron Products & Services, Inc. (herein after CARON) hereby warrants that equipment manufactured by CARON is free from defects in materials and workmanship when the equipment is used under normal operating conditions in accordance with the instructions provided by CARON.

COVERED:

- Parts for a period of two (2) years from date of shipment.
- Any part found defective will be either repaired or replaced at CARON's or their authorized representative's discretion. Parts that are replaced will become the property of CARON.
- If CARON or their authorized representatives determine that the customer's unit requires further service, CARON or the representative may, at its sole discretion, provide a service technician to correct the problem, or require the return of the equipment to the an authorized service depot.
- CARON or their authorized representative will have the right to inspect the equipment and determine the repairs or replacement parts necessary. The customer will be notified, within a reasonable time after inspection, of any costs incurred that are not covered by this warranty prior to initiation of any such repairs.

NOT COVERED:

- Calibration of control parameters.
- Improper installation; including electrical service, gas and water supply tubing, gas supplies, room ventilation, unit leveling, facility structural inadequacies or ambient conditions that are out of specification.
- Cost of express shipment of equipment or parts.
- Any customer modifications of this equipment, or any repairs undertaken without the prior written consent of CARON, will render this limited warranty void.
- CARON and their representative are not responsible for consequential, incidental or special damages; whether shipping damage or damages that may occur during transfer to the customer's point of use. When the equipment is signed for at the customer's site, ownership is transferred to the customer. Any damage claims against the shipping company become the responsibility of the customer.
- Repairs necessary because of the equipment being used under other than normal operating conditions or for other than its intended use.
- Repair due to the customer's failure to follow normal maintenance instructions.
- Parts considered consumable; including: light bulbs, filters, gases, etc.
- Damage from use of improper water quality.
- Damage from chemicals or cleaning agents detrimental to equipment materials.
- Force Majeure or Acts of God.

This writing is a final and complete integration of the agreement between CARON and the customer. CARON makes no other warranties, express or implied, of merchantability, fitness for a particular purpose or otherwise, with respect to the goods sold under this agreement. This warranty cannot be altered unless CARON agrees to an alteration in writing and expressly stated herein shall be recognized to vary or modify this contract.

Ohio Law governs this warranty.

Caron Products & Services, Inc.
PO Box 715 • Marietta, OH 45750
740-373-6809

INTERNATIONAL SYMBOLS AND DEFINITIONS



Help



Information



Warning of hazardous area



Warning of dangerous electric voltage



Earth (ground) protective
conductor

WARNINGS




Local government may require proper disposal

SECTION 2 – EQUIPMENT OVERVIEW


Congratulations! You have just purchased the latest technology in incubators. Before using the equipment, familiarize yourself with key components of the product and thoroughly read this manual.



SECTION 2 – EQUIPMENT OVERVIEW -- CONTINUED

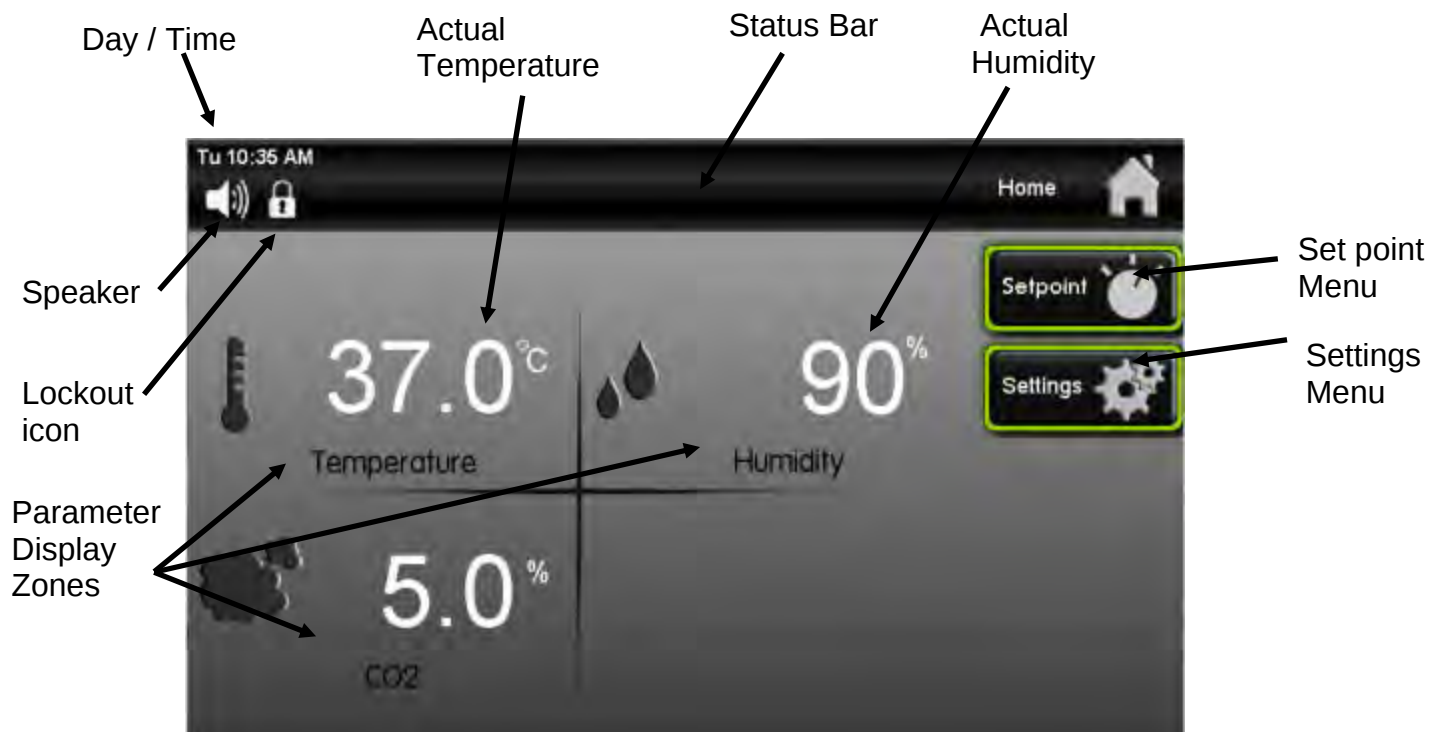

(Home Screen)

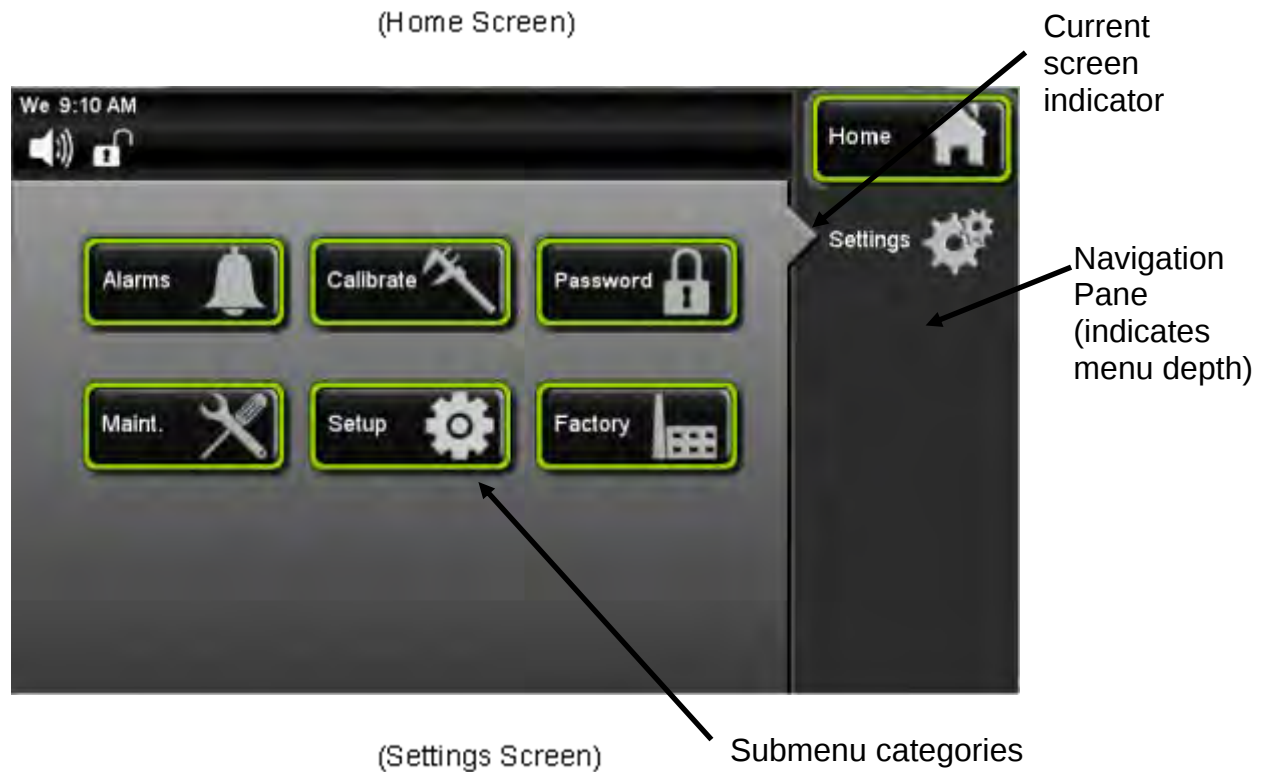

(Settings Screen)

SECTION 3 -- INSTALLATION

Unpacking

Your new unit has been thoroughly packaged to avoid shipping damage. However, the unit should be fully inspected upon arrival before signing for receipt. If the package has visual damage, notes should be made on the freight bill and signed by the delivery company. In the event of concealed damage after the unit is uncrated, keep the carton and packaging material. Call the shipping company within 7 days of receipt, request inspection and retain a copy of the inspection report.

Caron provides full on-site installation services for all models. Our installation services guarantees the proper set-up and startup of all equipment. Please contact the Service Department at 740-373-6809 or service@caronproducts.com for details.

Choosing a Location



This product weighs in excess of 400 pounds. Ensure that sufficient resources are available to safely move the product.

To ensure proper operation, the unit must be located on a firm level surface, capable of supporting approximately 500 pounds (1000 pounds if the units are to be stacked). The unit should be located in an 18°C – 25°C ambient area and where there is no direct airflow from heating and cooling ducts as well as out of direct sunlight. Allow four inches of clearance on all sides of the product to allow for connections and airflow.

The unit requires a dedicated electrical connection. Power requirements vary depending upon the incubator model, see Connecting Electrical Power section.

Choose a location where these facilities are, or can be made available. If a water source, or a drain is not available, contact CARON customer service and ask about our CRY5102 product line or click this web link for information on the product:

<http://www.caronproducts.com/65>

Preliminary Cleaning

Your new incubator was thoroughly cleaned prior to leaving the factory. It is recommended however, to disinfect all interior surfaces with a general purpose laboratory cleaning agent prior to using the product. After cleaning, dry all interior components with a sterile cloth as necessary.

Installing the Port Stoppers

The 7404-10 has an access port built into the right side of the cabinet. The port is designed to allow customer access for equipment validation and for installation of other equipment inside the incubator. These ports should be sealed with the provided silicone stoppers to allow the incubator to function properly. Install the stopper provided in the port on the right side of the unit.

Installing the Shelves

Each new incubator includes three perforated stainless steel shelves. Each shelf requires two shelf channels for installation. The left and right shelf tracks are the same. Prior to installation, take time to consider what the size of the product being placed in the incubator will be and set the shelf spacing accordingly. Additional shelving can be purchased through CARON customer service if necessary.

To install the shelf channels insert the rear tab on the shelf channel into the rear pilaster on the side wall of the incubator. Then insert the front tab into the front pilaster. Push the entire shelf channel towards the rear of the unit and snap it down into place.



Each shelf is capable of supporting a uniformly distributed load of 50 pounds. The maximum incubator capacity is 200 pounds. An optional re-enforced floor is available for heavy loads.



Do not have multiple loaded shelves out simultaneously or the incubator may tip.

Stacking two Units

The 7404-10 is designed to allow two units to be stacked. When units are stacked they must be bolted together for safety. A stacking adaptor kit, STCK301 with instructions is available through CARON customer service.



Failure to install the stacking adaptor kit can result in the top unit falling causing serious injury or death.

Leveling the Unit

Place a level on the middle shelf of the incubator. Adjust the cabinet leveling feet so the shelf is level. Units equipped with optional casters (CSTR301) can be leveled by adjusting the height of the lock nut on the caster. Adjust the feet or casters appropriately until the unit sits level left to right and front to back.

Connecting the Drain Line



When using a pressurized water source, failure to connect the unit to a drain could result in facility flooding.

The incubators control humidity by injecting water only as needed. This eliminates standing water which is a primary source of contamination and corrosion. There are several ways to take advantage of this feature. The simplest method is to connect the drain fitting and tubing supplied with the incubator to a local floor drain. During operation, any water that is not evaporated inside the cabinet will be sent to the cabinet drain to avoid standing water, minimizing the risk of contamination and corrosion.

The incubator drain connection is located in the bottom middle of the back of the incubator. A 3/8" NPT fitting and tubing are supplied in the unit parts kit. Thread the fitting into the drain connection and slide the tubing into the drain connection. Pull on the tubing after installation to make sure it is tight. Route the drain tubing to a local floor drain.



The drain line relies on gravity to remove water from the incubator. The drain line must remain below the incubator to drain properly. Kinks or elevations in the drain line above the cabinet drain will not allow the incubator to drain.

If a floor drain is not available, CARON offers a water recirculation system accessory (CRSY102) that acts as both a water supply and a drain for humidified incubators. This system continuously recycles any excess water not needed by the incubator, filters and conditions it, and reuses it to control humidity. www.caronproducts.com.

If neither a floor drain, nor a CRSY102 are available, another option is a carboy for a water source and a plug in the interior incubator drain. While this solution is not recommended due to the creation of standing water in the bottom of the incubator, it will allow the incubator to control humidity, with some limitations, while not requiring a drain. BOTL101 is a carboy accessory that can be purchased through CARON. A drain plug is provided in the shipping kit for each incubator.

Connecting the Water Supply

To ensure proper operation, distilled or deionized water is required as a supply on units that have humidity control. If these water sources are not available contact CARON customer service.



Use only distilled or deionized water with a resistivity between 50K Ω -CM and 1M Ω -CM and a pH of greater than 6.5. Using water outside this range will void your warranty.



Do not use water that contains chloramines. Chloramines can damage internal rubber gaskets resulting in leaks.

A water inlet fitting on the back of the unit and ¼" black tubing are provided to connect the water supply to the incubator. Connect an appropriate water supply to the fitting. Incoming line pressure should be regulated to not exceed 80 psi.

If a Condensate Recirculator water recycling system was purchased as a water supply, refer to its user's manual for proper installation of the water supply.

Connecting a CO₂ supply



High concentrations of carbon dioxide can cause asphyxiation. The use of CO₂ monitors and alarms is recommended for areas where CO₂ can collect.



The CO₂ gas supply should be 99.5% pure and should not contain a siphon tube. Gas pressure to the unit must be regulated to 15-20PSI. Failure to do so could cause tubing to burst.

The CO₂ supply should be 99.5% and not have siphon tubes. CO₂ pressure should be regulated to 15-20 psi. CO₂ tank regulators can be purchased through CARON customer service. Once the cylinder regulator is installed, connect the outlet of the regulator to the hose barb fitting using the tubing and clamps provided. An inline HEPA filter is provided to remove any contaminants in the CO₂ gas supply. Check the connections closely for leaks.

If the unit is equipped with a built in gas guard system, there will be 2 gas inlets. Each of the inlets should be connected to an individual gas tank as described above.

Connecting Electrical Power



Connect each incubator to a grounded circuit.
Failure to do so could result in electrical shock.

The unit requires a dedicated electrical outlet. See table below for model specific power required and connection.

Model #	Power Requirements	Plug Connection
-1	115V, 60Hz, 12A FLA	NEMA 5-15
-2	230V, 60Hz, 8A FLA	NEMA 6-15
-3	230V, 50Hz, 6A FLA	CEE 7/7

When the required electrical connection is available, plug the provided power cord into the unit and the electrical outlet.


SECTION 4 – ACCESSORY INSTALLATION

Connecting Alarm Contacts (ALRM302)

With the purchase of ALRM302, a set of terminals on the rear of the unit is provided to monitor temperature and humidity alarms.


With the alarm contacts, the terminals provided allow for a NO (normally open) output, a NC (normally closed) and COM (common) connection. In the event of an alarm condition or power failure, the NO contact will close, and the NC contact will open. Once the alarm is cleared, the contacts return to their normal conditions. Insert the appropriate wire into the terminal and tighten down the screw terminal on top of the connector.

Terminal Connection	Unit off	Normal	Alarm
N/O to C	Closed	Open	Closed
N/C to C	Open	Close	Open

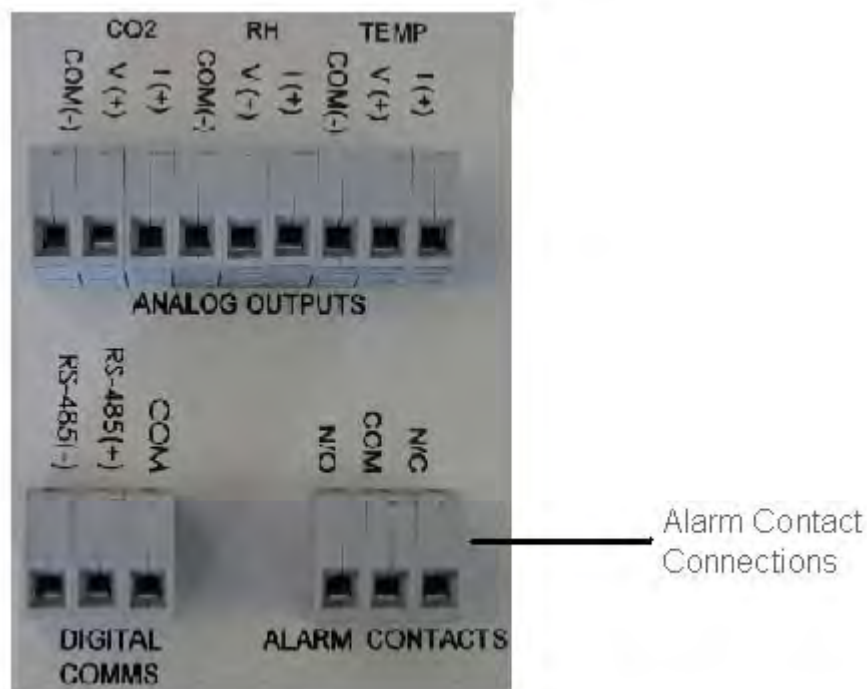

Installing Carboy Water System (BOTL301)

The optional 2.5 gallon carboy water system is preassembled and shipped inside the incubator. The four ¼" bolts required to mount the carboy to the unit will be mounted in the right hand side of the incubator. Remove the carboy assembly from inside the incubator and attach it to the incubator using the ¼" bolts.

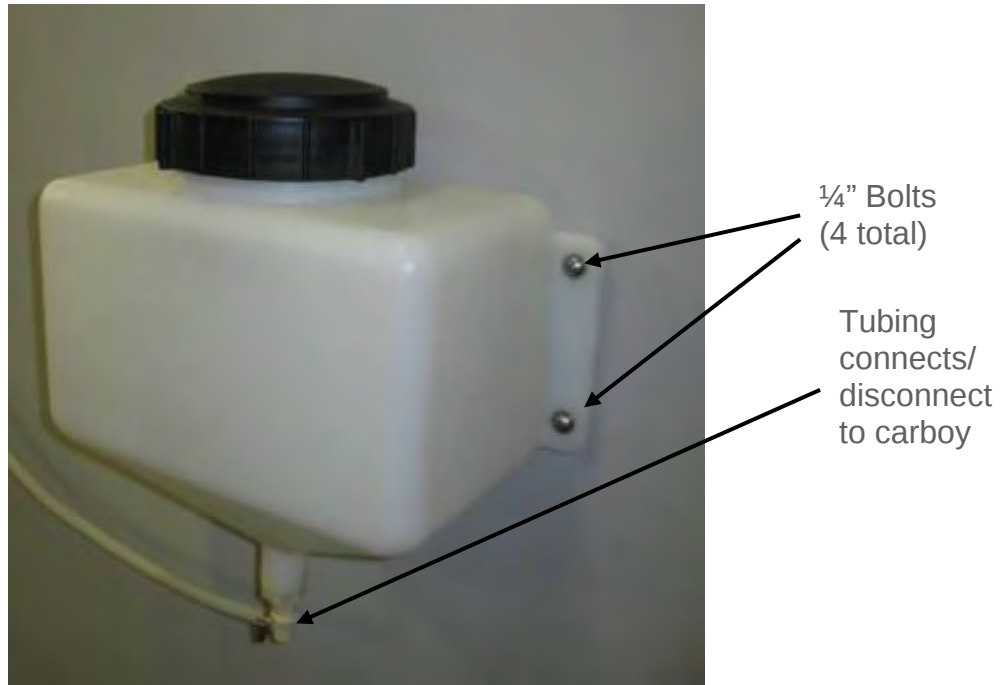

Attach the preassembled tubing provided with the carboy to the water inlet on the rear of the incubator. Fill the carboy with water as described in the "connecting a water supply" section of the manual.

Tubing to water
inlet




Connecting Analog Outputs (OUTP302, OUTP303)

With the purchase of OUTP302 or OUTP303, the controls are equipped with analog outputs. OUTP302 provides 2 connections for monitoring temperature and humidity or CO₂. OUTP303 provides 3 connections for monitoring temperature, humidity and CO₂.

Analog outputs are either milliamps (4-20mA) or voltage (0-5V) signal output that represents each of the displayed temperature, humidity or CO₂ values. These options can be used for connection to in-house data acquisition, recorder, or alarm system.

Parameter	Analog Output	Current	Corresponding Value
Temperature	0 – 5 V	4-20 mA	0 – 100 °C
Humidity	0 – 5 V	4-20 mA	0 – 100 %rh
CO ₂	0 – 5 V	4-20 mA	0 – 100 %CO ₂

Connect shielded wires to the appropriate signal terminals: I(+) for current (mA) or V(+) for voltage (DC). For both current and voltage outputs, COM(-) is common terminal.

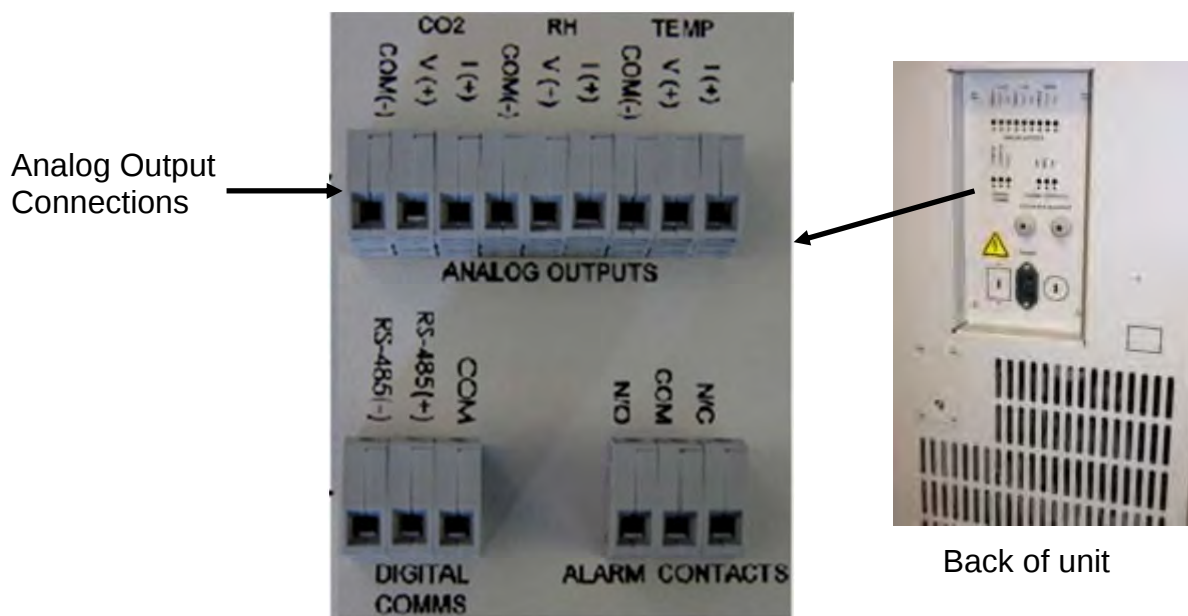

Installing Drain Water Pump (PUMP301)



In applications where a floor drain is not available and a CARON water recycling system is not being used, a drain pump can be purchased to pump any excess condensate from the chamber to a local sink or drain. The pump is located near the middle of the back of the chamber. Connect the supplied tubing from the pump to the sink / drain. The tubing may be run vertically into a ceiling but should not exceed 15 feet height. The pump is equipped with a small reservoir on the bottom of the pump with an internal level switch that will automatically turn the pump *ON* when it is full to drain the water out of the reservoir and into a floor or sink drain.

Installing the Stacking Kit (STCK301)

Two incubators can be stacked using a stacking kit. The kit contains brackets and bolts to secure them together.




Each incubator weighs in excess of 400 pounds. Ensure that sufficient resources are available to safely lift and move the product.

Place the bottom incubator into its location. Using a lift or jack, place the other incubator on top. Bolt into place both brackets (back side, right & left) and secure the two together with 12 screws.



SECTION 5 – OPERATION


With the chamber properly installed and the appropriate utilities connected, the power switch on the right side top wrap can be turned on. Within a few minutes, the temperature and humidity will begin to approach set-points. Here is an overview of the home screen.

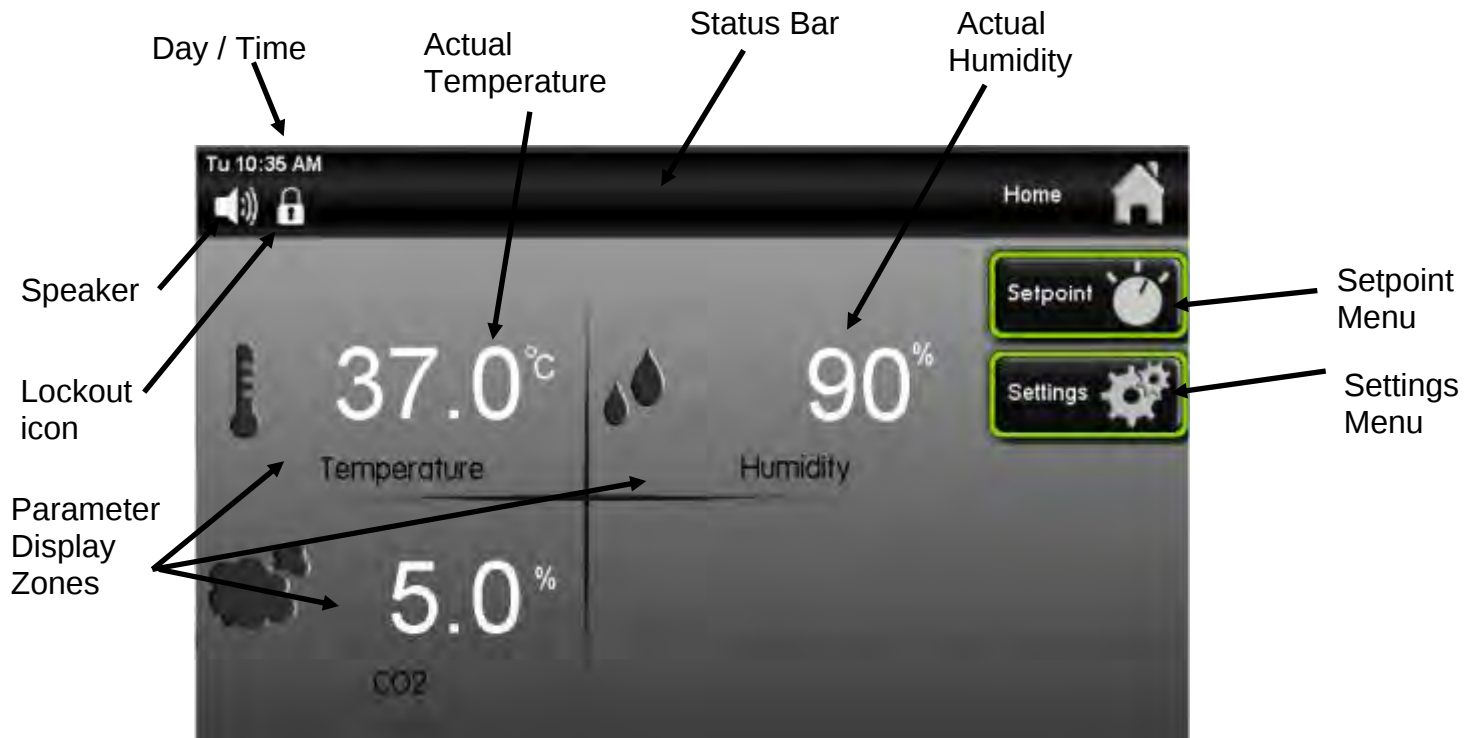

Main screen

Using the Keypad

This control system uses a numeric keypad to enter all parameter values. Similar to a calculator, this allows quick and precise entry of values. When any numeric value button is pressed, the keypad display will pop up over the current display.

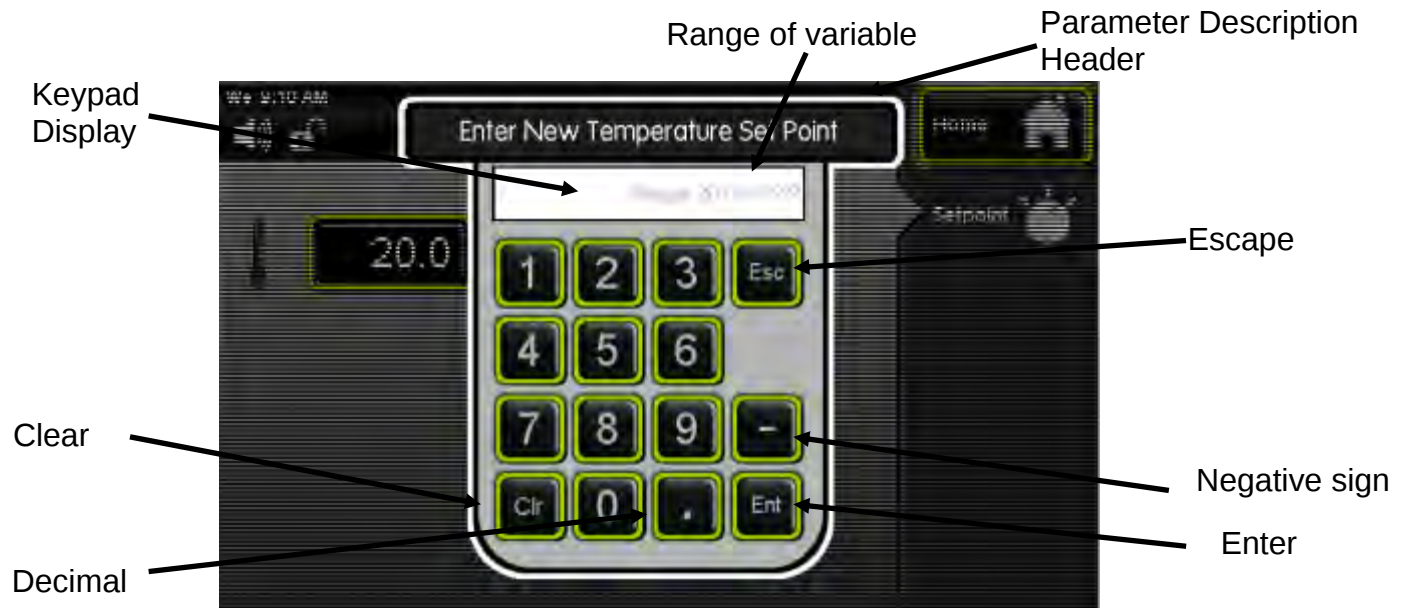

The Parameter Description Header tells what parameter is being changed. The Keypad Display shows allowable values of the parameter being changed (initially) and displays the entered value (when a button is pressed).

The Escape “Esc” button aborts the entry and returns to the previous screen without changing the value. The Clear “Clr” button erases the value that you have entered. After you have entered the value that you want, pressing the Enter “Ent” button and the new value will take effect. This also closes the keypad window. Other keypad buttons include a decimal point button and negative button.

If an invalid numeric button is pressed such that it would create an entry above the parameter’s range, the entered number will not display. For example, if the temperature set point range is 5.0 to 70.0, pressing ‘8’ followed by an ‘0’, only the ‘8’ will display.

If an invalid entry is made with an entry below the range (such as a ‘4’ followed by the ‘Ent’ button), then the entry will clear and the range will be re-displayed.

Learning the screen saver

To ensure long product life, the touchscreen display will automatically enter screen saver mode after 15 minutes. At this time, the screen will be completely blank (ie. black). The illuminated Caron logo (see Equipment Overview section) shows that the unit is powered on and functioning. To wake-up the touchscreen, simply press anywhere on the touchscreen and the main screen will display. If the unit has an alarm condition, the touchscreen will not go into screen saver mode. If an alarm condition occurs while in screen saver mode, the display will automatically wake up and display the alarm.


Changing the Temperature Set-point

The steps below walk through an example of changing the temperature set point from 37.0 °C to 20.0 °C. This example shows optional humidity control. Here is the display of the home screen.

Actual
Temperature



Setpoint Button



To set the temperature set-point, press the (Setpoint) button on the right side of the screen.

Temperature
Setpoint Button



Once the Setpoint screen appears, press the (Temperature Setpoint) button. (In this example the temperature set point initially has a value of '37.0'; this will vary with different initial set point values.)



A temperature setpoint window will appear. Enter the temperature setpoint by using the keypad. For a set point of 20, press  ('2'), then  ('0'), followed by the  (Enter) key. Correct any mistakes with the  (Clear button) and reenter the value.

Once the Enter key has been pressed, the pop-up keypad disappears and the screen returns to the Setpoint display with the new value of 20.0 °C in the temperature set point button.



Press the  (Home) button to return to the main screen.

Changing the Humidity Set-point

The steps below walk through an example of changing the humidity set point. Here is the display of the home screen.



To set the humidity set-point, press the  (Setpoint) button on the right side of the screen



Once the setpoint screen appears, press the  (Humidity Setpoint) button.



Enter the new humidity set point on the keypad as desired and press  (Enter) when complete.





Home Button


Press the  (Home) button to return to the main screen.

Changing the CO₂ Set-point

If an alternative CO₂ set-point is required, the following steps can be taken:

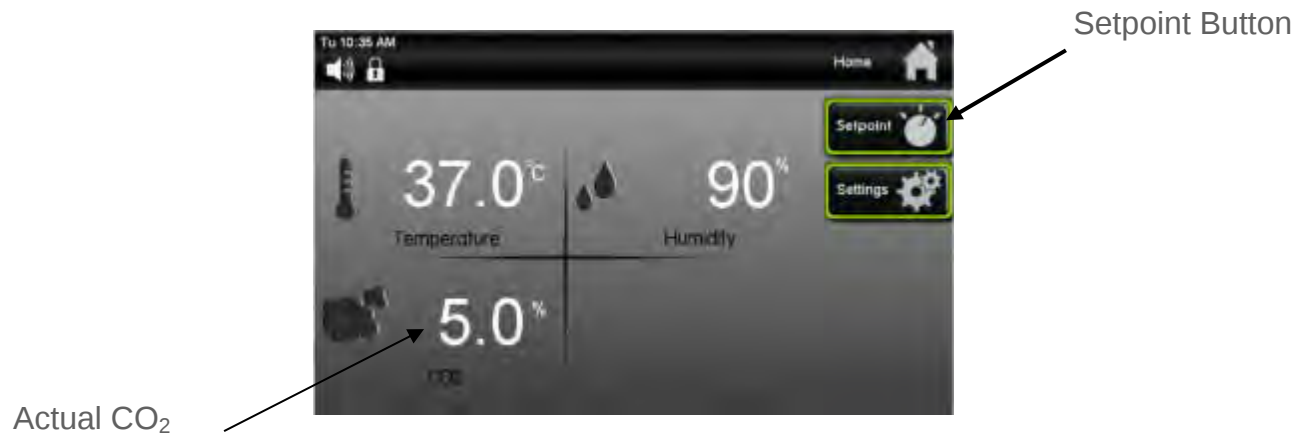


To set the CO₂ set-point, press the  (Setpoint) button on the right side of the screen

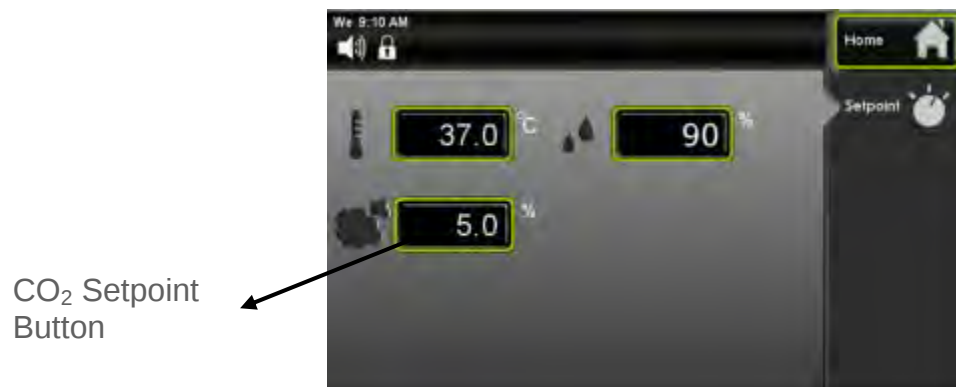


Once the setpoint screen appears, press the  (CO₂ Setpoint) button.



Enter the new CO₂ set point on the keypad as desired and press  (Enter) when complete.

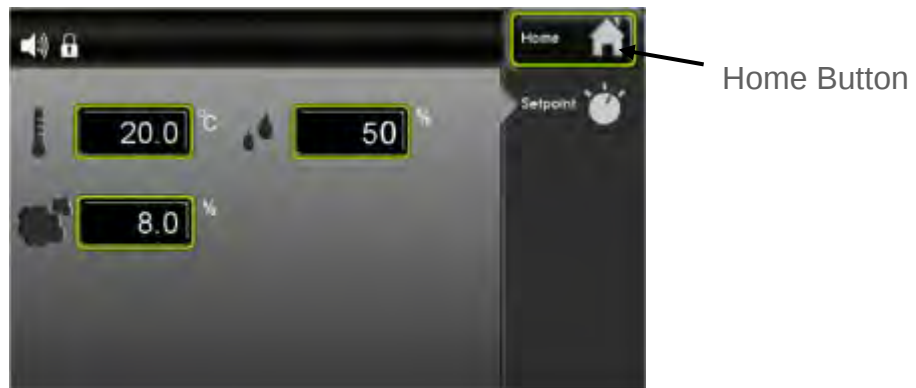

Press the  (Home) button to return to the main screen.

Decontamination Cycle

The 7404-10 incubator is equipped with a moist heat decontamination cycle. The purpose of the cycle is to eliminate common microbial contamination in your incubator and extend the time between manual cleaning cycles. The decontamination cycle is intended to be used as a reactive system to eliminate contamination. It is not necessary to run the cycle at a fixed time interval.

Before initiating a decontamination cycle, the following steps must be completed:

- 1) Remove all samples, products, equipment, etc ... from the incubator.
- 2) Power down the incubator.
- 3) If the unit is equipped with an internal outlet remove outlet from incubator before starting the decontamination cycle.
- 4) Locate the removable sensor access plate in the rear plenum of the incubator. Remove the plate by sliding the fasteners down.
- 5) With power off, remove the infrared CO₂ sensor by unscrewing the connector on the rear of the CO₂ sensor. The sensor unscrews where the orange cable meets the gray sensor housing.



Failure to remove the sensor will result in damage to the sensor and will not be covered by warranty.



- 6) Insert the orange cable into the grommet where the sensor was removed so that it is easily accessed when the sensor is replaced following the decon cycle.
- 7) Replace the CO₂ sensor plate and turn the incubator power switch back on.
- 8) The infrared CO₂ sensor can be disinfected using isopropanol. Spray the cleaner on a soft clean cloth and wipe the sensor.





Do not immerse the sensor in any type of cleaner as damage to the sensor may occur.

Starting the Decon Cycle process, from the home screen,
7404-10 Operations Manual

Rev B 02-24-15


Page 32 of 87

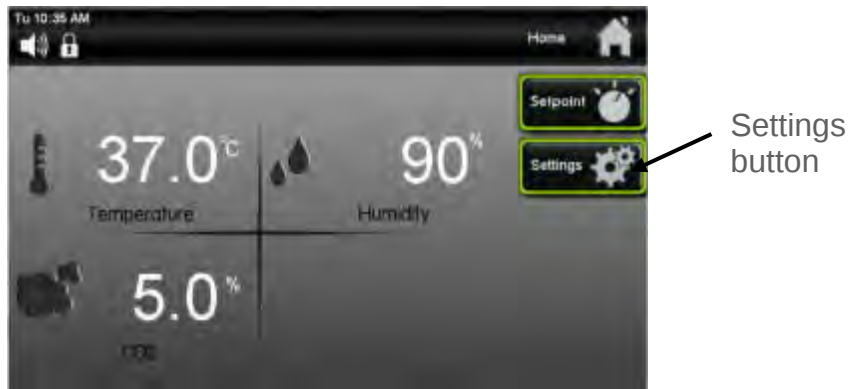

Press the  (Settings) button.



Press the  (Decon Cycle) button on the left side of the screen.

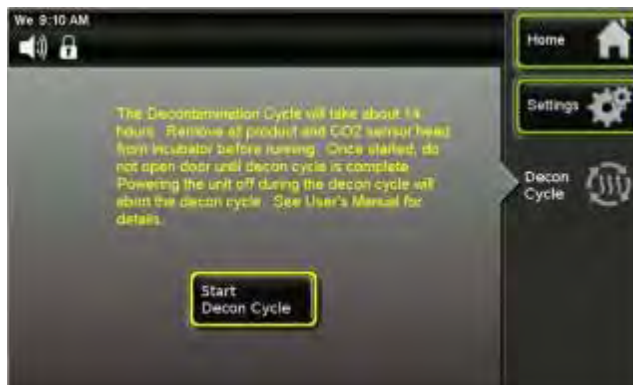

Be sure and read the information that is on the screen before starting the Decon Cycle. Not removing the sensor can cause damage to the CO2 sensor.



The decon cycle will heat the incubator interior surfaces to approximately 90C. Do not open the exterior door during the cycle, as contact with interior surfaces may result in burns. If the outer door is opening during the decon cycle, an audible warning alarm will occur.




Press the (Start Decon Cycle) button to start the Decon Cycle. The cycle will run for about 14 hours. Do not open the door until the cycle is complete. Powering the unit off during the Decon Cycle will abort the cycle.

During the Decon Cycle a “status icon” will appear in the Status Bar. At this time the screen is locked and the Setpoint and Settings buttons cannot be used.

Decon Cycle Info




To check the status of the Decon Cycle press the (Decion Info) icon in the Status Bar,

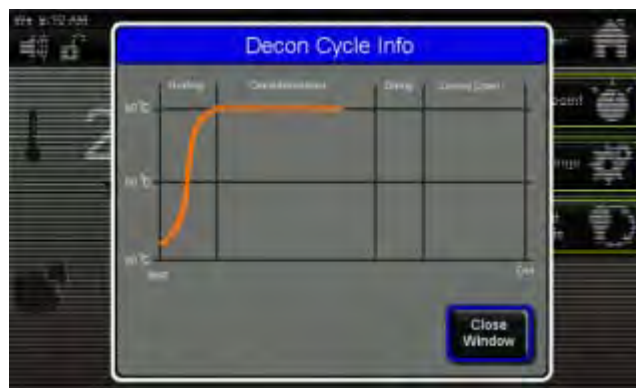

The Decon Cycle Info Screen will appear displaying the current stage that the Decon Cycle is in.

When the Decon Cycle is complete there is a message displayed on the Decon Cycle Info screen that tells you that the cycle is complete and that is safe to replace the CO2 sensor.

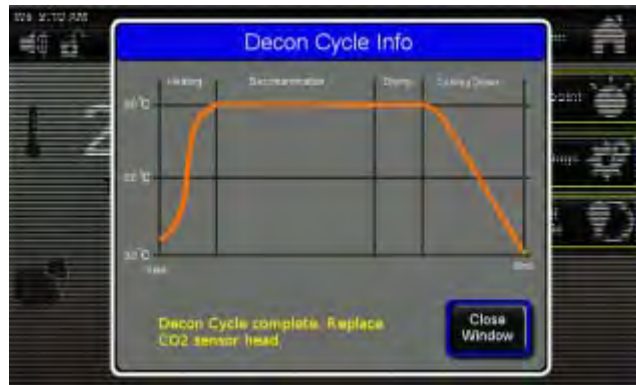

Press the (Close Window) button to return to the main screen.

Extended Temperature Range (EXTD301)


The extended temperature range is a factory installed option for model 7404-10. This extends the temperature range down to 10°C. Simply enter a lower temperature value when entering the temperature set point.

SECTION 6 – OPTIONAL ACCESSORY OPERATION

Using the Carboy Water System (BOTL301)

To fill the carboy while attached to the incubator, unscrew the cap. Fill carboy with distilled or deionized water (see Connecting the Water Supply section for details). The carboy holds 2.5 liters.

If the carboy must be removed in order to fill it up, first disconnect the tubing between the carboy and incubator by pressing the metal lever at the tubing connects / disconnects at the bottom of the carboy. Then unscrew the four mounting screws and remove the carboy. After re-attaching the carboy, connect the tubing by simply pressing the plastic fittings into each other.

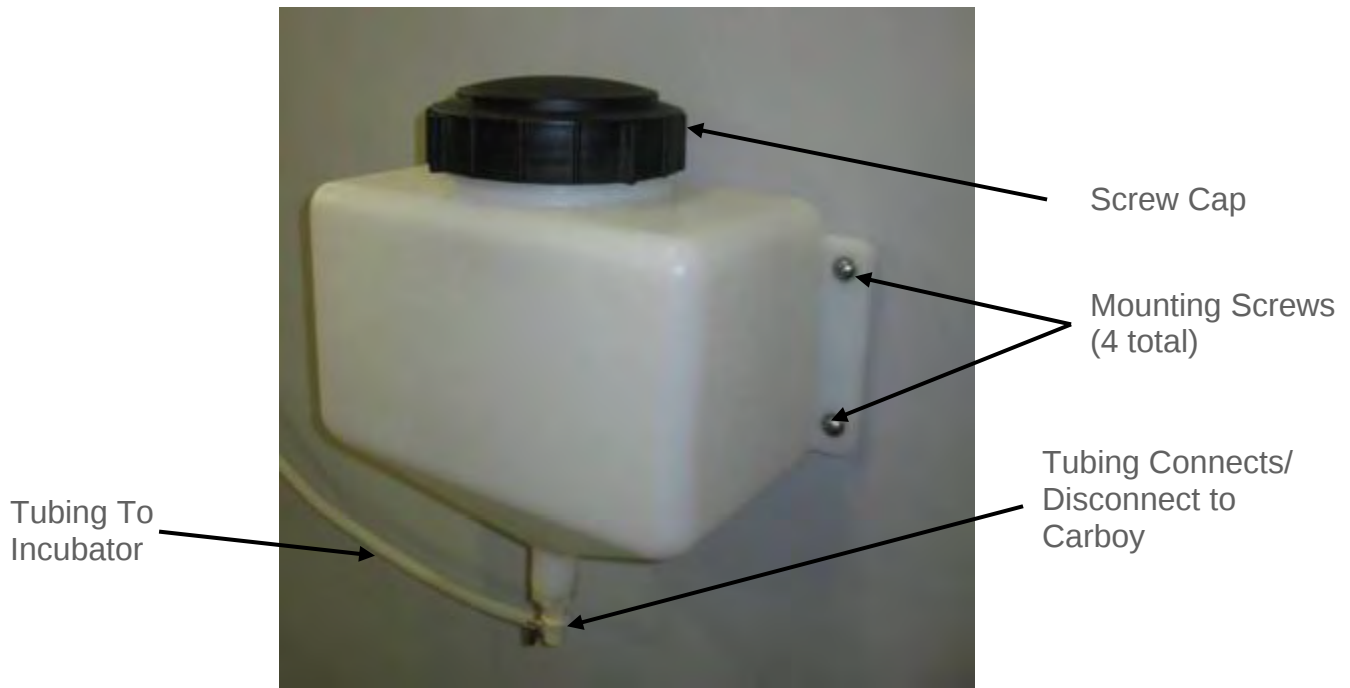

Operation of the Data Logger (DLOG301)



The DLOG301 option provides the customer with a means of logging data electronically for viewing at a later date. Logged variables are temperature, humidity, CO₂ and light intensity (but only if the chamber is equipped with those features.) All data is time-stamped with year, month, day of the month, hour, minute, 24 hour time (ISO 8601 format). This data is stored internally in the chamber in non-volatile memory.

Data is logged every 5 minutes (provided the chamber is on), more than 10 years of data can be stored in memory. If the internal memory fills up, new data overwrites the oldest data.



Continuous writing to the flash drive necessitates a high quality industrial grade device. Use only the flash drive provided by Caron (or equivalent: single level cell memory, wear leveling algorithms, error correcting code).




File name format is Data start YYYY_MM_DD HH_MM" (hours in 24 hour time)

When the chamber is on, the chamber's history data is being stored even when a flash drive is **not** inserted in the USB port. This data may be retrieved anytime using the provided USB flash drive.

Here are the methods for retrieving data:

Continuous logging of data

Insert the flash drive into the chamber's USB port. When first inserted, it creates a .csv file called 'DATA START' with the current date and time in the file name. At 5 min intervals, the chamber's process values are appended to the file. (The file will get as large as the flash drive will allow which would be years of data.)

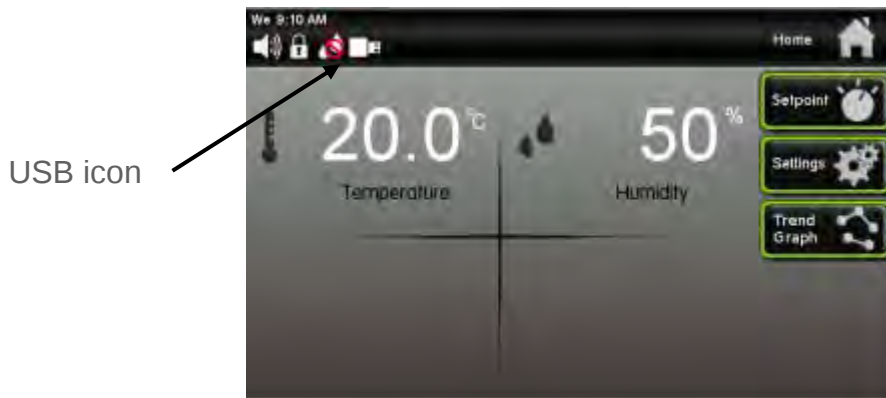

USB icon appears in in Status bar indicating that data is being written to flash drive.

To retrieve the data press the 'Eject' button. The flash drive is then inserted into a computer for uploading the data.

Upon re-insertion of the flash drive, a new .csv file is created, even if the old file is still present. File name nomenclature is "Data Start YYYY_MM_DD HH_MM" with hours in military time.

History Retrieval





Select the 'Auto Export' feature on the USB menu screen. Insert the flash drive into the chamber's USB port. A new .csv file is automatically created on the flash drive with all the stored history data. The file name nomenclature is "Data End YYYY_MM_DD HH_MM".



There is also an 'All Data' feature to indicate if the upload should include all data (since the unit has been used) or just the history data since a flash drive was inserted last. An 'Info' button will appear in the status bar warning the user not to remove the flash drive while the data is being uploaded. The length of time to upload the file will depend on the file size. When the 'Info' button disappears from the status bar, press the 'Eject' button to safely remove the flash drive. Now the data can be uploaded to a computer for viewing.

Using the Continuous Logging of Data method nothing on the touch screen has to be setup. However using the History Retrieval method of data will require going into the USB screen to select either the 'Auto Export' or 'All Data' buttons before inserting flash drive into USB port.

To select the 'Auto Export' and 'All Data' buttons.

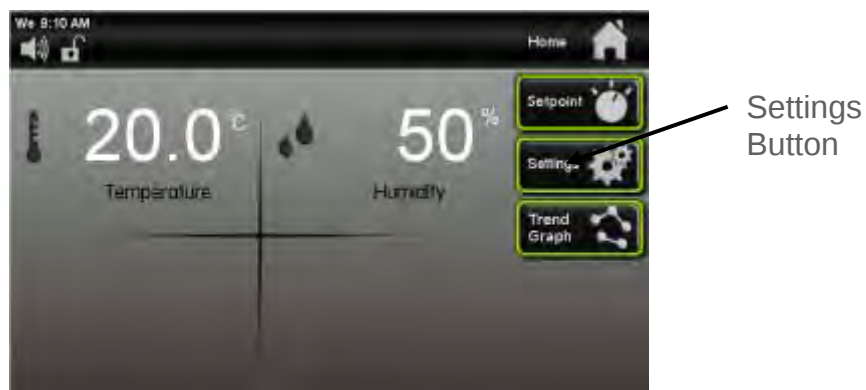

Press the (Settings) button.



Setup Button




Press the (Setup) button.



USB Button



Press the (USB) button.




When the 'All Data' button is selected this will retrieve all of the data from when the chamber was first turned on, up to the current time when flash drive was removed from USB port.



When the 'Auto Export' button is selected this will retrieve the data from the previous time when data was retrieved, up to the current time when flash drive was removed from USB port.

USB flash drive icon

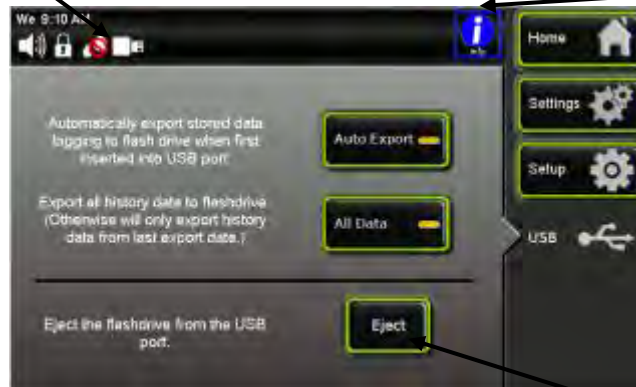

Info button

Eject button

When flash drive is inserted into the USB port a 'USB flash drive' icon and flashing 'Info' button appears in the status bar indicating that the data is being downloaded to the flash


drive. Once 'Info' icon stops flashing select the 'Eject' button.



Wait until the USB icon disappears to safely remove the flash drive from the USB port.

Note: Press the Eject button before removing the flash drive from the chamber, otherwise there could be the risk of corrupt data.

Here is a graphic to illustrate how the data retrieval works.

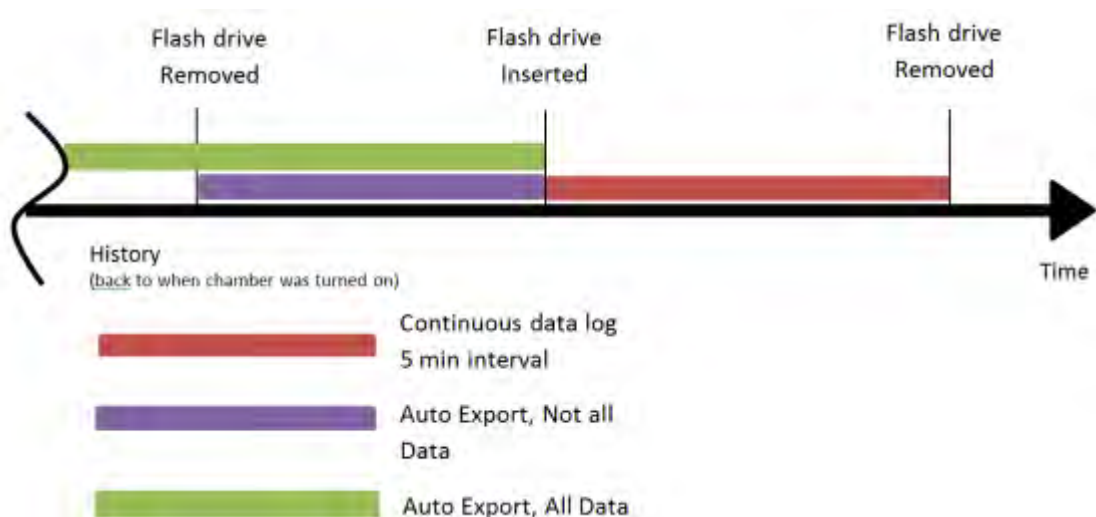

Built In Gas Guard System (GASG302)

An optional built in gas guard system is available to allow two tanks of CO₂ to be connected to an incubator requiring approximately 15 psig of gas pressure. The unit is designed to automatically switch from the primary tank to the secondary tank when low gas pressure of approximately 10 psig is detected on the primary tank. This allows for a continuous supply of CO₂ to an incubator after the primary tank is empty. In addition, the user is notified of a tank empty scenario via an audible and visual alarm.



The CO₂ gas supply should be 99.5% pure and should not contain a siphon tube. Gas pressure to the unit must be regulated to less than 30 psig. Failure to do so could cause tubing to burst.


The CO₂ gas supplies must be equipped with two stage regulators to ensure that the incoming gas to the unit is regulated to appropriate levels. The high pressure stage should have a 0-2000 psig range, and the low pressure gauge should adjust from 0-30 psig. When connecting the gas supplies, adjust each tank output to 20-25 psig. If the appropriate regulators are not available, contact CARON customer service to purchase them.

Once the cylinder regulators are installed and adjusted on each tank, connect the outlet of the regulator on Tank 1 to the hose barb fitting labeled Tank 1 on the back of the unit. Repeat the process for Tank 2. Turn on the regulated gas supplies and check the connections closely for leaks.

To access the internal Gas Guard,



Settings
Button




Press the (Settings) button.



Gas Guard
Button



Press the (Gas Guard) button.

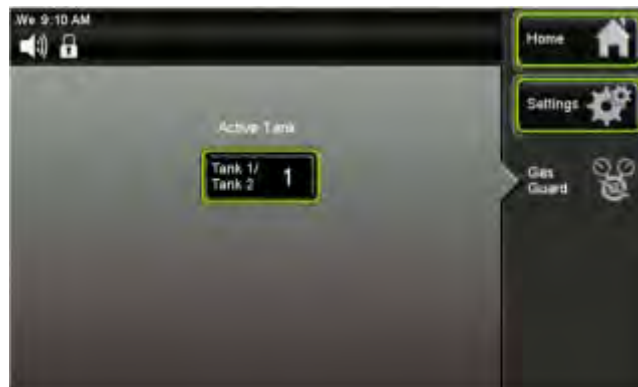

Press the (Tank 1 / Tank 2) button, will manually switch the tanks.

The factory default “master tank” is Tank 1. When the appropriate gas pressure is supplied to both tanks, the master tank will always be used as the gas source. The unit will swap from the master tank to the alternative tank whenever a low gas pressure condition is detected.

Ultraviolet Germicidal Lamp (LGHT602)



Before removing access panel(s), disconnect electrical power.



Avoid exposure to direct or reflected germicidal ultraviolet rays. Germicidal ultraviolet rays are harmful to the eyes and skin.

Replacing UV Light (optional accessory)

1. Turn off chamber and unplug power cord.
2. Remove left access panel.
3. Unclip green wire with ground clip from UV light housing.



UV Light Housing Cap

Green Wire with
Ground Clip

4. Pull UV light housing cap from UV light housing. Connected UV lamp will come out with it.





See separate ultraviolet light owner's manual for specific warnings and instructions.

5. Discard used UV lamp



Follow local regulations for disposing lamps.

6. Insert new UV lamp into lamp connector socket.
7. Install UV light housing cap (with attached new UV lamp) into UV light housing.
8. Re-attach ground clip.



Ground clip must be securely attached to UV light housing to reduce risk of electrical shock.


9. Install left access panel.
10. Plug power cord in and turn chamber on.

Interior Electrical Outlet (OUTL305 - OUTL309)

An optional interior duplex electrical outlet is available to supply power to small interior appliances such as shakers or stirrers. It is not intended to power high current draw devices. For incubators that have a single interior duplex outlet, the outlet is fused at 2.0 Amps. Incubators with two interior duplex outlets are fused at 4.0 Amps total. All outlets are resettable GFI protected. Other outlet configurations can be purchased..



OUTL305 US outlet is 115V/60Hz fused at 2.0A



OUTL306 European “Schuko” outlet is 220V/50Hz fused at 2.0A



OUTL307 UK, British outlet is 220V/50Hz fused at 2.0A



OUTL308 Australia outlet is 220V/50Hz fused at 2.0A



OUTL309 Brazil outlet is 220V/50Hz fused at 2.0A

Operation of Temp or Temp/Rh 6" Recorders (RCDR316/RCDR317)

Built in 6" ink pen temperature and or humidity recorders can be purchased with CARON incubators. The recorders are shipped installed on the outer door of the incubator from the factory and require no installation.

Changing the chart paper:

Press and hold the "change chart" button on the recorder (#3) for approximately one second until the pen begins to move to the left of the chart and then release the button. Wait until the pen has completely moved off of the chart. To remove the chart paper, unscrew (counter-clockwise) the chart "hub" knob at the center of the chart. Remove the old chart paper and position the new one so that the correct line coincides with the time line groove on the chart plate.

Re-attach the chart "hub" knob and fasten securely against the chart. Press and hold the "change chart" button (#3) again for approximately one second until the pen begins to move back onto the chart and then release the button. Check to make sure that the pen is marking on the chart paper. If it is not, then carefully adjust the pen arm to establish contact with the paper.


Chart recorder marking system:

This type of pen consists of a self contained ink reservoir with a porous plastic stylus which is snapped around the outer edge of the metal pen arm. A pen cap is provided to extend the life of the ink pen during shipping or when the recording unit is not in service. To remove the pen cap, gently lift the pen arm away from the chart paper. Remove the black plastic pen cap to expose the fiber tip of the ink pen and gently place the pen back onto the chart paper. Do not let the pen arm "snap" back onto the chart paper. This will flatten the fiber tip of the pen and will no longer give you a fine line marking on the chart paper. Place the pen cap in a safe place for future use. If the stylus does not touch the chart, adjustment can be made by slightly bending the metal pen arm in the center towards the chart paper. Do not use more pressure than is necessary to create a fine line marking on the chart paper. As the pen ink supply runs out, the pen color will become lighter. This indicates that the pen should be replaced.

Replacement of the Pen:

Recorders that are equipped with fiber tipped cartridge pens will have a cartridge that is color coded "red" to designate pen number one and an optional cartridge that is color coded "blue" to designate pen number two. The pen cartridge is securely fastened to the metal pen arm using a special "U" clip tab. For ease of replacement, it is suggested that the two screws that hold the pen arm be loosened and the pen cartridge and metal pen

arm be removed as an assembly. Unsnap the plastic "U" clip tab of the pen cartridge from the metal pen arm, remove and discard the old pen cartridge. Replace the new cartridge by opening the hinge and snapping it securely around the metal pen arm. Refer to the image below:

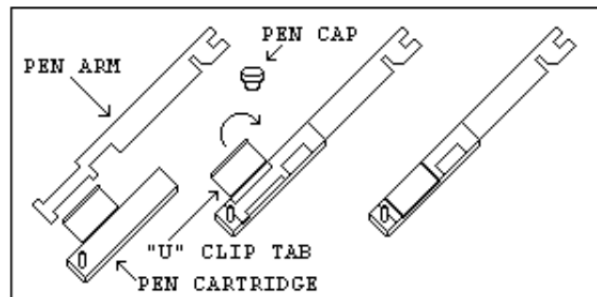

Pen Arm Calibration:

To check and/or adjust the recording pen(s) calibration to the outer most temperature graduation of the chart, press and hold the "change chart" button (#3) until the pen begins to move off of the chart. Once the pen(s) has moved off of the chart, again press and hold the "change chart" button (#3) until the pen begins to move back onto the chart. The pen should briefly stop at the outer most temperature graduation of the chart before continuing onto the chart to begin recording. If the pen does not stop exactly at this location on the chart, it can be adjusted or "calibrated" by using the left (#1) or right (#2) arrow buttons.

When the pen moves back onto the chart and briefly stops, you will have approximately five seconds in which to adjust the pen's position using the left and right arrow buttons of Figure 3.

On multiple pen recorders, each pen will move (one at-a-time) onto the chart briefly stopping at the outer most temperature graduation of the chart at which time the pen's position can be adjusted by using the left (#1) or right (#2) arrow buttons. When the time to adjust the position of the first pen has expired, the second pen will move onto the chart briefly stopping at the outer most temperature graduation of the chart at which time the second pen's position may be adjusted.

Each time the chart paper or fiber tip pen cartridge is changed, you should make sure that each pen stops at the outer most temperature graduation of the chart paper. Otherwise, this pen offset will cause the unit to record an incorrect temperature on the chart.

Recorder Calibration:

If a calibration adjustment is required for a single pen recorder, use the left (#1) and right (#2) arrow push buttons on the recorder to calibrate (or move) the pen's position on the chart to correspond to the temperature of the solution. The arrow buttons must be held for approximately five seconds before the pen will begin to move.

For two pen recorders, you must first select the pen that you wish to calibrate. This is done by pressing the left (#1) arrow button to select the red pen or the right (#2) arrow button to select the blue pen. The arrow button must be held down until the green LED light goes out. After the green LED light goes out, follow the instructions in step #3 above.

Battery Backup:

The green LED light remains a constant green color indicating that both the battery and the main power to the unit are good. Refer to Figure 5 for the location of the green LED indicating light. If the AC power were to fail or the battery becomes weak, then the green LED light will begin "flashing" indicating that either you have lost the main power to the unit or it is time to replace the battery. Having a 9 volt DC battery back-up in place, will allow the recorder to continue to function normally for approximately 24 hours in the event of a power failure.

Operation of Temp or Temp/Rh 10" Recorders (RCDR318, RCDR319)

Built in 10" thermal pen recorders can be purchased with CARON incubators. The recorders are shipped installed on the outer door of the incubator from the factory and require no further installation. Unlike ink pen recorders, the thermal recorders draw their own chart and control lines.

The 10" recorders have been setup at the factory in the following configuration: 7 Day / 24 Hour / Temperature 0-100°C / Humidity 0-100% (for dual input recorders). If this is not the ideal configuration for an application, the recorder may be reconfigured using the following process:

Configuring the recorder:

In order to configure the recorder, you will need to enter the set-up mode of the recorder. To enter the set-up mode of the recorder, press and hold the Change Chart button (#3) until the thermal pen arm begins to move off scale and then release the button.

Note: The green LED light will flash fast while the thermal pen arm is moving off scale.

Wait until the thermal pen arm has moved completely off scale and stops (the green LED light will stop flashing and will be steady On). Unscrew (counter clockwise) the chart "hub" knob at the center of the chart and remove the recording chart paper. Gently lift the thermal pen arm just enough to be able to slide the paper out from beneath it. Remove the recording chart paper and place the Setup Chart onto the recorder. This chart contains the configuration categories of the recorder (Probe Input, Inner Chart Temperature, Outer Chart Temperature, Temperature Scale, Chart Rotation Speed, Input Filtering, Optional Relay Contacts and Date/Time for internal clock).

Next, press and hold either button #1 or #2 until the green LED light goes out and release the button. If this step is successfully completed, the pen arm will move to the outermost graduation ring of the Setup Chart. Use the Left (#1) or Right (#2) arrow buttons to adjust the center of the thermal pen to be on this outermost graduation ring.

Position the Setup Chart so that the tip of the thermal pen is in the center of the Start circle. Tighten the chart hub knob to secure the chart in place. Next, press and release the Change Chart button to begin. The chart will rotate to the first category (Input #1). Use the Left and Right arrow buttons to move the thermal pen arm to the desired option of each category. Press and release the Change Chart button to accept the selection and advance to the next category. You must press and release the Change Chart button when you have finished configuring the last category in order to save all of the changes that have been made to the recorder's configuration. The thermal pen arm will

move off of the chart allowing you to place the recording chart paper onto the recorder. Press and release the Change Chart button to begin recording.

Changing the Chart Paper:

Press and hold the Change Chart button (#3) for approximately one (1) second until the pen begins to move off scale and then release the button.

Note: The green LED light will flash fast while the thermal pen arm is moving off scale.

Wait until the thermal pen arm has moved completely off scale and stops (the green LED light will stop flashing and will be steady On). To remove the chart paper, unscrew (counter clockwise) the chart "hub" knob at the center of the chart. Gently lift the thermal pen arm just enough to be able to slide the paper out from beneath it. Remove the old recording chart paper and position a new one.

Re-attach the chart "hub" knob and screw securely (by hand) against the chart. Press and hold the Change Chart button (#3) again for approximately one (1) second and the thermal pen arm will move back onto the chart and begin recording.

Green Light LED Status:

The green LED light (located just below the three button membrane switch) is used to show the recorder's status:

- 1.) LED on steady (not flashing) and input(s) recording within chart range, indicates unit is recording normally.
- 2.) LED on steady (not flashing) and pen arm above outermost graduation and not moving, indicates recorder is in Change Chart mode. Press and release Change Chart button to return to normal recording mode.
- 3.) LED flashing rapidly and one or both inputs recording at outermost or innermost graduation indicates a sensor break. Check or replace sensor(s). If sensor(s) are ok, make sure process temperature is within configured range of recorder.
- 4.) LED flashing slowly (.8 seconds ON / .8 seconds OFF) indicates recorder is in Set-Up mode. Refer to section CONFIGURING THE RECORDER.
- 5.) LED is Off indicates that there is no power to the recorder. Check A/C power to the recorder.

Recorder Calibration:

If calibration is required for single input recorders, use the Left (#1) and Right (#2) arrow buttons on the recorder to calibrate the temperature being recorded on the chart to correspond to the temperature of the solution. The arrow buttons must be held for approximately eight (8) seconds before the pen begins to move.

If calibration is required for dual input recorders, you must first select the input that you wish to calibrate. This is done by pressing and holding the Left (#1) arrow button to select Input #1 or the Right (#2) arrow button to select Input #2. The arrow button must be held down until the green LED light turns off, after which follow the instructions in single input instructions above.

Maximizing Pen Life:

In order to maximize the amount of life expected out of the thermal pen tip, follow these simple rules:

- 1) Never let the thermal pen tip ride on the chart plate when the chart paper is not present. This will damage the protective coating of the heating element.
- 2) Never use chart paper that is creased or that has been folded.
- 3) Periodically clean the thermal pen tip with a cotton swap dipped in alcohol. Clean more often when operating the recorder in a dusty environment.
- 4) Always keep the door closed while the unit is recording.
- 5) Never lift the pen arm more than is necessary to remove and replace the chart paper. Excessive lifting may cause a decrease in the pen tip pressure and cause light printing.

SECTION 7 – CALIBRATION

The temperature and humidity systems can all be calibrated as necessary. CARON recommends an annual calibration check of each system. Before making a calibration adjustment, allow the cabinet to stabilize a minimum of 12 hours from a power off condition. If the unit has been in operation, allow a minimum of 3 hours of stable operation at all set-points. If you do not have the appropriate reference instruments to perform calibration, contact CARON's service department for on-site calibration at service@caronproducts.com. Caron also provides validation services which ensures that the unit is functioning properly according to IQ, OQ and PQ protocols which satisfy FDA guidelines for qualification verification of equipment.




Be sure that all reference instruments are calibrated to an appropriate standard.

The Calibration Screen


To get to the calibration screen from the home page:



Main screen with HUMD304, HUMD307 option



Press the (Settings) button.




Once the settings screen appears, press the (Calibrate) button.



Calibrating the Temperature

If temperature calibration is needed, the following steps can be taken:

Locate the reference instrument's temperature sensor in close proximity to the cabinet's geometric center. Be sure that the stabilization times described earlier have been satisfied prior to performing calibration.

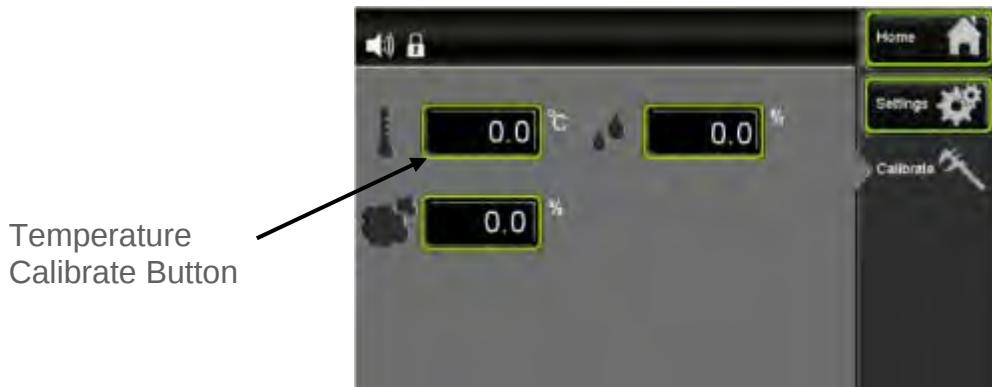

At the calibrate screen, press the  (Temperature Calibrate) button.



Enter the temperature offset by using the keypad and pressing  (Enter) when complete.

A positive value will move the temperature 'up' and a negative value 'down'. Press the 'home' button and verify the proper temperature is displayed.

Temperature calibration (example)

If the chamber temperature display reads 40.0°C and the calibrated independent sensor shows 40.3°C, set the temperature offset value to 0.3°C. If the calibrated independent sensor shows 39.6°C, then the entered offset should be negative. In this example the required offset to temperature would be -0.4°C.

Calibrating the Humidity

If humidity calibration is needed, the following steps can be taken:
Locate the reference instrument's humidity sensor in close proximity to the cabinet's geometric center. Be sure that the stabilization times described earlier have been satisfied prior to performing this calibration.

A positive value will move the humidity 'up' and a negative value 'down'. Press the 'home' button and verify the proper humidity is displayed.

Humidity calibration (example)

If the chamber humidity display reads 80% and the calibrated independent sensor shows 83%, set the humidity offset value to 3.0%. If the calibrated independent sensor shows 74%, then the entered offset should be negative. In this example the required offset to humidity would be -6.0%.

Calibrating CO₂

If CO₂ calibration is needed, the following steps can be taken:
Locate the reference instrument's CO₂ sensor in close proximity to the cabinet's geometric center. Be sure that the stabilization times described earlier have been satisfied prior to performing this calibration.

A positive value will move the humidity 'up' and a negative value 'down'. Press the 'home' button and verify the proper humidity is displayed.

SECTION 8 – ALARMS


Alarm System Overview

The incubator control system is equipped with an alarm system that constantly monitors temperature, CO₂ and humidity (on controlled humidified models) to ensure the user is notified if the cabinet goes into an alarm condition. Notification occurs via an alarm pop-up window and a buzzer. Each alarm condition has been factory programmed to minimize nuisance alarms while maximizing warning time. There is a 2 hour time delay at start-up and set point changes. To avoid nuisance alarms after a routine door opening, an alarm condition must be present for 15 minutes before the operator is alerted. If the optional remote alarm contacts are present, in an alarm condition, the dry contacts will change state.


The following alarm messages could be displayed:

- Chamber temperature is higher than set-point temperature
- Chamber temperature is lower than set-point temperature
- Chamber CO₂ is higher than set-point CO₂
- Chamber CO₂ is lower than set-point CO₂
- Temperature sensor error

In the event an alarm occurs, the alarm indicator will appear on the status bar and an audible alarm will occur. The flashing (Alarm) icon will appear on the status bar and the alarm pop-up window will automatically appear.

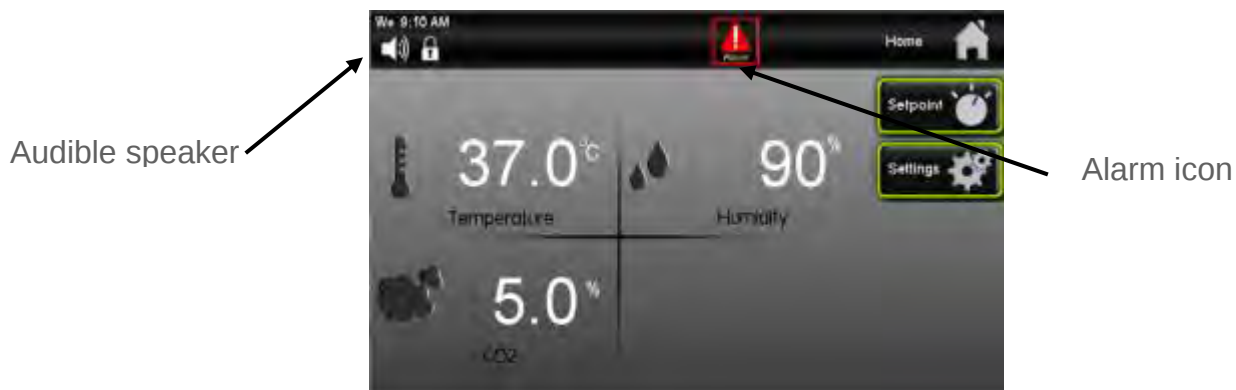


The flashing  (Alarm) icon will appear on the status bar.

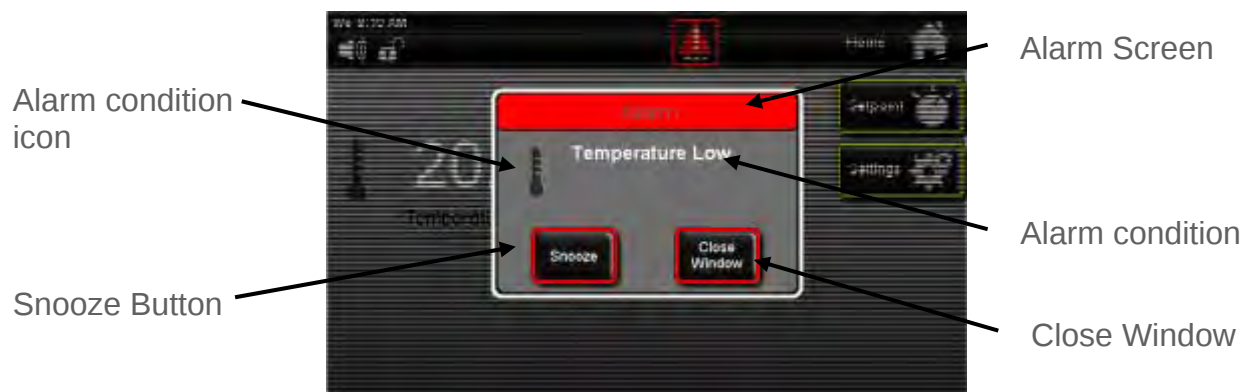

Snoozing the speaker:

When in an alarm condition, the speaker can be temporarily silenced to avoid being a nuisance to those nearby. The alarm will reappear after 60 minutes has passed, if the condition has not been corrected. (The audible alarm will not sound if the alarm speaker is muted)




Press the (Snooze) button, the audible alarm is silenced for a period of 60 minutes.


When the alarm condition is corrected the alarm indicator and the audible alarm will automatically turn off (unless there is another alarm condition).



To check what the alarm condition is, press the (Alarm) button on the status bar.



and the alarm window will be displayed. If the (Snooze) button has already been pushed and 60 minutes have not passed the Snooze button will be “greyed” out.




If you press the (Close Window) button, the Alarm Window will close, but the alarm will still be present as a flashing alarm icon on the status bar for the remainder of the 60 minutes time. It will not reset the 60 minutes alarm countdown time if the alarm condition is viewed on the pop up window.


After the 60 minutes time has passed for an alarm condition, the counter will reset itself to 60 minutes and repeat the countdown process again until the alarm has been resolved.

Muting the speaker:


By factory default, when an alarm condition is present, the speaker will sound. This speaker can be muted in an 'on/off' fashion eliminating all audible sounds. (Muting the speaker will silence it until manually 'un-muted'. This is different than 'snooze' in that fact that snooze can only be enabled when an alarm condition is present and only lasts for 1 hour.) When the speaker is muted, the alarm icon continues to flash and the remote alarm contacts (optional) remain in the 'alarm' state.

To mute the speaker:

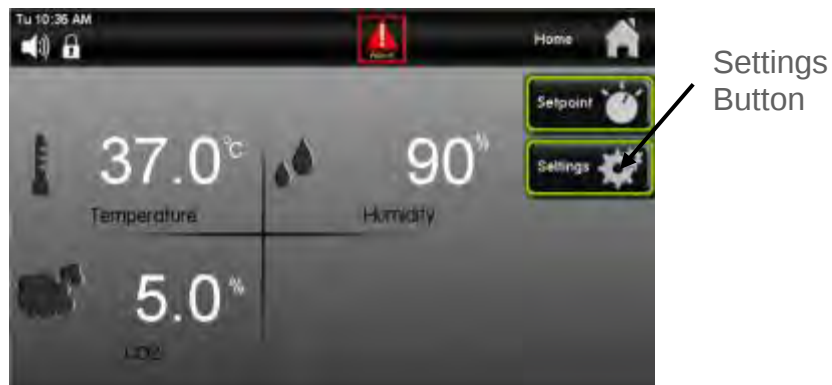

Press the  (Settings) button.




Press the  (Speaker Mute) button.



The Speaker Mute button toggles to the "on" position , and the speaker icon changes to  "Speaker Muted" icon.

Changing Alarm Set-points

All alarm set-points were pre-set at the factory to minimize nuisance alarms that could be created as a result of door openings. Alarm set-points can be changed based on individual user requirements. To change the alarm set points:

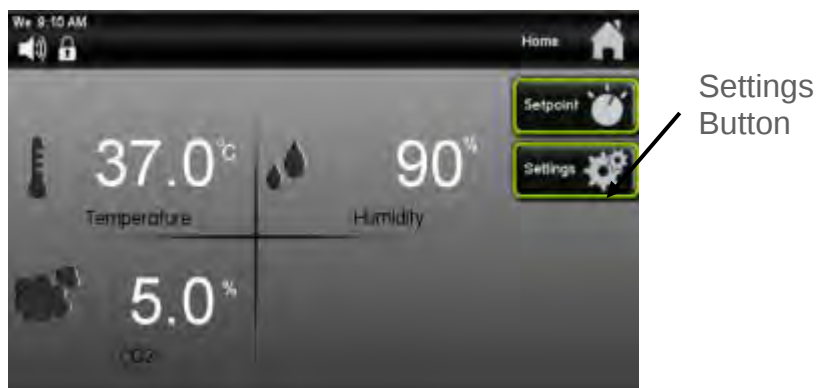

Press the (Settings) button.

Alarms Button




Press the (Alarms) button.

Temperature Alarm Button

Humidity Alarm Button




CO2 Alarm Button

Press the  (Temp Alarm) button.

Temperature
Alarm High Limit


Temperature
Alarm Low Limit

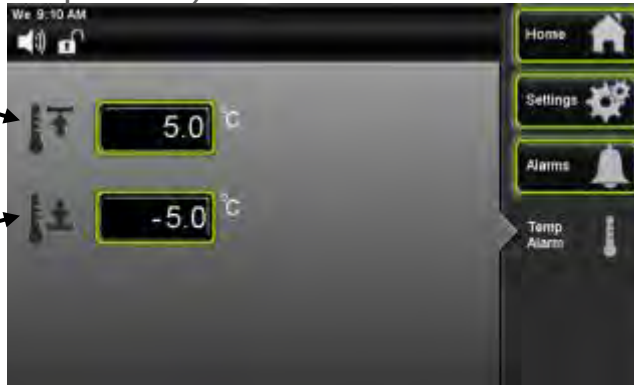


Once the alarm screen appears, press the  (Temp High Limit) button.



Keypad screen will appear. Enter the High Temp Alarm value; press  (Enter) when complete.

To change the CO2 Alarm, press the  (Alarms) button on the navigation

menu to go back to the Alarms screen. Press the  (CO2 Alarm) and

 (Humidity Alarm, *Controlled Humidity only*) buttons and repeat the same steps for CO2 and humidity.

SECTION 9 – ALERTS

Alert System Overview

The incubator control system is equipped with an Alert system that constantly monitors features of the incubator and to notify the user if the incubator needs any type of service that may need done, to ensure good running performance of the incubator. The intent is to notify the user that the incubator needs attention thus minimizing the risk of a failure or alarm condition. Some of the alert features are replace the atomizers (humidified units only), replace the air filter, and equipment calibration is due.


Notification occurs via an Alert icon on the status bar. When the Alert icon is pressed, a pop up window will display the alert condition(s). Each alert condition parameter is factory pre-set, no adjustment is necessary. The Alerts are cleared through the Maintenance screen.



Press the  (Alert icon).



The Alert pop up window will appear displaying the alert message.




Press (Close Window) button to make the pop up window disappear.

Resetting on the Maintenance Screen

Maintenance Menu Screen lets users check to see how much time is remaining on an item that may need routine service or calibration. This is very convenient to inform the user that a particular item will need to have service performed soon. After service has been completed, the item needs reset and the alert will disappear.



Press the (Settings) button.




Once the settings screen appears press the (Maintenance) button.



Once a Maintenance item is displayed on the Alert screen, it will continue to be present as an icon in the Status Bar until the Maintenance item is corrected and the (Reset) button is pressed resetting the replacement time to “new” status.



Press the  (Home) button to return to the main screen.

SECTION 10 – INFO


Info System Overview

The incubator control system is equipped with an Information system that constantly monitors the incubator and to notify the user when an automatic condition is occurring. This applies to conditions such as Decon Cycle or others that cannot be switched on and off by the user but is controlled automatically by the software of the control system. This notification cannot be disabled, it only lets the user know the incubator's current status.

Notification occurs via an Info pop-up icon on the status bar. When the Info icon is pressed a pop up window will display the Info condition(s).



The (Info) icon will appear on the status bar.

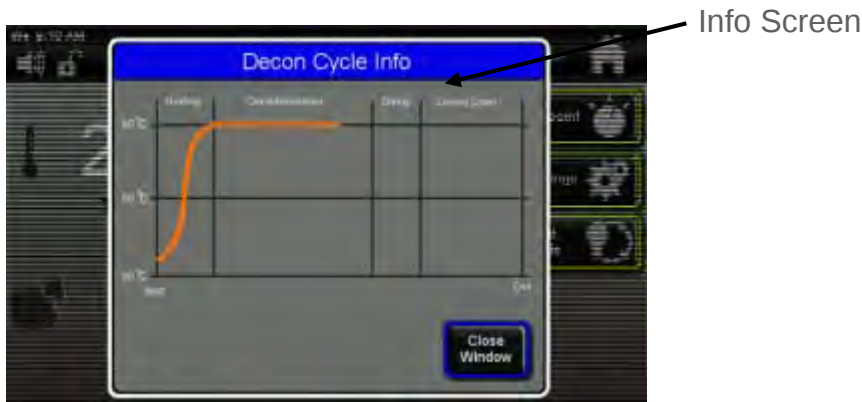


Press the (Close Window) button to return to the main screen.

SECTION 11 – ADVANCED FEATURES

Setting the time & day

The incubator has an internal real-time clock that keeps track of the day and time. It is set at the factory to Eastern Standard Time and may need adjusted for your time zone. To keep the clock accurate, it will need to be adjusted manually for daylight savings time changes. To set the day & time:

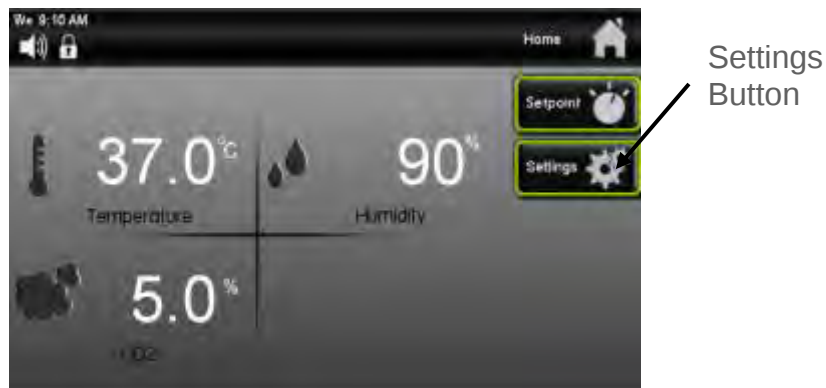

Press the (Settings) button.



Press the (Setup) button.

Day/Time Button



Press the  (Day / Time) button.

Hour Button

Minute Button

Day of the
Week Button



AM / PM
Button

Press the  (Hour) button.




The Enter New Time in Hours window will appear. Enter the hour by using the keypad and pressing  (Enter) when complete.

Follow same procedure for setting up minutes.

To setup AM/ PM, Press  (AM /PM) button and the words for AM and PM will toggle back and forth.


To set the Day of the Week, press the  (Day of the Week) button this button will scroll through the days of the week, press until the abbreviated letters correspond to the actual day of the week.


Press the  (Home) button to return to the main screen.

Locking the controls


To prevent un-authorized and accidental changes being made to the incubator, the touchscreen can be locked-out. The passcode is required to lock-out the controls and the same passcode is used to un-lock it. The factory default passcode is '1234'. This passcode can be changed by the user to create a unique 4-digit passcode. There is also a feature that will let you change the passcode from the factory default to a user defined passcode.

To lock the touchscreen,

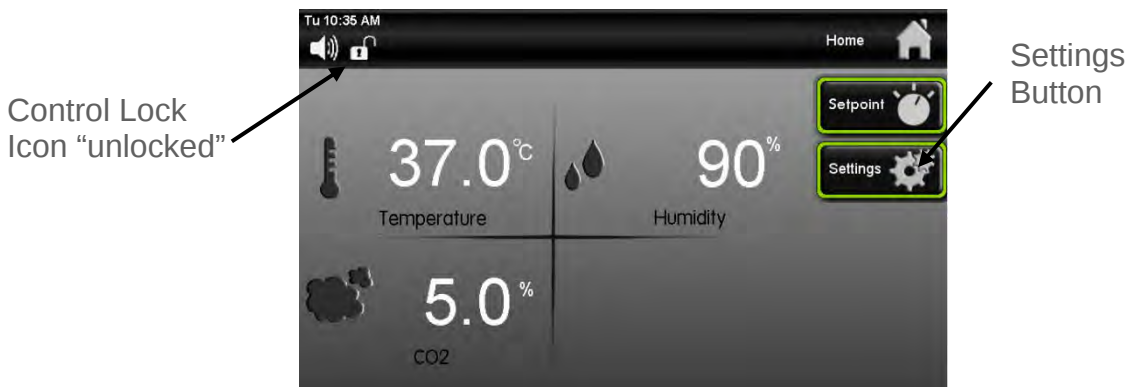

Press the  (Settings) button.




Press the  (Password) button.



Press the (Lock Keypad) button.




The Enter the Current Passcode Keypad screen will appear.




Enter digits "1 2 3 4"; press (Enter) when complete.

The screen will change back to the Home Screen and the Control Lock icon will change to the “locked” position.

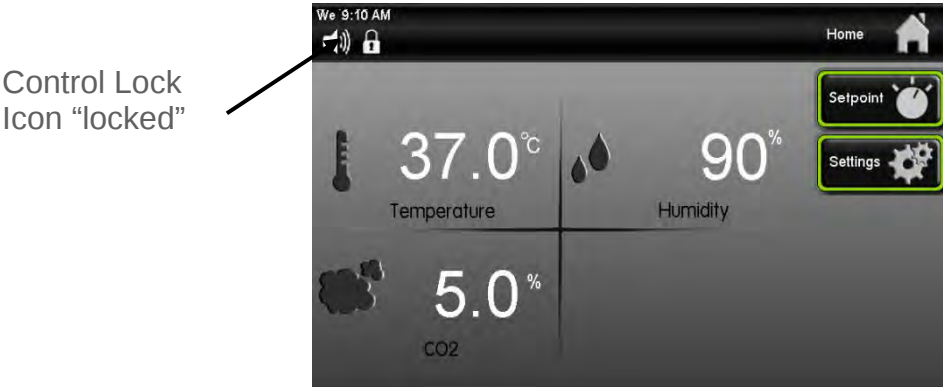

When any button is pressed on the home screen the following pop up window will appear. If the  button is pressed, the screen will change back to the Home Screen.

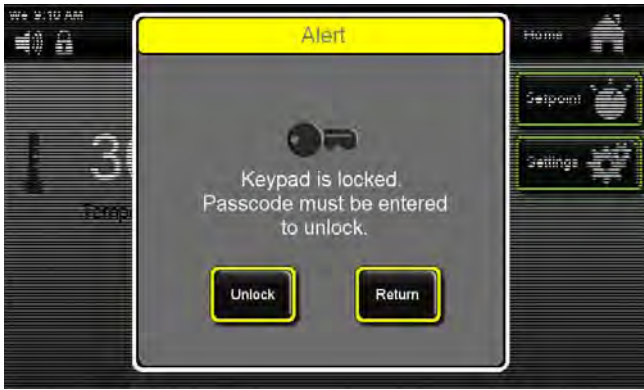

To un-lock the touchscreen,

From the previous Alert “Keypad is Locked” pop up screen, press the  (Unlock) button. The Enter New Passcode window will pop up.



Enter the digits “1 2 3 4”; press  (Enter) when complete. The Control Lock Icon will change back to the “unlocked” position.


Control Lock
Icon “unlocked”




Changing the passcode


To prevent un-authorized and accidental changes being made to the chamber, the touchscreen can be locked-out. The passcode is required to lock-out the controls and the same passcode is used to un-lock it. The factory default passcode is '1234'. This passcode can be changed by the user to create a unique 4-digit passcode. The current passcode is required to change the passcode.


To lock the touchscreen,

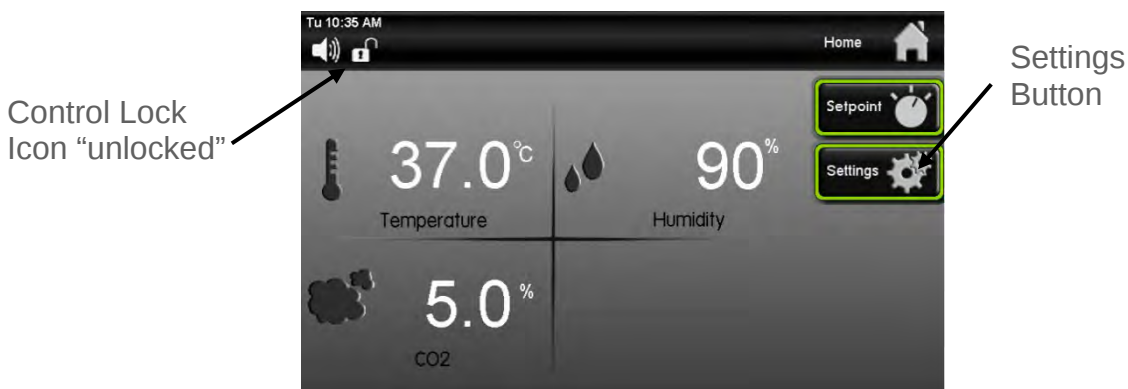

Press the  (Settings) button.



Press the  (Password) button.



Press the (Change Passcode) button.



The Enter *Current* Passcode Keypad screen will appear.



Enter digits “1 2 3 4”; press (Enter) when complete.



The Enter New Passcode Keypad screen will appear.

Enter any new four-digit passcode (example: “2 5 8 0”). Then press  (Enter) when complete.




The Lockout screen will tell you that the Passcode has been changed to a new value. *This is only time that the Passcode will be displayed on the Lockout screen.*


Factory menu & troubleshooting

The chamber control system is equipped with advanced diagnostics features which allow the user to manually turn 'on' & 'off' each electronically controlled system. The factory menu can be used to

- View the current chamber configuration
- See the percent output of the control system
- Manually and individually toggle any output



To access the Factory Menu,

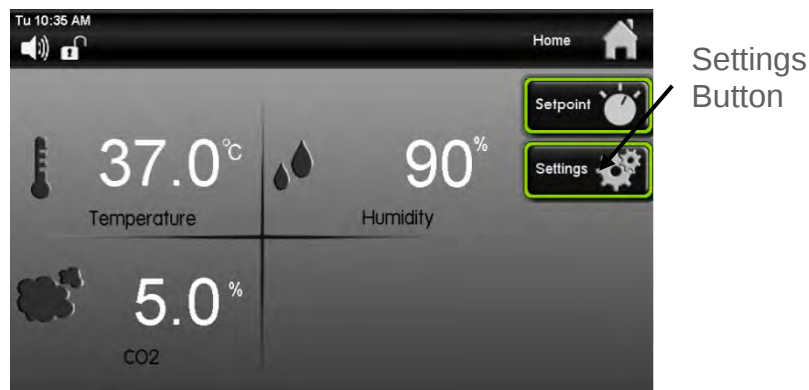



Press the  (Settings) button.



Press the  (Factory) button.

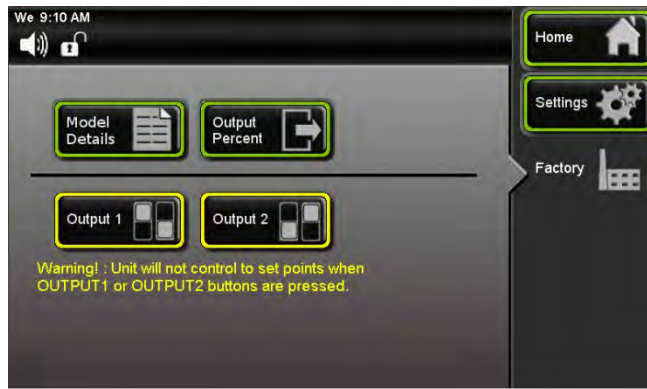


From the factory menu, four items can be selected. Press the (Configuration) button to view the chamber's configuration

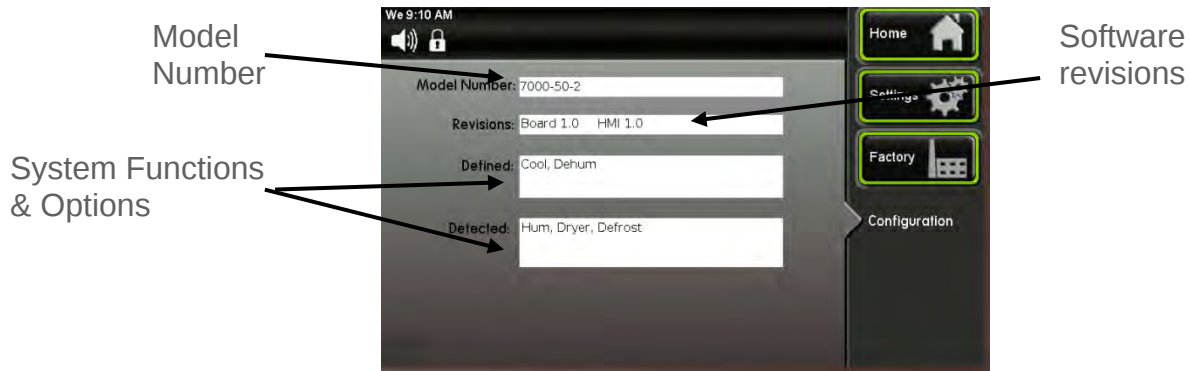

From the Factory screen, press the (Output Percent) button to view the current percent output level of each control parameter.



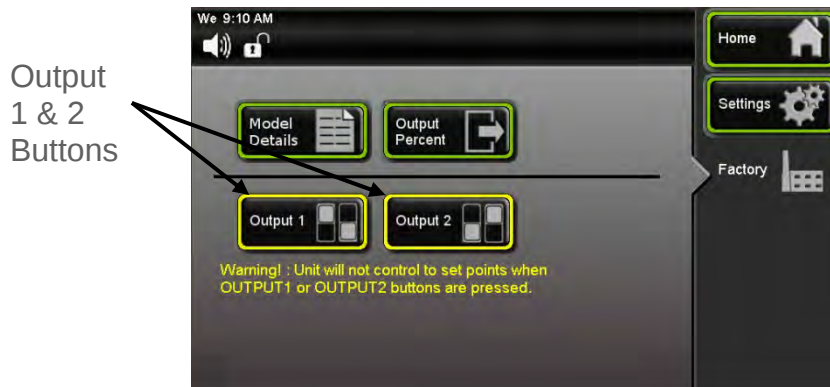

Navigating to the Output 1 or Output 2 screens in the factory page will temporarily halt chamber control & functionality.

To individually and manual control each output variable, from the factory screen press



the (Output 1) button. Note: Based on the chamber model number and options, not all functions will be present.




Each item can be turned on to check the condition of that device or parameter to aide in diagnosing a problem.



Press the (Output 2) button for other parameter buttons.



Chamber control & functionality is restored as soon as the screen is exited (Home, Settings, or Factory buttons) .When finished with diagnosis in Output 1 or Output 2



screen, press the (Factory) button to return to that screen. Once you go back to the Factory screen all parameters that were selected in Output 1 or Output 2 screens will reset to “off” position.



Press the (Home) button to return to the main screen.

SECTION 12 – PREVENTATIVE MAINTENANCE

Your CARON incubator has been robustly designed to minimize performance problems. However, regular maintenance is very important for continuous trouble free operation.

As a general rule, CARON recommends an annual calibration check of the temperature, humidity, CO2 systems. CARON offers a full range of on-site calibration and validation services. We also offer preventative maintenance contracts on our equipment. Contact our service department for details at 740-373-6809 or visit us on the web at www.caronproducts.com.

Recommended Daily Maintenance Checks

- Check the Temperature, humidity, and CO2 displays versus set-points.
- Check for and correct any alarm condition.

Recommended Monthly Maintenance Checks

- Check to ensure the drain in the bottom of the unit is draining properly.
- Check front air intake filter. If it is dirty replace it with CARON part number FLTR301. Washing the filter will result in poor performance.

Recommended Annual Maintenance Checks

- Disinfect all interior surfaces with a general purpose laboratory cleaning agent.
 - Perform a complete calibration of the temperature, humidity, and CO2 systems.
- A full validation is recommended for GMP facilities each time a unit is installed, moved or undergoes significant repair. Contact CARON's service department to schedule on-site validation.

SECTION 13 – SPECIFICATIONS

MODEL	7404-10
Temperature Range	Ambient +10°C to 60°C
Temperature Control	± 0.1°C
Temperature Uniformity	± 0.3°C
Temperature Sensor	3-wire RTD
Humidity Range	Ambient to 95% RH
Humidity Control	± 3% RH
Humidity Sensor	Capacitive
CO2 Range	0-20% CO2
CO2 Control	± 0.1% CO2
CO2 Sensor	Infrared
Interior Dimensions	23" W x 25.8" D x 29.8" H (58.4cm x 65.5cm x 75.7cm)
Interior Construction	Stainless Steel, Type 304, 2B Finish
Exterior Dimensions	44.2" W x 32.6" D x 36.5" H (112.3cm x 82.8cm x 92.7cm)
Exterior Construction	Cold Rolled Steel, Powder Coated
Work Space	10 Cu. Ft. (283 Liters)
# of Shelves	Three (3)
Shelf Construction	Perforated, Type 304, Stainless Steel, Electropolished
Shelf Dimensions	29.2" W x 26.4" D (74.2cm x 67.1cm)

	-1	-2	-3
Electrical	115V, 60 Hz, 12A	230V, 60 Hz, 8A	230V, 50 Hz, 6A
Shipping Weight	495 lbs. (225 kg)	495 lbs. (225 kg)	825 lbs.(374 kg)**

Specifications are subject to change without notice.

Environmental Conditions: Temperature 15°C to 25°C, Humidity non-condensing

*See graph for details

**Includes export shipping crate

This unit has forced internal air flow of 225 cfm (6,400 LPM)

SECTION 15 – TROUBLESHOOTING

Problem – Unit will not turn on

- Is the unit connected to a dedicated electrical circuit as defined in the installation section of the manual?
- Is there power at the electric outlet the unit is plugged into?
- Is the unit's power switch turned on?

Problem – Unit temperature is above / below temperature set-point

- Has the unit's temperature set-point been recently lowered / raised and if so has the unit been allowed 12 hours stabilize at the new set-point?
- Has the inner door been recently opened for an extended period of time?
- Is the access port stopper in the right side of the cabinet installed?
- Is the condenser filter on the front of the cabinet clean?

Unit humidity level is above / below humidity set-point

- Is the unit connected to a water source as specified in the installation section of the manual?
- Has the unit been leveled to insure the cabinet drain works correctly?
- The cabinet's drain line uses gravity to remove water. Does the drain line have any rises in it above the cabinet's drain level that could be trapping water?
- Has the unit's humidity set-point been recently lowered / raised and if so has the unit been allowed time to stabilize at the new set-point?
- Has the inner door been recently opened for an extended period of time?
- Is the access port stopper in the right side of the cabinet installed?
- Is the condenser filter on the front of the cabinet clean?

Unit CO2 level is above / below the CO2 set-point

- Is the unit connected to a pressure regulated CO2 source as specified in the installation section of the manual?
- Has the unit's CO2 set-point been recently lowered / raised and if so has the unit been allowed time to stabilize at the new set-point?
- Has the inner door been recently opened for an extended period of time?
- Is the access port stopper in the right and left side of the cabinet installed?

SECTION 16 – SPARE / REPLACEMENT PARTS

General

Part Number	Description
MTR-130	Blower Motor
BLW-113	Blower Wheel
CTR-140	Main Controller Board
CTR-141	CO2 Controller Board
CTR-142	Light Controller Board
CTR-144	7" Touchscreen, HMI
POW-108	24V DC Power Supply
FLTR303	Condenser Filter Replacement Kit
CRD-113	Power Line Cord
STP-101	2" Rubber Port Stopper

Temperature Related

Part Number	Description
HTR-150	Air Heater
RMT-114	107C Air Heater Thermostat
RMT-116	121C Air Heater Thermostat
RTD-101	Temp Sensor -- RTD 100 Ohm Platinum
REL-103	Heater Solid State Relay
CND-135	115V / 60Hz Condensing Unit
CND-137	230V / 60Hz Condensing Unit
CND-138	230V / 50Hz Condensing Unit
SOL-108	Refrigeration Cooling Solenoid

Humidity Related

Part Number	Description
HUM-110	RH Sensor
PMP-150	24VDC RH Pressure Pump
NOZ-101	Precision RH Spray Nozzle
SOL-135	Humidification Solenoid
REL-152	Humidification Solid State Relay
TUB-168	Drain Tubing, Blue, 3/8"
TUB-132	Water Supply Tubing, Black, 1/4"

SECTION 16 – SPARE REPLACEMENT PARTS (CONTINUED)

CO2 Related

Part Number	Description
CO2-101	Carbon Dioxide Sensor
SOL-135	CO ₂ Injection Solenoid
FIL-213	In-line CO ₂ HEPA Filter
FIL-115	HEPA Filter

Fuse Related

ID	Description	115V	230V
SW1	Main circuit breaker switch	CBR-116 (12A)	CBR-115 (10A)
FUS1	Heater fuse	FUS-103 (10A)	FUS-104 (5A)
FUS3*	Internal outlet fuse (single duplex)	FUS-151 (2A)	FUS-151 (2A)
FUS3*	Internal outlet fuse (double duplex)	-	FUS-163 (4A)
FUS5	Internal outlet transformer fuse	-	FUS-164 (3A)

* Fuse size varies depending upon whether the chamber has a single internal duplex outlet or two internal duplex outlets

Options Related

Part Number	Description	Option
CLM-132	Nylon tube clamp	GASG301, REGL101
FIT-348	1/4" barb-1/4" push-in adapter	GASG301, REGL101
MEM-103	USB Flash Drive	DLOG301
PEN-103	Red pen for 6 inch recorder	RCDR316, RCDR317
PEN-104	Blue pen for 6 inch recorder	RCDR317
PPR-104	6 inch recorder paper, 7 day 0-60C	RCDR316
PPR-105	6 inch recorder paper, 7 day 0-100C	RCDR317
PPR-106	10 inch recorder thermal paper	RCDR318, RCDR319
TUB-174	1/2" I.D. silicone tubing	PUMP301
TUB-145	1/4" I.D. vinyl tubing	GASG302, REGL101
TUB-174	1/2" I.D. silicone tubing	PUMP301
WIR-102	20/3 conductor shielded wire	ALRM302



DECLARATION OF CONFORMITY

Caron Products and Services, Inc.
27640 State Route 7
Marietta, OH 45750 USA



Declares that the product:

Designation:	7404
Model Numbers:	7404-10-3
Classification:	Electrical equipment intended for residential, commercial and lighting industrial environments
Rated Voltage:	220-240 ~ (ac)
Rated Frequency:	50Hz

Meets the essential requirements of the following European Union Directive(s) using the relevant section(s) of the normalized standards and related documents shown:

EMC

EN 61326 (CISPR 11: 2004 Class B) Laboratory Equipment, Immunity Measurement & Control requirements

Performed according to

EMC Directive 2004/108/EC

IEC/CISPR 11: 1997, +A1: 1999, +A2: 2002

EN 55011: 1998, +A1: 1999, +A2: 2002

FCC CFR47 Part 18

Safety

EN 61010-1 Safety requirements for electrical equipment for measurement, control, and laboratory use part 1: General Requirements

By: Dave Figel
Engineering/Production Manager
CARON Products & Services, Inc.