


Raz Rehab Shower Commode Chairs AP600 / SP600 Heavy Duty Models

User's Manual

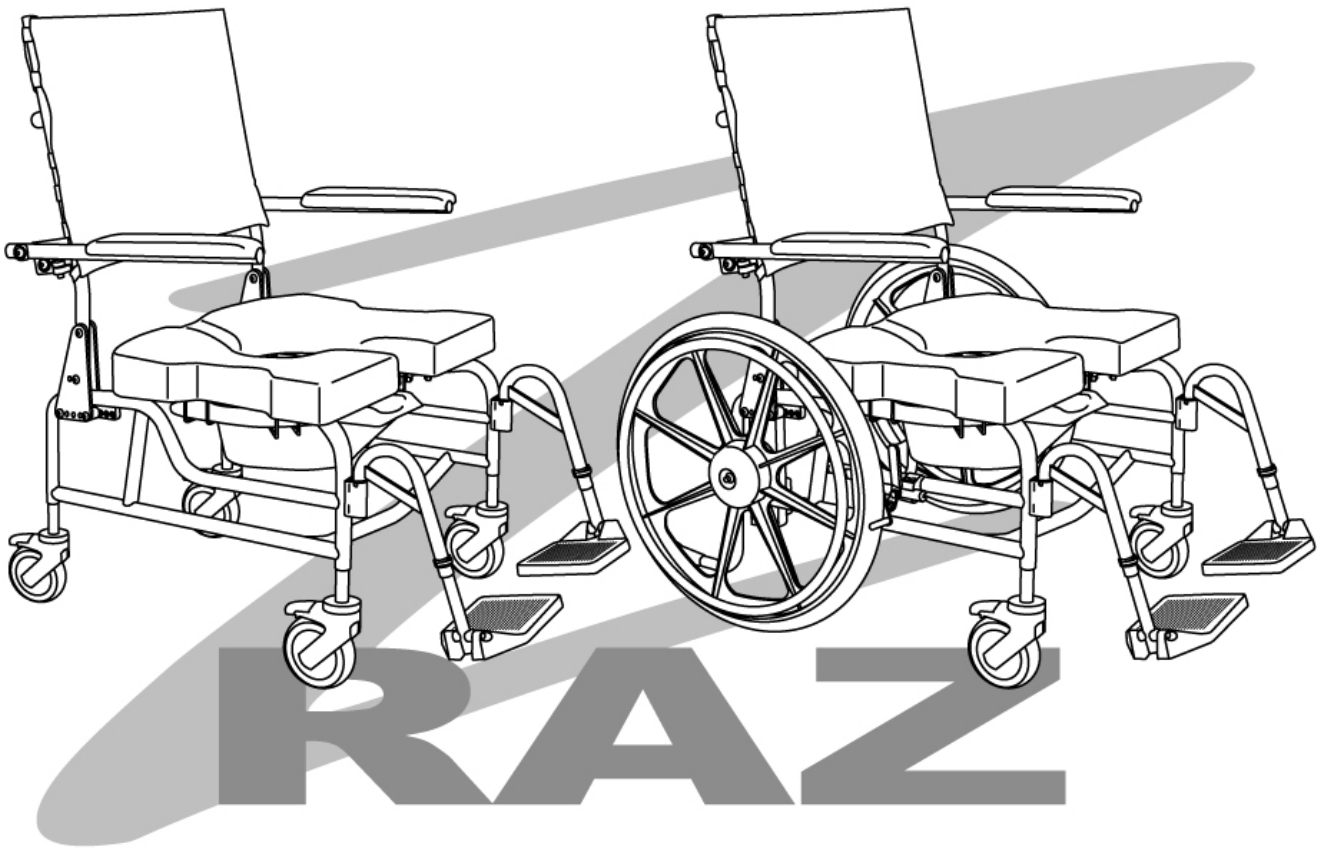

**A guide to help users and caregivers in the safe usage and
maintenance of Raz Rehab Shower Chairs**

SAFETY PRECAUTIONS

Failure to comply may cause injury or damage!

It is important that the user(s), and/or the caregivers of the user(s) read and thoroughly understand the User's Manual. If there are any parts of the User's Manual that are not understood, clarification should be sought prior to using the product.

CHAIR CLASSIFICATION BASED ON MAXIMUM USER WEIGHT	
AP600 / SP600	600 lbs (272 kg)

SAFETY WARNINGS TO CONSIDER FOR USE PURPOSES

Forward Stability

The casters on all models are equipped with dual-locks. The step-on lever activates both the roll lock and the swivel lock. ***It is essential that all casters on the shower chair be in the outward position before engaging the locks for optimal forward and lateral stability.*** If so equipped, disengage the optional Directional Caster Lock first before rotating the rear caster to the rearward position and applying the caster's dual-locks.

USERS MUST NOT lean forward while sitting in the Raz Shower Chair as this may cause the chair to tip forward.

USERS MUST NOT wheel down a ramp (SP600 Model) without an attendant who can hold onto the chair during the descent.

WHEEL LOCKS ARE NOT BRAKES! Never use wheel locks to slow down the shower chair when descending inclines as this could cause the chair to tip in the direction of travel.



Lateral Stability

USERS MUST NOT lean over the edge of a Raz Shower Chair.

USERS MUST NOT attempt to pick up objects from the floor by leaning over and reaching – a reacher or assistance from others should be employed.

USERS MUST NOT position the shower chair on a side slope as this could cause the chair to tip.




Rearward Stability

USERS MUST NOT wheel up an incline on a Raz SP600 without ensuring that the optional rear anti-tippers are in place. The optional anti-tippers must be ordered with the Raz SP600 and properly installed before wheeling on uneven surfaces.

Anti-Tippers (SP600 Model Only)

Anti-tippers are an option for the Raz SP600 Shower Chairs. These are recommended whenever the chairs are to be used on uneven surfaces such as ramps or sloped floors. If the stability of the Raz SP600 is ever in question, anti-tippers should be installed by the dealer that supplied the chair.



IMPORTANT !

THE REARWARD STABILITY OF THE RAZ SP600 IS AFFECTED BY THE MOUNTING LOCATION OF THE REAR WHEELS, THE PHYSICAL AND CLINICAL CHARACTERISTICS OF THE USER AND THE ANGLE OF THE BACKREST. THE NEED FOR ANTI-TIPPERS SHOULD HAVE BEEN DETERMINED AT THE TIME OF THE PRESCRIPTION OF THE RAZ SP600 WITH CONSIDERATION FOR THE USER'S PHYSICAL ATTRIBUTES AND ENVIRONMENT.

Ramps and Other Inclines

Ramps and other surfaces that are not level (such as slopes into wheel-in showers) must be tested with an attendant to ensure that they do not compromise the chair's stability. A qualified healthcare professional should be consulted to assist with this process.

DO NOT push or pull the Raz AP600 up or down an incline or ramp that exceeds a 1:12 grade (5° slope). If unsure of the ramp grade, contact your authorized Raz dealer for assistance.

DO NOT allow any user to be propelled (pushed or pulled) in a Raz AP600 Shower Chair in any other manner than by an attendant.



Immersion

The Raz Shower Chair is not designed to be used as a pool chair. Do not immerse the shower chair in whole or in part, in water or any other liquid, otherwise damage to the shower chair components may result.



Transfers

The most dangerous part of using any shower chair is the transfer. Since every chair has different stability characteristics, it is essential to carefully review and test the transfer technique to ensure that the procedure is safe. Consult a healthcare professional if safe, reliable transfer techniques have not been learned. Individuals who have not learned this skill must seek assistance during transfers and may require the use of a mechanical lift.

Transferring onto a Raz AP600 Shower Chair – **ALWAYS** lock all four casters in their outward position (front casters positioned in the forward position/rear casters positioned to the rear) for maximum chair stability.

Transferring onto a Raz SP600 Shower Chair – **ALWAYS** lock both front casters in their outward position (positioned forward) and fully apply both rear wheel locks so that they securely engage the rear wheels.



The wheel locks are designed to prevent the self-propelling wheels from rotating. The dual-locks on the casters are designed to prevent the casters from rotating and the caster forks from swivelling. Caster locks **DO NOT and CANNOT** prevent the casters from sliding and the shower chair from moving if the floor is slippery. A slippery floor can be caused by dust, water, soap or any substance that does not allow the casters to grip the floor securely. **Transfers should never be attempted with the shower chair positioned on slippery surfaces.** It is recommended that transfers be performed on clean, dry non-slippery surfaces; a fully-carpeted surface is optimal. Be aware that area rugs and shower mats can slide on floors and thereby present a hazardous surface.

NEVER use the footplates to assist in transfers. This could cause the chair to tip. The footrests should be swung to the side or removed entirely during transfers to provide unobstructed access to the shower chair.

DO NOT stand on any part of the frame of the Raz Shower Chair.

The Raz Shower Chair **is NOT** intended for use as a transportation device or a long-term seating system.

USERS SHOULD NEVER be left unattended in a Raz Shower Chair.

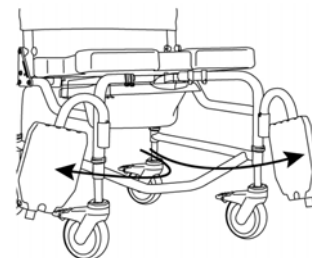

IMPORTANT !

IF IT IS EVER FELT THAT ANY ASPECT OF THE RAZ SHOWER CHAIR IS IN NEED OF MAINTENANCE, CONTACT YOUR DEALER. ANY PROBLEMS THAT COULD AFFECT THE SAFE USAGE OF THE CHAIR MUST BE ATTENDED TO IMMEDIATELY. THE DEALER THAT PROVIDED THE SHOWER CHAIR MUST BE CONTACTED SO THAT REPAIRS CAN BE MADE PRIOR TO USING THE CHAIR. IT MUST BE MADE CLEAR TO THE DEALER THAT THE SHOWER CHAIR IS IN NEED OF MAINTENANCE AND IS UNAVAILABLE FOR USE UNTIL REPAIRS HAVE BEEN UNDERTAKEN AND ALL PROBLEMS RESOLVED.

USER'S MANUAL TABLE OF CONTENTS

Page

1.0 GENERAL INFORMATION

1.1	Raz Rehab Shower Chair Models AP600 and SP600 Overview	6
1.2	Raz Rehab Shower Chair Models AP600 and SP600 Specifications	6

2.0 USE AND OPERATION

2.1	Multi-Position Backrest	7
2.2	Adjustable Tension Back Upholstery	7
2.3	Molded Seat	8
2.4	Casters	9
2.5	Directional Caster Lock	9
2.6	Self Propel Wheels - SP600 Model Only	10
2.7	Anti-Tippers - SP600 Model Only	10
2.8	Adjustable Footrests	10
2.9	Lateral Supports	11
2.10	Leg Adductors	11
2.11	Armrests	12
2.12	Chest Positioning Strap	12
2.13	Pelvic Positioning Strap	13
2.14	H-Strap	13
2.15	Heel Loops	13
2.16	Commode Pan	13
2.17	Fasteners	14


3.0 CLEANING AND MAINTENANCE

3.1	Cleaning After Each Use	15
	Commode Pan	15
	Molded Seat	15
3.2	Cleaning As Needed	15
	Adjustable Tension Back Upholstery	15
	Frame, Armrests, Adjustable Footrests, and Other Components	15
3.3	Suggested Cleaning Products	16

4.0	LIMITED WARRANTY	17
-----	------------------------	----

1.0 GENERAL INFORMATION

1.1 Raz Rehab Shower Chair Models AP600 and SP600 Overview

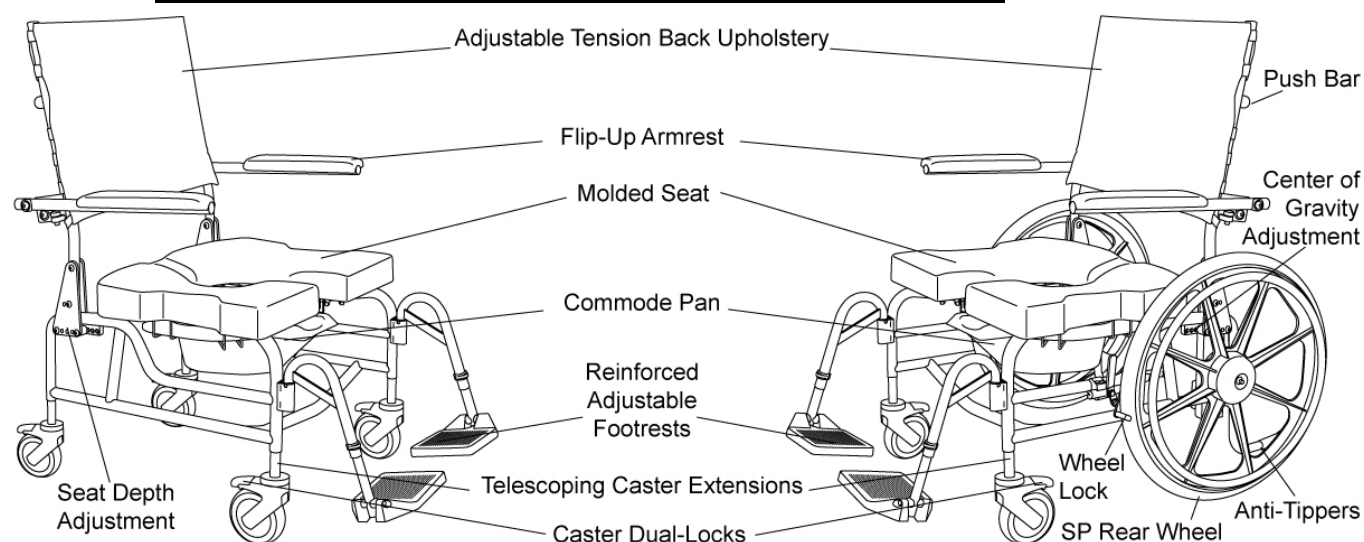

1.2 Raz Rehab Shower Chair Models AP600 and SP600 Specifications

SPECIFICATION	RAZ-AP600	RAZ-SP600
WEIGHT CAPACITY	600 lbs.	600 lbs.
FRAME WIDTH	22"	22"
SEAT WIDTH	23"	23"
SEAT DEPTH ADJUSTMENT	18" – 20"	18" – 20"
CENTER OF GRAVITY ADJUSTMENT	Back Position: Up to 1" fore/aft	Wheel Axle: Up to 1½" fore/aft Back Position: Up to 1" fore/aft
SEAT HEIGHT (seat to floor)		
Standard 5" Caster:	19¼", 20¼", 21¼", 22¼", 23¼"	20¼", 21¼", 23¼"
Optional 6" Caster:	20¼", 21¼", 22¼", 23¼", 24¼"	20¼", 21¼", 23¼"
CLEARANCE HEIGHT		
5" Caster (under pan):	10¼", 11¼", 12¼", 13¼", 14¼"	11¼", 12¼", 14¼"
5" Caster (under frame):	15½", 16½", 17½", 18½", 19½"	16½", 17½", 19½"
6" Caster (under pan):	11¼", 12¼", 13¼", 14¼", 15¼"	11¼", 12¼", 14¼"
6" Caster (under frame):	16½", 17½", 18½", 19½", 20½"	16½", 17½", 19½"
BACK HEIGHT	20"	20"
BACK ANGLE	95°, 100°	95°, 100°
ARMREST HEIGHT	8"	8"
WIDTH BETWEEN ARMPADS	22½"	22½"
LATERAL SUPPORT (adjustment range)	1¼" - 2½" offset 1" fore/aft ±5° pad angle	1¼" - 2½" offset 1" fore/aft ±5° pad angle
FOOTREST ADJUSTMENT (seat to footplate)	16"-20½" (Z709) 18"-22½" (Z711)	16"-20½" (Z709) 18"-22½" (Z711)
STANDARD CASTER:	Dual-locking 5" casters (x4)	Dual-locking 5" casters (x2)
OPTIONAL CASTER:	Dual-locking 6" casters (x4)	Dual-locking 6" casters (x2)
REAR WHEELS (with molded handrims)	Optional Retrofit Kit (Z618)	24" Wheels
OVERALL WIDTH	26" (w/ standard armpad) 29½" (w/ Z715 armpad)	30" (outside handrim)
OVERALL LENGTH (with footrests)	39" - 40½"	44" - 45¼"
OVERALL LENGTH (without footrests)	29½"	32" - 34½"
PRODUCT WEIGHT	54 lbs. (w/ 5" casters) 56 lbs. (w/ 6" casters)	68 lbs. (w/ 5" casters) 69 lbs. (w/ 6" casters)
FRAME AND HARDWARE MATERIAL	Stainless Steel	Stainless Steel


2.0 USE AND OPERATION

IMPORTANT !

ADJUSTMENTS SHOULD NEVER BE ATTEMPTED WITH THE USER IN THE CHAIR.

2.1 Multi-Position Backrest

The Raz AP600 and SP600 Shower Chairs come with a 20" Multi-Position Backrest. It can be moved fore/aft within a 1" range to improve center of gravity and weight distribution, and the backrest angles can be set at 95°, or 100°. The armrests on this back type flip-up for transfers and are adjustable in angle, but are fixed at a height of 8".

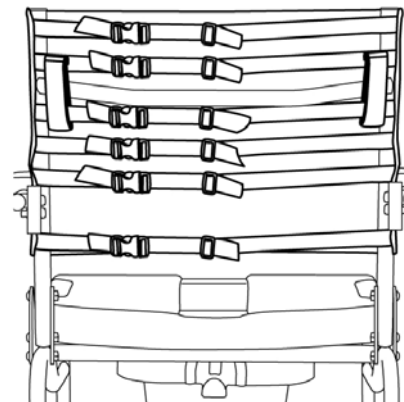


2.2 Adjustable Tension Back Upholstery

The Raz AP600 and SP600 Shower Chairs come with a 20" Adjustable Tension Back Upholstery which provides trunk support for optimal positioning and comfort. The Adjustable Tension Back Upholstery is available in a polyester fabric for comfort, and a vinyl material ideal for clinical facilities. In both cases the upholstery has double stitched straps for heavy-duty use and is removable for machine washing.

To install the Adjustable Tension Back Upholstery:

1. Remove the grey fabric upholstery from the accessory box.
2. Place the fabric against the front of the backrest canes making sure that when wrapped around, the clips on the straps face away from the fabric, and the loops point downwards.
3. Clip up the lowest strap below the armrest weldment.
4. The second and third lowest straps can be clipped up above the armrest weldment.
5. The fourth strap from the bottom of the backrest must be fed through the loop on the strap above it, and can then be clipped up below the push bar.
6. The last two straps can be clipped up above the push bar.
7. Adjust all of the straps to meet the user's needs.

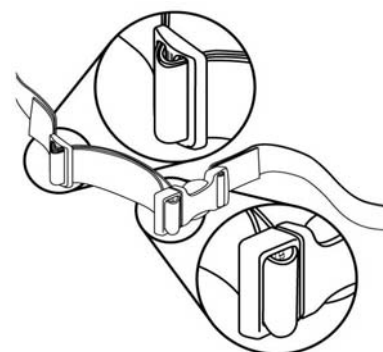

To adjust the Adjustable Tension Back Upholstery, each strap can be tightened or loosened at the buckles to achieve a wide range of positions. For example, the second and third straps from the bottom can be tightened further to create more pronounced support in the lumbar area of the back. The looser the straps of the back upholstery, the more the fabric will sling into the chair.


To remove the Adjustable Tension Back Upholstery, release the buckles on the straps.

NOTE: The bottom strap should be fastened below the armrest weldment on the back frame. In order to remove this strap, it may help to raise the armrests.

2.3 **Molded Seat**

The unique seat on all Raz Shower Chairs was designed to help stabilize the pelvis and was contoured for pressure reduction. The seat is made from a soft, integral-skin foam and measures 23" wide by 18" deep. The seat is an element of the unique Ischial Pelvic Alignment System (IPAS), it provides 1½" of fore and aft adjustment so that the seat can be aligned with the pelvis. The Molded Seat readily locks in place for transfers but also removes easily for cleaning. The seat-to-floor height achievable on the Raz AP600 and SP600 Shower Chairs is between 19¼" and 24¼" and the chair fits over most standard toilet bowls when the commode pan is not in place.




NOTE: 23" x 18" seat comes standard with the Raz Rehab Shower Chair AP600 and SP600 models.

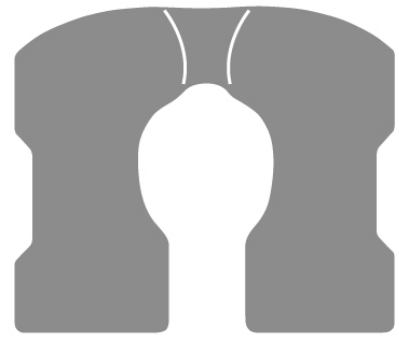

23" WIDE SEAT

To install the seat:

1. Open the spring clips by squeezing each inward to unlatch the free end from the seat bracket.
2. Slide the rear of the seat over the rear crosstube as the front of the seat is lowered onto the frame. Check to make sure that the rear seat brackets hook below the crosstube.
3. Lower the front of the seat until the front seat brackets nestle onto the front seat support tubes.
4. To secure the seat in place, squeeze each clip inward while moving the free end towards the seat until the spring clips click into the seat bracket under the front support tubes.

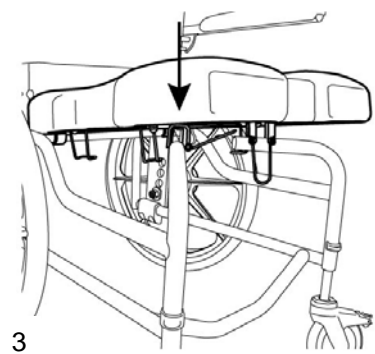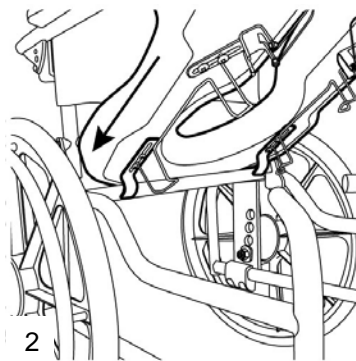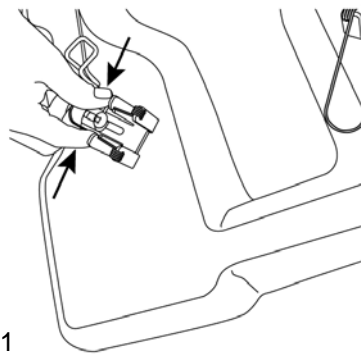

To remove the seat:


1. Unlatch the spring clips from the front seat brackets.
2. Lift the front of the seat directly up.
3. Pull the seat towards the front of the chair to unhook the rear brackets.

IMPORTANT !

NEVER ATTEMPT TO CHANGE THE SEAT HEIGHT WITHOUT THE HELP OF A QUALIFIED DEALER. ADJUSTED SEAT POSITIONS WILL REDUCE THE CHAIR'S STABILITY AND MAY RESULT IN TIPPING AND INJURY.

2.4 Casters

Raz AP600 Shower Chairs are built for each order with four 5" casters (standard), however four 6" heavy-duty casters may be ordered as an option. Raz SP600 Shower Chairs come equipped with two 5" casters and 24" wheels (two 6" heavy-duty casters may be ordered as an option on the SP600). Each caster is equipped with a dual-lock feature, which stops the caster from swivelling and rolling simultaneously.

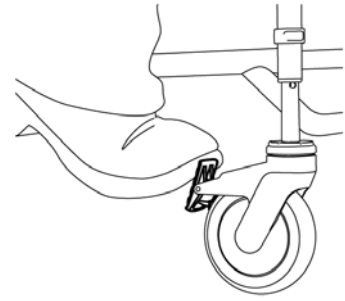

To engage the dual-lock, step on the end of the caster lock lever until it latches in the on position.


To disengage the dual-lock, step on the raised end of the caster lock lever until it latches in the off position.

IMPORTANT !

FRAME AND SEAT ADJUSTMENTS SHOULD BE PERFORMED ONLY BY TECHNICIANS FROM QUALIFIED RAZ DEALERS. NEVER ATTEMPT TO CHANGE THE FRAME ANGLE BY CHANGING THE CASTER POSITION. THE FRAME SHOULD ALWAYS BE LEVEL. IMPROPER CASTER POSITIONS MAY REDUCE THE CHAIR'S STABILITY AND RESULT IN TIPPING. THIS HAS THE POTENTIAL TO CAUSE SERIOUS HARM TO THE USER AND/OR DAMAGE TO THE CHAIR.

2.5 Directional Caster Lock

A Directional Caster Lock can be added to one caster on the Raz AP600 and SP600 Shower Chairs to facilitate linear movement of the commode and manipulation in confined environments. The flip-down directional lock keeps one rear caster aligned in a forward direction. This feature is available for both 5" and 6" casters and facilitates the pushing of the chair by reducing unwanted sideways movement. Close-quarters manoeuvrability may be easier with the Directional Caster Lock in the off (*upwards*) position.

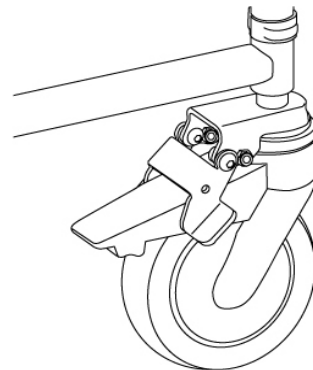

To engage the Directional Caster Lock:

1. Ensure that the dual-locks are not activated and that each caster can swivel and roll freely.
2. Pull the shower chair rearward until the rear casters swivel to their forward positions, directly under the frame tube.
3. Flip the directional lock guide latch down to its on position so that it cradles and holds the caster in the forward position.

NOTE: If the caster is not perfectly in-line with the frame, the spring-loaded latch, once activated, will engage if the rear caster is slowly swung around.


To disengage the Directional Caster Lock, flip the spring-loaded latch up, to its off position.

IMPORTANT !

ALWAYS RELEASE THE DIRECTIONAL LOCK AND SWIVEL ALL FOUR CASTERS TO THEIR OUTWARD POSITION (LOCKING THEM) FOR MAXIMUM STABILITY BEFORE EVER TRANSFERRING A USER.

2.6 Self Propel Wheels – SP600 Model Only

The wheels included with every Raz SP600 Model are 24" in size. These wheels have improved non-slip molded handrims which outperform vinyl handrims for utility and durability. All Raz SP600 Chairs come standard with fixed, self-propel wheels. An AP600 chair with a Multi-Position Back can also be ordered with a SP600 Conversion Kit to facilitate the conversion between attendant and self propulsion. The seat to floor height range of a Raz SP600 Model is between 20¼" and 23¼" with the rear wheels installed. The self propel wheels also have a fore and aft adjustment range of 1½".

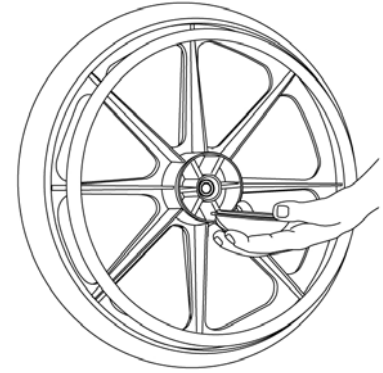

2.7 Anti-Tippers – SP600 Model Only

Anti-Tippers are an option for all Raz SP600 Shower Chairs, these are recommended whenever the shower chairs are to be used on uneven surfaces such as shower ramps or sloped floors, or for lower-extremity amputees. A dealer can adjust the Anti-Tippers up or down and further outward from the chair in order to increase rearward stability as required by the user.

IMPORTANT !

THE ADJUSTMENT OF ANTI-TIPPERS ON A RAZ SP600 MODEL COULD RESULT IN SERIOUS INJURY. IT IS STRONGLY RECOMMENDED THAT ONLY A QUALIFIED RAZ DEALER MAKE ADJUSTMENTS TO THE POSTIONS OF ANTI-TIPPERS. A STABILITY CHECK MUST ALSO BE PERFORMED IN ORDER TO ENSURE SAFETY FOR THE USER IN HIS/HER ENVIRONMENT.

2.8 Adjustable Footrests


Reinforced Adjustable Footrests are available as an option on AP600 and SP600 Raz Shower Chairs. Adjustable Footrests are recommended for users who need an extra level of comfort, positioning, or pressure relief in the thighs. For transfers, the footrests can be flipped up, rotated away, or removed entirely. Adjustable Footrests can be extended for users with long legs with a 2" longer tube that can be ordered for any Raz Shower Chair.

To insert the Adjustable Footrests:

1. Place the footrest hanger tubes into the receiving sleeves at.
2. If the support tubes are aligned forward, the pins on the tubes will engage with grooves in the sleeves and lock in place.

To adjust the length of the Adjustable Footrests:

1. Remove the snap-pin from one footrest hanger tube.
2. Reposition the footplate to a length suitable for the user.
3. Insert the snap-pin through the footrest hanger tube and through the inner tube. *Ensure that the snap-pin is completely through the tube and that the grey plastic clip is snapped securely around the outside of the hanger tube.*

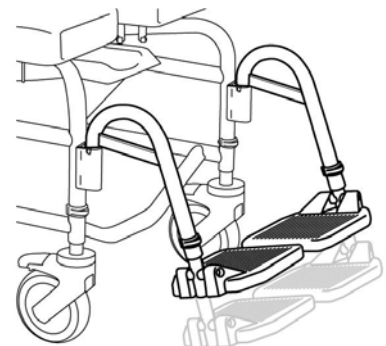


To rotate the Adjustable Footrests:

1. Lift the footrest hanger tube up to disengage the pins.
2. Rotate the footrests outward or inward.

To remove the Adjustable Footrests, lift the footrests out of the receiving sleeves on the frame.

2.9 Lateral Supports

Raz Shower Chairs may be fitted with optional lateral supports. Lateral Supports are designed to assist a user in maintaining an upright posture in the Raz Shower Chair. One or two Lateral Supports may be mounted on any Raz Model. The molded foam pads have a soft foam exterior, contoured to hug the torso, and have a solid insert to provide strength for positioning. An extension plate can be ordered as an option to attain additional extension of the Lateral Support Pad. The Lateral Pads can be adjusted medially up to 1" on both sides of the chair for individuals requiring more support (up to 4" with an optional extension plate). The laterals can also be adjusted towards or away from the chair's backrest within a range of 1". The Lateral Support Pads can also be angled to meet the user's needs. Both Lateral Support Pads lock in front of, and behind, the backrest.

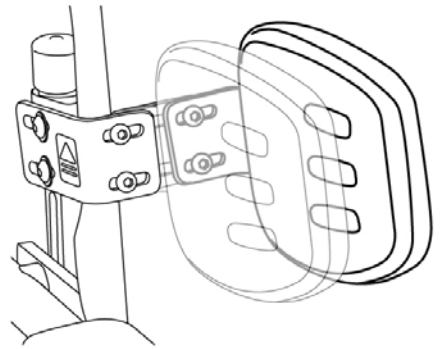


To release a Lateral Support Pad from the forward position:

1. Grasp one pad bracket at the blue arrow decal and lift up.
2. Once raised, rotate the lateral pad to a position behind the back and press down above the decal to lock the pad in place.
3. Repeat for the other lateral support if desired.
4. Ensure that the laterals are locked in place before use.

To release a Lateral Support Pad from the rearward position:

1. Grasp the pad bracket near the mounting post and lift up.
2. Once raised, rotate the lateral pad around to the front and press down above the decal to lock the pad in place.
3. Repeat for the other lateral support if desired.
4. Check to ensure that the laterals are locked in place before use.

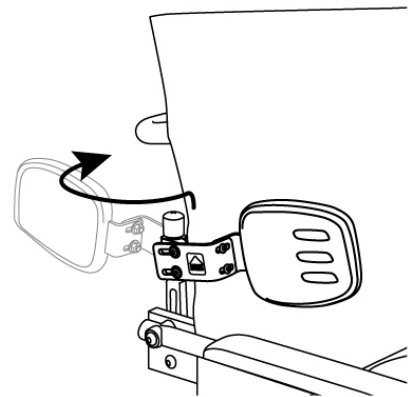

IMPORTANT !


ALL ADJUSTMENTS TO LATERAL SUPPORT PADS (UP/DOWN, MEDIAL/LATERAL, AND ANGLE) MUST BE PERFORMED BY A QUALIFIED TECHNICIAN. ALL ADJUSTMENTS PERFORMED MUST NOT IMPEDE THE OPERATION OF OTHER COMPONENTS.

2.10 Leg Adductors

Leg Adductors are available as an option on AP600 and SP600 Raz Shower Chairs. Leg Adductors are recommended for users who need assistance with leg positioning. For transfers, the adductor pads can be removed entirely. Leg Adductors have a comfortable 6"x5" molded foam pad and are multi-axis adjustable to meet users' unique needs.

To insert the Leg Adductors:

1. Loosen the tri-lobe knob on the adductor clamp mounted on the side of the chair frame.
2. Insert the leg adductor mounting post into the clamp.
3. Move the adductor pad to the desired height for the user.
4. Tighten the tri-lobe knob
5. Repeat steps 1 to 4 for the other Leg Adductor if necessary.

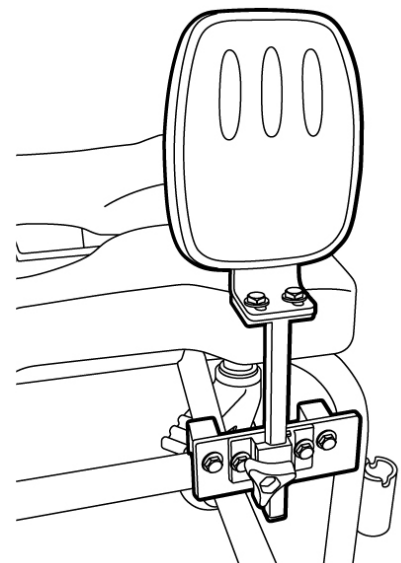

To adjust the Leg Adductors:

1. Loosen the tri-lobe knob on the Leg Adductor clamp mounted on the side of the chair frame.
2. Reposition the adductor pad to a height suitable for the user.
3. Tighten the tri-lobe knob
4. Repeat steps 1 to 3 for the other Leg Adductor if necessary.

To remove the Leg Adductors, loosen the tri-lobe knob and lift the adductor out of the adductor clamp on the frame.

2.11 Armrests

The Raz Shower Chair comes standard with flip-up padded armrests. Also available are 3¼" Molded Flat Armpads as an alternative to the standard 2¼" wide armpads. The armrests on Multi-Position Backs are fixed at one height (8") but are adjustable in angle (up to 10°).

IMPORTANT !

ARMRESTS ON RAZ AP600 AND SP600 MODELS ARE NOT INTENDED TO SUPPORT THE ENTIRE BODY WEIGHT OF AN INDIVIDUAL. TOO MUCH WEIGHT MAY CAUSE DAMAGE TO THE ARMRESTS OR MAY CAUSE THE CHAIR TO TIP.

2.12 Chest Positioning Strap


An optional one-piece Chest Positioning Strap can be attached to any Raz Model. The 2" wide heavy-duty webbing can be used to support a user in a forward leaning position for hygiene access to the user's back. The back upholstery includes loops that are intended as strap guides.

To install the Chest Positioning Strap:

1. Insert one side of the strap through both back upholstery loops.
2. With the user seated in the chair, thread one end of the strap through the plastic loop on the other end of the chest strap.
3. Secure the strap in front of the user with the Velcro closure.

To adjust the Chest Positioning Strap:

1. Open the Velcro on the strap.
2. Tighten or loosen the strap around the user as needed.
3. Fasten the chest strap to secure the user.

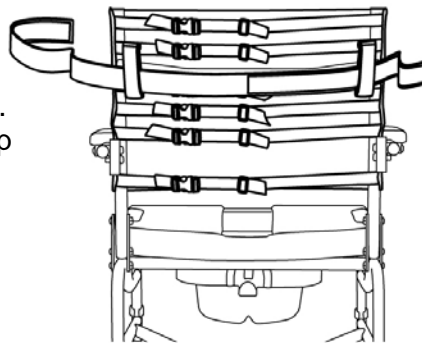

IMPORTANT !

ANY ADJUSTMENTS TO THE CHAIR'S STRAPS SHOULD BE PERFORMED WITH EXTREME CAUTION AS THE USER'S SAFETY MAY BE DEPENDENT ON SECURE POSITIONING STRAPS.

2.13 Pelvic Positioning Strap

An optional two-piece Pelvic Positioning Strap can be ordered with the shower chair and can be attached to any Raz Model. The pelvic strap uses 2" wide heavy-duty webbing and a buckle for one-handed operation.

To install the Pelvic Positioning Strap:

1. Weave one strap end through a DD-ring and slide the ring several inches from the end.
2. Feed the strap through the slot in the triangular strap plate – **from the inside to the outside** and then weave the loose end back through the DD-ring.
3. Repeat steps 1 and 2 for the other side of the strap.
4. Adjust the DD-rings and tighten the pelvic strap as necessary.



To adjust the Pelvic Positioning Strap:


1. Loosen both straps through the "double D" ring on one side of the pelvic strap.
2. Adjust by pulling/pushing the strap end in/out of the DD-ring.
3. Repeat step 2 for the other side of the strap.
4. Pull tightly on each strap to ensure that it is secured properly.

2.14 H-Strap

An optional one-piece H-Strap can be attached to the footrests on any Raz Model. The H-Strap is recommended for individuals who require additional support for the legs and feet.


To install the H-Strap:

1. With the Velcro facing towards the chair, center the strap horizontally between both footrest hanger tubes and wrap the loop side around the tubes until it engages with the hook side.

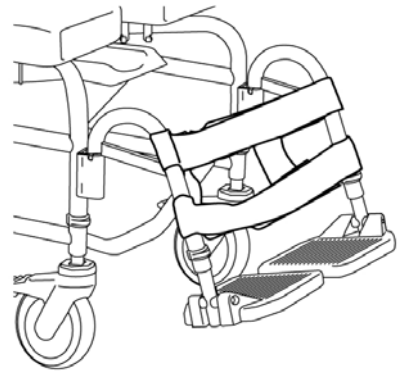

To adjust the H-Strap:

1. Disconnect the Velcro from the back of the H-strap and adjust to sling or tighten the H-Strap to suit the user's needs.
2. Press firmly on the Velcro to secure the H-Strap prior to use.

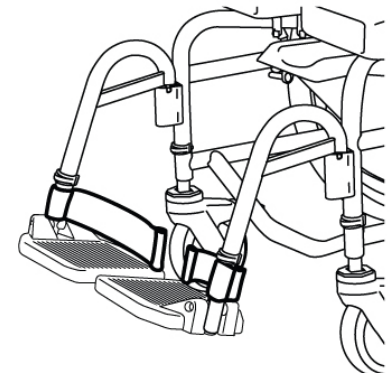


2.15 Heel Loops

Heel Loops can be attached to one or both footrests on any Raz Shower Chair. They provide added support, positioning, and comfort for the user.

2.16 Commode Pan


The Raz Commode Pan was designed with an elongated form that fits directly under the seat to minimize backspray. A unique splash-reduction ridge is located at center of the pan. The high gloss surface facilitates cleaning and rinsing, while the pouring spout and handle facilitate emptying the contents. Removal of the Commode Pan is achieved by sliding the pan rearward.

NOTE: When re-inserting the pan, ensure that the pan clicks into the stainless steel brackets and is centered under the seat aperture. If the brackets do not hold the pan under the seat securely, squeeze the metal brackets inward for realignment.

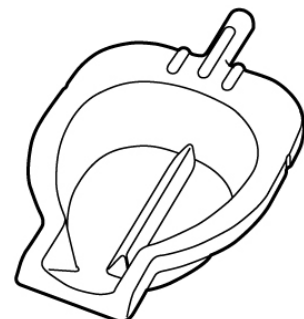

2.17 Fasteners

All fasteners (locknuts, screws, and washers) should be checked periodically to ensure that they are snug and do not pose risk to the user. All nuts used on your Raz Shower Chair are locknuts or are used in conjunction with lock washers. Locknuts that are removed for any reason should be replaced rather than re-used. The fasteners should be checked periodically to ensure a secure fit.



IMPORTANT !

A QUALIFIED RAZ DEALER SHOULD BE CONTACTED TO CHECK ALL FASTENERS, CASTER AND WHEEL LOCKS, HARDWARE, AND OTHER MOVING PARTS AT LEAST ONCE PER YEAR.

3.0 CLEANING AND MAINTENANCE

3.1 Cleaning After Each Use

Commode Pan

1. Remove the Commode Pan and empty its contents.
2. Wash the pan with a multi-purpose disinfectant cleaning solution. Use a toilet brush if needed.
3. Rinse well before storage or re-use.

NOTE: A soapy hot water wash followed by a disinfectant spray can be substituted for a multi-purpose disinfectant cleaning solution

Molded Seat

1. Spray with a multi-purpose disinfectant cleaner and scrub with a soft brush as required.
2. Rinse with a water spray before storage or re-use.

DO NOT IMMERSE the shower chair seat in water or cleaning solutions.

3. For a more thorough cleaning, remove the seat from the shower chair to allow better access to the underside of the seat around the opening or aperture area of the seat.

See section 2.1 for seat removal instructions.

3.2 Cleaning As Needed

Adjustable Tension Back Upholstery

1. Remove the plastic buckles and tri-glides from the back upholstery straps, paying attention to how the straps are wound through each component as they are removed.
2. Remove the back upholstery from the back frame and machine wash with a mild detergent in warm water on a normal or gentle wash cycle. Include the H-strap, pelvic and chest straps if they were ordered with the chair and require cleaning.
3. Install the back upholstery and other positioning straps on the chair and allow to dry. **DO NOT** dry the back upholstery in a clothes dryer or damage to the upholstery may occur.
4. Install the back upholstery on the back frame and assemble all plastic buckles and tri-glides onto the straps.
5. Adjust the backrest upholstery straps to the desired tension.

Frame, Armrests, Adjustable Footrests, and Other Components

1. Spray the frame and components with a multi-purpose disinfectant cleaner, and scrub with a soft brush and rinse with water.
2. If necessary, spray the frame and components with a diluted (10 parts water to 1 part solution) calcium/lime removal solution, scrub with a soft brush, and rinse thoroughly with water. **DO NOT** mix a calcium/lime remover with any other liquid or toxic fumes may result.

It is recommended that a qualified Raz dealer check over all fasteners and subassemblies on a continuing basis or if there is cause for concern to the shower chair's performance.

It is highly recommended that the rinsing of Raz Shower Chair components occur in a well drained area with an industrial steam cleaner (e.g. Intersteam) or a commercial pressure washer.

Several times each year the chair and its components should be wiped down with a diluted calcium/lime removal solution to reduce deposits, followed by a hot water rinse.

To minimize the risk of mildew buildup the entire chair should be wiped down with a soft dry cloth after the final rinse and before storage or use.

3.3 Suggested Cleaning Products

Task	Recommended Products
General Cleaning	Antibacterial Detergent
Tuberculocidal Surface Cleaner and Intermediate Level Disinfectant	Accel TB (Virox Technologies Inc.), SepteFX 7D-11 (Titan Worldwide Inc.)
Calcium and Lime Deterrent	CLR Outdoor Furniture Cleaner

IMPORTANT !

DO NOT USE ABRASIVE POWDERS OR SCOURING PADS ON THE RAZ SHOWER CHAIR.

DO NOT SUBMERGE THE RAZ SHOWER CHAIR IN WATER.

RINSE THOROUGHLY AFTER CLEANING TO ENSURE THAT ANY SOAP OR DETERGENT RESIDUE IS REMOVED.

DO NOT USE CLEANING PRODUCTS WITHOUT CONSULTING THE PRODUCTS' INSTRUCTIONS AND TAKING APPROPRIATE PRECAUTIONS FOR HUMAN EXPOSURE TO CHEMICALS.

4.0 LIMITED WARRANTY

This warranty is extended only to the original purchaser/user of Raz Rehab Shower Chairs from a qualified Raz dealer.

This warranty gives you specific legal rights, but you may have additional legal rights depending on your region and country.

This warranty shall be extended to comply with regional laws and requirements.

With regards to the original purchaser/user only, Raz Design warrants its base and back frame components to be free of defects in materials and workmanship for a period of two (2) years from the date of purchase. All other components on the Raz Rehab Shower Chair are covered for a period of one (1) year and are subject to normal wear and tear exclusions. If within such warranty period any such product shall be proven to be defective, the part will be repaired or replaced, at Raz Design's discretion. This warranty does not include any labour or shipping charges incurred in replacement, part installation, or repair of any such product.

For warranty service, please contact the dealer from whom you purchased your Raz Rehab Shower Chair. In the event that you do not receive satisfactory warranty service, please contact Raz Design directly using the contact information located in either the beginning or the end of this manual. In your correspondence please provide your dealer's name and address, the product type, the date of purchase, the chair's serial number (on a grey label located on the chair frame), as well as the nature of the product defect. Do not return products to the manufacturer without prior authorization.

Limitations and Exclusions:

The foregoing warranty shall not apply to serial numbered products if the serial number has been removed or defaced, and to products subjected to negligence or an accident. Improper operation, maintenance, or storage may void the warranty coverage on the Raz Rehab Shower Chair.

The warranty does not apply to products modified without Raz Design's express written consent. This includes, but is not limited to, modification through the use of unauthorized parts or attachments, products damaged by repairs made to any component without the specific consent of Raz Design, or to a product damaged by circumstances beyond Raz Design's control. Only Raz Design will have the authority to determine whether or not the circumstances are eligible for warranty coverage. The warranty will not apply to problems arising from normal wear or failure to adhere to the instructions contained in this manual.

The foregoing warranty is exclusive and in lieu of any other warranties, whether express or implied, including the implied warranties of merchantability and fitness for a particular purpose. The sole remedy for violations of any warranty whatsoever will be limited to repair or replacement of the defective product in compliance to the terms contained in this document.

The application of any implied warranty shall not extend beyond the duration of the express warranty provided herein. Raz Design will not be liable for any consequential or incidental damages to part or whole of a Raz Rehab Shower Chair.