

MGMT Pyro[®] Kit Handbook

For quantitative measurement of methylation
of four CpG sites in exon 1 of the human
MGMT gene



REF 970061

H B 1069131EN

 QIAGEN GmbH, QIAGEN Strasse 1, D-40724 Hilden

R1 **MAT** 1069131EN



QIAGEN Sample and Assay Technologies

QIAGEN is the leading provider of innovative sample and assay technologies, enabling the isolation and detection of contents of any biological sample. Our advanced, high-quality products and services ensure success from sample to result.

QIAGEN sets standards in:

- Purification of DNA, RNA, and proteins
- Nucleic acid and protein assays
- microRNA research and RNAi
- Automation of sample and assay technologies

Our mission is to enable you to achieve outstanding success and breakthroughs. For more information, visit www.qiagen.com.

Contents

Intended Use	5
Summary and Explanation	5
Principle of the Procedure	6
Controls	6
Materials Provided	7
Kit contents	7
Materials Required but Not Provided	8
Warnings and Precautions	9
Safety information	9
General precautions	9
Reagent Storage and Handling	10
Specimen Handling and Storage	10
Procedures	11
DNA isolation and bisulfite conversion	11
Protocols	
■ 1: Run setup for the PyroMark Q24 System	12
■ 2: PCR using the reagents supplied with the MGMT Pyro Kit	14
■ 3: Immobilization of PCR products to Streptavidin Sepharose High Performance beads	17
■ 4: Preparation of samples prior to Pyrosequencing analysis on the PyroMark Q24	19
■ 5: Running the PyroMark Q24 System	23
Interpretation of Results	26
Analysis of a PyroMark Q24 run	26
Troubleshooting guide	29
Quality Control	31
Limitations	31
References	31
Symbols	32
Contact Information	32
Appendix A: Setting Up MGMT Assays	33

Appendix B: Emptying the Waste Container and Troughs	34
Ordering Information	35

Intended Use

The MGMT Pyro Kit is intended for molecular biology applications.

This product is not intended for the diagnosis, prevention, or treatment of a disease or for patient management.

Summary and Explanation

The MGMT Pyro Kit is intended for quantitative measurements of methylation in four CpG sites in exon 1 of the human MGMT gene (genomic sequence on chromosome 10 from 131,265,519 to 131,265,537:

CGACGCCCGCAGGTCCTCG). Bisulfite converted genomic DNA is amplified by PCR and sequenced through the defined region in the forward direction (Figure 1). Sequences surrounding the defined positions serve as normalization and reference peaks for quantification and quality assessment of the analysis.

The product consists of PCR primer mix and sequencing primer, two vials of each. The primers are delivered in solution. Each vial contains 24 μ l of primer or primer mix. The kit contains primers and reagents for amplification of the genes, plus buffers, primers, and reagents for quantitative methylation detection in real time using Pyrosequencing[®] technology on the PyroMark[®] Q24 System.

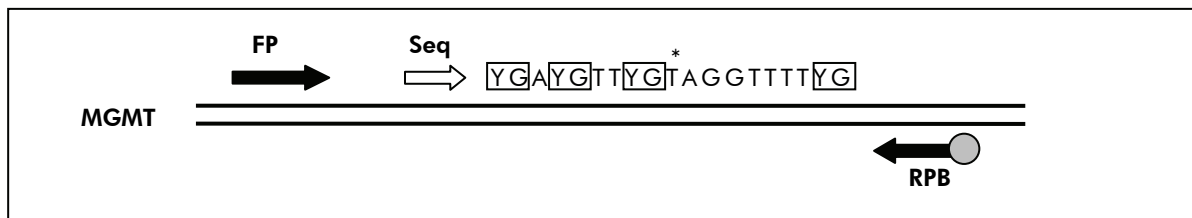



Figure 1. Illustration of the MGMT assay. The sequence indicated is the analyzed sequence after bisulfite conversion. Y indicates the potentially methylated sites and boxes indicate the analyzed CpG sites. The asterisk indicates the site for bisulfite conversion control. **FP**: Forward PCR primers; **RPB**: Reverse PCR primers (**B** indicates biotinylation); **Seq**: Sequencing primers.

Note: The workflow has been slightly modified compared to the *PyroMark Q24 User Manual* (see “Protocol 4: Preparation of samples prior to Pyrosequencing analysis on the PyroMark Q24”, page 19).

Principle of the Procedure

The workflow illustrates the assay procedure. After PCR using primers targeting the defined region of exon 1, the amplicons are immobilized on Streptavidin Sepharose® High Performance beads. Single-stranded DNA is prepared, and the sequencing primers anneal to the DNA. The samples are then analyzed on the PyroMark Q24 System using a run setup file and a run file.

Workflow of MGMT Pyro procedure

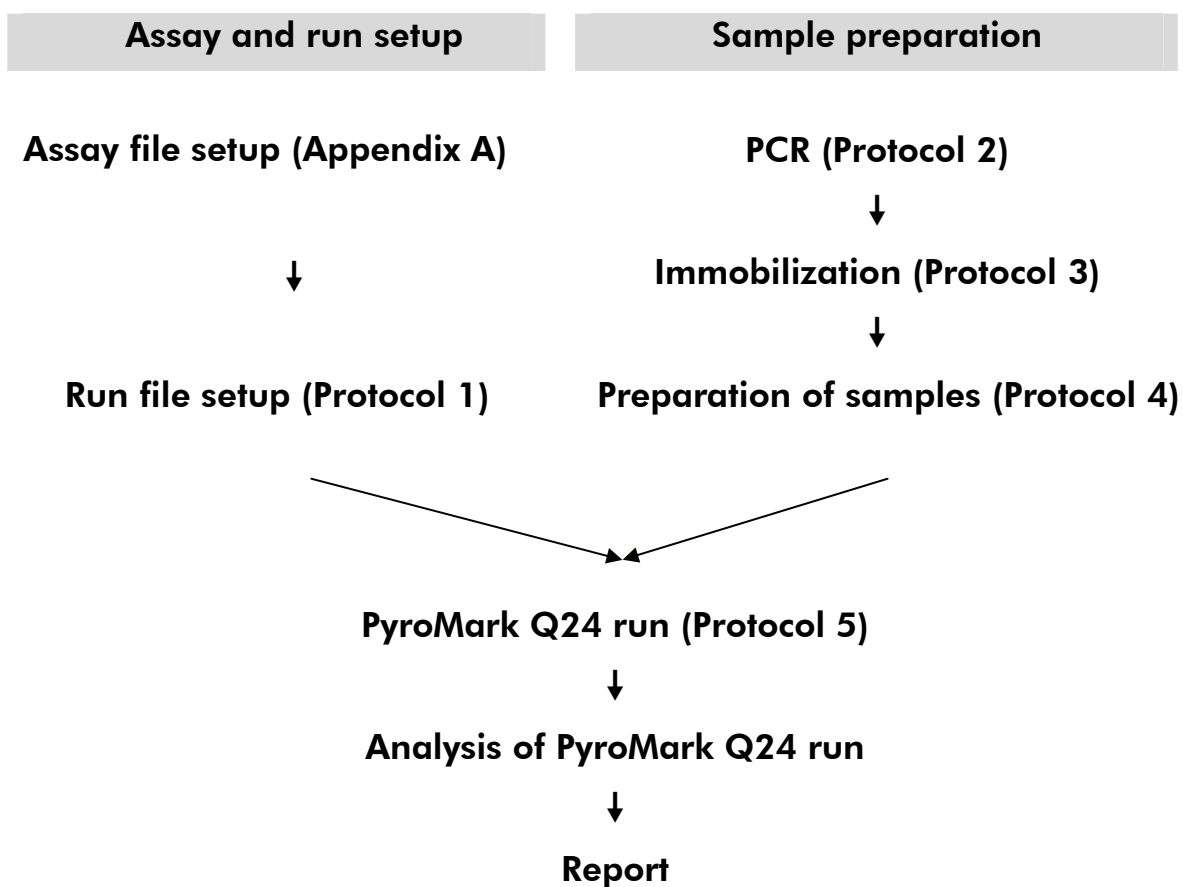

Controls

Methylated control DNA is included in the kit as a positive control for PCR and sequencing reactions. It is also recommended that a DNA sample derived from a healthy blood donor is included in every Pyrosequencing run for comparison. In addition, a negative control (without template DNA) should always be included in every PCR setup.


Materials Provided

Kit contents

MGMT Pyro Kit (box 1/2)

MGMT Pyro Kit	(48)
Catalog no.	970061
Number of reactions	48
PCR Primer Mix MGMT	2 x 24 μ l
Seq Primer MGMT	2 x 24 μ l
PyroMark PCR Master Mix, 2x	850 μ l
CoralLoad [®] Concentrate, 10x	1.2 ml
H ₂ O	3 x 1.9 ml
Methylated Control DNA, 10 ng/ μ l	100 μ l

Pyro buffers and reagents (box 2/2)

Buffers and reagents	
PyroMark Binding Buffer	10 ml
PyroMark Annealing Buffer	10 ml
PyroMark Denaturation Solution*	250 ml
PyroMark Wash Buffer, 10x	25 ml
Enzyme Mixture	1 vial
Substrate Mixture	1 vial
dATP α S	1180 μ l
dCTP	1180 μ l
dGTP	1180 μ l
dTTP	1180 μ l
Handbook	 1

* Contains sodium hydroxide.

Materials Required but Not Provided

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

- DNA isolation kit (see “DNA isolation and bisulfite conversion”, page 11)
- Reagents for bisulfite conversion of DNA (see “DNA isolation and bisulfite conversion”, page 11)
- Pipets (adjustable)
- Sterile pipet tips (with filters for PCR setup)
- Benchtop microcentrifuge
- Thermal cycler and appropriate PCR tubes
- Streptavidin Sepharose High Performance (GE Healthcare, cat. no. 17-5113-01; www.gelifesciences.com)
- PyroMark Q24 (cat. no. 9001514)
- PyroMark Q24 Software (cat. no. 9019062)
- PyroMark Q24 Plate (cat. no. 979201)
- PyroMark Q24 Cartridge (cat. no. 979202)
- PyroMark Q24 Vacuum Workstation (cat. no. varies depending on region, see “Ordering Information”, page 35)
- Plate mixer for immobilization to beads (see “Recommended plate mixers”, page 11)
- Heating block capable of attaining 80°C
- 24-well PCR plate or strips
- Strip caps
- High-purity water (Milli-Q® 18.2 MΩ x cm or equivalent)

Note: Sufficient water is provided in the product for PCR, DNA immobilization, and for dissolving the Enzyme Mixture and the Substrate Mixture; additional high-purity water is required to dilute PyroMark Wash Buffer, 10x

- Ethanol (70%)*

* Do not use denatured alcohol, which contains other substances such as methanol or methylethylketone.

Warnings and Precautions

Safety information

When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, please consult the appropriate material safety data sheets (MSDSs). These are available online in convenient and compact PDF format at www.qiagen.com/Support/MSDS.aspx where you can find, view, and print the MSDS for each QIAGEN kit and kit component.

The following risk and safety phrases apply to components of the MGMT Pyro Kit.

PyroMark Denaturation Solution

Contains sodium hydroxide: Irritant. Risk and safety phrases:* R36/38, S26-36/37/39-45

24-hour emergency information

Emergency medical information in English, French, and German can be obtained 24 hours a day from:

Poison Information Center Mainz, Germany

Tel: +49-6131-19240

General precautions

The user should always pay attention to the following.

- Note that the workflow has been slightly modified compared to the *PyroMark Q24 User Manual* (see "Protocol 4: Preparation of samples prior to Pyrosequencing analysis on the PyroMark Q24", page 19).
- The components of this product are sufficient to perform the 48 reactions in up to 5 independent runs.
- Use sterile pipet tips with filters (for PCR setup).
- Store and extract positive materials (specimens, positive controls, and amplicons) separately from all other reagents and add them to the reaction mix in a spatially separated facility.

* R36/38: Irritating to eyes and skin; S26: In case of contact with eyes, rinse immediately with plenty of water and seek medical advice; S36: Wear suitable protective clothing; S37: Wear suitable gloves; S39: Wear eye/face protection; S45: In case of accident or if you feel unwell, seek medical advice immediately (show the label where possible).

- Thaw all components thoroughly at room temperature (15–25°C) before starting an assay.
- When thawed, mix the components (by pipetting repeatedly up and down or by pulse vortexing) and centrifuge briefly.
- Failed results are not a basis for judgment of methylational status.

Reagent Storage and Handling

The MGMT Pyro Kit is shipped in two boxes. The MGMT Pyro Kit (box 1/2) is shipped on dry ice. PyroMark PCR Master Mix, CoralLoad Concentrate, methylated control DNA, and all primers should be stored at –15 to –25°C upon arrival.

The Pyro Buffers and Reagents (box 2/2) containing buffers, Enzyme Mixture, Substrate Mixture, dATP α S, dCTP, dGTP, and dTTP (the reagents for Pyrosequencing analysis) is shipped on cool packs. These components should be stored at 2–8°C upon arrival. To minimize loss of activity, it is advisable to keep both the enzyme mixture and the substrate mixture in the vials supplied.

Reconstituted enzyme and substrate mixtures are stable for at least 5 days at 2–8°C. Reconstituted enzyme and substrate mixtures can be frozen and stored in their vials at –15 to –25°C. Frozen reagents should not be subjected to more than 3 freeze–thaw cycles.

Important: Nucleotides should not be frozen.

The MGMT Pyro Kit is stable until the kit expiration date when stored under these conditions.

Specimen Handling and Storage

All samples must be treated as potentially infectious material.

Specimen material is human DNA extracted from blood or formalin-fixed paraffin-embedded samples.

Samples from humans undergoing heparin treatment must not be used. Blood samples that have been collected in tubes containing heparin as an anticoagulant should not be used. Heparin affects the PCR.

Procedures

DNA isolation and bisulfite conversion

The QIAGEN kits shown below are recommended for DNA purification from the indicated human sample types for use with the MGMT Pyro Kit. Carry out the DNA purification according to the instructions in the kit handbooks. For bisulfite conversion, the EpiTect® Bisulfite Kit (cat. no. 59104) or EpiTect Plus FFPE Bisulfite Kit (cat. no. 59144) from QIAGEN is recommended.

Table 1. DNA purification kits recommended for use with the MGMT Pyro Kit

Sample material	Nucleic acid isolation kit	Catalog number (QIAGEN)
Paraffin-embedded tissue	QIAamp® DNA FFPE Tissue Kit (50)	56404
	EZ1® DNA Tissue Kit (48)	953034
Blood	QIAamp DSP DNA Blood Mini Kit	61104

Recommended plate mixers

The plate mixers shown in Table 2 are recommended for use with the MGMT Pyro Kit.

Table 2. Plate mixers recommended for use with the MGMT Pyro Kit

Manufacturer	Product	Catalog number
Eppendorf	Basic mixer	5355 000.011
	Thermoblock for MTP	5363 000.012
	Adapter plate for 96 x 0.2ml PCR tubes to insert in blocks for microtiter plates	5363 007.009
H+P Labortechnik GmbH	Variomag® Teleshake	51410 (115 V = 51410 U)
	Variomag Monoshake	51110 (115 V = 51110 U)

Protocol 1: Run setup for the PyroMark Q24 System

Things to do before starting

- Create an Assay Setup as described in Appendix A. This needs to be done only once, before running the MGMT assay for the first time (see “Appendix A: Setting Up MGMT Assays”, page 33).

Procedure


1. Click  in the toolbar.

A new run file is created.

2. Enter the run parameters (see “Run parameters”, page 13).
3. Set up the plate by adding the assay to wells corresponding to the samples to analyze.

A negative sample (without template DNA) should be included in every PCR setup.

It is also recommended to include a control sample with DNA from a healthy blood donor in each Pyrosequencing run.

4. When the run is set up and ready to run on the PyroMark Q24 System, print a list of required volumes of enzyme mix, substrate mix, and nucleotides, and the plate setup. Select “Pre Run Information” from the “Tools” menu and, when the report appears, click .

5. Close the run file and copy it to a USB stick (supplied with the system) using Windows® Explorer.

The printed Pre Run Information can be used as a template for the sample setup (see “Protocol 3: Immobilization of PCR products to Streptavidin Sepharose High Performance beads”, page 17).

To run the plate on PyroMark Q24, see “Protocol 5: Running the PyroMark Q24 System”, page 23.

Run parameters

Run name:	The name of the run is given when the file is saved. Renaming the file also changes the name of the run.
Instrument method:	Select the instrument method according to the reagents and cartridge that will be used for the run; see the instructions supplied with the products.
Plate ID:	Optional: Enter ID of the PyroMark Q24 Plate.
Bar code:	Optional: Enter a bar code number for the plate or, if you have a bar code reader connected to your computer, place the mouse cursor in the "Barcode" text box (by clicking the box) and scan the bar code.
Reagent ID:	Optional: Enter the lot number for the MGMT Pyro Kit to be used. The lot number can be found on the product label. Note: We recommend entering the lot number so that any unexpected problems with the MGMT Pyro Kit can be traced.
Run note:	Optional: Enter a note about the contents or purpose of the run.

Add assay files

To add an assay to a well, you can either:

- Right-click the well and select "Load Assay" from the context menu.
- Select the assay in the shortcut browser and click-and-drag the assay to the well.

A well is color-coded according to the assay loaded to the well.

Enter sample IDs and notes

To enter a sample ID or note, select the cell and enter the text.

To edit a sample ID or note, either select the cell (the current contents will be selected) or double-click the cell.

Protocol 2: PCR using the reagents supplied with the MGMT Pyro Kit

This protocol is for PCR amplification of a region of bisulfite converted DNA using the MGMT Pyro Kit.

Important points before starting

- The HotStarTaq[®] DNA polymerase in the PyroMark PCR Master Mix requires an activation step of **15 minutes at 95°C**.
- Set up all reaction mixtures in an area separate from that used for DNA purification, adding template DNA to the PCR, PCR product analysis, or preparation of samples prior to Pyrosequencing analysis.
- Use disposable tips containing hydrophobic filters to minimize cross-contamination.
- Bisulfite converted DNA must be used as template DNA. The EpiTect Bisulfite Kit (cat. no. 59104) or EpiTect Plus FFPE Bisulfite Kit (cat. no. 59144) from QIAGEN are recommended.

Things to do before starting

- Before opening the tube with PCR primer, centrifuge briefly to collect contents at the bottom of the tubes.
- Adjust the concentration of the sample and control DNA, if necessary, to 2–10 ng/ μ l.

Procedure

1. Thaw all necessary components.

Mix well before use.

2. Prepare a reaction mix according to Table 3.

The reaction mix typically contains all of the components needed for PCR, except the sample.

Prepare a volume of reaction mix greater than that required for the total number of PCR assays to be performed.

Table 3. Preparation of reaction mix

Component	Volume/reaction (μl)
PyroMark PCR Master Mix, 2x	12.5
CoralLoad Concentrate, 10x	2.5
PCR Primer Mix MGMT	1.0
Water (H ₂ O, supplied)	4.0
Total volume	20.0

3. Mix the reaction mix thoroughly and dispense 20 μ l into each PCR tube.

It is not necessary to keep PCR tubes on ice since HotStarTaq DNA polymerase is inactive at room temperature.

4. Add 5 μ l template DNA (10–50 ng of genomic DNA measured before bisulfite conversion) to the individual PCR tubes (see Table 4) and mix thoroughly.

A negative control sample (without template DNA) should be included in every PCR setup.

It is also recommended to include a control sample with DNA from a healthy blood donor in each Pyrosequencing run.

Table 4. Preparation of PCR

Component	Volume/reaction (μl)
Reaction mix	20
Sample DNA	5
Total volume	25

5. Program the thermal cycler according to the manufacturer's instructions using the conditions outlined in Table 5.

Table 5. Optimized cycling protocol

			Comments
Initial activation step:	15 minutes	95°C	HotStarTaq DNA polymerase is activated by this heating step.
3-step cycling:			
Denaturation	20 seconds	95°C	
Annealing	30 seconds	53°C	
Extension	20 seconds	72°C	
Number of cycles	42		
Final extension:	5 minutes	72°C	

6. Place the PCR tubes in the thermal cycler and start the cycling program.
7. After amplification, proceed with "Protocol 3: Immobilization of PCR products to Streptavidin Sepharose High Performance beads", page 17.

Protocol 3: Immobilization of PCR products to Streptavidin Sepharose High Performance beads

This protocol is for immobilization of template DNA to Streptavidin Sepharose High Performance (GE Healthcare) prior to analysis on the PyroMark Q24 System.

Important points before starting

- Allow all required reagents and solutions to reach room temperature (15–25°C) before starting.

Procedure

1. Gently shake the bottle containing Streptavidin Sepharose High Performance until it is a homogeneous solution.
2. Prepare a master mix for DNA immobilization according to Table 6. Prepare a volume 10% greater than that required for the total number of reactions to be performed.

Table 6. Master mix for DNA immobilization

Component	Volume/sample (µl)
Streptavidin Sepharose High Performance	2
PyroMark Binding Buffer	40
Water (H ₂ O, supplied)	28
Total volume	70

3. Add 70 µl of the master mix to wells of a 24-well PCR plate (or strips) as predefined in the run setup (see "Protocol 1: Run setup for the PyroMark Q24 System", page 12).
4. Add 10 µl of biotinylated PCR product from Protocol 2 to each well containing master mix, as predefined in the run setup (see "Protocol 1: Run setup for the PyroMark Q24 System", page 12).
The total volume per well should be 80 µl after addition of the master mix and PCR product.
5. Seal the PCR plate (or strips) using strip caps.
Ensure that no leakage is possible between the wells.

6. Agitate the PCR plate at room temperature (15–25°C) for 5–10 minutes at 1400 rpm.

During this step, prepare the PyroMark Q24 Vacuum Workstation for sample preparation as described in the *PyroMark Q24 User Manual*.

7. Proceed immediately with “Protocol 4: Preparation of samples prior to Pyrosequencing analysis on the PyroMark Q24”, page 19.

Sepharose beads sediment quickly. Capturing of the beads must take place immediately following agitation.

If more than 1 minute has elapsed since the plate (or strips) was agitated, agitate again for 1 minute before capturing the beads.

Protocol 4: Preparation of samples prior to Pyrosequencing analysis on the PyroMark Q24

This protocol is for preparation of single-stranded DNA and annealing of the sequencing primer to the template prior to Pyrosequencing analysis on the PyroMark Q24.

Important points before starting

- Add the sequencing primer in the same pattern as predefined for the plate in the run setup (see “Protocol 1: Run setup for the PyroMark Q24 System”, page 12).
- Note that the workflow has been slightly modified compared to the *PyroMark Q24 User Manual* (step 18). Do not shorten the time for cooling down the samples after heating to 80°C.
- Perform the function test for filter probes as described in the *PyroMark Q24 Handbook* on a regular basis and exchange filter probes if indicated.

Things to do before starting

- Before opening the tube with sequencing primer, centrifuge briefly to collect contents at the bottom of the tubes.
- Place one PyroMark Q24 Plate Holder on a preheated heating block at 80°C for use in step 17. Leave a second PyroMark Q24 Plate Holder at room temperature (15–25°C) for use in step 18.
- PyroMark Wash Buffer is supplied as a 10x concentrate. Before using for the first time, add high-purity water to 25 ml 10x PyroMark Wash Buffer to achieve a final volume of 250 ml and obtain a 1x working solution.

Note: The 1x PyroMark Wash Buffer working solution is stable at 2–8°C until the marked expiration date.

Procedure

1. Dilute a sufficient amount of the sequencing primer, Seq Primer MGMT, in PyroMark Annealing Buffer as shown in Table 7.

Prepare a volume of diluted sequencing primer greater than that required for the total number of samples to be sequenced (for the number of samples + one extra).

Table 7. Example of dilution of the sequencing primer

Component	Volume/sample (μl)	Volume for 9 + 1 reactions (μl)
Seq Primer MGMT	0.8	8
PyroMark Annealing Buffer	24.2	242
Total volume	25	250

- 2. Add 25 μ l of diluted sequencing primer to each well of the PyroMark Q24 Plate according to the run setup (see “Protocol 1: Run setup for the PyroMark Q24 System”, page 12).**

Keep one of the PyroMark Q24 Plate Holders (supplied with the PyroMark Q24 Vacuum Workstation) at room temperature (15–25°C) and use it as support when preparing and moving the plate.

- 3. Place the PCR plate (or strips) from Protocol 3 and the PyroMark Q24 Plate on the worktable (Figure 2).**

Ensure that the plate is in the same orientation as when samples were loaded.



Figure 2. Placement of PCR plate (or strips) and PyroMark Q24 plate on the vacuum workstation.

- 4. Apply vacuum to the vacuum tool by opening the vacuum switch.**

- 5. Carefully lower the filter probes into the PCR plate (or strips) to capture the beads containing immobilized template. Hold the probes in place for 15 seconds. Take care when picking up the vacuum tool.**

Sepharose beads sediment quickly. Capturing of the beads must take place immediately following agitation.

If more than 1 minute has elapsed since the plate (or strips) was agitated, agitate again for 1 minute before capturing the beads.

- 6. Transfer the vacuum tool to the trough containing 40 ml 70% ethanol (Figure 2). Flush the filter probes for 5 seconds.**
- 7. Transfer the vacuum tool to the trough containing 40 ml Denaturation Solution (Figure 2). Flush the filter probes for 5 seconds.**
- 8. Transfer the tool to the trough containing 50 ml Wash Buffer (Figure 2). Flush the filter probes for 10 seconds.**
- 9. Raise the vacuum tool up and back, beyond 90° vertical, for 5 seconds to drain liquid from the filter probes (Figure 3).**



Figure 3. Illustration of the vacuum tool raised to beyond 90° vertical.

- 10. While the vacuum tool is held over the PyroMark Q24 Plate, close the vacuum switch on the tool (Off).**
- 11. Release the beads into the PyroMark Q24 Plate by lowering the filter probes into the diluted sequencing primer and moving the tool gently from side to side.**

Do not damage the surface of the PyroMark Q24 Plate by scratching it with the filter probes.
- 12. Transfer the vacuum tool to the trough containing high-purity water (Figure 2) and agitate the tool for 10 seconds.**
- 13. Wash the filter probes by lowering the probes into high-purity water (Figure 2) and applying vacuum. Flush the probes with 70 ml high-purity water.**
- 14. Raise the tool up and back, beyond 90° vertical, for 5 seconds to drain liquid from the filter probes (Figure 3).**

- 15. Close the vacuum switch on the tool (Off), and place the tool in the Parking (P) position.**
- 16. Turn off the vacuum pump.**

At the end of a working day, liquid waste and remaining solutions should be discarded and the PyroMark Q24 Vacuum Workstation should be checked for dust and spillage (see “Appendix B: Emptying the Waste Container and Troughs”, page 34).
- 17. Heat the PyroMark Q24 Plate with the samples at 80°C for 2 minutes using the prewarmed PyroMark Q24 Plate Holder.**
- 18. Remove the PyroMark Q24 Plate from the hot plate holder and place it on a second PyroMark Q24 Plate Holder that was kept at room temperature (15–25°C) to let the samples cool to room temperature (15–25°C) for 10–15 minutes.**
- 19. Proceed with “Protocol 5: Running the PyroMark Q24 System”, page 23.**

Protocol 5: Running the PyroMark Q24 System

This protocol describes the preparation and loading of PyroMark Gold Q24 Reagents into the PyroMark Q24 Cartridge, and starting and finishing a run on the PyroMark Q24 System. For a detailed description on how to set up a run, see the *PyroMark Q24 User Manual*.

Important point before starting

- Switch on the PyroMark Q24. The power switch is located at the rear of the instrument.
- The Pre Run information report, found in the “Tools” menu at run setup (see “Protocol 1: Run setup for the PyroMark Q24 System”, page 12), provides information about the volume of nucleotides, enzyme, and substrate buffer needed for a specific assay.

Procedure

- 1. Dissolve each of the freeze-dried enzyme and substrate mixtures in 620 μ l water (supplied).**
- 2. Mix by swirling the vial gently. Do not vortex!**
To ensure the mixture is fully dissolved, leave it at room temperature (15–25°C) for 5–10 minutes. Make sure that the solution is not turbid before filling the PyroMark Q24 Cartridge. If the reagents are not to be used immediately, place the reagent vials on ice* or in a refrigerator.
- 3. Allow the reagents and the PyroMark Q24 Cartridge to reach ambient temperature (20–25°C).**
- 4. Place the PyroMark Q24 Cartridge with the label facing you.**
- 5. Load the PyroMark Q24 Cartridge with the appropriate volumes of nucleotides, enzyme, and substrate mixes according to Figure 4.**
Make sure that no air bubbles are transferred from the pipet to the cartridge.

* When working with chemicals, always wear a suitable lab coat, disposable gloves, and protective goggles. For more information, consult the appropriate material safety data sheets (MSDSs), available from the product supplier.

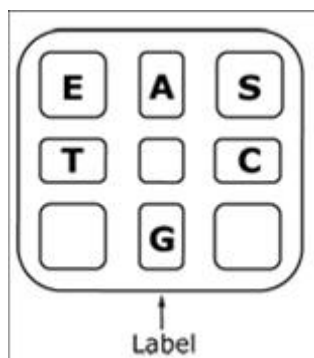


Figure 4. Illustration of the PyroMark Q24 Cartridge, as seen from above. The annotations correspond to the label on the reagent vials. Add enzyme mixture (**E**), substrate mixture (**S**), and nucleotides (**A**, **T**, **C**, **G**) according to the volume information given in the Pre Run information report found in the “Tools” menu at run setup.

6. **Open the cartridge gate and insert the filled reagent cartridge with the label facing out. Push the cartridge in fully and then push it down.**
7. **Ensure the line is visible in front of the cartridge and close the gate.**
8. **Open the plate-holding frame and place the plate on the heating block.**
9. **Close the plate-holding frame and the instrument lid.**
10. **Insert the USB stick (containing the run file) into the USB port at the front of the instrument.**
Do not remove the USB stick before the run is finished.
11. **Select “Run” in the main menu (using the ▲ and ▼ screen buttons) and press “OK”.**
12. **Select the run file using the ▲ and ▼ screen buttons.**
To view the contents of a folder, select the folder and press “Select”. To go back to the previous view, press “Back”.
13. **When the run file is selected, press “Select” to start the run.**
14. **When the run is finished and the instrument confirms that the run file has been saved to the USB stick, press “Close”.**
15. **Remove the USB stick.**
16. **Open the instrument lid.**
17. **Open the cartridge gate and remove the reagent cartridge by lifting it up and pulling it out.**
18. **Close the gate.**
19. **Open the plate-holding frame and remove the plate from the heating block.**
20. **Close the plate-holding frame and the instrument lid.**

- 21. Discard the plate and clean the cartridge, as per the instructions in the product sheet supplied with the cartridge.**
- 22. Analyze the run according to "Analysis of a PyroMark Q24 run", page 26.**

Interpretation of Results

Analysis of a PyroMark Q24 run

This protocol describes the methylation analysis of a completed MGMT run using PyroMark Q24 Software.

Procedure

1. **Insert the USB stick (containing the processed run file) into the computer's USB port.**
2. **Move the run file from the USB stick to the desired location on the computer using Windows Explorer.**
3. **Open the run file in CpG mode of the PyroMark Q24 Software either by selecting "Open" in the "File" menu or by double-clicking the file (✓) in the shortcut browser.**
4. **To analyze the run and get an overview of the results, click one of the Analyze buttons.**



Analyze all wells.



Analyze the selected well.

The analysis results (methylation frequencies) and quality assessment are displayed above the variable position in the Pyrogram[®] trace. For more details on how to analyze a run, see the *PyroMark Q24 User Manual*.

5. **To generate a report, select "CpG Full Report" or "CpG Analysis Results" in the "Reports" menu.**

For reliable results, we recommend single peak heights above 30 RLU. Set 30 RLU as the "required peak height for passed quality" in assay setup (see Appendix A, page 33, and the *PyroMark Q24 User Manual*).

The CpG Analysis results report should be used for documentation and interpretation of methylation quantification. The numbers shown in the Pyrogram are rounded and do not show the exact quantification.

The Pyrogram should always be compared to the histogram which can be displayed by right-clicking in the Pyrogram window. The measured peaks should match the height of the histogram bars.

Interpretation of results

It is recommended that a DNA sample derived from a healthy blood donor is included in every run for comparison. The samples can also be compared with each other to reveal low methylation frequencies.

The limit of blank (LOB) values represent methylation frequencies obtained from healthy blood donor samples with a probability of 95%. LOB values have been determined using samples from healthy blood donors (Table 8). The α - and β -errors (false positive and false negative, respectively) were set to 5%.

Table 8. LOB determined for specific methylation sites using samples from healthy blood donors

Position	LOB (% units)
CpG site 1	1.5
CpG site 2	1.8
CpG site 3	3.2
CpG site 4	3.4
Mean of CpG site 1 to 4	2.1

These values were based on runs where the signal was over 30 relative light units (RLU), as routinely obtained from 10 ng of DNA isolated from blood (measured before bisulfite conversion). We recommend that the method performance is confirmed in the laboratory.

Representative results

Representative Pyrogram results are shown in Figures 5–6.

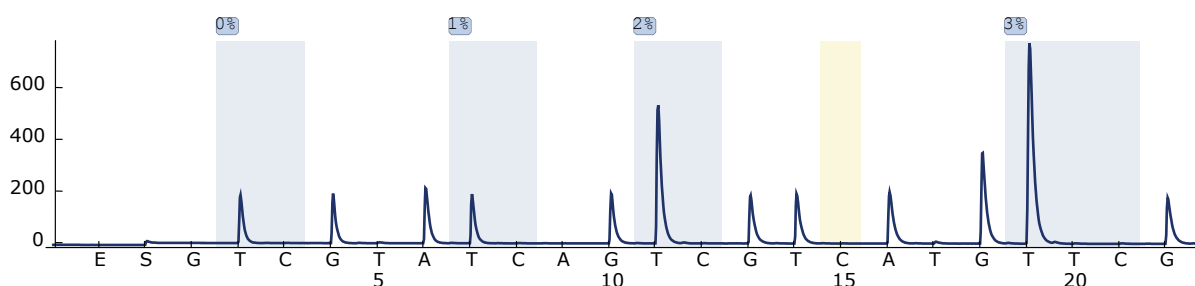


Figure 5. Pyrogram trace obtained after analysis of unmethylated bisulfite converted DNA from a healthy blood donor sample. The bar at dispensation 15 represents the control for completion of bisulfite conversion.

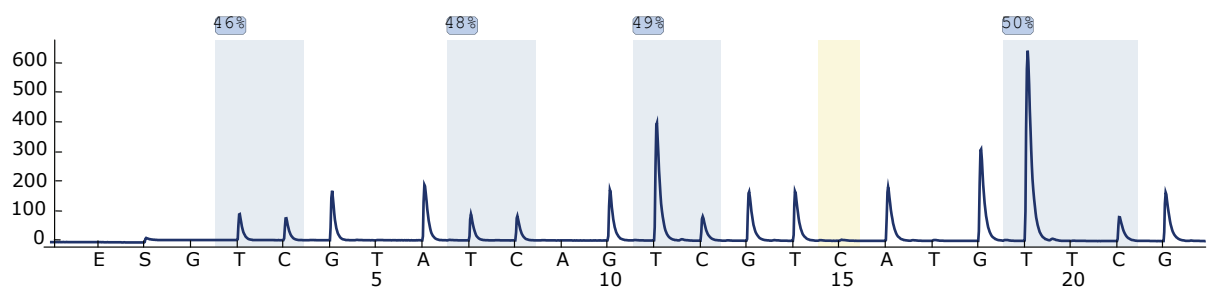


Figure 6. Pyrogram trace obtained after analysis of a methylated bisulfite converted DNA. The bar at dispensation 15 represents the control for completion of bisulfite conversion.

Troubleshooting guide

This troubleshooting guide may be helpful in solving any problems that may arise. For more information, see also the Frequently Asked Questions page at our Technical Support Center: www.qiagen.com/FAQ/FAQList.aspx. The scientists in QIAGEN Technical Services are always happy to answer any questions you may have about either the information and protocols in this handbook or sample and assay technologies (for contact information, see back cover or visit www.qiagen.com).

Refer to the *PyroMark Q24 User Manual* for general troubleshooting of the instrument.

Comments and suggestions

Signals in the no template control (negative control)

- | | |
|-----------------------------|---|
| a) Cross-talk between wells | Signal from one well is detected in a neighboring well. Avoid placing samples with high signal intensities next to “no template” control wells. |
| b) PCR contamination | Use sterile pipet tips with filters. Store and extract materials such as specimens, plasmid controls, and amplicons separately from PCR reagents. |

Poor or unexpected sequence

- | | |
|-------------------------------|--|
| a) Low quality of genomic DNA | Low-quality genomic DNA can cause the PCR to fail. Analyze PCR samples using an electrophoretic technique (for example, the QIAxcel [®] System or agarose-gel electrophoresis). |
|-------------------------------|--|

“Check” or “failed” result

- | | |
|--------------------------------|--|
| a) Low peak height | Handling errors in PCR setup or sample preparation prior to Pyrosequencing can result in low peaks. Perform the function test for filter probes as described in the <i>PyroMark Q24 Handbook</i> on a regular basis and exchange filter probes when indicated.

In case of a “Check” warning, carefully compare the Pyrogram to the histogram which can be displayed by right-clicking in the Pyrogram window. If the measured peaks match the height of the histogram bars, the result is valid. Otherwise it is recommended to rerun the sample. |
| b) Signal in bisulfite control | The bisulfite conversion was not complete. It is recommended to use the EpiTect Bisulfite Kit (cat. no. 59104) or EpiTect Plus FFPE Bisulfite Kit (cat. no. 59144) from QIAGEN, and to strictly follow the protocol for conversion. |

High background

- | | |
|---|---|
| a) Incorrect storage of nucleotides | Store nucleotides at 2–8°C. Storage at –20°C can cause an increase in the background. |
| b) Short cooling time of samples prior to Pyrosequencing analysis | Keep the samples on a PyroMark Q24 Plate Holder at room temperature for 10–15 minutes. Do not shorten the cooling time. |
| c) Contamination of cartridge | Carefully clean the cartridge as described in the product sheet. Store the cartridge protected from light and dust. |

No signals in positive controls

- | | |
|---|--|
| a) Insufficient enzyme or substrate mix for all wells | Make sure to fill the PyroMark Q24 Cartridge according to the “Pre Run Information” in the “Tools” menu. |
| b) Reagents incorrectly stored or diluted | Prepare the PyroMark Q24 Gold Reagents according to the instructions. |

- c) PCR or sample preparation failure Handling errors in PCR setup, programming of the PCR cycler, or sample preparation prior to Pyrosequencing analysis can result in no signal. Perform the function test for filter probes as described in the *PyroMark Q24 Handbook* and exchange filter probes when needed. Repeat the PCR and Pyrosequencing analysis.

Quality Control

In accordance with QIAGEN's ISO-certified Quality Management System, each lot of the MGMT Pyro Kit is tested against predetermined specifications to ensure consistent product quality.

Limitations












The purchaser and user of the MGMT Pyro Kit should refer to the Limited License Agreement on the inside back cover of the *MGMT Pyro Kit Handbook* for additional information concerning the use of this product.

References

QIAGEN maintains a large, up-to-date online database of scientific publications utilizing QIAGEN products. Comprehensive search options allow you to find the articles you need, either by a simple keyword search or by specifying the application, research area, title, etc.

For a complete list of references, visit the QIAGEN Reference Database online at www.qiagen.com/RefDB/search.asp or contact QIAGEN Technical Services or your local distributor.

Symbols

	Contains reagents sufficient for <N> reactions
	Use by
	Catalog number
	Lot number
	Material number
	Components
	Contains
	Number
	Temperature limitation
	Manufacturer
	Consult instructions for use



Contact Information

For technical assistance and more information, please see our Technical Support Center at www.qiagen.com/Support or call one of the QIAGEN Technical Service Departments or local distributors (see back cover or visit www.qiagen.com).

Appendix A: Setting Up MGMT Assays

Before running the MGMT assay for the first time, the assay file needs to be set up as described below.

Procedure

1. Set up the assay for MGMT by using the PyroMark Q24 Software.
2. Click  in the toolbar and select "New CpG Assay".
3. Type the sequence "YGAYGTTYGTAGGTTTTYGT" in "Sequence to Analyze".
4. Manually enter the following "Dispensation Order"; "GTCGTATCAGTCGTCATGTTTCG".
5. Click the "Analysis Parameters" tab and increase "Peak Height Threshold - Required peak height for Passed quality:" to 30.
6. In the "Analysis Parameters" tab, set the "Allowed percentage for passed quality" and "Allowed percentage for check quality" to 7.0 and 10.0, respectively.
7. Click  in the toolbar, and save the assay as "MGMT".

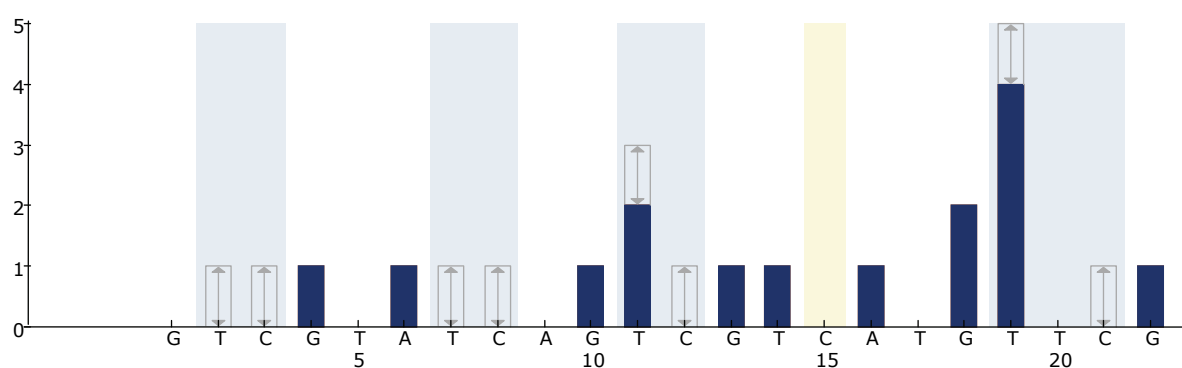



Figure 7. Histogram for the MGMT Pyro Kit assay. The bar at dispensation 15 indicates the control for completion of bisulfite conversion.

Appendix B: Emptying the Waste Container and Troughs

WARNING 	Hazardous chemicals <p>The Denaturation Solution used with the vacuum workstation contains sodium hydroxide, which is irritating to eyes and skin. Always wear safety glasses, gloves, and a lab coat.</p> <p>The responsible body (e.g., laboratory manager) must take the necessary precautions to ensure that the surrounding workplace is safe and that the instrument operators are not exposed to hazardous levels of toxic substances (chemical or biological) as defined in the applicable Material Safety Data Sheets (MSDSs) or OSHA,* ACGIH,[†] or COSHH[‡] documents.</p> <p>Venting for fumes and disposal of wastes must be in accordance with all national, state, and local health and safety regulations and laws.</p>
---	---

* OSHA: Occupational Safety and Health Administration (United States of America)

[†] ACGIH: American Conference of Government Industrial Hygienists (United States of America)

[‡] COSHH: Control of Substances Hazardous to Health (United Kingdom)

Be sure to observe federal, state, and local environmental regulations for the disposal of laboratory waste.

Procedure

1. **Ensure that no vacuum is applied to the vacuum tool. Make sure that the vacuum is closed (Off) and the vacuum pump is switched off.**
2. **Discard any solutions left in the troughs.**
3. **Rinse the troughs with high-purity water, or replace them if necessary.**
4. **Empty the waste container.**
5. **The cap can be removed without disconnecting the tubing.**
6. **If the vacuum workstation must be cleaned (for example, due to dust or spillage), follow the instructions in the *PyroMark Q24 User Manual*.**

Ordering Information

Product	Contents	Cat. no.
MGMT Pyro Kit (48)	For 48 reactions on PyroMark Q24 Systems: Seq Primers, PCR Primers, Methylated Control DNA, PyroMark PCR Master Mix, CoralLoad Concentrate, PyroMark Binding Buffer, PyroMark Annealing Buffer, PyroMark Denaturation Solution, PyroMark Wash Buffer, Enzyme Mixture, Substrate Mixture, dATP α S, dCTP, dGTP, dTTP, and H ₂ O	970061
Accessories		
PyroMark Q24 Plate (100)	24-well sequencing reaction plate	979201
PyroMark Q24 Cartridge (3)	Cartridges for dispensing nucleotides and reagents	979202
PyroMark Vacuum Prep Filter Probe (100)	Reusable filter probes for PyroMark Vacuum Workstation Q96 and Q24	979010
PyroMark Control Oligo	For installation check of system	979203
PyroMark Q24 Validation Oligo	For performance confirmation of system	979204
Related products		
PyroMark Q24	Sequence-based detection platform for Pyrosequencing of 24 samples in parallel	9001514
PyroMark Q24 Vacuum Workstation	Vacuum Workstation for preparing 24 samples in parallel, from PCR product to single-stranded template	9001518 (220 V); 9001516 (110 V); 9001519 (100 V)

Product	Contents	Cat. no.
PyroMark Q24 Software	Analysis software	9019062
QIAamp DNA FFPE Tissue Kit (50)	For 50 DNA preps: 50 QIAamp MinElute® Columns, Proteinase K, Buffers, Collection Tubes (2 ml)	56404
EZ1 DNA Tissue Kit (48)	For 48 preps: Reagent Cartridges (Tissue), Disposable Filter-Tips, Disposable Tip-Holders, Sample Tubes (2 ml), Elution Tubes (1.5 ml), Buffer G2, Proteinase K	953034
QIAamp DSP DNA Blood Mini Kit	For 50 preps: QIAamp Mini Spin Columns, Buffers, Reagents, Tubes, VacConnectors	61104
EpiTect Bisulfite Kit	For 48 preps: EpiTect Bisulfite Spin Columns, Reaction Mix, DNA Protect Buffer, Carrier RNA, Buffers	59104
EpiTect Plus FFPE Bisulfite Kit	For 48 preps: MinElute DNA spin columns, Bisulfite mix, DNA Protect Buffer, Carrier RNA, Buffers, Deparaffinization Solution, Lysis Buffer FTB	59144

For up-to-date licensing information and product-specific disclaimers, see the respective QIAGEN kit handbook or user manual. QIAGEN kit handbooks and user manuals are available at www.qiagen.com or can be requested from QIAGEN Technical Services or your local distributor.

This page intentionally left blank

This page intentionally left blank

Trademarks: QIAGEN®, QIAamp®, QIAxcel®, CoralLoad®, EpiTect®, EZ1®, HotStarTaq®, MinElute®, Pyro®, Pyrogram®, PyroMark®, Pyrosequencing® (QIAGEN Group); Milli-Q® (Millipore Corporation); Sepharose® (GE Healthcare); Variomag® (Thermo Fisher Scientific); Windows® (Microsoft Corporation).

Limited License Agreement

Use of this product signifies the agreement of any purchaser or user of the MGMT Pyro Kit to the following terms:

1. The MGMT Pyro Kit may be used solely in accordance with the *MGMT Pyro Handbook* and for use with components contained in the Kit only. QIAGEN grants no license under any of its intellectual property to use or incorporate the enclosed components of this Kit with any components not included within this Kit except as described in the *MGMT Pyro Handbook* and additional protocols available at www.qiagen.com.
2. Other than expressly stated licenses, QIAGEN makes no warranty that this Kit and/or its use(s) do not infringe the rights of third-parties.
3. This Kit and its components are licensed for one-time use and may not be reused, refurbished, or resold.
4. QIAGEN specifically disclaims any other licenses, expressed or implied other than those expressly stated.
5. The purchaser and user of the Kit agree not to take or permit anyone else to take any steps that could lead to or facilitate any acts prohibited above. QIAGEN may enforce the prohibitions of this Limited License Agreement in any Court, and shall recover all its investigative and Court costs, including attorney fees, in any action to enforce this Limited License Agreement or any of its intellectual property rights relating to the Kit and/or its components.

© 2011 QIAGEN, all rights reserved.

www.qiagen.com

Australia ■ Orders 1-800-243-800 ■ Fax 03-9840-9888 ■ Technical 1-800-243-066

Austria ■ Orders 0800-28-10-10 ■ Fax 0800-28-10-19 ■ Technical 0800-28-10-11

Belgium ■ Orders 0800-79612 ■ Fax 0800-79611 ■ Technical 0800-79556

Brazil ■ Orders 0800-557779 ■ Fax 55-11-5079-4001 ■ Technical 0800-557779

Canada ■ Orders 800-572-9613 ■ Fax 800-713-5951 ■ Technical 800-DNA-PREP (800-362-7737)

China ■ Orders 86-21-3865-3865 ■ Fax 86-21-3865-3965 ■ Technical 800-988-0325

Denmark ■ Orders 80-885945 ■ Fax 80-885944 ■ Technical 80-885942

Finland ■ Orders 0800-914416 ■ Fax 0800-914415 ■ Technical 0800-914413

France ■ Orders 01-60-920-926 ■ Fax 01-60-920-925 ■ Technical 01-60-920-930 ■ Offers 01-60-920-928

Germany ■ Orders 02103-29-12000 ■ Fax 02103-29-22000 ■ Technical 02103-29-12400

Hong Kong ■ Orders 800 933 965 ■ Fax 800 930 439 ■ Technical 800 930 425

Ireland ■ Orders 1800 555 049 ■ Fax 1800 555 048 ■ Technical 1800 555 061

Italy ■ Orders 800-789-544 ■ Fax 02-334304-826 ■ Technical 800-787980

Japan ■ Telephone 03-6890-7300 ■ Fax 03-5547-0818 ■ Technical 03-6890-7300

Korea (South) ■ Orders 080-000-7146 ■ Fax 02-2626-5703 ■ Technical 080-000-7145

Luxembourg ■ Orders 8002-2076 ■ Fax 8002-2073 ■ Technical 8002-2067

Mexico ■ Orders 01-800-7742-639 ■ Fax 01-800-1122-330 ■ Technical 01-800-7742-436

The Netherlands ■ Orders 0800-0229592 ■ Fax 0800-0229593 ■ Technical 0800-0229602

Norway ■ Orders 800-18859 ■ Fax 800-18817 ■ Technical 800-18712

Singapore ■ Orders 1800-742-4362 ■ Fax 65-6854-8184 ■ Technical 1800-742-4368

Spain ■ Orders 91-630-7050 ■ Fax 91-630-5145 ■ Technical 91-630-7050

Sweden ■ Orders 020-790282 ■ Fax 020-790582 ■ Technical 020-798328

Switzerland ■ Orders 055-254-22-11 ■ Fax 055-254-22-13 ■ Technical 055-254-22-12

UK ■ Orders 01293-422-911 ■ Fax 01293-422-922 ■ Technical 01293-422-999

USA ■ Orders 800-426-8157 ■ Fax 800-718-2056 ■ Technical 800-DNA-PREP (800-362-7737)

