New as of:

02.2013



inCoris TZI

Translucent zirconia ceramic blocks for inLab Processing instructions: Restoration production for crowns and bridges



Table of contents

1	Gene	eral	4
2	Mate	rial	5
3	Chen	nical composition	6
4	Tech	nical data	7
5	Indica	ation and preparation instructions	8
	5.1	Indication	8
	5.2	Contraindications	8
	5.3	General preparation instructions	8
	5.4	Preparation of premolars and molars	8
	5.5	Preparation of anterior and posterior tooth crowns	9
6	Crea	ting the restoration	10
	6.1	Scanning, designing and milling	10
	6.2	Reworking the milled restoration	10
	6.3	Pre-drying	10
	6.4	Coloring	11
		6.4.1 Brush technique (multicoloring)	11
		6.4.2 Dipping	13
	6.5	Drying before sintering	14
	6.6	Sintering	14
	6.7	Additional notes: procedure after sintering	16
	6.8	Rework	16
	6.9	Painting and coating	16
7	Reco	mmended tools and materials	17
8	Faste	ening instructions	18
9	Rem	Removal of inserted restorations and Trephination1	

10	Refer	ences	20
	10.1	Materials science	20
	10.2	CEREC/ inLab	21

CE 0123

General

The inCoris TZI product bears the CE mark in accordance with the provisions of Council Directive 93/42/EEC of June 14, 1993 concerning medical devices.

inCoris TZI blocks are intended for use in manufacturing individually designed fully anatomical restorations, which can be polished or veneered after milling and sintering.

Rx only	CAUTION: Federal law (USA) restricts sale of this device to or on the
	order of a physician, dentist, or licensed practitioner.

2 Material

inCoris TZI ceramics constitute blocks comprised of zirconia ceramics.

The blocks are initially manufactured in a partially sintered state; then, enlarged by the inLab CAD/CAM system, they are individually processed to specification, and finally, densely sintered.

The aesthetic features of inCoris TZI enable application as fully anatomical crowns and bridges.

The advantages of inCoris TZI include:

- High strength
- Resistance to corrosion
- Good biological compatibility of the product,
- Translucency

3 Chemical composition

Component	inCoris TZI
ZrO ₂ +HfO ₂ +Y ₂ O ₃	≥ 99.9%
Y ₂ O ₃	5.4%
Al ₂ O ₃	≤ 0.35%
Fe ₂ O ₃	≤ 0.01%
Other oxides	≤ 0.2%



4 Technical data

The following specifications apply to material that is densely sintered in an inFire HTC / inFire HTC speed sintering furnace.

Density:	6.08 g cm ⁻³
Fracture toughness K _{IC}	6.4 MPa m ^{1/2}
Thermal expansion coefficient (20 - 500 °C):	10.4 10 ⁻⁶ K ⁻¹
Bending strength:	> 900 MPa

5 Indication and preparation instructions

5.1 Indication

Classic sintering and speed sintering

- Fully anatomic crowns and bridges in the anterior and posterior tooth region.
- Bridges containing up to 9 units and no more than 2 pontics.

Super speed sintering

- Fully anatomic crowns, maximum wall thickness of 2 mm
- Single caps

5.2 Contraindications

- Insufficient oral hygiene
- Insufficient preparation results
- Insufficient tooth structure
- Insufficient space available

5.3 General preparation instructions

- The preparation must be performed with either a chamfer or a shoulder with rounded internal angle.
- The vertical preparation angle should be at least 3°. All transitions from the axial to the occlusal or incisal areas must be rounded off. Flat or plane surfaces are advantageous.

5.4 Preparation of premolars and molars

A simplified occlusal relief is recommended for posterior teeth to allow sufficient space for the veneer ceramic. A minimum of 1.5 mm of occlusal substance must be removed.

≥ 1,5 mm

5.5 Preparation of anterior and posterior tooth crowns

Preparation of anterior teeth

The incisal wall thickness should be at least 1.5 mm, the circular wall thickness at least 1.0 mm.

The tapering crown edge should be 0.8 mm thick.

≥ 1.5 mm 1.0 mm - 1.5 mm ≥ 1.5 mm 0.8 mm

Preparation of posterior teeth (premolars and molars)


At the lowest point of the main fissure, the material thickness should be 1.5 mm.

For the cusp design, a material thickness of at least 1.5 mm should be ensured.

The circular wall thickness should be 1.0 - 1.5 mm.

The tapering crown edge should be 0.8 mm thick.

Connector surface on	Minimum connector surface in mm ²
Posterior tooth bridge restoration with a pontic	9
Posterior tooth bridge restoration with two pontics	12
Free-end bridge	12



6 Creating the restoration

6.1 Scanning, designing and milling

inCoris TZI can only be processed with software version 3.88 or higher.

If you are using software version 3.88, you must first install the material ("Material Pack inCorisTZI.exe"). The files are available for downloading at "www.sirona.de/incoristzi".

Software version 3.88

inCoris TZI is only available in the *"Bridge"*1 *"Biogeneric"* selection dialog. Even if single crowns are to be created, *"Bridge"* must be selected as the restoration type. In this case, select only one tooth in the odontogram.

Details are documented in the "inLab 3D User Manual".

Software 4.x

If you are using software 4.x, select Sirona/inCoris TZI in the material dialog.

Details are documented in the "inLab SW User Manual".

6.2 Reworking the milled restoration

After the milling process and prior to sintering, a diamond burr milling tool has to be used to separate the restoration.

To prevent milling residues from remaining in the fissures, the restoration can be briefly steamed off or cleaned with water and a soft toothbrush.

6.3 Pre-drying

To prevent inhomogeneous coloring of the restorations caused by varying liquid penetration characteristics, the restorations need to be dried first of all.

Predrying can be carried out in various ways. We recommend one of the following:

• 30 minutes at 80°C (176°F) in the drying cabinet

or

• 10 minutes at 150 °C (302°F) in the drying cabinet

NOTICE

In the case of high humidity

In an environment with a high level of humidity, the restorations can absorb moisture after drying. For this reason, sintering must take place within a maximum of one hour after drying.

6.4 Coloring

Prior to sintering, the uncolored restorations can be dyed to the desired tooth color using inCoris TZI coloring liquids.

There are two ways to color inCoris TZI crowns and bridges:

- Brush technique (multicoloring)
- Dipping

Items 6.1 - 6.3 of the inCoris TZI processing instructions apply to both of the above possibilities prior to coloring.


6.4.1 Brush technique (multicoloring)

With dipping you obtain a completely monochrome tooth color. In order to achieve a natural color gradient, it is advisable to brush on inCoris TZI coloring liquids instead of dipping entire restorations.


Please take the following points into consideration when using the brush technique:


- Use a size 8 to 10 modeling brush for the overall application and a size 1 to 2 brush for applying the paint to the fissures.
- Use a separate brush for each color or wash the brush out thoroughly after use and then let it dry. Residual moisture influences the coloring.
- Hold the restorations using only a pair of plastic tweezers.
- Never place the restorations on metallic surfaces as this can lead to shifts in the color concentration and therefore discoloration.
- Always move the brush from the occlusal/incisal to the cervical direction.

Coloring a posterior tooth

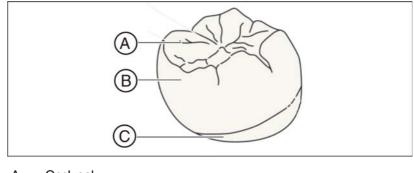


- A Occlusal
- B Body
- C Cervical






- Brush the entire tooth 1x. Direction of brush stroke: From the occlusal (A) area across the body (B) to the cervical area (C).
- Paint the body (B) and the cervical area (C) 5x. Omit the occlusal surface.
 Direction of brush stroke: From the body (B) to the cervical area (C). The colors shown in this figure are only visible after sintering and not during painting.



- For light colors: Paint the cervical area (C) 3x. Direction of brush stroke: cervical. For dark colors (A3.5, A4, B4, C4, C3, C4): Paint the cervical area (C) 4x.
- 4. Paint the central fissures 1-2x for a natural color gradient.
- 5. Treat the palatal surfaces in the same way as the vestibular surfaces.

Coloring an anterior tooth

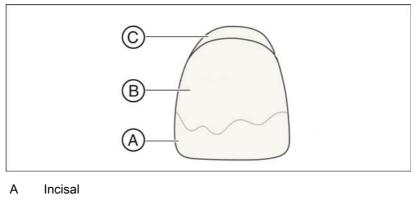



- B Body
- C Cervical

(A)

B

C





- Brush the entire tooth 1x. Direction of brush stroke: From the incisal area (A) across the body (B) to the cervical area (C).
- Paint the body (B) and the cervical area (C) 5x. Omit the incisal surface.
 Direction of brush stroke: From the body (B) to the cervical area (C).
- C B A A C C Dire For 4x. 4. Tre
 - For light colors: Paint the cervical area (C) 3x. Direction of brush stroke: cervical. For dark colors (A3.5, A4, B4, C4, C3, C4): Paint the cervical area (C) 4x.
 - 4. Treat the palatal surfaces in the same way as the vestibular surfaces.

6.4.2 Dipping

NOTICE

With the speed and super speed sintering processes, the restorations are lighter in color than with the classic long-term sintering process.

Recommendation: When using the speed and super speed sintering processes with an inCoris TZI coloring solution, dye the restorations one color level darker than desired.

- 1. To color the restoration, use a vessel in which the milled restoration can be fully submerged into the coloring solution, e.g. the inCoris TZI dip tanks.
- 2. Allow the restoration to absorb the coloring solution for five minutes. Leaving it submerged for less than 5 minutes will produce a lighter end result and leaving it for longer will produce a darker result.
- **3.** Then remove the restoration from the vessel using a pair of plastic tweezers.

IMPORTANT

All parts which have come into contact with coloring solution must be cleaned afterwards, as discolorations could result if they are used again. Always keep dip tanks and bottles containing coloring solution closed following use, since the liquid otherwise will evaporate, thus resulting in a higher color concentration.

6.5 Drying before sintering

To avoid damage during sintering, the restoration must be dried in the drying cabinet.

- 30 minutes at 80°C (176°F) or
- 10 minutes at 150°C (302°F)

NOTICE

Risk of damaging the restoration

Drying at temperatures above 150°C (302°F) can damage the restoration.

All restorations to be sintered must be dried thoroughly first, especially for super speed sintering. Any residual moisture can cause the parts to burst.

6.6 Sintering

Restorations made from inCoris TZI have to be sintered in dry conditions.

The sintering process should only be performed in Sirona inFire HTC/ inFire HTC speed with the pre-programmed inCoris ZI programs. As an alternative, the sintering process can be carried out in the compatible VITA Zyrcomat or Ivoclar Vivadent Sintramat high temperature furnace. In any case, the details in the manuals for the respective furnaces are to be adhered to.

🕂 WARNING

The "Super Speed" program of the inFire HTC speed furnace can only be used for the following:

- Fully anatomic crowns with a maximum wall thickness of 2 mm and single caps.

- Materials labeled "SUPER SPEED authorized".

The classic program for sintering with inCoris TZI is the same as for inCoris ZI. The sintering result from furnaces other than those specified here cannot be guaranteed by Sirona:



Heating rate °C/min	Holding temperature °C	Holding time min
25	800	0
15	1510	120
30	200	0

Since speed and super speed sintering are only permitted in inFire HTC speed furnaces with inCoris ZI and inCoris TZI materials and these programs are permanently installed in the furnace, the programs are not described here. Classic and speed sintering are carried out in the sintering tray provided with the inFire HTC speed furnace. Super speed sintering can only be carried out with the sintering boats specially designed for this process. The crowns must be placed on these boats at least 1 cm apart.

We recommend following the instructions below precisely because, especially in the sintering processes for occlusally very curved restorations, the correct bead layer is a decisive factor in subsequent fitting on the model:

Restoration on sintering bead layer

- Only use the sintering trays and beads intended for the respective high temperature furnaces when sintering inCoris TZI.
- Make sure that the restorations are lying completely on the bed of beads.
- Remove beads lying interdentally with a probe, so that shrinking is unhindered.
- If several restorations are sintered at the same time, these must not touch the edge of the sintering tray or each other.

"Embedded" bridge restoration

 In order to prevent the sintering beads from sticking (e.g. interdental on the bridge pontic), the restorations must not be pressed or "embedded" into the sintering beads too hard.

Very occlusally curved bridge restorations lying on buccal restoration side

- Position crown and bridge restorations on the occlusal side of the restoration.
- Very occlusally curved bridge restorations (e.g. Spee's curve) are always to be placed on the **buccal** / **labial** side of the restoration so that the center bend of the restoration is lying on the sintering beads.
- Use additional sintering beads to support ends of restorations which have hollow areas.

Non-supported bridge restoration (with hollow area)

 Support every restoration pontic with at least one sintering bead so that bridge restorations are adequately supported along the entire length of the restoration and do not "lie hollow".

6.7 Additional notes: procedure after sintering

In the case of yellow staining of restorations after the sintering process, the high-temperature furnace should be cleansed by performing an empty run. The details in the manuals for the respective furnaces are to be adhered to in this case.

Sintering beads that adhere are to be removed carefully.

After the sintering process, the restorations must be cooled down to room temperature before further processing.

6.8 Rework

The surface condition of ceramic materials is decisive for their bending strength. Reworking sintered restorations with milling tools, especially in the connector region, must be avoided at all costs.

Therefore make corrections to the milled restoration if possible before sintering.

However, if reworking should be necessary, comply with the following basic rules:

- Reworking in the sintered condition should be performed with a wet grinding turbine (approx. 2.5 3 bar) or rubber polishers (low speed) or for primary telescopes with a grinding unit using water cooling and with low grinding pressure. As an alternative it is possible to rework with soft, diamond rubber polishers and a handpiece at low speed and low pressure. The tool must be applied flat and must not "chatter."
- New diamond burrs with varied grain size should be used if possible.
- Areas that are under tension in clinical use, i.e. primarily the connectors in bridge structures, should not be ground.

The sintered restorations should also be polished prior to applying the enamel coating in order to prevent abrasion to the antagonist following potential loss of shine.

The inCoris TZI can be polished with all standard polishing agents for zirconia ceramics. Subsequent heat treatment (regeneration firing) is not necessary.

6.9 Painting and coating

Restorations made from inCoris TZI can be finalized using all standard paint and gloss colors for zirconia ceramics, e.g. VM9 from Vita. In this case the manufacturer's processing instructions must be observed without fail.

Recommended tools and materials

- Modeling wax
 - Scan wax (Sirona) (suitable for scans with the inLab scanner, not for exposures with inEos)
- Wet grinding turbines:
 - KaVo K-AIR plus (KaVo);
 - IMAGO (Steco-System-Technik GmbH & Co.KG);
 - NSK Presto Aqua (Girrbach);
 - Turbo-Jet (Acurata)
- Grinding tools for reworking with the wet grinding turbine/with handpiece
 - Diamond grinding element sets Ceramic-Line, Telescope-Line (Sirius Dental Innovations).
 - Diamond porcelain polisher for handpiece, green-orange (Hager & Meisinger, Art. No. HP 803 104 372 533 170).
 - Diamond polisher for handpiece (green and orange), EVE Diacera.
- Other:
 - Suitable colored contact materials
- Preparation sets:
 - Preparation set acc. to Küpper (Hager & Meisinger, Art. No. 2560);
 - Preparation set acc. to Baltzer and Kaufmann (Hager & Meisinger, Art. No. 2531);

8 Fastening instructions

Restorations made from inCoris TZI can be fastened non-adhesively with glasionomer or zinc phosphate cements, or adhesively with the selfcuring PANAVIA 21 TC composite or the dual-curing PANAVIA F composite (Kuraray). Both products contain the special MDP monomer, which forms a durable chemical compound with the shot blasted surface of the restorations without having to silicatize and silanize its surface.

The use of plastic-reinforced or modified glasionomer cements is not advised, since no adequate clinical data is currently available.

Pre-treatment of the restoration before adhesive bonding:

- Sand-blast the internal surfaces of the restoration in the one-way blasting process with maximum 50 µm corundum (Al2O3). Pressure
 2.5 bar.
- Do not touch the sandblasted surface if at all possible.

NOTICE

Observe usage information

Etching with hydrofluoric acid does not produce a retentive surface. Silanization is not required

Please observe the information on use of the fastening materials of the corresponding manufacturers.

9 Removal of inserted restorations and Trephination

Removal of inserted restorations

In order to remove a fixed zirconia restoration, we recommend using a cylinder-shaped diamond tool with the maximum amount of water cooling and a speed of 120,000 rpm to separate the restoration.

Trephination

The restoration can be trephined with a coarse-grained, spherical diamond with maximum water cooling and a speed of 120,000 rpm.

In this case, it is recommended that the instrument is applied in a circular motion at an angle of 45° when drilling through the restoration.

References

10.1 Materials science

Baltzer, A.; Kaufmann-Jinoian, V.: The toughness of VITA In-Ceram. Quintessenz Zahntech 29, 11, 1318-1342 (2003)

Blatz, M.; Sadan, A.; Kern, M.: Adhesive bonding of high-strength full ceramic restorations.

Quintessenz 55, 1, 33-41 (2004)

Geis-Gerstorfer, J; Päßler, P.: Investigations of the fatigue behavior of dental ceramics – zirconium dioxide TZP and In-Ceram. Dtsch Zahnärtzl Z 54, 692- 694 (1999)

Kappert, H.F.: On the high strength of dental ceramics. Zm 93, 7, 2003

Kern, M.: Fracture quota lower than the "divorce rate" ZWL 04, 2004, Luthard, R.; Herold, V et al.: Crowns made of high-performance ceramics. Dtsch Zahnärztl Z 53, 4 280-285 (1998)

Luthard et al.: Comparison of various techniques for the manufacture of crown frameworks from high-performance ceramics. State of the art of the CAD/CAM supported production of full ceramic crowns from oxide ceramics.

Swiss Dent, 19, 6 5 -12 (1998)

Marx, R. et al.: Crack parameters and Weibull modules: subcritical crack growth and long-term strength of full ceramic materials. Dtsch Zahnärtzl Z 56, 2 90 - 98 (2001)

Report by DGZMK/DGZPW: Are full ceramic crowns and bridges scientifically recognized? Dtsch Zahnärtzl Z 56 10 575 - 576 (2001)

Schweiger, M.: Zirconium oxide. High-strength and break-resistant structural ceramics. Ästh. Zahnmedizin 5, 2004, 248-257

Tinschert, J; Natt, G.; Spiekermann, H.: Current positioning of dental ceramics.

Dental-Praxis XVIII, 9/10 293 - 309 (2001)

Vollmann, M.: Innovative DeguDent full ceramic system as a benchmark for the processing of zirconium oxide. IJCD 2004, 7, 279-291

10.2 CEREC/ inLab

CEREC[®]/ inLab[®]

Baltzer, A.; Kaufmann-Jinoian, V.: CAD/CAM in dentistry CEREC inLab. Dental-Labor, XLIX, Volume 5 (2001)

David, A.: CEREC inLab - The CAD/CAM System with a Difference. CJDT Spectrum, September/October, 24 - 28 (2002)

Kurbad, A.; Reichel, K.: CEREC inLab - State of the Art. Quintessenz Zahntech 27, 9, 1056 -1074 (2001)

Kurbad, A.: Manufacturing In-Ceram bridge frameworks with the new CEREC technology. Quintessenz Zahntech 27, 5, 504 - 514 (2001)

Tsotsos, St.; Giordano, R.: CEREC inLab: Clinical Aspects, Machine and Materials. CJDT Spectrum January/February, 64 - 68 (2003) Preparation illustrations on p. 5 accd. to Dr. Andres Baltzer, CH-Rheinfelden

Kern, M.: Computer-aided crown and bridge technology with new perspectives. Quint. Zahnt. 30, 9, 966-973 (2004)

Rudolph, H., Quaas, S., Luthard, R.G.: CAD/CAM – New technologies and developments in dentistry. DZZ 58 (2003)10

We reserve the right to make any alterations which may be required due to technical improvements.

© Sirona Dental Systems GmbH 2011-2013 D3487.201.06.05.02 02.2013

Sprache: englisch Ä.-Nr.: 116 686

Printed in Germany

Sirona Dental Systems GmbH

Fabrikstraße 31 64625 Bensheim Germany www.sirona.com in the USA: Sirona Dental Systems LLC 4835 Sirona Drive, Suite 100 Charlotte, NC 28273 USA

Order No 63 59 801 D3487