

HBV Quantitative Real Time PCR Kit

User Manual

For In Vitro Diagnostic Use Only

REF HD-0002-02-A+B

**For use with ABI Prism®7000/7300/7500/7900/Step One Plus; iCycler iQ™4/iQ™5;
Smart Cycler II; Bio-Rad CFX 96; Rotor Gene™6000; Mx3000P/3005P; MJ-Option2/Chromo4;
LightCycler®480 Instrument**



Shanghai ZJ Bio-Tech Co., Ltd.

www.liferiver.com.cn Tel: +86-21-34680596

trade@liferiver.com.cn Fax: +86-21-34680595

2nd floor, No.15 Building, No.188 Xijunhuan road,

PuJiang Hi-tech Park Shanghai China

1. Intended Use

HBV quantitative real time PCR kit is used for the detection of HBV in serum or plasma by using real time PCR systems.

Its characteristics:

High sensitivity: lower detection line 500 IU/ml; LOQ: $10^3 \sim 10^8$ IU/ml

(Note: Analysis sensitivity depends on the sample volume, elution volume, nucleic acid extraction methods and other factors. If you use the DNA extraction buffer in the kit, the analysis sensitivity is the same as it declares. However, when the sample volume is dozens or even hundreds of times greater than elution volume by some concentrating method, it can be much higher.)

High specificity: test result will be positive, only to hepatitis B virus.

Short operating time: One and a half hours totally

Good stability: kept for 12 months at -20°C; CV≤5%;

2. Principle of Real-Time PCR

The principle of the real-time detection is based on the fluorogenic 5' nuclease assay. During the PCR reaction, the DNA polymerase cleaves the probe at the 5' end and separates the reporter dye from the quencher dye only when the probe hybridizes to the target DNA. This cleavage results in the fluorescent signal generated by the cleaved reporter dye, which is monitored real-time by the PCR detection system. The PCR cycle at which an increase in the fluorescence signal is detected initially (Ct) is proportional to the amount of the specific PCR product. Monitoring the fluorescence intensities during Real Time allows the detection of the accumulating product without having to re-open the reaction tube after the amplification.

3. Product Description

Chronic hepatitis B virus (HBV) infection affects over 350 million people worldwide and over 1 million die annually of HBV-related chronic liver disease. Although many individuals eventually achieve a state of nonreplicative infection, the prolonged immunologic response to infection may lead to the development of cirrhosis, liver failure, or hepatocellular carcinoma (HCC) in up to 40% of patients. HBV is an enveloped virus in the family Hepadnaviridae, with partially double-stranded DNA and 42nm in diameter. Its antigenic components includes hepatitis B surface antigen (HBsAg), hepatitis B core antigen (HBcAg), and hepatitis B e antigen (HBeAg). Virus replicates in liver and sheds into blood in high concentration. HBV is transmitted through blood and body fluid.

HBV real time PCR kit contains a specific ready-to-use system for HBV detection (for genotype A~H) through polymerase chain reaction (PCR) in the real-time PCR system. The master contains reagents and enzymes for the specific HBV DNA amplification. Fluorescence is emitted and measured by the real time systems' optical unit during PCR. The detection of amplified HBV DNA fragment is performed in fluorimeter **channel FAM** with the fluorescent quencher BHQ1. DNA extraction buffer is available in the kit. In addition, the kit contains a system to identify possible PCR inhibition by measuring the HEX/VIC/JOE fluorescence of the internal control (IC). Four quantitation standards are supplied, allows the determination of the gene load.

4. Kit Contents

	Ref.	Cap Color	Type of reagent	Presentation 25rxns
PCR System	1	Blue	DNA Extraction Buffer	1 vial, 1.8ml
	2	Gray	HBV Reaction Mix	1 vial, 950μl
	3	Blue	PCR Enzyme Mix	1 vial, 12μl
	4	Yellow	Molecular Grade Water	1 vial, 400μl
	5	Orange	Internal control (IC)	1 vial, 30μl
QS ★ System	6	Pink	HBV QS1 (5×10^7 IU/ml)	1 vial, 20μl
	7	Purple	HBV QS2 (5×10^6 IU/ml)	1 vial, 20μl
	8	Orange	HBV QS3 (5×10^5 IU/ml)	1 vial, 20μl
	9	Yellow	HBV QS4 (5×10^4 IU/ml)	1 vial, 20μl

★QS: Quantitation Standard

5. Storage

- All reagents should be stored at -20°C. Storage at +4°C is not recommended.
- All reagents can be used until the expiration date indicated on the kit label.
- Repeated thawing and freezing (> 3x) should be avoided, as this may reduce the sensitivity of the assay.
- Cool all reagents during the working steps.
- Reaction mix should be stored in the dark.

6. Additionally Required Materials and Devices

- Biological cabinet
- Real time PCR reaction tubes/plates
- Pipets (0.5 μl – 1000 μl)
- Disposable gloves, powderless
- Biohazard waste container
- Sterile filter tips for micro pipets
- Desktop microcentrifuge for "ependorf" type tubes (RCF max. 16,000 x g)
- Real time PCR system
- Vortex mixer
- Cryo-container
- Sterile microtubes
- Refrigerator and freezer
- Tube racks

7. ⚠Warnings and Precaution

Carefully read this instruction before starting the procedure.

- For in vitro diagnostic use only.
- This assay needs to be carried out by skilled personnel.
- Clinical samples should be regarded as potentially infectious materials and should be prepared in a laminar flow hood.
- This assay needs to be run according to Good Laboratory Practice.
- Do not use the kit after its expiration date.
- Avoid repeated thawing and freezing of the reagents, this may reduce the sensitivity of the test.
- Once the reagents have been thawed, vortex and centrifuge briefly the tubes before use.
- Prepare quickly the Reaction mix on ice or in the cooling block.
- Set up two separate working areas: 1) Isolation of the RNA/ DNA and 2) Amplification/ detection of amplification products.
- Pipets, vials and other working materials should not circulate among working units.
- Use always sterile pipette tips with filters.
- Wear separate coats and gloves in each area.

- Avoid aerosols

8. Sample Collection, Storage and transport

- Collect samples in sterile tubes;
- Specimens can be extracted immediately or frozen at -20°C to -80°C.
- Transportation of clinical specimens must comply with local regulations for the transport of etiologic agents

9. Procedure


9.1 DNA-Extraction

DNA extraction buffer is supplied in the kit, please thaw the buffer thoroughly and spin down briefly in the centrifuge before use. It's better to use commercial kits for nucleic acid extraction.

- 1) Take 50ul serum or plasma, add 50ul DNA extraction buffer, and close the tube then vortex for 10 seconds. Spin down briefly in a table centrifuge.
- 2) Incubate the tube for 10 minutes at 100°C.

9.3 PCR Protocol

The Master Mix volume for each reaction should be pipetted as follows:

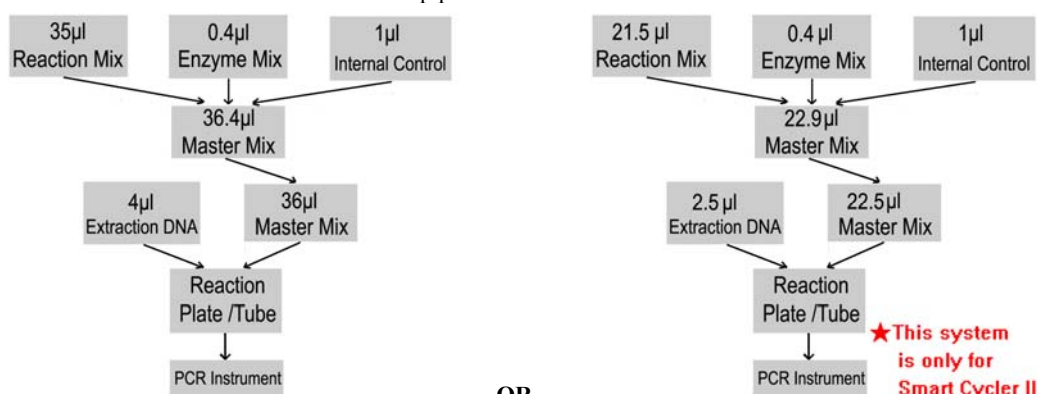

OR

※PCR system without HEX/VIC/JOE channel may be treated with 1ul Molecular Grade Water instead of 1ul IC.

- 1) The volumes of Reaction Mix and Enzyme Mix per reaction multiply with the number of samples, which includes the number of controls, standards, and sample prepared. Molecular Grade Water is used as the negative control. For reasons of unprecise pipetting, always add an extra virtual sample. Mix completely then spin down briefly in a centrifuge.
- 2) Pipet 36ul (22.5ul for Smart Cycler II) Master Mix with micropipets of sterile filter tips to each Real time PCR reaction plate/tubes. Separately add 4ul (2.5ul for Smart Cycler II) DNA sample, QS1, QS2, QS3, QS4 and negative control to different reaction plate/tubes. Immediately close the plate/tubes to avoid contamination.
- 3) Spin down briefly in order to collect the Master Mix in the bottom of the reaction tubes.
- 4) Perform the following protocol in the instrument:

37°C for 2 min, 1 cycle; 94°C for 2 min, 1 cycle; 93°C for 15 sec, 60°C for 60 sec, 40 cycles.

Fluorescence is measured at 60°C; FAM and HEX/VIC/JOE channels should be chosen.

- 5) ⚠ If you use ABI Prism® system, please choose “none” as passive reference and quencher.

10. Threshold setting: just above the maximum level of molecular grade water.

11. Calibration for quantitative detection: Input each concentration of standard controls at the end of run, and a standard curve will be automatically formed.

12. Quality control:

Channel	Ct value	
	FAM (Target Nucleic Acid)	HEX/VIC/JOE (IC)
Molecular Grade Water	UNDET	25~35
QS1/QS2/QS3/QS4	≤38, and Correlation coefficient of QS curve ≤ -0.98	—

13. Data Analysis and Interpretation

The following results are possible:

- 1) The Ct value in channel FAM shows ≤38. **The result is positive: The sample contains HBV DNA. Quantitative value of samples is automatically reported according to the standard curve.**

Quantitative Value	Data Analysis and Suggestion
$< 5 \times 10^2$ IU/ml	HBV DNA Positive; its concentration lower than 5×10^2 IU/ml
$5 \times 10^2 \sim 10^3$ IU/ml	HBV DNA Positive; the quantitative value for recommendation only
$10^3 \sim 10^8$ IU/ml	HBV DNA Positive; the quantitative value is valid
$> 10^8$ IU/ml	1) HBV DNA Positive but the quantitative value for recommendation only 2) Re-test the sample after dilute the sample by several times, making the quantitative value within $10^3 \sim 10^8$ IU/ml

- 2) The Ct value in channel FAM shows 38~40, please repeat again. **If the result still shows 38~40, it can be considered negative.**
- 3) In channel FAM no signal is detected, at the same time, a HEX/VIC/JOE signal from the Internal Control appears. **The sample does not contain any HBV DNA. It can be considered negative.**
- 4) Neither in channel FAM nor in channel HEX/VIC/JOE signal is detected. **A diagnostic statement can not be made.** Inhibition of the PCR reaction.

For further questions or problems, please contact our technical support at trade@liferiver.com.cn