



# Human EGFR (Total) Singleplex Bead Kit

## Technical Data Sheet

Catalog #: LHR9061 Lot #:\* 1003596

\*Note: A letter at the end of the lot number signifies an additional packaging of this same lot.

### Intended Use

This kit is comprised of components for the measurement of EGFR in cell lysates. Buffer reagents needed to complete the reaction are sold separately under Catalog #LHB0002. These reagents are intended for use in the **Luminex® 100™/200™** and the **FlexMAP 3D® System**. **This kit is configured for research use only and is not to be used in diagnostic procedures.**

**Note: This kit uses a Co-Incubation Assay format.** Refer to the User Manual included in the Intracellular Protein Buffer Reagent Kit (Cat # LHB0002) for further information. **Before attempting to multiplex this kit with any other kits, please contact Technical Support.**

### Reagents Provided

Human EGFR

1. **Part #:** LM197    **Description:** Antibody Bead Concentrate (10X)    **Lot:** 1079861    **Size:** 0.25 mL-100 tests  
**Bead Region:** 68  
**Form:** 0.25 mL 10X bead concentrate solution in storage buffer. Contains 0.05% sodium azide as a preservative.  
**Storage:** **Light sensitive material.** Store at 2 to 8°C, in the dark, until the expiration date indicated on the kit.

Human EGFR (Total)

2. **Part #:** DN197    **Description:** Detection Ab Concentrate (10X)    **Lot:** 1079860    **Size:** 0.50 mL-100 tests  
**Form:** 0.5 mL of a 10X stock of Detection Antibody Concentrate. Contains 0.1% sodium azide as preservative. Concentration of antibody is matched to this lot of beads. Do not mix lots of Coated Beads and Detection Antibody.  
**Storage:** Store at 2 to 8°C until the expiration date indicated on the kit.

3. **Part #:** SM0572    **Description:** EGFR (Total) Standard    **Lot:** 1071653    **Size:** 2 Vials  
**Form:** Lyophilized. The protein in this standard has been calibrated against the masses of highly purified recombinant protein. Contains 0.1% sodium azide as a preservative.  
**Storage:** Store at 2 to 8°C. Use within 1 hour after reconstitution. The remaining reconstituted standard should be discarded or frozen in aliquots at -80°C for further use. The standard can be frozen and thawed one time without loss of immunoreactivity.

**Concentration of Reconstituted Standard\*\*:**  
EGFR Total (5,350 pg/mL)

**\*\*Important note: The concentrations of reconstituted standard are lot-specific. Please verify all concentration values entered in data analysis software.**

**Reconstitution:** Reconstitute in **2.0 mL Assay Diluent**.

**Recommended Starting Concentration for Standard Curve:** Upon reconstitution, the starting concentration of standard is the value cited above. Make 2-fold serial dilutions in *Assay Diluent*. Refer to the User Manual included in the kit for further information.

**Calibration:** Standards have been normalized to previous lot to allow consistency of quantitation.

**Species Reactivity:** This reagent set recognizes human proteins. Other species have not been tested.

# Human EGFR (Total) Singleplex Bead Kit

## Technical Data Sheet

### Performance Characteristics

#### Typical Standard Curve

Protein	EGFR Total
Sensitivity (ng/mL) <sup>1</sup>	0.001

**For Research Use Only. CAUTION: Not for human or animal therapeutic or diagnostic use.**

[www.invitrogen.com](http://www.invitrogen.com)


Life Technologies Corporation • 7335 Executive Way, Frederick, MD 21704 • Tel: 800.955.6288 • E-mail: [techsupport@invitrogen.com](mailto:techsupport@invitrogen.com)

LHR9061

(Page 1 of 2) MAN0005531 Rev 1.00 Effective Date: 27 OCT 2011

#### Limited Use Label License: Research Use Only

The purchase of this product conveys to the purchaser the limited, non-transferable right to use the purchased amount of the product only to perform internal research for the sole benefit of the purchaser. No right to resell this product or any of its components is conveyed expressly, by implication, or by estoppel. This product is for internal research purposes only and is not for use in commercial applications of any kind, including, without limitation, quality control and commercial services such as reporting the results of purchaser's activities for a fee or other form of consideration. For information on obtaining additional rights, please contact [outlicensing@lifetech.com](mailto:outlicensing@lifetech.com) or Out Licensing, Life Technologies, 5791 Van Allen Way, Carlsbad, California 92008.

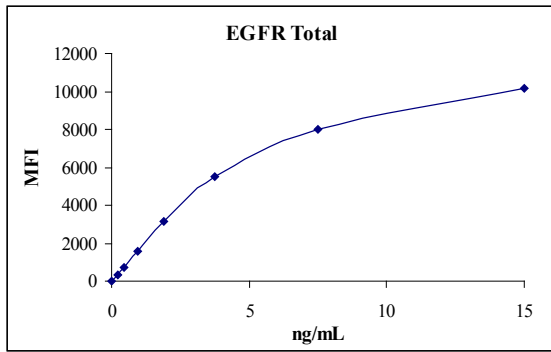

Note: This is a representative standard curve.  
Absolute MFI values will vary.


Recovery (10% FNN0011) <sup>2</sup>	85.9
Recovery (10% FNN0021) <sup>2</sup>	94.8
Intra-assay variation (n=16)	5.35
Inter-assay variation (n=32)	5.83

<sup>1</sup>**Analytical Sensitivity:** The analytical sensitivity was determined by adding two standard deviations to the median fluorescence intensity obtained when the zero standard was assayed 32 times.


<sup>2</sup>**Recovery:** To evaluate recovery, analytes were spiked at 3 different concentrations into 10% Cell Extraction Buffer (Cat. # FNN0011) and 10% NP40 Cell Lysis Buffer (Cat. # FNN0021).

**Sample Preparation:** This kit has been validated with cell lysates prepared in Cell Extraction Buffer (Cat. # FNN0011) and NP40 Cell Lysis Buffer (Cat. # FNN0021). Optimization of cell stimulation and cell lysis procedures may be required for each specific application. Refer to User Manual included in the Buffer Reagent Kit for detailed instructions.

**Example Data:** To evaluate the performance of this kit, natural EGFR from A431 cell lysate was serially diluted in *Assay Diluent*. The median fluorescence intensity of each dilution was plotted against the EGFR standard curve. Parallelism is presented in the figure to the right and indicates that the standard accurately reflects EGFR content in samples.

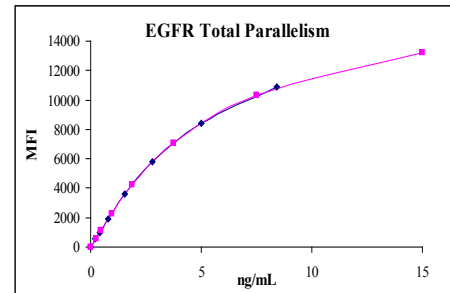

The data presented to the right demonstrate the impact of the *Sample Treatment Buffer* pre-incubation step on the observed signal. In this study, A431 cells were lysed in Cell Extraction Buffer. Lysates were either treated with *Sample Treatment Buffer* (+STB) or the *Sample Treatment Buffer* incubation step was omitted (-STB).

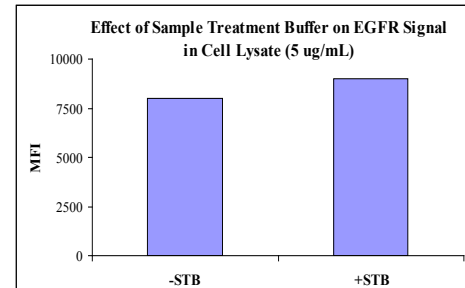

#### Explanation of symbols

Symbol	Description	Symbol	Description
	Catalogue Number		Batch code
	Research Use Only		<i>In vitro</i> diagnostic medical device
	Use by		Temperature limitation
	Manufacturer		European Community authorised representative
	Without, does not contain		With, contains
	Protect from light		Consult accompanying documents
	Directs the user to consult instructions for use (IFU), accompanying the product.		

**For Research Use Only. CAUTION: Not for human or animal therapeutic or diagnostic use.**

[www.invitrogen.com](http://www.invitrogen.com)

Life Technologies Corporation • 7335 Executive Way, Frederick, MD 21704 • Tel: 800.955.6288 • E-mail: [techsupport@invitrogen.com](mailto:techsupport@invitrogen.com)

LHR9061

(Page 2 of 2) MAN0005531 Rev 1.00 Effective Date: 27 OCT 2011

#### Limited Use Label License: Research Use Only

The purchase of this product conveys to the purchaser the limited, non-transferable right to use the purchased amount of the product only to perform internal research for the sole benefit of the purchaser. No right to resell this product or any of its components is conveyed expressly, by implication, or by estoppel. This product is for internal research purposes only and is not for use in commercial applications of any kind, including, without limitation, quality control and commercial services such as reporting the results of purchaser's activities for a fee or other form of consideration. For information on obtaining additional rights, please contact [outlicensing@lifetech.com](mailto:outlicensing@lifetech.com) or Out Licensing, Life Technologies, 5791 Van Allen Way, Carlsbad, California 92008.