

US-1


Ultrasound Examination Training Model “ECHOZY”

Production supervision:

Dr.Hitoshi Asai,Director
Osaka Kyoiku University,Health Administration Center
Dr.Shigeru Nakamura
Nagayashi General Hospital Clinical Examination Department

Caution:

Don't mark on the phantom with pen or leave printed materials contacted on its surface.
Ink marks on the phantom will be irremovable.

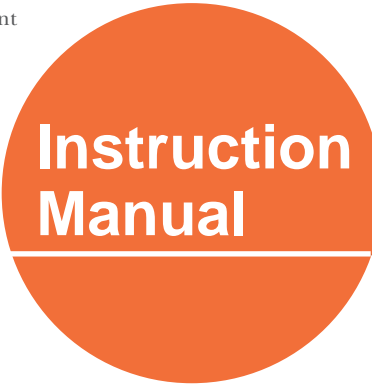

Contents



- Please read before training
General information P. 1
- Preparation
1 Befor training P. 2
- Training
2 Training session P. 2
3 After training P. 2


Unique high-fidelity ultrasound phantom facilitates effective training in abdominal ultrasound scanning with your own clinical devices.

● **Features**

- Inanimate tool for training of a novice to demonstration by an expert.
Any ultrasound device with a convex probe can be used for the phantom.
- Detailed hepatobiliary, pancreatic and other abdominal anatomy meeting requirement for excellent training; Eight Couinaud's hepatic segments can be localized.
- Near real-size organs, structures and abnormal lesions.
- Durable long-life phantom materials.

Set includes:

Before your first use, please ensure that you have all components listed below.

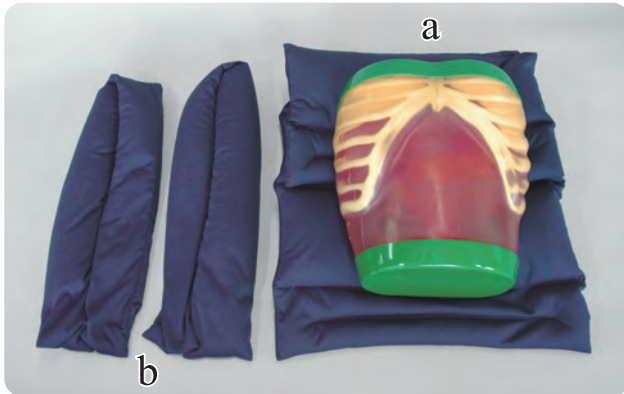

- a. Ultrasound abdominal phantom 1
 - the liver (segmental anatomy, portal and hepatic venous systems, ligamentum teres and ligamentum venosum), biliary tract (gallbladder, cystic duct, intrahepatic and extrahepatic bile ducts), pancreas (pancreatic duct), spleen, kidneys, detailed vascular structures (aorta, vena cava, celiac artery and its branches, portal vein and its branches, superior mesenteric vessels, renal vessels, etc)
- b. Positioning pillows 3

DOs and DON'T s

DO s

Handle with care.

The materials for phantom and models are special composition of soft resin. Please handle with care at all

Cleaning and care

Please clean the phantom completely every time after you finish the training.
The remaining lubricating gel may deteriorate the phantom.

Keep the training set at room temperature, away from heat, moisture and direct sunlight.

DON'Ts

Never wipe the phantom or models with thinner or organic solvent.

Don't mark on the phantom with pen or leave printed materials contacted on their surface.
Ink marks on the models will be irremovable.

Please note: The color of the phantom may change over time, though, please be assured that this is not deterioration of the material and the ultrasonic features of the phantom stay unaffected.

This phantom has a thin layer of coating for protective purposes which may cause minor wrinkling.
However, it has no effect on the ultrasound image.

1 Before training



① Place the phantom stably on the positioning



② Spread lubricant gel on the phantom body.


2 Training session



The phantom can be scanned with actual ultrasound devices.



Midsagittal plane



Liver



Kidney

3 After training



Wipe the remaining gel completely by wet cloth.
If remaining gel gets dried up on the body, it may cause scratches and tears on the phantom material.



Caution

Don't mark on the phantom with pen or leave printed materials contacted on its surface.
Ink marks on the phantom will be irremovable.

The contents of this manual are subject to change without prior notice.

No part of this instruction manual may be reproduced or transmitted in any form without permission from the manufacturer. Please contact manufacturer for extra copies of this manual which may contain important updates and revisions.

Please contact manufacturer with any discrepancies, typos, or mistakes in this manual or product feedback. Your cooperation is greatly appreciated.

KYOTO KAGAKU co.,LTD

URL:<http://www.kyotokagaku.com> e-mail:rw-kyoto@kyotokagaku.co.jp

Worldwide Inquiries & Ordering

Kyotokagaku Head Office and Factories:

15 Kitanechoya-cho, Fushimi-ku, Kyoto, 612-8388, JAPAN

Tel: +81-75-605-2510 Fax: +81-75-605-2519

Kyotokagaku USA Office: USA and Canada sales and services

3109 Lomita Boulevard, Torrance, CA 90505-5108, USA

Tel: 1-310-325-8860 Fax: 1-310-325-8867