

**RS-232/422/485 to 100Base-FX
Device Server/Managed Media
Converter**

**IRF-634
User's Manual**

(September 2006)



COPYRIGHT

All rights reserved. No part of this publication may be reproduced, stored in a retrieval system, or transmitted in any form or by any means, whether electronic, mechanical, photo copying, recording or otherwise, without the prior written permission of the publisher.

FCC WARNING



This equipment has been tested and found to comply with the limits for a class A device, pursuant to part 15 of FCC rules. These limits are designed to provide reasonable protection against harmful interference in a commercial installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communication. Operation of this equipment in a residential area is likely to cause harmful interference, in which case, the user will be required to correct the interference at the user's own expense.



This is a Class A product. In a domestic environment, this product may cause radio interference in which case the user may be required to take adequate measures.

Take special note to read and understand all the content in the warning boxes:



Warning

TABLE OF CONTENTS

1 ABOUT THIS GUIDE.....1

 1.1 Welcome1

 1.2 Purpose1

 1.3 Terms/Usage1

 1.4 Features.....1

 1.5 Specifications2

 1.6 Package Contents.....3

2 HARDWARE DESCRIPTION4

 2.1 Product Overview4

 2.2 Product Illustrations.....4

3 INSTALLATION.....5

 3.1 Location.....5

 3.2 Wall Mount Installation.....5

 3.3 Din Rail Mount Installation.....5

 3.4 Powering On Unit.....6

 3.5 Connecting Fiber Cable.....7

 3.6 DB9 Male Connector Pin Assignments.....7

 3.7 Serial Connection8

4 LED INDICATORS9

5 USER INTERFACE STARTUP.....10

 5.1 Console Port Access10

 5.2 Telnet Access.....12

 5.3 Web Access.....13

6 CONFIGURATION MANAGEMENT.....14

 6.1 Menu-driven User Interface.....14

 6.1.1 System Information15

 6.1.2 DHCP Configuration16

 6.1.3 RS-232/422/485 Transfer Configuration17

 6.1.4 Monitor Menu19

 6.1.5 TFTP Firmware Upgrade19

 6.1.6 SNMP Configuration.....20

 6.1.7 System Restart.....21

 6.2 Command Line Interface22

 6.3 Web Graphic User Interface.....23

 6.3.1 System Information23

 6.3.2 Master Information23

6.3.3	RS-232/422/485 Transfer Configuration	23
6.3.4	Serial Connect Status.....	26
6.3.5	User Configuration	27
6.3.6	Firmware Download	27
6.3.7	SNMP Community Configuration	28
6.3.8	IP Trap.....	28
6.3.9	System Restart.....	29
7	APPENDIX: SERIAL IP REDIRECTOR	30
8	CONTACT INFORMATION	34

1 About This Guide

1.1 Welcome

Thank you for selecting the RS-232/422/485 to 100Base-FX Device Server / Managed Media Converter. This unit is designed to provide a RS-232/422/485 connection over twisted-pair cable where the connected devices have RS-232/422/485 interfaces. Enabling serial devices such as CNCs and PLCs to instantly connect to an existing Ethernet/ Fast Ethernet network, the Serial-to-Ethernet Device Server / Managed Media Converter represents a robust solution for devices controllers for MIS personnel. This product can either be used as Device Server or Managed Media Converter.

1.2 Purpose

This guide discusses how to install and configure your RS-232/422/485 to 100Base-FX Device Server / Managed Media Converter.

1.3 Terms/Usage

In this guide, the term “Device Server / Managed Media Converter ” (first letter upper case) refers to your RS-232/422/485 to 100Base-FX Device Server / Managed Media Converter , and “device server / media converter” (first letter lower case) refers to other device servers / media converters.

1.4 Features

- Device Server & Managed Media Converter Mode option
- Complies with EIA/TIA and IEEE standards
- 100Mbps Fast Ethernet fiber port
- Supports 4 wires full duplex asynchronous serial data transmission (RS-422/485)
- Supports 2 wires half-duplex asynchronous serial data transmission (RS-485)
- Supports serial port asynchronous data rates up to 115.2 Kbps
- Extended distances up to 1.2 km (24 AWG) using RS-422/485
- Terminator feature improves signal quality and distance
- LEDs for ‘at-a-glance’ device status
- Wall mount or Din-Rail mountable installation
- Power range 9~32V DC
- FCC Class A & CE approved

1.5 Specifications

Standards:	IEEE 802.3 (10BASE-T Ethernet); IEEE 802.3u (100BASE-TX/ Fast Ethernet); EIA/TIA RS-232/422/485; EIA/TIA-5744
Ports:	1x Fiber; Single Mode / Multi-Mode 1x 9-pin serial connector; D-sub, Male
Max. Distance:	Fiber: Up to 120,000 meters Serial: 15 meters (RS-232) 1,200 meters (RS-422, RS-485)
Data Rates:	Fiber: 100 Mbps Serial: 115.2 kbps (asynchronous)
Signals:	RS-232: TxD, RxD, CTS, RTS, DTR, DSR, RI, DCD, GND RS-422: TxD+/-, RxD+/-, GND RS-485: Data+, Data-, GND
Configuration:	Bits Per Second: 38400 Parity: None Data bits: 8 Stop bits: 1 Flow Control: None (The console connection is only available once the DIP switch 1 is ON)
Switches:	DIP 1: Enables / disables console / data communication mode DIP 2: Enables / disables RS-232 DIP 3: Enables / disables RS- 422/485 (4-wire) DIP 4: Enables / disables RS-485 (2-wire) DIP 5: N/A DIP 6: N/A DIP 7: Enables / disables termination (TMR)
Power:	External power adapter; 9~32V DC @800mA Frequency: 47Hz to 63Hz
Environment:	Temperature: Operating: 0°C to 50°C Relative Humidity: 10% to 80%, non-condensing Storage: -20°C to 80°C Relative Humidity: 5% to 90%, non-condensing
Emissions:	FCC Part 15 of Class A & CE approved
Dimensions:	109.2 x 90 x 30mm (L x W x H)
Weight:	280 grams

1.6 Package Contents

The package should include the following:

- One IRF-634 Device Server / Managed Media
- One power adapter (please check connector type and input power specification)
- Four self-adhesive pads
- DIN Rail Kit
- Screws for wall-mount installation
- Quick Installation Guide
- User's Manual CD
- Serial IP Redirector software CD

2 Hardware Description

2.1 Product Overview


The Device Server/Managed Media Converter features complete Ethernet and TCP/IP network support that allows devices in industry with RS-232/422/485 connectors such as milling machines, measurement instruments, and robots to connect to LAN based automation. Other devices typically found on campus networks such as card readers, code readers, lab equipment, medical equipment, and other similar serial devices can now instantly migrate to a TCP/IP network. Additionally, by deploying the device server mode, enable users to monitor and manage up to 256 serial devices from single PC with the help of Serial IP Redirector software.

2.2 Product Illustrations

Front Panel



Rear Panel

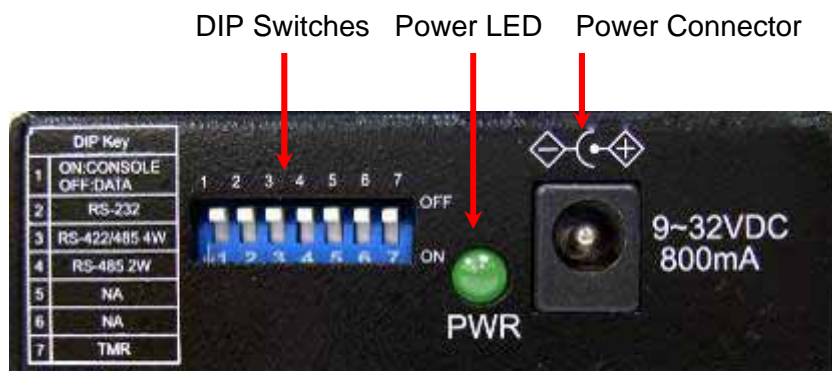

3 Installation

To install your Device Server / Managed Media converter, please see the following procedures:

- Location
- Din Rail Mounting
- Desktop Installation
- Powering On Unit
- Connecting Fiber Cables
- DB9 Male Connector Pin Assignment
- Serial Connection

3.1 Location

The location selected for installing the Device Server / Managed Media Converter may greatly affect its performance. When selecting a site, we recommend considering the following rules:

1. Install the Device Server / Managed Media Converter in a fairly cool and dry place. See *Technical Specifications* for the acceptable temperature and humidity operating ranges.
2. Install the Device Server / Managed Media Converter in a location free from strong electromagnetic field generators (such as motors), vibration, dust, and direct exposure to sunlight.
3. Leave at least 5cm of space at the front and rear of the unit for ventilation.
4. Affix the provided rubber pads to the bottom of the Device Server / Managed Media Converter for grip, and to protect the case from scratching.


3.2 Wall Mount Installation

IRF-634 can also be installed by wall mounting. The backside casing provides space for two screws each side. Identify the exact location at wall by placing the Device Server / Managed Media Converter and marking the screw positions. Use the screw (include in the package) and snug them well to fix the Device Server / Managed Media Converter.

3.3 Din Rail Mount Installation

The aluminum DIN Rail attachment plate should already be affixed to the back panel of the Device Server / Managed Media Converter. If you need to attach the DIN Rail plate, assure that the stiff metal spring is situated towards the top. Attaching the Device Server / Managed Media Converter to the DIN rail is easy, just align, and attach the top rail, then press down and snap forward the Device Server / Managed Media Converter to snap in the bottom rail, as shown in the figures below.

Use following steps set up the Device Server / Managed Media Converter:

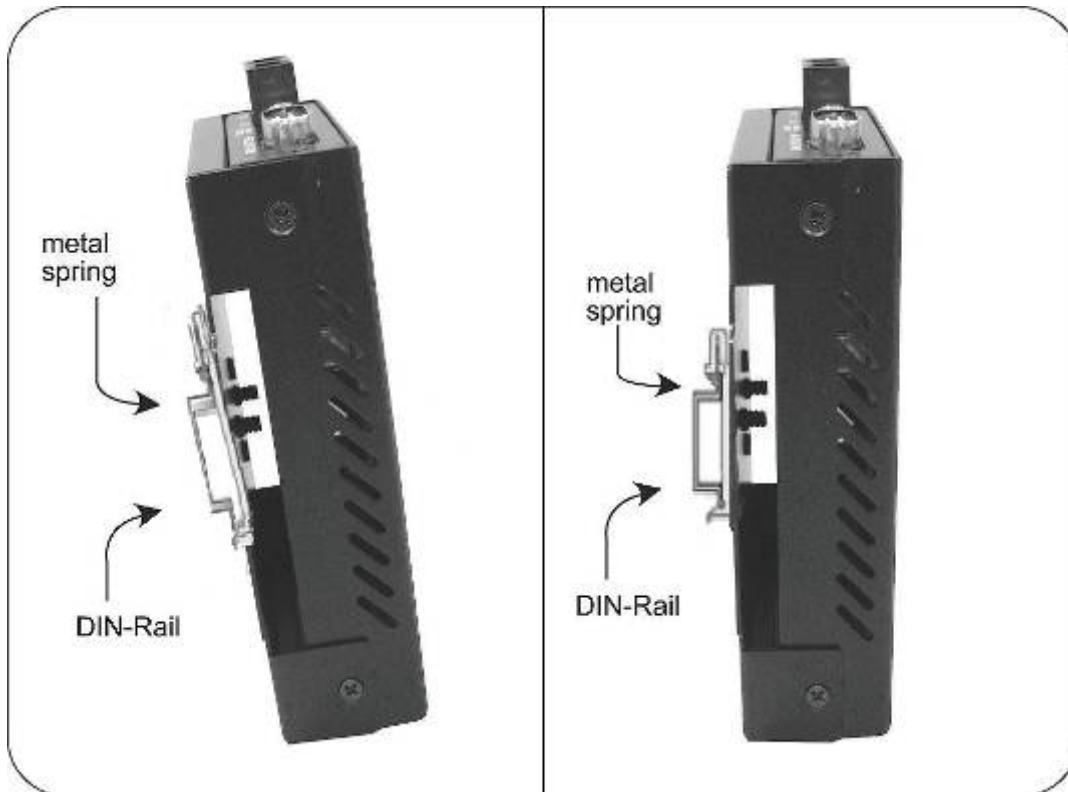

- The surface must support at least 500 gm for the Device Server / Managed Media Converter.
- The power outlet should be within 1.82 meters (6 feet) of the Device Server / Managed Media Converter.
- Visually inspect the power adapter and make sure that it is properly connected. Make sure that there is proper heat dissipation from and adequate ventilation around the Device Server / Managed Media Converter. Do not place heavy objects on the product.



Warning Please exercise caution when using power tools. Also, install this unit away from damp or wet locations, or in close proximity to very hot surfaces. These types of environments can have a detrimental effect on the unit and cables.

3.4 Powering On Unit

The Device Server / Managed Media Converter uses external power supply 9~32V DC @ 0.8A 50~60 Hz.

1. Insert the power cable plug directly into the receptacle located at the back of the device.
2. Plug the power adapter into an available socket.
3. Check the rear-panel LEDs as the device is powered on to verify that the Power LED is lit. If not, check that the power cable is correctly and securely plugged in.

NOTE: The RJ-45 port accepts both 'straight-through' and 'cross-over' Ethernet cables without the need to re-configure the port.

3.5 Connecting Fiber Cable

When connecting fiber cable to a 100BASE-FX port on the product, be sure the correct type – ST, SC, or WDM - connector is used. Follow the steps below to properly connect fiber cable:

1. Remove and keep the ST/SC/WDM port's rubber cover. When not connected to a fiber cable, the rubber cover should be replaced to protect the optics.
2. Check that the fiber terminators are clean. You can clean the cable plugs by wiping them gently with a clean tissue or cotton ball moistened with a little ethanol. Dirty fiber terminators on fiber optic cables will impair the quality of the light transmitted through the cable and lead to degraded performance on the port.
3. Connect one end of the cable to the ST/SC/WDM port on the Device Server / Managed Media Converter and the other end to the ST/SC/WDM port on the other device.


NOTE: When inserting the cable, be sure the tab on the plug clicks into position to ensure that it is properly seated.

4. Check the corresponding port LED on the Device Server / Managed Media Converter to be sure that the connection is valid. (Refer to the LED chart in next section)



Warning Because invisible laser radiation may be emitted from the aperture of the fiber port when no cable is connected, avoid exposure to laser radiation and do not stare into the open apertures.

3.6 DB9 Male Connector Pin Assignments

	PIN	RS-232 (Full-duplex)	RS-422/485 4-wire (Full-duplex)	RS-485 2-wire (Half-duplex)	Signal Direction
1	1	DCD			OUT
2	2	RX	RX-	**DATA B(-)	IN
3	3	TX	TX-		OUT
4	4	DTR			IN
5	5	GND	GND	GND	--
6	6	DSR			OUT

NOTE: Bi-directional RS-485 BUS line.

3.7 Serial Connection

This Device Server / Managed Media Converter features DIP switches on the rear panel that sets the unit to the correct type of cable configuration to support connection with a RS-232 / 422 / 485 device.

Definition of DIP Switches

No	Dip description	Default
1	ON: Console / OFF: Data	OFF
2	RS-232	ON
3	RS-422 / 485 (4W)	OFF
4	RS-485 (2W)	OFF
5	NA	OFF
6	NA	OFF
7	TMR (Terminator)	OFF

For setting the control function of the serial port, see the table below:

DIP 1	Serial Connection
ON	RS-232 Console
OFF	Data Communication

NOTE:

1. If using console mode turn the DIP Switch 1 to ON position. For data communication from the serial device keep the switch to OFF position. In case of ON position data communication will be blocked and at OFF position console port access.
2. For some RS-422/485 devices, which may not be designed to provide DB-9 connection, please check the pin definition to connect the devices.
3. For the first time installation, you have to use console mode to setup the IP and TCP port configuration with RS-232 cable. Always use Cross Over cable, if using Straight Through, you must use "Null Modem" to use Telnet option.


4 LED Indicators

This Device has LED indicators located at the front of the device. The LEDs have been designed to give easy at-a-glance network status, and provides 'real-time' connectivity information. Please see below for an interpretation of their functions:

LED Indicators		
LED	Condition	Status
PWR	On (Green)	Unit is receiving power
	Off	Power off or failure
LNK / ACT	On (Green)	Receiving data packets
	Flashing (Green)	Data packets being transmitted or received via fiber port
	Off	Fiber cable is not connected
ACT	On (Green)	Serial connector attached and link signals received
	Flashing	Data traffic passing through serial port
	Off	Serial port is idle or no link established

5 User Interface Startup

There are two separate methods for configuring this Device Server / Managed Media Converter for use. In the first section of this chapter, the Command line Interface (CLI) or Menu-driven interface via the *Console Port* to set the device IP and TCP configuration to monitor/managed the attached serial device via Serial IP Redirector software. The second section will describe *CLI or Menu-driven via Telnet* configuration. Firstly, make the connection below:

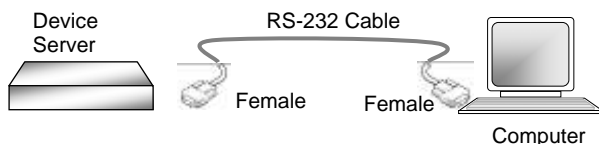

DIP Switch 1 set to 'ON' position

5.1 Console Port Access

The Device Server / Managed Media Converter is accessible via a terminal emulator attached to the RS-232 console port. Please follow the step below.

1. Attaching the serial cable to COM port of computer and serial port of device server.
2. Select Hyper Terminal from (start menu → programs → Accessories → communication) a window will appear, assign the connection name. Then select the correct available COM port (COM1 or COM2). After this enter the port settings as below.
 Bits per seconds: 38400
 Data bits: 8
 Parity: None
 Stop bits: 1
 Flow Control: None
3. Once connection is established, you will see a log in screen.


```
VOLKTEK Corporation
Firmware version: 1.00.02 (built at Jan 9 2006 11:17:12)
Press <ENTER> key to start.
```

4. Press **ENTER** and on the following screen, type the default username **admin**, leave the password field blank since there is no default value and press **ENTER** to proceed.

```
VOLKTEK Corporation
Firmware version: 1.00.02 (built at Jan 9 2006 11:17:12)
Press <ENTER> key to start.

Username:admin
Password:
```

5. Select either CLI User Interface or Menu-driven Interface option by using the associated number key or using the **TAB** key and pressing **ENTER**. A relevant Main Menu screen appears.

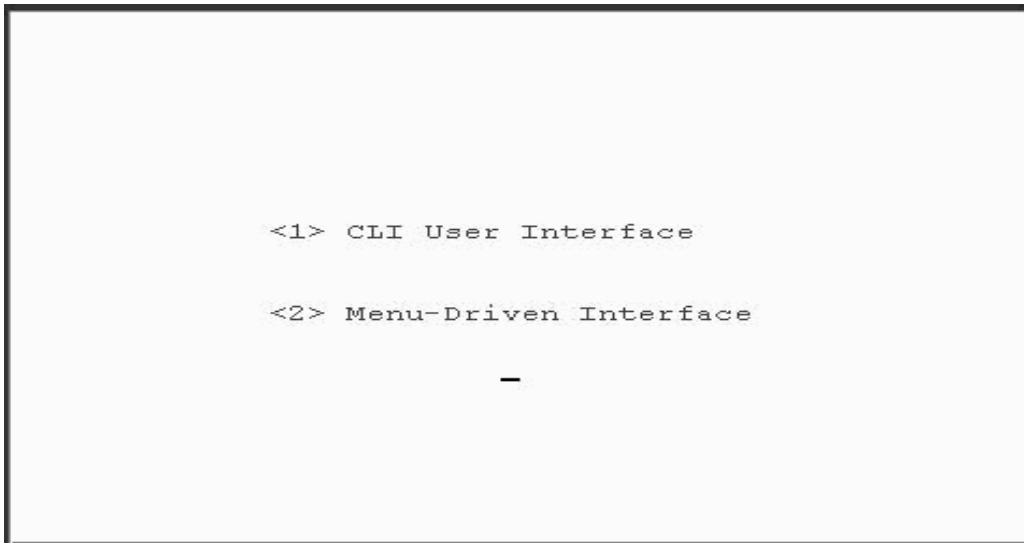

The Device Server / Managed Media Converter is preset with a factory IP address (192.168.0.254) that must be configured to the user's individual IP address. It is important to do this so that the device server / managed media converter doesn't conflict with other devices with the same defaults.

NOTE:

Prior to following the instructions for HyperTerminal Configuration, ensure that a serial cable connection between the device server / managed media converter and workstation exists.

Type the following command line to change the device IP address in CLI mode where **xxx**'s represent values between **0** and **254** and the user should enter their own IP address in this form.

- a) set eth0 ip **xxx.xxx.xxx.xxx**

If using the Menu-driven interface. Select the **System Information** from the Main Menu and following screen will appear. Use **TAB** key to move the cursor and **<Enter>** to change the value. Once change the value, select **<SAVE>** to apply the changes.

```
System Information
=====

Description      : Serial/IP Device Server
Model Name       : RS-232/422/485 To ETH Device Server
Company Name     : VOLKTEK Corporation
Board Name       : 6700-00634-0100
MAC-1 Address    : 00:0B:04:FF:EE:EE

DHCP Client      : Disabled
IP Address       : 192.168.0.200
Subnet Mask      : 255.255.0.0
Gateway          : 192.168.0.1

<SAVE>          <ESC>

<Tab> to move | <Enter> to select
```

After entering the new IP address. The system will confirm whether the operation is successful.

NOTE:

Copy the new address down on a piece of paper. You will need the address when you are going to use Telnet or set up data transfer/communication connection.



Warning

IP addresses are unique! If an address isn't available, please contact the appropriate authorities to apply for one.

5.2 Telnet Access

The Device Server / Managed Media Converter is accessible via a Telnet. At the command prompt type **telnet 192.168.0.254** (If connecting with default IP). You will be prompted to Enter user name and password as mentioned and shown in the topic Console Port Access. Use CLI or Menu-driven interface to perform the changes.

NOTE:

The only limitation of Telnet Access is that users can not assign new IP address to device server. Please use Console Port Access or Web Access to assign new IP address.


5.3 Web Access

The Device Server / Managed Media Converter is accessible via a web browser once connected to the network. Type the IP address at web browser **192.168.0.254** (if connecting with default IP). A window will be prompted to Enter user name and password.



(Note: We use IP 192.168.0.200 to write this manual)

After successful login, the main screen will appear.

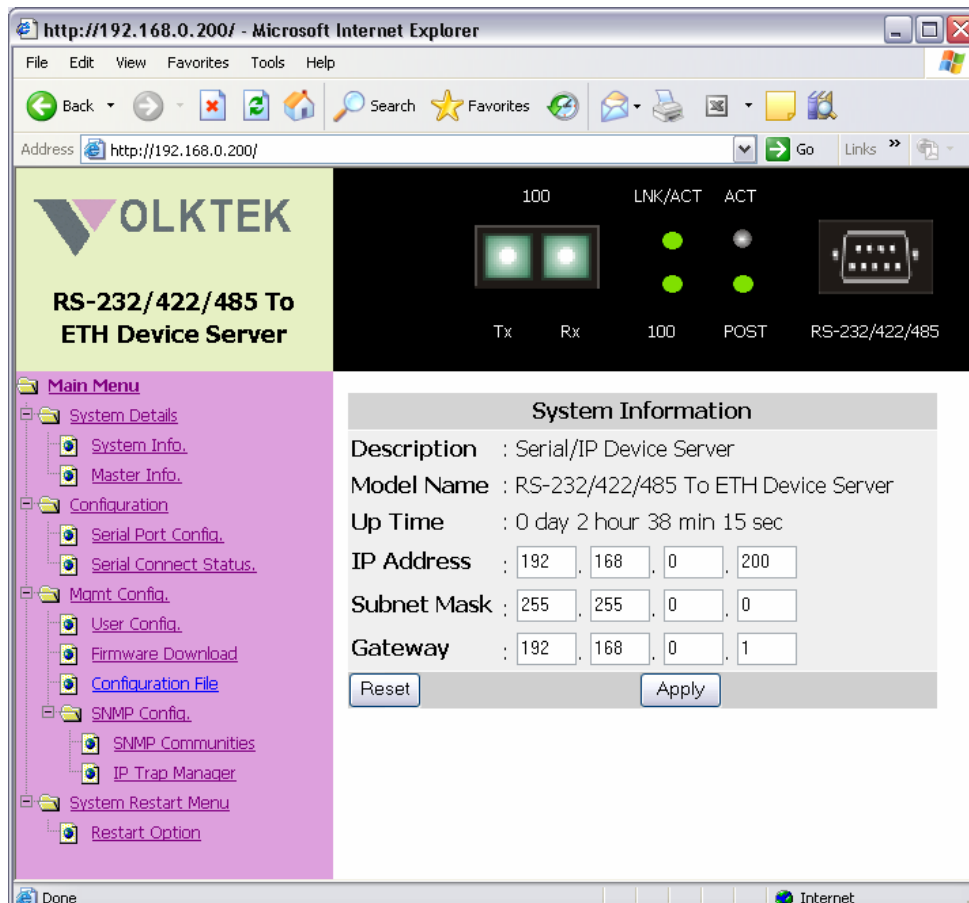


6 Configuration Management

Users can manage the Device Server via menu-driven interface or command line interface from Telnet or serial console, or Web graphic user interface.

6.1 Menu-driven User Interface

The figure below shows the Main Menu screen. From this screen the configuration options available provide the user to quickly access and adjust the device server settings as required.

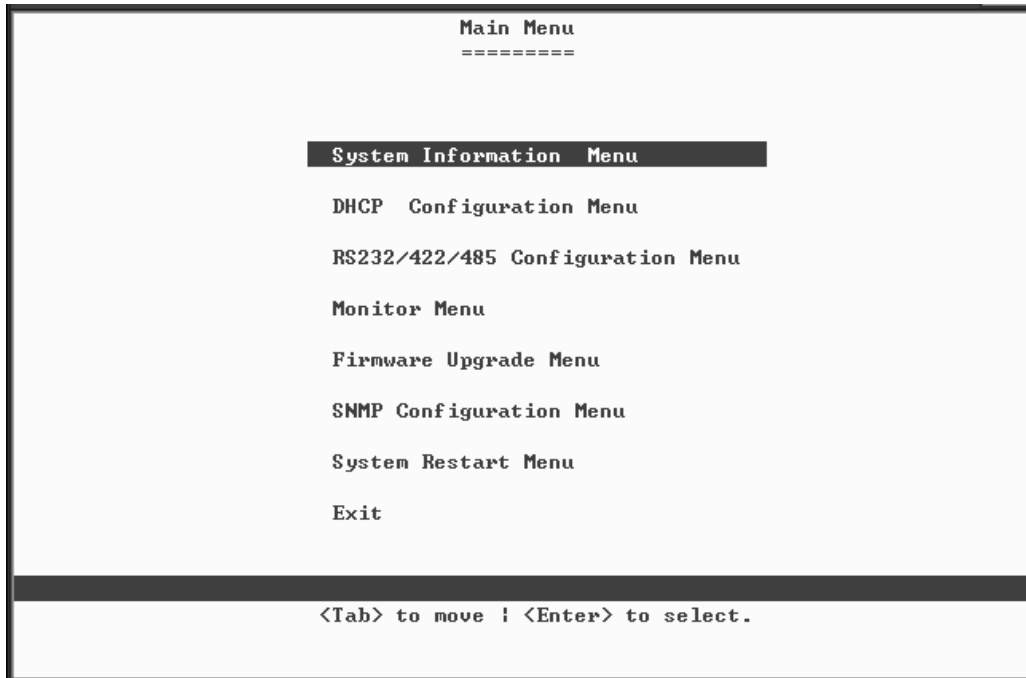

Main Menu Screen

Use **TAB** key to move the cursor to different fields and press **Enter** to select/edit the option.

6.1.1 System Information

From this menu, the user can view some system related information and default IP address. The user should set up appropriate IP address, subnet mask and Gateway for his own network. After entering a new IP address, Telnet and data communication will be based on the 'new' address.

```
System Information
=====
Description      : Serial/IP Device Server & Converter
Model Name       : RS-232/422/485 To ETH Device Server & Converter
Company Name     : VOLKTEK Corporation
Board Name       : 6700-00633-0120
MAC-1 Address    : 00:0B:04:FF:EE:EE

DHCP Client      : Disabled
IP Address       : 192.168.0.200
Subnet Mask      : 255.255.0.0
Gateway         : 192.168.0.1

<SAVE>          <ESC>
-----
<Tab> to move | <Enter> to select
```

System Information menu

Once changes are made, move the cursor to **<SAVE>** by using **TAB** key and press **Enter** to save the settings. Change of IP will lead to restart the Device Server / Managed Media Converter.

NOTE:

In Telnet mode you can't change the IP address.

6.1.2 DHCP Configuration

DHCP(Dynamic Host Configuration Protocol) allows the Device Server / Managed Media Converter to obtain an IP address from DHCP server automatically.

NOTE:

A DHCP server must exist and be available in your local network prior to enabling the DHCP client.



DHCP Configuration menu

Use **Spacebar** to enable the DHCP Client settings. Select **<SAVE>** to apply the settings and **<ESC>** to move to the previous menu. If you don't want to save the changes made, just select **<ESC>** and you will move to previous menu without making any changes.

6.1.3 RS-232/422/485 Transfer Configuration

The RS-232/422/485 menu is applicable to all RS-232/RS-422/RS-485 modes. Before using data transfer mode option for the Device Server / Managed Media Converter, move the DIP Switch 1 to OFF position.

In case the device is used in Device Server Mode:

You can assign the TCP port number to monitor and access the serial device via device server over the network/Internet from a workstation using Serial IP Redirector software. (The TCP port number can be of any number from 1024 to 65535).

The 2 screenshots below show the different screen options when selecting Device Server mode in the DS/CR Mode setting (top) or Converter mode (bottom):

```
RS232/422/485 Transfer Configuration
=====
Server/Client Type : SERVER
TCP Port Number   : 1234
DS/CR Mode       : Device Server
Packet Mode(serial) : Disable
Packet Mode timeout(ms) : 20
```

```
RS232/422/485 Transfer Configuration
=====
Server/Client Type : AUTO
Remote IP          : 192.168.0.155
TCP Port Number   : 1234
Connection Idle Time(sec): 600
DS/CR Mode       : Converter

Serial Port Configuration
=====
Operation Mode: Console Mode
Baud Rate      : 38400
Parity         : None
Word Length    : 8
Stop Bits      : 1
Flow Control   : NONE
```

RS-232/422/485 Transfer Configuration (Explanation follows below)

EXPLANATION: Server/Client Mode Configuration	
Server/Client Type	A read-only attribute. In Device Server mode, the device will have a Server role as a TCP Server. In Media Converter mode, the "Server" and "Client" roles of the two ends will be decided automatically.
Remote IP	In Media Converter mode, set the IP address of the other end device. Ignore if in Device Server mode.
TCP Port Number	The TCP port number that the TCP Server is "bound" to.
Connection Idle Time	In seconds. This is valid for Media Converter mode only. The Client will disconnect the TCP session if no packets are transmitted in the set period.
DS/CR Mode	DS: Device Server mode – the Device Server acts as TCP Server and the Serial IP Redirector software acts as TCP Client. CR: Media Converter mode – two Device Servers communicate with each other through point-to-point architecture.
Packet mode of serial input	This is valid for Device Server mode only. Enabled – input data from the serial interface is treated as serial packets. Disabled – input data from the serial interface is treated as bit streams.
Packet mode inter-packet timeout	In milliseconds. This is valid for Device Server mode only. It is the delimiter value for recognizing the timeout gap between serial packets if Packet Mode is enabled.
Serial Port Configuration	
Operation Mode	A read-only attribute. It shows the RS232/422/485 mode set by the DIP switch.
Baud Rate	The speed of the serial interface.
Parity	Select or disable the parity checking method
Word Length	The length of data in bits
Stop Bits	The bit length of stop bits
Flow Control	The flow control method for informing the correspondent

For Device Server Mode, in case you are using a serial device with a 2-wire RS-485 application or Modbus RTU protocol, do not forget to "Enable" the "Packet" mode of serial input. Also enter the appropriate inter-packet timeout value to enable smooth data communication.

To set the timeout value via console mode, first "Enable" the packet mode and "Save" the settings. Once settings are applied, you will be able to change the timeout value.

In case you are using the product as a Managed Media Converter, keep "Packet Mode" **Disabled**. In Managed Media Converter mode, the device must be paired with another device.



Changes to the settings are saved to a system flash memory and do NOT take effect until a system reset or reboot has occurred. This action validates the new settings. Please note that you can't change the Device Server / Media Converter mode by using Telnet. Always use Web Interface or Console access to change the Mode.

6.1.4 Monitor Menu

This screen provides at-a-glance system status information.

```

Connection Status                               RS232/422/485 Transfer Configuration
=====
Connect Status : Not connected                 Server/Client Type : AUTO
Peer IP Address  : 0.0.0.0                     Remote IP          : 192.168.1.220
Dest/Srce port number : 0/0                   TCP Port Number   : 1234
Byte counts from UART : 0                     Connection Idle Time(sec): 600
Byte counts to network : 0                    DS/CR Mode       : Converter
Byte counts from network: 0
Byte counts to UART   : 0

                                           Serial Port Configuration
                                           =====
                                           Operation Mode: RS232 Mode
                                           Baud Rate      : 38400
                                           Parity         : None
                                           Word Length    : 8
                                           Stop Bits     : 1
                                           Flow Control   : NONE

                                           <Clear>           <ESC>

                                           <Tab> to move | <Enter> to select

```

Monitor Menu

6.1.5 TFTP Firmware Upgrade

From this menu, the user can upgrade the existing firmware to newer firmware available from a TFTP server. Simply enter the file name of the updated firmware in the file name field and enter the IP address of the TFTP server in the IP address field to perform the upgrade. Selecting **<update>** will start downloading the newer firmware and system will restart to apply the firmware.

```

TFTP FIRMWARE UPGRADE
=====

File Name   : ████████████████████████████████████████████████████████████
IP address  : 192.168.0.206

                                           <Update>           <ESC>

                                           <Tab> to move | <Enter> to select_

```

TFTP Firmware Upgrade menu

6.1.6 SNMP Configuration

Use the SNMP Configuration screen to display and modify parameters for the Simple Network Management Protocol (SNMP). The product includes an onboard SNMP agent that monitors the status of its hardware as well as the traffic passing through its ports. A computer attached to the network, called a Network Management Station (NMS), can be used to access this information. Community strings control access rights to the agent module. To communicate with the Device Server / Managed Media Converter, the NMS must first submit a valid community string for authentication.

```

SNMP Configuration
=====

System Name   : RS-232/422/485 To ETH Device Server & Converter
Location      : VOLKTEK Corporation
Contact name  : service@volktek.com.tw
Get Community : public
Set Community : private

[SNMP Trap]

Index  Status  IP address  Community
1     Disabled  0.0.0.0    public
2     Disabled  0.0.0.0    public
3     Disabled  0.0.0.0    public
4     Disabled  0.0.0.0    public
5     Disabled  0.0.0.0    public

<SAVE>      <ESC>

<Tab> to move ; <Enter> to select ; <Esc> to Cancel_

```

SNMP Configuration

The options for configuring community strings and related trap functions are described as below.


Use the <Tab> and <Enter> keys as previously. Enter the IP address of computers for when abnormalities on a connection occur and an alarm to be sent. Enter their community names and disable or enable their alarm function accordingly. See descriptions below:

Parameter	Description
Index	Number assigned to each trap
Status	Disable or enable their alarm function accordingly
IP Address	Enter the IP address of computers for when abnormalities on a connection occur and an alarm to be sent. Enter their community names and disable or enable their alarm function accordingly
Community	Enter their community names

You can use an external SNMP-based application to configure and manage the Device Server / Managed Media Converter. This management method requires the SNMP agent on the Device Server / Managed Media Converter and the SNMP Network Management Station to use the same community string. This management method, in fact, uses two community strings: the get community string and the set community string. If the SNMP Network Management Station only knows the set community string, it can read and write to the MIBs. However, if it only knows the get community string, it can only read MIBs. **The default get and set community strings for the product are public.**

6.1.7 System Restart

This menu allows users to restore the factory default setting for the Device Server / Managed Media Converter and/or to reset the system manually. Selecting this option will lead to another window with the following two options to select.

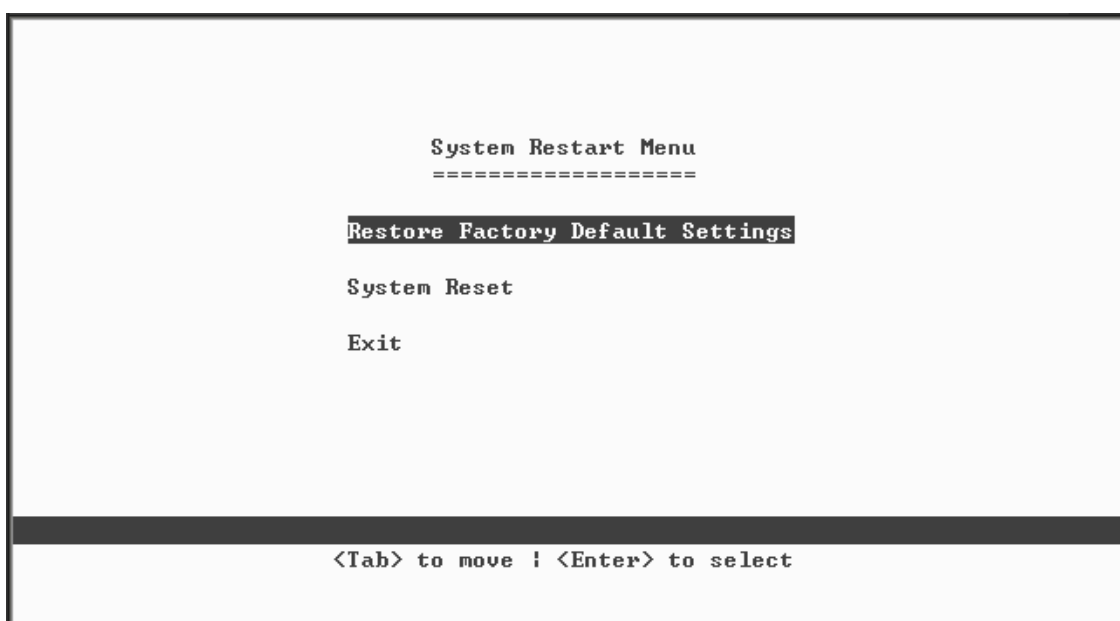

System Restart Menu

Restore Factory Default Settings

Selecting this option will lead to restore factory default settings to the device server / managed media converter. Highlight the field and hit the **<ENTER>** key to execute.

System Restart

The System Restart allows a user to perform a 'warm' restart and validate newly saved configuration to the device server / managed media converter. Highlight the System Restart field and hit the **<ENTER>** key to reset the unit.



After each configuration session, be sure to set DIP switch 1 to the 'OFF' position. Otherwise, the unit will not transmit any data.

6.2 Command Line Interface

Once you logged in and select the option of Command Line Interface, a window with command prompt will appear. Type **?** or **help** and it will show you the command list.

```

CLI>?
[Command List]
?..... Help commands
backup..... backup configuration file
exit..... Logout
help..... Help commands
logout..... Logout
ping..... Ping a specified host with IP address
reset..... Reset system or reset factory default setting
set..... Set commands
show..... Show commands
upgrade..... Upgrade run-time firmware or configuration file
CLI>

```

Command List

Command Definitions

backup: Use this command to save configuration settings to file.

exit: Type exit or logout and press **ENTER** to quit the program.

help: To access help commands list.

logout: To logout from the device server.

ping: Type **ping** followed by a **space**, and then the **IP address** of the device to send a test signal. If a response is received, then the device is connected. To view a full list of **ping** options, type ping and press **ENTER**.

reset: Type **reset config** and press **ENTER** to load factory default settings, or type **reset system** and press **ENTER** to restart the system.

show: Type **show** to display variety of device server settings.

set: To configure the management settings, type the commands below, followed by the **ENTER** key.

NOTE: Separate each port of the command line with a space.

set admin - follow the prompts to change user name and password

set eth0 - the command is for factory setting use **set eth0 ip** (new IP address) **network mask** (new network mask) **gateway** (new gateway). Use this command to set new Ethernet settings.

set idle - (time in seconds) – set automatic logout. when the program or communication is idle

set xfer - the command is for RS-232 configuration and data communication setting. The command syntax is as below.

```
set xfer [arg_1 data_1] [arg_2 data_2]
[arg_n data_n]
[Argument List]
Port..... Set TCP port number
statistics..... Clear statistics
```

upgrade - Use this command to upgrade the firmware.
i.e upgrade firmware xxx.xxx.xxx.xxx Soft2.bin

set snmp - Use this command to set SNMP settings of the device server.



After each configuration session, be sure to set DIP switch 1 to the 'OFF' position. Otherwise, the unit will not transmit any data.

6.3 Web Graphic User Interface

Please see previous chapter to log-in the Device Server / Managed Media Converter via web browser.

6.3.1 System Information

System information will show IP Address, Subnet Mask and Gateway settings. After editing the setting press **Apply** to implement the settings.

System Information				
Description	: Serial/IP Device Server			
Model Name	: RS-232/422/485 To ETH Device Server			
Up Time	: 0 day 0 hour 36 min 34 sec			
IP Address	: 192	: 168	: 0	: 200
Subnet Mask	: 255	: 255	: 0	: 0
Gateway	: 192	: 168	: 0	: 1
<input type="button" value="Reset"/>		<input type="button" value="Apply"/>		

6.3.2 Master Information

Master Info will show the hardware and firmware version.

Master Information
Hardware Version : 6700-00633-0100
Firmware Version : 1.00.02 (built at Jan 9 2006 11:17:12)

6.3.3 RS-232/422/485 Transfer Configuration

This page offers the selection between Device Server and Media Converter mode. Please select the appropriate required for your application. User can also monitor the serial port status and configure TCP port number from this menu.

- A. **Serial Port Config.** window will show you the serial port configuration and allow to assign the TCP port number to operate via Serial IP Redirector software for Device Server mode.
- B. The unit also offers two modes (Device Server Mode / Media Converter). Please restart the unit after selecting the mode to take effect.

Note: In case of using Media Converter Mode, recommend to keep Packet Mode option **Disable**.

A detailed explanation of the setting choices are given underneath the following screenshot:

RS232/422/485 Transfer Configuration	
Server Client Mode Configuration	
Server/Client Type	: Auto
Remote IP	: <input type="text" value="192.168.0.1"/>
TCP Port Number	: <input type="text" value="1234"/> (value=1024~65535)
Connection Idle Time (sec)	: <input type="text" value="60"/> s (value=30~3600)
DS/CR Mode	: <input type="text" value="Device Server"/>
Packet mode of serial input	: <input type="text" value="Disable"/>
Packet mode inter-packet timeout	: <input type="text" value="30"/> mS (value=1~5000)
Serial Port Configuration	
Operation Mode	: CONSOLE MODE
Baud Rate	: <input type="text" value="38400"/>
Parity	: <input type="text" value="None"/>
Word Length	: <input type="text" value="8"/>
Stop Bits	: <input type="text" value="1"/>
Flow Control	: <input type="text" value="None"/>
<input type="button" value="Reset"/>	<input type="button" value="Apply"/>

EXPLANATION: Server/Client Mode Configuration	
Server/Client Type	A read-only attribute. In Device Server mode, the device will have a Server role as a TCP Server. In Media Converter mode, the "Server" and "Client" roles of the two ends will be decided automatically.
Remote IP	In Media Converter mode, set the IP address of the other end device. Ignore if in Device Server mode.
TCP Port Number	The TCP port number that the TCP Server is "bound" to.
Connection Idle Time	In seconds. This is valid for Media Converter mode only. The Client will disconnect the TCP session if no packets are transmitted in the set period.
DS/CR Mode	DS: Device Server mode – the Device Server acts as TCP Server and the Serial IP Redirector software acts as TCP Client. CR: Media Converter mode – two Device Servers communicate with each other through point-to-point architecture.
Packet mode of serial input	This is valid for Device Server mode only. Enabled – input data from the serial interface is treated as serial packets. Disabled – input data from the serial interface is treated as bit streams.
Packet mode inter-packet timeout	In milliseconds. This is valid for Device Server mode only. It is the delimiter value for recognizing the timeout gap between serial packets if Packet Mode is enabled.
Serial Port Configuration	
Operation Mode	A read-only attribute. It shows the RS232/422/485 mode set by the DIP switch.
Baud Rate	The speed of the serial interface.
Parity	Select or disable the parity checking method
Word Length	The length of data in bits
Stop Bits	The bit length of stop bits
Flow Control	The flow control method for informing the correspondent

While using as Device Server mode, in case you are using a serial device with a 2-wire RS-485 application or Modbus RTU protocol, do not forget to "Enable" the "Packet" mode of serial input. Also enter the appropriate inter-packet timeout value to enable smooth data communication.

Note: You will not be able to change the serial port settings (Baud Rate, Parity, Stop bits etc) while working in Device Server mode; they are managed through IP Serial Redirector software.

6.3.4 Serial Connect Status

Serial Connect Status will show the serial port connection to the serial device. Serial port settings can only be changed when using Media Converter mode.

RS232/422/485 Connection Status	
Connect Status	: Server-Type
Peer IP Address	: 192.168.0.21
Dest/Srce Port Number	: 1753 / 1234
Byte Counts From UART	: 543
Byte Counts To Network	: 543
Byte Counts From Network	: 9
Byte Counts To UART	: 9

Clear

User can get the instant information about the connectivity.

Connect Status: Server or Client

Peer IP Address: IP of remote PC access the serial device via Device Server

Dest/Srce Port Number: Showing the destination and source Port numbers. Source port number will be as configured.

Byte Counts From UART: Displaying the number of bytes transmitted from serial device.

Byte Counts to Network: Displaying the number of bytes received to TCP/IP network.

Byte Counts From Network: Displaying the number of bytes transmitted from Network.

Byte Counts to UART: Displaying the number of bytes received to serial device.

Mgmt. Configuration: This category offers multiple management options.

6.3.5 User Configuration

This option will allow user to change the “username” and “user password” for the device server / managed media converter management.

User Configuration	
User Name	User Password
<input type="text" value="admin"/>	<input type="text"/>
<input type="button" value="Reset"/>	<input type="button" value="Apply"/>

Type the new user name in the “User Name” and password to “User Password”. Selecting **Apply** will implement the new user name and password, which will be required to manage the device server / managed media converter.



It is recommended to keep a written record in a safe place for the User Name and Password. In case, you lost the both or either one, you need to reset the system to default setting. This can be done by pressing a button at S1 location of PCB (near to capacitor) after removing the casing.

6.3.6 Firmware Download

The user can download the newer/latest firmware to upgrade the device server / managed media converter once available. The user has two options, either they can upgrade via HTTP with browse option to select the firmware file.

Upgrade System by HTTP	
File Name :	<input type="text"/> <input type="button" value="Browse..."/>
<input type="button" value="Start Upgrade by HTTP"/>	
Upgrade System by TFTP	
IP Address :	<input type="text"/> . <input type="text"/> . <input type="text"/> . <input type="text"/>
File Name :	<input type="text"/>
<input type="button" value="Start Upgrade by TFTP"/>	

If using TFTP method, user must provide the valid IP address of TFTP server and the file name, i.e. VK413.bin.

Once enter the parameters press “Start Upgrade by HTTP / TFTP” to upgrade the firmware. The window will appear to show the time to before restarting the device server to implement the upgraded firmware.

6.3.7 SNMP Community Configuration

You can use an external SNMP-based application to configure and manage the Device Server / Managed Media Converter. This management method requires the SNMP agent on the Device Server / Managed Media Converter and the SNMP Network Management Station to use the same community string. This management method, in fact, uses two community strings: the **Get** community string and the **Set** community string. If the SNMP Network Management Station only knows the **Set** community string, it can read and write to the MIBs. However, if it only knows the **Get** community string, it can only read MIBs. The default **Get** and **Set** community strings for the Device Server / Managed Media Converter are public and private respectively.

SNMP Communities	
	Community Name
GET	<input type="text" value="public"/>
SET	<input type="text" value="private"/>
<input type="button" value="Reset"/>	<input type="button" value="Save"/>

If needed, assign the new parameters and press **Save** to implement the settings.

6.3.8 IP Trap

The following figure and table describe how to specify management stations that will receive authentication failure messages or other trap messages from the Device Server / Managed Media Converter. Up to 5 trap managers may be assigned.

IP Trap Manager		
IP Address	Community Name	Status
<input type="text" value="192.168.0.59"/>	<input type="text" value="public"/>	Enabled <input type="button" value="v"/>
<input type="text" value="192.168.1.112"/>	<input type="text" value="private"/>	Disable <input type="button" value="v"/>
<input type="text" value="0.0.0.0"/>	<input type="text" value="public"/>	Disable <input type="button" value="v"/>
<input type="text" value="0.0.0.0"/>	<input type="text" value="public"/>	Disable <input type="button" value="v"/>
<input type="text" value="0.0.0.0"/>	<input type="text" value="public"/>	Disable <input type="button" value="v"/>
<input type="button" value="Reset"/>	<input type="button" value="Save"/>	

Click on each parameter field to modify the desired setting, then click on **Undo** to restore previously saved configurations or click on **Save** to retain newly entered information. See descriptions below:

Parameter	Description
IP Address	Enter the IP address of terminals for when abnormalities on a connection occur and an alarm to be sent. Enter their community names and disable or enable their alarm function accordingly
Community Name	Enter their community names
Status	Disable or enable their alarm function

6.3.9 System Restart

Users can restart/reset the system via software from a remote location.

Restart Options

System Restore Factory Default Settings

Restore the factory default settings of the Device.

System Reset

Press "Reset" if the device is abnormally functioning.




Clicking on the Restore button will set the device server / managed media converter back to factory defaults. All saved configurations will be lost.

7 Appendix: Serial IP Redirector

Install the Serial IP Redirector software from CD-Rom. Once it's installed, you can read the "documentation" to get assistance related to Serial IP Redirector. The documentation will be installed to your PC with the software.


The serial IP icon can be found at the right corner of system tray. Right click the icon and select **Configure**, the following window will appear.

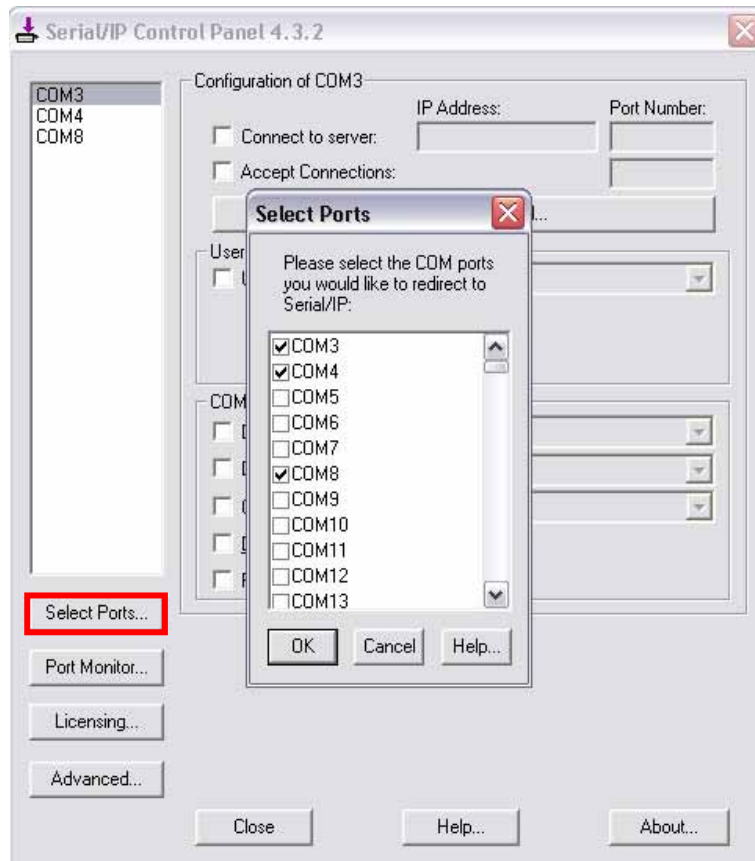

Note: Serial IP Redirector software will only work while using the unit as a Device Server. Do not install or use the software while using the unit as Managed Media Converter.


Click on **Select Ports** option to configure the Virtual COM ports. You can select up to 256 virtual COM ports. COM1 and COM2 are normally physical ports, so will not appear here. The selected ports will be shown on the left top corner of the Configure screen.

Selecting the “Connect to server” will allow you to enter IP address and port number. Enter the correct IP address and port number assigned to the Device Server.

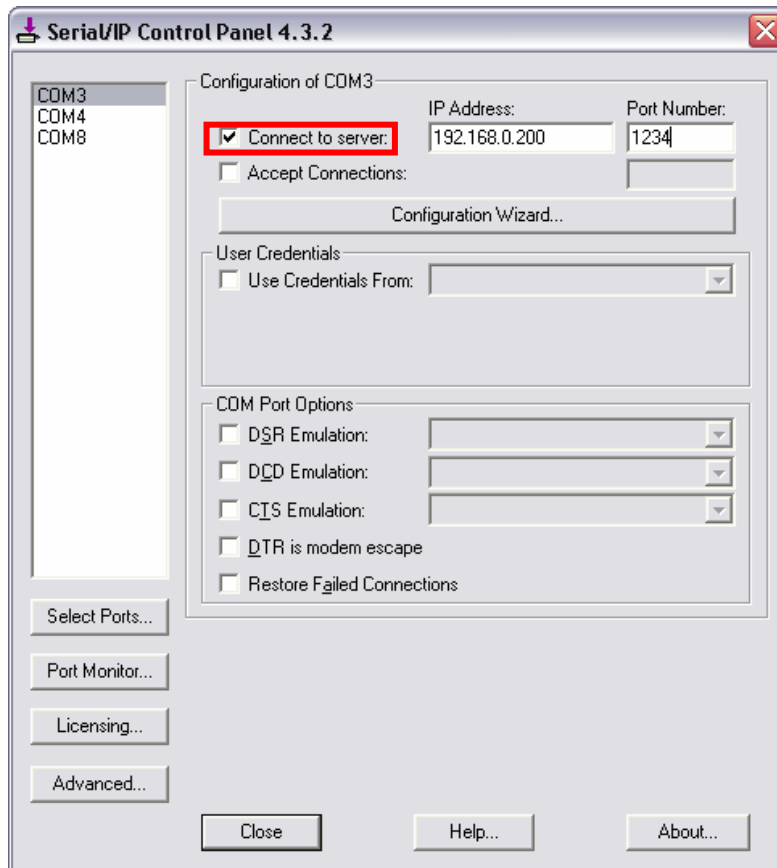

After assigning the IP address and port number, press **Configuration Wizard** button to check if the link is established.

On the following screen, press **Start** button. If the link is function well, the following screen will appear.

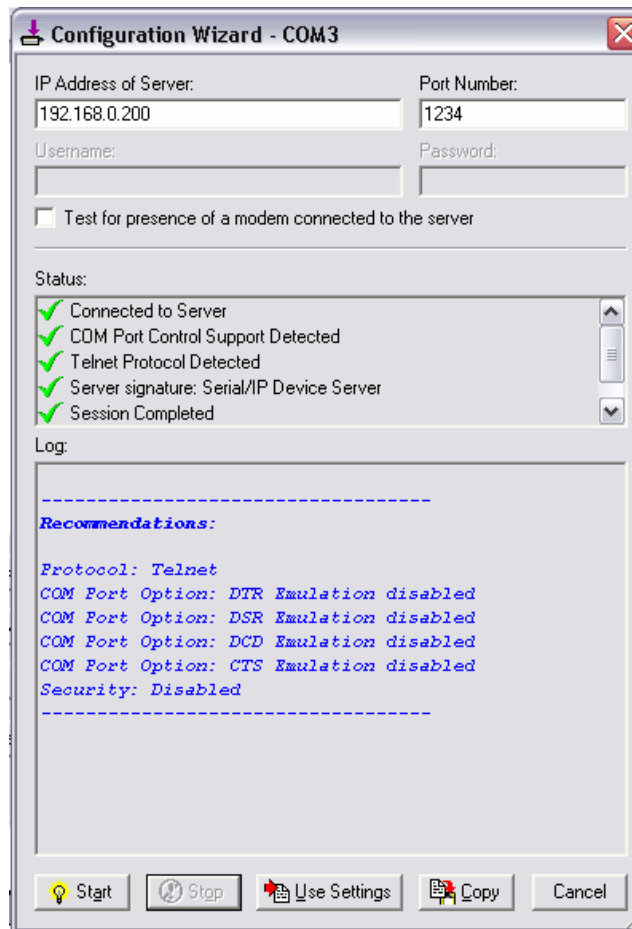


If the link has trouble, the error message will appear. To solve the problem, please check the following:


- a) Whether IP address and Port numbers are correct.
- b) Fiber cable is properly connected to Ethernet.
- c) DIP Switch 7 is correctly selected (4Wire and 2Wire Mode).

Once the link is established, you can manage the serial device attached to the device server from remote workstation installed Serial IP Redirector software.

From the Serial IP **“Port Monitor”** option, you can see the connectivity status and IP address of the device server.

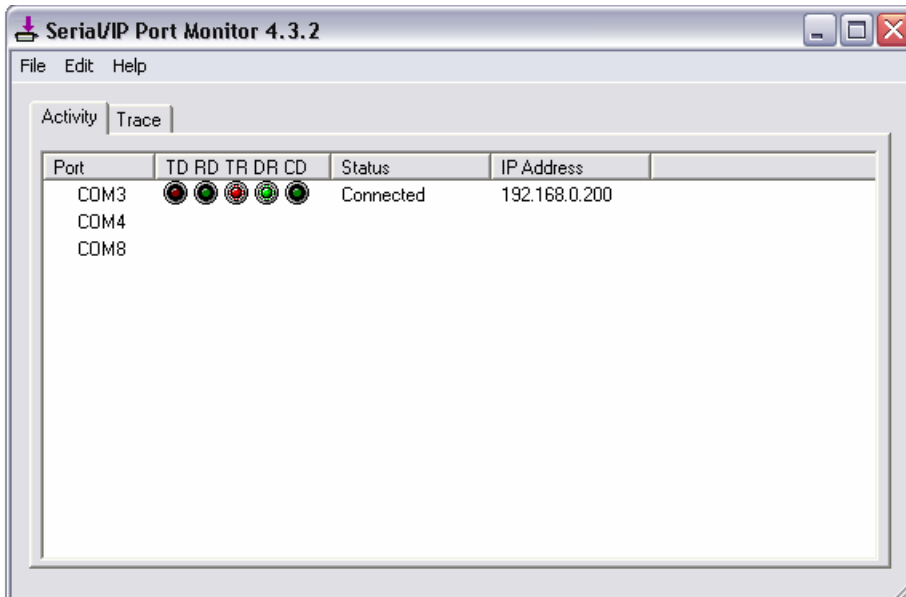

If more devices are attached and connected, the status and IP address of those devices will also be showed against each Virtual COM port as shown below.

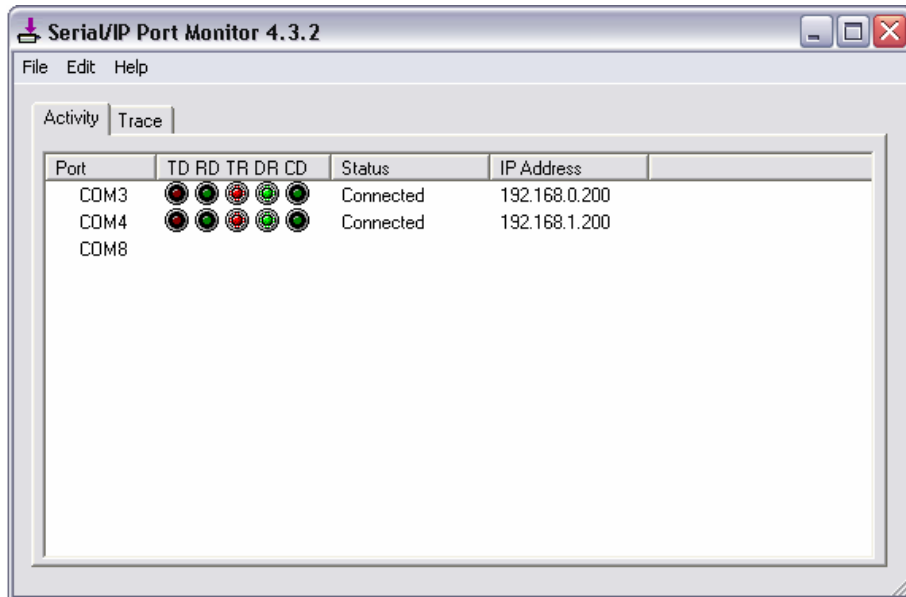

8 Contact Information

VOLKTEK CORPORATION

4F, No. 192 Lian-Cheng Road
Chung-Ho, Taipei 235, Taiwan ROC

TEL: +886 (2) 8242-1000

FAX: +886 (2) 8242-3333

ISO 9001 Certified