


Leer manual that came

	Phospho-p53 Ser392 ELISA Kit User's Manual For Research Use Only, Not for use in diagnostic procedures LISA Kit for Measuring Phosphorylated Human p53 Ser392	
GI	Phospho-p53 Ser392 ELISA Kit	
vclex	User's Manual	
G	For Research Use Only, Not for use in diagnostic procedures	
	S S	
EI	LISA Kit for Measuring Phosphorylated Human p53 Ser392	
CvcLe		
	$\begin{array}{c} \text{Cat# CY-7051} \\ Cat$	
-		
	ssay 2-3	
	ed4	
Materials Require	ed but not Provided	
	Recommendations	
Detailed Protocol		
Calculations		
Measurement Ra	nge	
-		
	stics	
	Results	
T (1 1 T		

Intended Use

The CycLex Research Product CycLex Phospho-p53 Ser392 ELISA Kit is designed to detect and quantify the level of human p53 protein that is phosphorylated at serine 392. Since the amino acid sequence surrounding serine 392 is got conserved in mouse and rat p53, this ELISA kit can not be used for mouse and rat cells. This assay is intended for the detection of phosphorylated human p53 at serine 392 from cell lysate.

This assay kit is for research use only and not for use in diagnostic or therapeutic procedures.

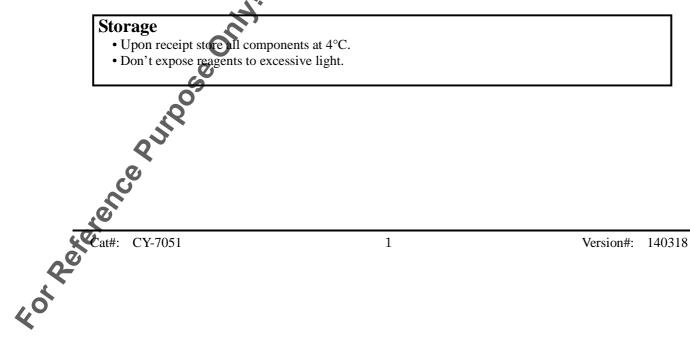



User's Manual

For Research Use Only, Not for use in diagnostic procedures

Introduction


p53 is a short-lived, non-abundant protein that regulates the response of cells to DNA damage, in part through transcriptional activation of genes involved in cell cycle control, DNA repair, and apoptosis (1). p53 is a tumor suppressor protein; consequently, mice in which the p53 gene has been disrupted develop tumors with high frequency (2, 3), and deletions or mutations in the p53 gene are prevalencin a majority of human cancers (4, 5). The protein level and activity of p53 are regulated, and this is accomplished by MDM2 (murine double minute 2) (6–10). The MDM2 gene is induced by p53, and MDM2 prevents apoptosis by inhibiting p53 activity and promoting its degradation (6, 9, 11).

In response to DNA damage, the p53 protein is phosphorylated on each of the seven serines and one threonine the in the first 50 amino acids of its N-terminal transactivation domain as well as at several sites in its C-terminal tetramerization/regulatory domain (12, 13). As a transcription factor, p53 induces or represses several genes that regulate cell cycle arrest, DNA repair or apoptosis, including p21WAF1, MDM2, GADD45, p53R2, and p53AIP1. Recent studies suggest that specific p53 phosphorylation events are important for the activation or repression of specific promoters (14-17).

Phosphorylation of human p53 Ser-392 C-terminal regulatory domain occurs following UV but not gamma irradiation (18, 19) and results in enhancement of sequence-specific binding activity in vitro (20), possibly by promoting stable tetramer formation (21).

Principle of the Assay

The CycLex Research **CycLex Phospho-p53 Ser392 ELISA Kit** is a solid phase sandwich ELISA. An antibody specific for human p53 has been coated onto the wells of the microtiter strips provided. Samples, including a standard containing phosphorylated form of p53 at Serine 392, control specimens, and unknowns, are pipetted into these wells. During the first incubation, p53 protein binds to the capture antibody on the well. After washing, mouse monoclonal antibody, specific for phosphorylated p53 Ser392 as a detection antibody, is added to the wells. During the second incubation, this antibody serves as a detector by binding to the immobilized phosphorylated p53 protein at Ser392 captured during the first incubation. After removal of excess detection antibody, followed by binding with horseradish peroxidase conjugated anti-mouse IgG which then catalyzes the conversion of the chromogenic substrate tetra-methylbenzidine (TMB) from a colorless solution to a blue solution (or yellow after the addition of stopping reagent). The color is quantitated by spectrophotometry and reflects the relative amount of acetylated form of p53 at serine 392 present in the original specimen.

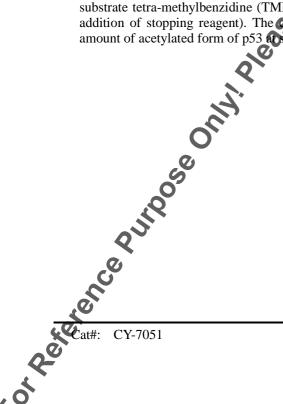

Version#: 140318



Summary of Procedure

with your product Culture cells in culture flask or dish at 50-70 % confluency Incubate O/N at 37°C in CO2 incubator Add appropriate amount of the drug for induction of p53 Ser392 phosphory ation Sall Incubate appropriate time at 37°C in CO₂ incubator Harvest the cells by scraping and centrifugation Make cell lysate by adding extraction buffer and centrifugation July, Add 100 µL of diluted cell lysate to the wells Incubate for 1 hour at room temp. Wash the wells Ť Add 100 µL of Primary Antibody Solution (ant Phospho-p53 Ser392 monoclonal antibody) Ţ Incubate for 1hour at room temp. Wash the wells Ť Add 100 µL of Secondary Antibody Solution (HRP conjugated anti-mouse IgG antibody) Incubate for thour at room temp. T Wash the wells Add 100 µL of Substrate Reagent Add 100 µL op Solution ence percentions teat#: CY-7051 Measure absorbance at 450 nm 3 Version#: 140318



User's Manual

For Research Use Only, Not for use in diagnostic procedures

Materials Provided

All samples and standards should be assayed in duplicate. The following components are supplied and are sufficient for the one 96-well microplate kit.

Microplate: One microplate supplied ready to use, with 96 wells (12 strips of 8-wells) in a foil, zip-lock bag with a desiccant pack. Wells are coated with anti-human p53 antibody as a capture anabody.

10X Wash Buffer: One 100 mL bottle of 10X buffer containing 2% Tween[®]-20

Cell Extraction Buffer: One bottle containing 20 mL of 1X buffer. For long term storage (over 3 months), store at -20°C.

Dilution Buffer: One bottle containing 50 mL each of 1X buffer; use for sample dilution. Ready to use.

Phospho-p53 Ser392 Standard: One vial containing 240 units of lyophilized phosphorylated p53 Ser392.

Primary Antibody Solution (Anti-Phospho-p53 Ser392 Monoclonal Antibody FPS392): One vial containing 12 mL of Anti-Phospho-p53 Ser392 monoclonal antibody. Ready to use.

Secondary Antibody Solution (HRP conjugated Anti-Mouse IgG): One vial containing 12 mL of HRP (horseradish peroxidase) conjugated anti-mouse IgG antibody. Ready to use.

Substrate Reagent: One bottle containing 20 mL of the chromogenic substrate, tetra methylbenzidine (TMB). Ready to use.

Stop Solution: One bottle supplied ready to use, containing 20 mL of 1 N H₂SO₄.

Materials Required but not Provided

- **Protease inhibitor cocktail:** ex Sigma Cat. # P-2714 (reconstituted according to manufacturer's guideline). Add 250 µL per 5 mCcell Extraction Buffer.
- Orbital microplate shaker
- Pipettors: 2-20 µL, 20-200 µL and 200-1000 µL precision pipettors with disposable tips.
- Precision repeating pipettor
- Microcentrifuge and tubes for sample preparation.
- Vortex mixer
- Microplate washer: optional (Manual washing is possible but not preferable)
- **Plate reader** capable of measuring absorbance in 96-well plates at dual wavelengths of 450 nm/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. The plate can also be read at a single wavelength of 450 nm, which will give a somewhat higher reading.
- Software package facilitating data generation and analysis :optional
- 500 or 1000 mL graduated cylinder
- Reagent reservoirs
- · Deionized water of the highest quality
- Disposable paper towels

CY-7051



Precautions and Recommendations

- All microplate strips that are not immediately required should be returned to the zip-lock pouch, which must be carefully resealed to avoid moisture absorption.
 Do not use kit components beyond the indicated kit expiration date.
 Use only the microtiter wells provided with the kit.
 Rinse all detergent residue from glassware.
 Use deionized water of the highest quality.

- Use deionized water of the highest quality.
- Do not mix reagents from different kits.

CY-7051

- The buffers and reagents in this kit may contain preservatives where chemicals. Care should be taken to avoid direct contact with these reagents.
- Do not mouth pipette or ingest any of the reagents.
- Do not smoke, eat, or drink when performing the star or in areas where samples or reagents are handled.
- Dispose of tetra-methylbenzidine (TMB) containing solutions in compliance with local regulations.
- Avoid contact with the acidic Stop Solution and Substrate Solution, which contains hydrogen peroxide.
- Wear gloves and eye protection when handling immunodiagnostic materials and samples of human origin, and these reagents. In case of contact with the Stop Solution and the Substrate Solution, wash skin thoroughly with water and secondical attention, when necessary. \mathcal{D}
- Biological samples may be cataminated with infectious agents. Do not ingest, expose to open wounds or breathe aerosole. Wear protective gloves and dispose of biological samples properly.
- CAUTION: Sulfuric Arid is a strong acid. Wear disposable gloves and eye protection when handling Stop Solution. The Putpose

Version#: 140318



Detailed Protocol

The CycLex Research Product **CycLex Phospho-p53 Ser392 ELISA Kit** is provided with removable strips of wells so the assay can be carried out on separate occasions using only the number of strips required for the particular determination. Since experimental conditions may vary, an about of the Phospho-p53 Standard within the kit, should be included in each assay as a calibrator. Disposable pipette tips and reagent troughs should be used for all liquid transfers to avoid cross-contamination of reagents or samples.

Preparation of Working Solutions

All reagents need to be brought to room temperature prior to the assay. Assay reagents are supplied ready-to-use, with the exception of 10X Wash Buffer, Cell Extraction Buffer and Phospho-p53 Ser392 Standard.

- 1. Prepare a working solution of Wash Buffer by adding 100 mL of the **JOX Wash Buffer** to 900 mL of deionized (distilled) water (ddH₂O). Mix well.
- 2. Prepare a working solution of Cell Extraction Buffer by addine 250 μL of Protease inhibitor cocktail (Sigma Cat. # P-2714) to 5 mL of **Cell Extraction Buffer**. Mix well.
- 3. Reconstitute **Phospho-p53 Ser392 Standard** with **1** of **ddH**₂**O**. The concentration of the phospho-p53 Ser392 in vial should be <u>200 units/mL</u>, which is referred as a **Master Standard** of phospho-p53 Ser392.

Prepare Standard Solutions as follows:

Use the **Master Standard** to produce a **diu**tion series (below). Mix each tube thoroughly before the next transfer. The 100 units/mL standard (Std.1) serves as the highest standard. The **Dilution Buffer** serves as the zero standard (**Blant**).

	Volume of Standard	Dilution Buffer	Concentration
Std.1	300 µL of Master Standard	300 µL	100 units/mL
Std.2	300 µL of Std (100 units/mL)	300 µL	50 units/mL
Std.3	300 µL of Std. 2 (50 units/mL)	300 µL	25 units/mL
Std.4	300 µL of Std. 3 (25 units/mL)	300 µL	12.5 units/mL
Std.5	300 µL of Std. 4 (12.5 units/mL)	300 µL	6.25 units/mL
Std.6	300 µL of Std. 5 (6.25 units/mL)	300 µL	3.13 units/mL
Std.7	200 µL of Std. 6 (3.13 units/mL)	300 µL	1.56 units/mL
Blank	-	300 µL	0 units/mL

Note: Do not use a Repeating pipette. Change tips for every dilution. Wet tip with Dilution Buffer before dispensing. Unused portions of Standards should be aliquoted and stored at below -70°C immediately. Avoid multiple freeze and thaw cycles.

CY-7051



hat came with your out of the second Phospho-p53 Ser392 ELISA Kit User's Manual For Research Use Only, Not for use in diagnostic procedures

Assay Procedure

A. Treatment of Cells with compounds

- 1. Plate adherent cells or non-adherent cells in culture flasks at 50-70 % confluency.
- 2. Incubate the culture flasks at 37°C over night in CO₂ incubator.
- 3. Add appropriate amount of test compounds to each flask.
- 4. Incubate the culture flasks at 37°C for appropriate time.

B. Cell Extraction

- Note: This protocol has been successfully applied to several cell lines. Users should optimize the cell extraction procedure for their own applications.
- 1. Collect cells in PBS by centrifugation (non-adherent cells) of craping from culture flasks (adherent cells).
- 2. Wash cells twice with cold PBS.
- 3. Remove and discard the supernatant and collect the sel pellet. At this point the cell pellet can be frozen at below $-70^{\circ}C$ and lyse at a later date.
- 4. Lyse the cell pellet in 0.5 mL* of Cell Extraction Buffer for 30 minutes, on ice, with vortexing at 10-minute intervals.

* To get a rough idea you could adjust the cell concentration to around 2 x 10^7 cells/mL. Resulting protein concentration of the cell lysate should be 2-4 mg/mL using this Cell Extraction Buffer.

* The volume of Cell Baraction Buffer depends on the cell number in cell pellet and phosphorylation level p53. For example, <u>1.2 x 10⁷</u> MCF-7 cells (in 10 cm dish) can be extracted in 0.5 mL & Cell Extraction Buffer. Under these conditions, the protein concentration should be <u>2-4 mg/mL</u>, and use of <u>5-10 μ L</u> of the clarified cell extract diluted to a volume of 100 μ l/well in Dilution Buffer is sufficient for the detection of phospho-p53 Ser392.

- 5. Transfer the lysates b microcentrifuge tubes and centrifuge at 13,000 rpm for 10 minutes at 4°C.
- 6. Aliquot the clear lysate to clean microfuge tubes. These samples are ready for assay. The lysates can be stored at below -70°C. Avoid multiple freeze/thaw cycles.

NOTE: THE ABOVE PROCEDURES ARE INTENDED ONLY AS A GUIDELINE. THE **OPTIMAL EXPERIMENTAL CONDITIONS WILL VARY DEPENDING ON THE** PARAMETERS BEING INVESTIGATED, AND MUST BE DETERMINED BY THE INDIVIDUAL USER. NO WARRANTY OR GUARANTEE OF PERFORMANCE USING THESE PROCEDURES IS MADE OR IMPLIED.


CY-7051



C. ELISA

- 1. Remove the appropriate number of microtiter wells from the foil pouch and place them into the well holder. Return any unused wells to the foil pouch, refold, seal with tape and store at 4°C.
- 2. Dilute the lysate 1:10* with Dilution Buffer (e.g. $30 \,\mu\text{L}$ sample + $270 \,\mu\text{L}$ Dilution Buffer)
- * Lysates prepared in Cell Extraction Buffer must be diluted 1:10 or greater in Diluter Buffer. While a 1:10 lysate dilution has been found to be satisfactory, higher dilutions such as 1:40 may be optimal. The dilution chosen should be optimized for each experimental system.
- 3. Pipette 100 µL of Standard Solutions (Std1-Std7, Blank) and diluted lysates in duplicates, into the appropriate wells.
- 4. Incubate the plate <u>at room temperature (ca. 25°C) for 1 hour</u>, shaking at ca. 300 rpm on an orbital <u>microplate shaker</u>.
- 5. Wash 4-times by filling each well with Wash Buffer (350 µc using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer*.
- 6. Add 100 μL of Primary Antibody Solution into each well
- 7. Incubate the plate <u>at room temperature (ca. 25°C) for 1 hour</u>, shaking at ca. 300 rpm on an orbital <u>microplate shaker</u>.
- 8. Wash 4-times by filling each well with Wash Buffer (350 μL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
- 9. Add 100 µL of Secondary Antibody Solution into each well.
- 10. Incubate the plate <u>at room temperature (ca. 25°C) for 1 hour</u>, shaking at ca. 300 rpm on an orbital <u>microplate shaker</u>.
- 11. Wash 4-times by filling each well with Wash Buffer (350 µL) using a squirt bottle, multi-channel pipette, manifold dispenser or microplate washer.
- 12. Add **100** μ L of **Substrate Reagent**. (Avoid exposing the microtiter plate to direct sunlight Covering the plate with e.g. alumnum foil is recommended). Return Substrate A to 4°C immediately after the necessary volume is removed
- 13. Incubate the plate at room temperature (ca. 25°C) for 10-20 minutes, shaking at ca. 300 rpm on an orbital microplate shaker. (The incubation time may be extended up to 30 minutes if the reaction temperature is below than 20°C).
- 14. Add **100 µL of Stop Solution** to each well in the same order as the previously added Substrate Reagent.
- 15. Measure absorbance in each well using a spectrophotometric microplate reader at dual wavelengths of 450/540 nm. Dual wavelengths of 450/550 or 450/595 nm can also be used. Read the microplate at 450 nm if only a single wavelength can be used. Wells must be read within 30 minutes of adding the Stop Solution.

CY-7051 Cat#:





User's Manual

For Research Use Only, Not for use in diagnostic procedures

- **Note-1:** Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
- **Note-2:** Reliable standard curves are obtained when either O.D. values do not exceed the units for the blank (zero concentration), or 2.5 units for the highest standard concentration. The plate should be monitored at 5-minute intervals for approximately 30 minutes.
- **Note-3**: If the microplate reader is not capable of reading absorbance greater than the absorbance of the highest standard, perform a second reading at 405 nm. A new standard curve, constructed using the values measured at 405 nm, is used to determine Phospho-p53 Ser392 concentration of off-scale samples. The readings at 405 nm should not replace the on-scale readings at 450 nm.


Calculations

Average the duplicate readings for each standard, control, and sample and subtract the average zero standard optical density. Plot the optical density for the standards versus the concentration of the standards and draw the best curve. The data can be linearized by using log/log paper and regression analysis may be applied to the log transformation. To determine the Phospho-p53 Ser392 concentration of each sample, first find the absorbance value on the y-axis and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the x-axis and read the corresponding Phospho-p53 Ser392 concentration. If the samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

- A. The dose-response curve of this assay fits best to a sigmoidal 5-parameter logistic equation. The results of unknown samples can be calculated with any computer program having a 5-parameter logistic function. It is important to make an appropriate mathematical adjustment to accommodate for the dilution factor.
- B. Most microtiter plate readers perform automatic calculations of analyte concentration. The calibration curve is constructed by plotting the absorbance (Y) of calibrators versus log of the known concentration (X) of calibrators, using the four-parameter function. Alternatively, the logit log function can be used to linearize the calibration curve (i.e. logit of absorbance (Y) is plotted versus log of the known concentration (X) of calibrators).

Measurement Range

The measurement range is 1.56 units/mL to 100 units/mL. Any sample reading higher than the highest standard should be diluted with Dilution Buffer in higher dilution and re-assayed. Dilution factors need to be taken into consideration in calculating the phospho-p53 Ser392 concentration.

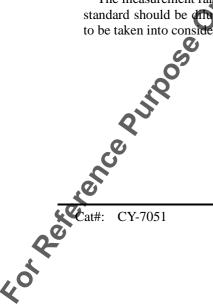



User's Manual

For Research Use Only, Not for use in diagnostic procedures

Troubleshooting

- 1. The Human Phospho-p53 Ser392 Standard should be run in duplicate, using the protocol described in the **Detailed Protocol**. Incubation times or temperatures significantly different from those specified may give erroneous results.
- 2. Poor duplicates, accompanied by elevated values for wells containing no sample, indicate insufficient washing. If all instructions in the **Detailed Protocol** were followed accurately, such results indicate a need for washer maintenance.
- 3. Overall low signal may indicate that desiccation of the plate has occurred between the final wash and addition of Substrate Reagent. <u>Do not allow the plate to dry out</u>. Add Substrate Reagent immediately after wash.

Reagent Stability

All of the reagents included in the CycLex Research Product **CycLex Phospho-p53 Ser392 ELISA Kit** have been tested for stability. Reagents should not be used beyond the stated expiration date. Upon receipt, kit reagents should be stored at 4°C, except the reconstituted Human Phospho-p53 Ser392 Standard must be stored at below -70°C. Coated assay plate should be stored in the original foil bag sealed by the zip lock and containing a desiccant pack.

For research use only, not for use in diagnostic or the apeutic procedures

Assay Characteristics

1. Sensitivity

The limit of detection (defined as such a concentration of Phospho-p53 Ser392 giving absorbance higher than mean absorbance of blank* Ous three standard deviations of the absorbance of blank: A blank + 3*SD blank) is better than 1.413 units/ml of sample.

* Dilution Buffer is pipetted into blank wells.

Eighty assays were evaluated and the minimum detectable dose (MDD) of Phospho-p53 Ser392 ranged from 0.723 - 1.624 units/mL. The mean MDD was 1.413 units /mL. The MDD was determined by adding three standard deviations to the mean optical density value of twenty zero standard replicates and calculating the corresponding concentration.

2. Specificity

The antibodies in the CycLex Phospho-p53 Ser392 ELISA Kit are highly specific of human Phospho-p53 Ser392, with no detectable cross-reactivity to mouse and rat Phospho-p53.

3. Linearity

To assess the linearity of the assay, samples containing and/or spiked with high concentrations of Phospho.p53 Ser392 were serially diluted with the Dilution Buffer to produce samples with values within the dynamic range of the assay.

CY-7051



Example of Test Results

Fig.1 Typical standard of phospho-p53 Ser392


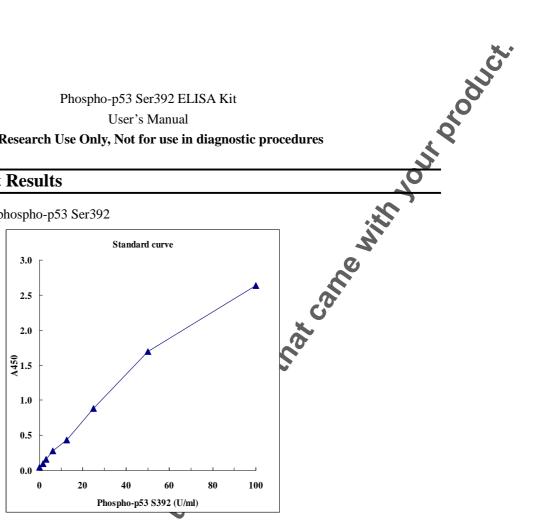


Fig.2 Phospho-p53 Ser392 ELISA using breast cancer cell line MCF-7 that expresses wild type p53, which have been treated with 10 μ M SN-38 for indicated time

140318



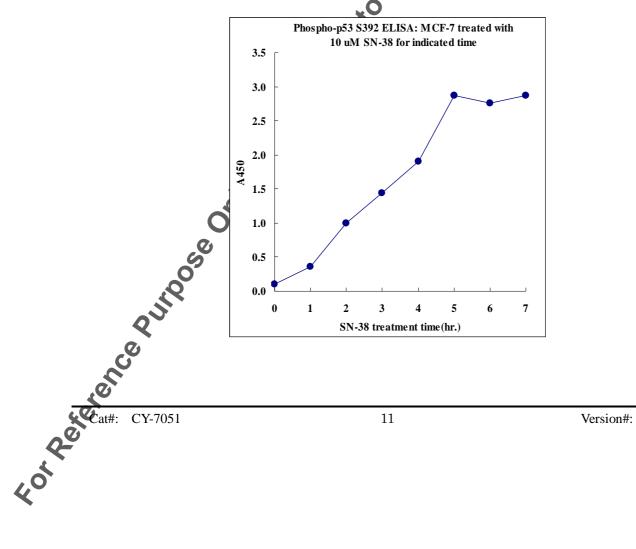

User's Manual

For Research Use Only, Not for use in diagnostic procedures

References

- 1. Levine, A. J. (1997) Cell 88, 323-331
- 2. Donehower, L. A., Harvey, M., Slagle, B. L., McArthur, M. J., Montgomery, C. A., Jr., Butel, J. S., and Bradley, A. (1992) Nature 356, 215-221
- 3. Harvey, M., McArthur, M. J., Montgomery, C. A., Jr., Bradley, A., and Donehower L. A. (1993) FASEB J. 7, 938-943
- 4. Hollstein, M., Sidransky, D., Vogelstein, B., and Harris, C. C. (1991) Science 253,
- 5. Greenblatt, M. S., Bennett, W. P., Hollstein, M., and Harris, C. C. (1994) *Cancer Res.* 54, 4855–4878
- 6. Chen, H. E., Chang, S., Trub, T., and Neel, B. G. (1996) Mol. Cell. Biol. 16, 3685-3697
- 7. Honda, R., Tanaka, H., and Yasuda, H. (1997) FEBS Lett. 420, 25-27
- 8. Kubbutat, M. H., Jones, S. N., and Vousden, K. H. (1997) Nature 387, 299
- 9. Haupt, Y., Maya, R., Kazaz, A., and Oren, M. (1997) Nature 387, 296-299
- 10. McCoy, M. A., Gesell, J. J., Senior, M. M., and Wyss, D. F. (2003) Prop Natl. Acad. Sci. U. S. A. 100, 1645-1648
- 11. Barak, Y., Juven, T., Haffner, R., and Oren, M. (1993) EMBO J. 14,461-468
- 12. Appella, E., and Anderson, C. W. (2001) Eur. J. Biochem. 268, 2764-2772
- 13. Wahl, G. M., and Carr, A. M. (2001) Nat. Cell Biol. 3, E277-E286
- 14. Buschmann, T., Potapova, O., Bar-Shira, A., Ivanov, V. N., Fuchs, S. Y., Henderson, S., Fried, V. A., Minamoto, T., Alarcon-Vargas, D., Pincus, M. R., Gaarte W. A., Holbrook, N. J., Shiloh, Y., and Ronai, Z. (2001) Mol. Cell. Biol. 21, 2743-2754
- 15. Dumaz, N., and Meek, D. W. (1999) EMBO J. 18, 70027010
- 16. Jabbur, J. R., Huang, P., and Zhang, W. (2000) Oncorene 19, 6203-6208
- 17. Oda, K., Arakawa, H., Tanaka, T., Matsuda, K., Chinikawa, C., Mori, T., Nishimori, H., Tamai, K., Tokino, T., Nakamura, Y., and Taya, Y. (2000) Cell 102, 849-862
- 18. Kapoor, M. and Lozano, G., (1998) Proc. Nat Cad. Sci. USA 95, 2834–2837.

- Lu, H., Taya, Y., Ikeda, M. and Levine, A.J. (1998) *Proc. Natl. Acad. Sci. USA* **95**, 6399–6402.
 Hupp, T.R., Meek, D.W., Midgley, C.A. and Lane, D.P. (1992) *Cell* **71**, 875–886.
 Sakaguchi, K., Sakamoto, H., Lewis, M.S., Anderson, C.W., Erickson, J.W., Appella, E. and Xie, D. tot



For Research Use Only, Not for use in diagnostic procedures

Related Products

- * CycLex Total p53 ELISA Kit: Cat# CY-7049
- * CycLex Phospho-p53 Ser46 ELISA Kit: Cat# CY-7050
- * CycLex Phospho-p53 Ser392 ELISA Kit: Cat# CY-7051
- * Anti-Phospho-p53 Ser46 (TK-4D4) monoclonal antibody: Cat# CY-M1022

PRODUCED BY

CycLex Co., Ltd. 1063-103 Terasawaoka Ina, Nagano 396-0002 Japan Fax: +81-265-76-7618 e-mail: info@cyclex.co.jp URL: http://www.cyclex.co.jp

CycLex/CircuLex products are supplied for research use only. CycLex/CircuLex products and components thereof may not be resold, modified for resale, or used to manufacture commercial products without prior written approval from CycLex Co., Ltd.. To inquire about licensing for such commercial use, please contact us via email.

