

Warranty Information

Days Healthcare *Escape* manual wheelchairs are warranted for 12 months from the date of purchase on frame and crossbars.

- During the warranty period any parts that have become defective due to faulty workmanship or material will be repaired or replaced without charge by Days Healthcare supplier/dealer
- The warranty excludes tyres, punctures and items that become worn due to normal wear and tear such as upholstery and armrest pads
- The warranty excludes all items that have been subject to undue wear and tear and misuse
- Unauthorised changes or modifications will forfeit your warranty
- If a defect or fault is discovered, the Days Healthcare supplier/dealer from whom the Wheelchair was purchased should be notified immediately
- The maximum user weight is 100 kg (16 stone)

Limitation of liability

The warranty does not extend to the consequential costs resulting from fault clearance, in particular freight and travel costs, loss of earnings, expenses, etc.

The manufacturer will not accept responsibility for any damage or injury caused by misuse or non-observance of the instructions set out in this user manual.

Dealer Stamp



Days Healthcare Ltd • North Rd • Bridgend Industrial Estate • Bridgend • CF31 3TP
Tel: +44 (0) 1656 664700 • Fax: +44 (0) 1656 664750 • Email: info@dayshealthcare.com

www.dayshealthcare.com



Escape

338 *Escape* LITE

Aluminium Manual Wheelchair



Technical Specifications

	338N	338
Seat Width	41 cm	46 cm
Seat Depth	41 cm	41 cm
Seat Height (front)	50 cm	50 cm
Backrest Height	41 cm	41 cm
Backrest Height (folded)	26 cm	26 cm
Footrest Length (min)	37 cm	37 cm
Footrest Length (max)	53 cm	53 cm
Armrest Height	21 cm	21 cm
Overall Length	90 cm	90 cm
Overall Length (without footrest)	64 cm	64 cm
Overall Width (open)	53 cm	58 cm
Overall Width (folded)	28 cm	28 cm
Overall Height	92 cm	92 cm
Folding Handle Length	20 cm	20 cm
Chair Weight	11.5 kg	11.5 kg
Maximum User Weight	100 kg	100 kg

Maintenance & Inspection

We recommend that your wheelchair is serviced by your local dealer every twelve months. It is in your best interests, not only to ensure your personal safety but also to ensure long life and reliability. Regular service will identify early damage and worn components avoiding unnecessary faults occurring.

Weekly check that:

- Manual brakes do not rub the tyres and secure the wheel when locked
- Castor bolts are tight and all fasteners are secure
- Arms operate and lock securely in front of rear sockets
- The drive wheels axles are secure and there is no excessive side movement or binding when spun
- Tyres do not show excessive wear or damage
- Castors for proper tension, i.e. spinning castors should come to gradual stop

Monthly check that:

- Tyres are not excessively worn
- Handrims do not have sharp edges or any abrasion
- The chair rolls straight (no excessive drag or pull to one side)
- Pivot points are free of wear or looseness
- Seat and backrest upholstery is not for ripped or sagging
- Frames are not worn or bent

Cleaning

Paintwork and plastic mouldings can be cleaned with a damp soft cloth of warm soapy water. Do not use any harsh abrasive cleaners, bleach base fluids or solvents.

Seat and back upholstery can be cleaned with a general purpose upholstery cleaner or sponged with warm soapy water.

Table of Contents

Introduction	4	Footrests	9
Intended Use	4	Manual Brake	9
Technical Description	4	Folding Back	9
Feature Guide	5	Folding the Chair	10
Safety Guidelines	6	Unfolding the Chair	10
Safe Operation	7	Transferring to and from the Chair	11
Adjustment Procedures	8	Tyres	11
Footrest Adjustments	8	Slopes & Gradients	11
Heel and Calf Straps	8	Wheelchair Assistance	12
Backrest Height	8	Transportation	13
Seat Belt	8	Maintenance Inspection	14
Anti-tippers	8	Cleaning	14
Operations of Use	9	Technical Specifications	15

Introduction

Welcome to the Days Healthcare *Escape* manual wheelchair and thank you for choosing our product. This latest model has been designed with specific practical user needs in mind. It combines solid, rugged construction, safety and performance. We are confident that it will prove a reliable companion in your home as well as outdoors.

This manual contains some useful tips and information on safety, operation and maintenance. Please read it carefully to ensure that you get maximum enjoyment and benefit from your new independence and mobility.

Whenever you require special advice and attention do not hesitate to contact your local Days Healthcare dealer. He has all the equipment and know-how to provide an expert service and assistance on technical and clinical applications to suit your particular need.

Intended Use

The *Escape* manual wheelchairs are intended to assist and improve mobility for those individuals who are less able or have walking difficulties who wish to maintain their independence and freedom.

Your day to day activities will depend on your physical capabilities and your own specific circumstances. If in doubt seek medical advice first.

The information in this booklet provides a general guide on how to use your chair safely and correctly. Do not use the chair without reading this manual first.

Technical Description

The Days Healthcare *Escape* manual wheelchair has a maximum carrying capacity of 100 kg (16 stone) which must never be exceeded. It is classified as an 'Invalid Carriage' for use indoors, on pavements, footpaths, pedestrian zones and areas free from motor traffic. Use on the road or highway is not allowed except for the purpose of crossing.

Transportation

We recommend that you do not sit on your wheelchair when in a vehicle, but transfer to a vehicle seat. A wheelchair secured in a vehicle will not provide the equivalent safety level and security as the vehicle's seating systems.

However, when transfer is not practical or impossible, ensure the following:

- 1) Check that the vehicle is suitably designed, insured and equipped to transport a passenger seated in a wheelchair
- 2) Remove any part of the wheelchair (accessories, etc.) that can be easily detached and store it in the vehicle's luggage hold
- 3) Make sure the wheelchair is transported in a forward facing direction. Rearward facing is only acceptable if the passenger's head and back can be supported by a suitable bulkhead
- 4) Use the buckle seat belt (if fitted) with your chair as additional restraint



To assist you in storing the chair for transportation. First remove the footrests, fold down the rear push handles and fold the chair as described in earlier paragraph.

Ensure the back upholstery folds to the rear of the chair and in a tidy manner.

Wheelchair Assistance

Practical Use

Many activities require the wheelchair owner to reach, bend and transfer in and out of the wheelchair. These movements will cause a change to the normal balance, the centre of gravity and weight distribution of the wheelchair.

To determine and establish your particular safety limits, activities involving reaching, bending and transferring should first be practised with a qualified health care professional.

Tilting

WARNING! Do not tilt the wheelchair without assistance.

- 1) The attendant should grasp the push handles securely, making sure that the handle grips are firmly attached.
- 2) Inform the chair occupant before tilting the chair and remind him/her to lean back. Be sure the occupant's feet and hands are clear of all wheels.
- 3) Place one foot on the tipping lever and apply a continuous motion until the balance point is achieved. At this point, the attendant will feel a difference in weight distribution (this usually occurs at about 14° angle).
- 4) Turn the wheelchair in the direction required.
- 5) Lower the front end, placing one foot on the tipping lever and grasping the push handles to **slowly** lower to the ground.



NOTE: After mastering the techniques of tilting the chair, use this procedure to tackle kerbs, steps, etc.

Kerbs

- 1) The attendant should stand on the pavement and turn the chair so that the rear wheels are against the kerb.
- 2) The chair should be tilted back to the balance point and in one continuous movement, the rear wheels should be pulled up and over the kerb.

NOTE: We recommend that two attendants are utilised for this procedure.



Feature Guide

Model No: 338




Safety Guidelines

- ➔ Do not use on the road, except when crossing between pavements. When crossing the carriageway of a public road always take extra care and observe the Highway code
- ➔ Do not ride over deep, soft terrain (soft dirt, loose gravel, deep grass)
- ➔ Do not attempt to mount a kerb without assistance
- ➔ Do not carry passengers
- ➔ We recommend that you do not sit on your wheelchair when in a vehicle, but transfer to a vehicle seat
- ➔ Always engage a slow speed when going down gradients
- ➔ Do not ride in reverse down a slope or kerb
- ➔ Always keep your feet on the footplate when moving
- ➔ Do not stand on the footplate when getting in or out of the chair
- ➔ We recommend the use of safety belt
- ➔ Always keep your pneumatic tyres to the correct pressures
- ➔ Do not use parts, accessories or adapters other than those authorised by Days Healthcare Ltd
- ➔ Keep the wheelchair away from children. It is not intended to be used as a toy
- ➔ The manual parking brakes are not designed for slowing-down

Transferring to and from the Chair

Circumstances and individual needs will vary from person to person, but if there are difficulties we advise you to consult your therapeutic advisor who will help you to develop your skill for appropriate transfer method that suits you.

During transfer always make sure that the brakes are in a locked position and the wheelchair is manoeuvred as close as possible to the transfer seat.



Tyres


Regularly check the condition of front & rear tyres for wear and tear. Contact your supplier for replacements.

If you have pneumatic tyres fitted, the pressure indicated on the side of the tyre wall should not be exceeded.

Slopes and Gradients

Do not attempt to climb or descend beyond your limitations to avoid tipping over.

Note: - When travelling down or up a slope, avoid sharp turns, zigzag movements or moving across the slope

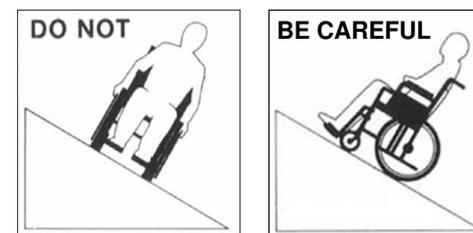


Do not hang or store objects, shopping bags on the push handles or on the back of the chair, as this will affect rear stability.

Folding the Chair

The wheelchair is folded by grasping the seat canvas at the front centre with one hand and at the rear with the other. A simple lifting action will draw both sides of the chair together into the folded position.

Unfolding the Chair

When both wheels have been secured, grasp both side frames of the wheelchair and pull apart as far as possible or at least until there is sufficient room to push down on the sides of the seat canvas.

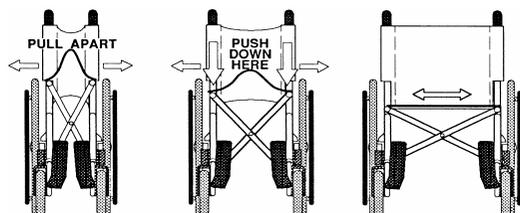

Safe Operation

When using indoors beware of narrow doors, steps, high surfaces, protruding wall fittings and everyday household items such as children's toys, electrical appliances etc. Take extra care in kitchen environments.



To ensure stability and safe control you must maintain proper balance at all times. The wheelchair is designed to remain stable during normal use as long as you do not move your centre of gravity outside the normal seating position.

When reaching/bending forward do not lean your body out of the wheelchair further than the length of the armrests. Do not attempt to reach objects by sliding forwards to the edge of the seat.

When reaching/bending backwards do not reach any further than your arm will extend without changing your seating position.

Never attempt to use an escalator or stairway, always use a lift.

Occasionally check that the adjustments of the footrests are secure and are set in the most comfortable position for use.

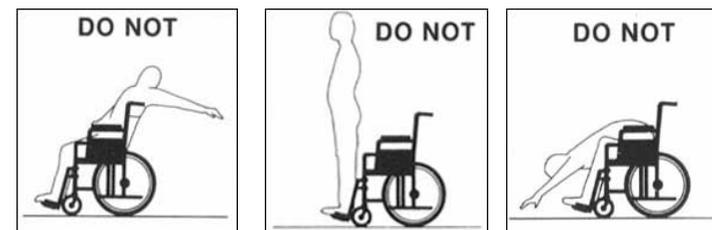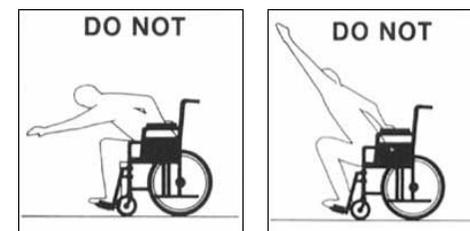


Adjustment Procedures

Footrest Adjustments

Length Adjustment

Adjustments are made with the user sitting in the wheelchair with feet on footplates.

- 1) Use a spanner to loosen the bolt at the bottom of the footrest support hanger.
- 2) Adjust the footplate up or down as needed to provide maximum support of thighs on the seat upholstery, then re-tighten the bolt.



WARNING! Ensure that desired length adjustment does not cause pressure to legs at front of seat upholstery.

Backrest Height

Height adjustment is not available on this model of chair.

Seat Belt (if fitted)

Hold the bayonet end in one hand, and pull on the webbing to increase or decrease belt length with the other. When length is correct, adjust slide buckle to suit.

Anti-tippers (if fitted)

These are fitted at the rear of the chair, adjacent to the rear wheels and Days Healthcare recommends that these are fitted, especially when climbing kerbs and gradients.

Operations of Use

Footrests

Your footrests are capable of being rotating outwards. To achieve this pull the release lever towards you and rotate footrest in the required direction. Lift-off from the two pivot points to remove.



Manual Brake

This is a parking brake which is applied manually to the tyres when the chair is parked or stationary, by an attendant. To apply the brake, pull the lever upwards. The ratchet mechanism will lock the brakes on. To release the brake, pull the small lever upwards, which unlocks the ratchet.

Warning! - Do not push down on the brake lever to avoid damage or breakages



Brake Adjustment

The operation of the brakes can be adjusted to suit. Attached to the brake shoe is an adjusting screw which will vary the tension applied to the brake lever



Folding Back

This is available to reduce the overall height of the chair. Whilst at the rear of the chair, grip the small lever and push down to release pin allowing the handle section to be folded.

