

Genie™ Plus

Syringe Pump

User's Manual

Cat# GENIE Plus



WEEE/RoHS Compliance Statement

EU Directives WEEE and RoHS

To Our Valued Customers:

We are committed to being a good corporate citizen. As part of that commitment, we strive to maintain an environmentally conscious manufacturing operation. The European Union (EU) has enacted two Directives, the first on product recycling (Waste Electrical and Electronic Equipment, WEEE) and the second limiting the use of certain substances (Restriction on the use of Hazardous Substances, RoHS). Over time, these Directives will be implemented in the national laws of each EU Member State.

Once the final national regulations have been put into place, recycling will be offered for our products which are within the scope of the WEEE Directive. Products falling under the scope of the WEEE Directive available for sale after August 13, 2005 will be identified with a "wheelie bin" symbol.

Two Categories of products covered by the WEEE Directive are currently exempt from the RoHS Directive – Category 8, medical devices (with the exception of implanted or infected products) and Category 9, monitoring and control instruments. Most of our products fall into either Category 8 or 9 and are currently exempt from the RoHS Directive. We will continue to monitor the application of the RoHS Directive to its products and will comply with any changes as they apply.



- Do Not Dispose Product with Municipal Waste.
- Special Collection/Disposal Required.

Table of Contents

1

SUBJECT	PAGE NO.
Table of Contents	1
General Information - Warranty and Repairs	2
General Safety Summary	3-4
Introduction	5-6
Theory of Operation	5
Features	5
Genie Plus, Front and Rear Views	6
Installation	7
Initial Setup & Location Requirements	7
Loading the Syringe	7
Limit Switch Calibration	7
Operation.....	8
Getting Started	8
Turn Pump ON	8
Function Keys and Run Indicator.....	8
Entering Syringe Size	9
Entering Flow Rate Range	9
Entering Flow Rate	9
Press Run	9
Check Syringe	9
Advanced Features	10
Volume Mode	10
Power Failure	10
Changing Rates	11
Infuse/Withdraw Switch.....	11
Maintenance.....	11
Protecting Small, Fragile Syringes	12
Remote Communication.....	12
Appendices	
A. Specifications	13
B. Table of Popular Syringe Diameters	14
C. Table of Minimum and Maximum Flow Rates.....	15
D. Serial Communications; Commands, Queries and Responses.....	16,17
E: Serial Port Connections: RS-232	18
Daisy-Chain.....	18
F: Genie Plus to PC Connection	19

General Information

Serial Number

All inquiries concerning our product should refer to the serial number of the unit. Serial numbers are located on the rear of the chassis.

Calibration

All syringe pumps are designed and manufactured to meet their performance specifications at all rated voltages and frequencies. A calibration certificate is available upon request. Contact customer service for details and pricing.

Warranty

Kent Scientific warrants this instrument for a period of one year from date of purchase. At its option, Kent Scientific will repair or replace the unit if it is found to be defective as to workmanship or material.

This warranty does not extend to damage resulting from misuse, neglect or abuse, normal wear and tear, or accident.

This warranty extends only to the original customer purchaser.

IN NO EVENT SHALL KENT SCIENTIFIC BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES. Some states do not allow exclusion or limitation of incidental or consequential damages so the above limitation or exclusion may not apply to you. **THERE ARE NO IMPLIED WARRANTIES OF MERCHANTABILITY, OR FITNESS FOR A PARTICULAR USE, OR OF ANY OTHER NATURE.** Some states do not allow this limitation on an implied warranty, so the above limitation may not apply to you.

If a defect arises within the one-year warranty period, promptly contact your local distributor or **Kent Scientific, 1116 Litchfield St., Torrington, CT 06790-6029, (860) 626-1172.** Goods will not be accepted for return unless an RMA (returned materials authorization) number has been issued by our customer service department. The customer is responsible for shipping charges. Please allow a reasonable period of time for completion of repairs, replacement and return. If the unit is replaced, the replacement unit is covered only for the remainder of the original warranty period dating from the purchase of the original device.

This warranty gives you specific rights, and you may also have other rights which vary from state to state.

Repair Facilities and Parts

Kent Scientific stocks replacement and repair parts. When ordering, please describe parts as completely as possible, preferably using our part numbers. If practical, enclose a sample or drawing. We offer a complete reconditioning service.

CAUTION

This pump is not registered with the FDA and is not for clinical use on human or veterinary patients. It is intended for research use only.

CAUTION
FOR RESEARCH USE ONLY
NOT FOR CLINICAL
USE ON PATIENTS

General Safety Summary

Please read the following safety precautions to ensure proper use of your syringe pump. To avoid potential hazards and product damage, use this product only as instructed in this manual. If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.

To Prevent Hazard or Injury:

Use Proper Power Supply

The pump is supplied with an approved power supply and line cord. To maintain the safety integrity of the device, use only one of the following power supplies:

Ault Inc.

Model:	PW118
Output:	12 VDC, 1.5 A
Input:	100-250 VAC, 50-60 Hz, 0.5A

Cui Inc.

Model:	SA06N12-V
Output:	12 VDC, 2.0 A
Input:	100-240 VAC, 50-60 Hz, 0.8A

Globtek Inc

Model:	GT-4201D-12
Output:	12 VDC, 1.66 A
Input:	100-240 VAC, 50-60 Hz, 0.6A

Use Proper Line Cord

Use only the line cord shipped with the product and make sure line cord is certified for country of use.

Ground the Product

This product is grounded through the return path of the DC power supply. To avoid electric shock, use only approved power supply and line cord with the product.

Make Proper Connections

Make sure all connections are made properly and securely.

Observe all Terminal Ratings

Review the operating manual to learn the ratings on all connections.

General Safety Summary

Avoid Exposed Circuitry

Do not touch any electronic circuitry inside of the product.

Do Not Operate with Suspected Failures

If damage is suspected on or to the product do not operate the product. Contact qualified service personnel to perform inspection.

Observe all Warning Labels on Product

Read all labels on product to ensure proper usage.



CAUTION
Refer to Manual



*Functional Ground
Terminal*

Environmental Conditions

Indoor Use Only

Temperature 4°C to 40°C (40°F to 104°F)

Humidity 20% to 80% RH

Well Ventilated Room

Altitude up to 2000 meters

Mains Voltage Fluctuation not to Exceed $\pm 10\%$ of Nominal

Transient Overvoltage, Category II

Pump is Rated Pollution Degree 2 in Accordance with IEC 664

Introduction

Theory of Operation:

The Genie Plus is designed as a low cost, single or dual syringe infusion pump capable of low to moderate back pressures. The Genie Plus is standard with an infuse limit switch and anti-siphon brackets. Includes an RS232 interface, reversing switch, and a withdraw limit switch.

The pump can hold syringes of any make from 0.5 μ l to 50/60 ml. The diameter of the syringes is entered via the keypad and the internal micro-processor drives a precision stepper motor to produce accurate fluid flow.

Nonvolatile memory stores the last syringe diameter and flow rate along with other configuration data.

The "Power Failure Mode" can be set to either turn the pump off in the event of power failure or to resume pumping when power resumes.

Features:

Bright Display and Easy-To-Use Interface

A two-line 16 character LCD display check along with six membrane keys make this a most attractive but powerful, easy-to-use syringe pump. Only two entries required to start pumping; syringe Inside Diameter (mm) and pumping flow rates. The Flow rate can be changed while the Pump is running.

Two Modes of Operation, Constant Flow Rate and Volume Dispense

The Genie Plus will operate continuously in RATE mode or accurately dispense a specific amount of fluid in VOLUME mode.

Smooth Flow

Enhanced micro-stepping pump profiles deliver very smooth and consistent flow, that is virtually pulse free.

Nonvolatile Memory

The pump remembers its last syringe size, flow rate used and configuration settings.

Power Fail Mode

In a power failure the Pump can either RESUME or STOP pumping when power is returned.



CE Mark Approved

The Genie Plus meets all relevant European EMC and Safety requirements for laboratory equipment.

Genie Plus Front and Rear Views

6

Kent Scientific Genie Plus Syringe Pump

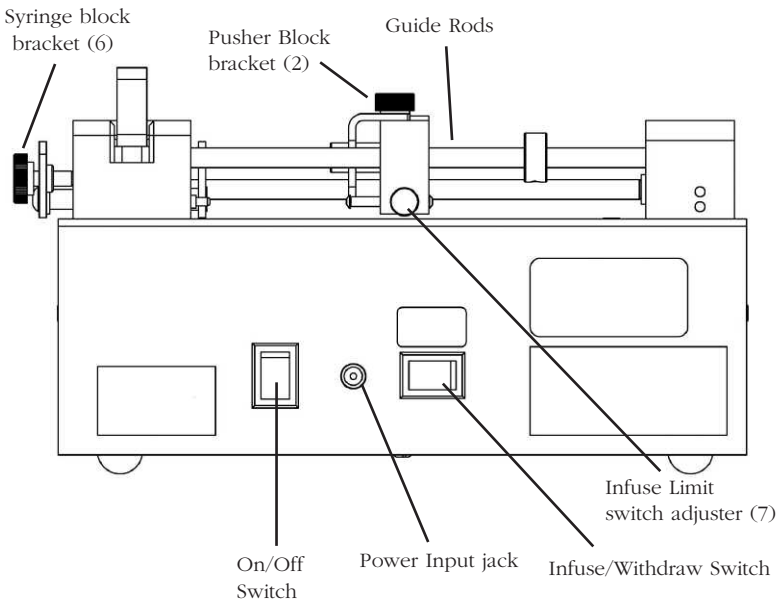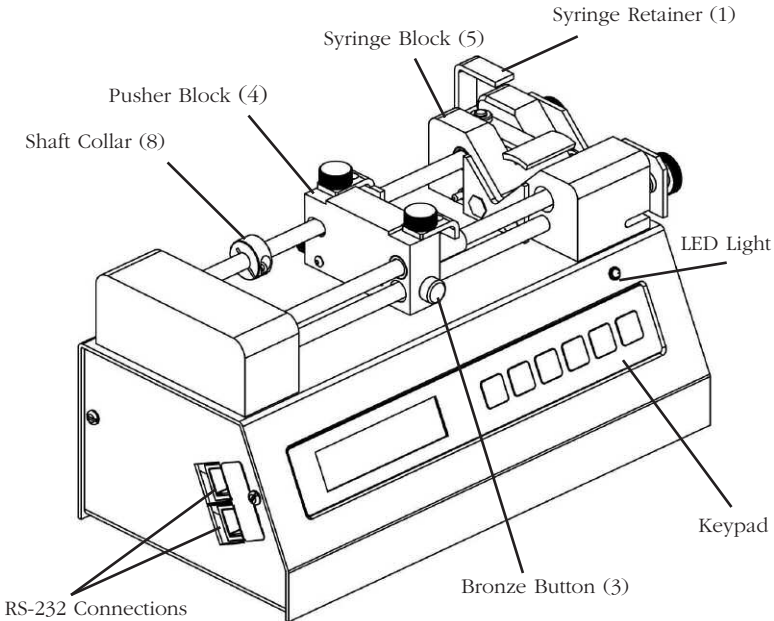

Installation

Initial Setup

1. Read the manual to become familiar with all features and functions of the Genie Plus.
2. Connect the external DC Power Supply and line cord to the pump and main supply.
3. Turn on main power switch located on the rear panel. The display will now illuminate indicating that the power connections are correct. The display will indicate POWER FAIL. (this is normal as the pump indicates on the display if power was disrupted since last use.)

Location Requirements for the Syringe Pump

- A sturdy, level, clean and dry surface
- Minimum of one inch (2 cm) clearance around the pump
- Appropriate environmental conditions
- A well ventilated room

Loading the Syringe & Limit Switch Calibration

1. Release the Syringe pusher block (4) by pressing the bronze button (3) on the side of the pusher.
2. While holding the bronze button 'in', slide the pusher to the right.
3. Raise the spring loaded syringe retainer (1) and swing it out of the way.
4. Lay the loaded syringe in the 'V' shaped syringe block (5).
5. Swing the syringe retainer (1) so it holds the syringe in place.
6. Move the pusher so it makes contact with the syringe plunger.
7. Adjust pusher block thumbscrews and bracket (2) until the syringe plunger is completely captured.
8. Tighten down thumbscrews on syringe block bracket (6) so that it captures flanges on syringe barrel.
9. The Infuse limit switch can be easily adjusted by loosening the thumbscrew (7) on the pusher block and sliding the dowel pin in or out to the desired position. Tighten thumbscrew into place when switch is set.
10. The Withdraw limit switch is adjusted via the shaft collar (8). Slide the collar to the desired position, and use the hex key provided to lock it into place.


Operation: Getting Started

8

Getting started

1. Turn Pump 'ON'

Turn on power using the switch on rear of the pump, the display will light, and indicate POWER FAIL. (this is normal as the pump indicates on the display if power was disrupted since last use.)



2. Function Keys and Run Indicator

Refer to the colored keypad at the front of the pump to identify the following functions starting from the right.

RUN/STOP – This turns the pump motor on and off.

ENTER – This key enters the data that is on the display into the memory of the pump. Also used to query the flow rate.

DIAM – Used to enter or query the syringe diameter.

SET – This key is used to select which digit of the display is to be changed, to move the decimal point and to move between modes. Each time the set key is pressed the underline cursor below the digit or character on the display moves one step to the right. It is used in conjunction with the ascending and descending keys. When it the display shows the desired the correct value the set key will advance right to the next digit.

△▽ – The ascending and descending keys are used to change the numbers on the display. △ Up key makes numbers increase, ▽ Down Key makes numbers decrease. When the underline cursor is placed below the decimal point, the △▽ keys shift the decimal one place up or down.

Run Indicator – When the pump is running, the highly visible, green LED above the RUN/STOP key will illuminate.

Operation: Getting Started

3. *Enter Syringe Size*

Enter the inside diameter (ID) of the syringe you wish to use. Units are in millimeters (mm).

If you do not know your syringe diameter, refer to appendix B for nominal inside diameters of most popular syringes. For the greatest accuracy or if your syringe is not listed in appendix B, measure the inside diameter with a vernier caliper or other precision measuring tool. Record this value for future use.

Press SET followed by the DIAM key. The previously used diameter will appear on the display. The underline cursor will appear under the left-most digit or decimal point. The Δ and ∇ keys are used to scroll to the desired number and the SET key moves the underline cursor one place to the right. Once the desired diameter is displayed, press the ENTER key to place this value into memory.

4. *Enter Flow Rate Range*

Choose your flow rate units; either microliters or milliliters, per minute or per hour.

From the initial RATE VOL CONFIG menu, using the Δ or ∇ key, move the underline cursor under the CONFIG mode menu prompt. Press the SET key to enter the CONFIG mode. Press the SET key again to move the underline cursor to the flow rate choices. Choose your flow rate units while in the SET:UNITS mode by pressing the Δ or ∇ keys to scroll the four flow rate choices; ml/min, μ l/min, ml/hr, μ l/hr. Once the desired flow rate units are displayed, press the ENTER key to return to the main SET:CONFIG mode. Press SET or ENTER again to put your desired flow rate units into memory and return to the RATE VOL CONFIG menu. These units will be the same for infuse and withdraw.

5. *Enter Flow Rate*

From the initial RATE VOL CONFIG menu, press the SET key to enter the SET:RATE mode. Each time you change the syringe diameter, the previously used flow rate is erased. If the syringe diameter is unchanged, the previously used flow rate will appear on the display. The underline cursor will appear under the left-most digit or decimal point. The Δ and ∇ keys are used to scroll to the desired number and the SET key moves the underline cursor one place to the right. Once the desired rate is displayed, press the ENTER key to place this value into memory. This value will be the same for infuse and withdraw.

Operation: Advanced Features

6. **Press RUN**

Press the RUN/STOP key to start pump and begin pumping. The Run Indicator (Green LED above the RUN/STOP key) will light when the pump is on and pumping.

7. **Check Syringe Often**

The Genie Plus will shut itself off via the limit switches. It will not shut off if the switches are set incorrectly, and the syringe is empty or otherwise overloaded. Although this presents no hazard to the user or the pump, it is prudent to check the syringe from time to time.

1. **Volume Mode**

The Genie Plus can be set to dispense a precise volume and then stop. To activate the volume dispense mode a target volume must be set.

To set a target volume, at the RATE VOL CONFIG display, move the underline cursor, using the Δ or ∇ key, to VOL. Press the SET key to enter the VOL set mode. Use the Δ or ∇ key and the SET key to display a target volume from 00.01 to 99.99. Volume units are either ml (milliliters) or μ l (microliters). Target volume units are established in the CONFIG SET:UNITS mode; example: if your pumping units are ml/ min or ml/ hr, then the volume dispense units will be ml's. Press the ENTER key to select the desired target volume. Exit the VOL mode by pressing the ENTER key.

Once you press the RUN key, the pump will run until the target volume is delivered. The display will show the actual volume dispensed along with the target volume. Press the RUN key each time you want to repeat the volume dispense. If you press the STOP key during a volume dispense, you can restart the pump at the place you stopped by pressing the RUN key again.

To exit the volume dispense mode, set the target volume to 00.00 or turn off and on the pump via the main power switch. NOTE: In the event of a power failure, the actual dispensed volume and the target volume are not retained in memory. This means that while in volume dispense mode, if a power failure occurred, the pump would not resume volume dispense pumping even if the POWER ON mode was set to run. This mode will function for both infuse and withdraw.

Operation: Advanced Features

2. *Power Failure*

In the event of a momentary or prolonged power failure, the Genie Plus can be set to either;

- a) Resume pumping when power is returned, with “POWER FAIL” on the display.
- b) Not start pumping when power is returned, with “POWER FAIL” on the display.

To set the power fail mode, at the RATE VOL CONFIG display, move the underline cursor, using the Δ or ∇ key, to CONFIG. Press the SET key to enter the CONFIG mode options. Use the Δ or ∇ key to scroll the CONFIG options until you reach the SET:POWER ON: display. Press the SET key again moving the underline cursor to the right. Use the Δ or ∇ key to scroll the POWER:ON choices; ‘stop’ or ‘run’. Press the ENTER key to select either mode. Exit the CONFIG mode by pressing the ENTER key again and save the POWER:ON setting in memory.

3. *Changing Rates*

If the pump is running at an existing rate it will continue to do so until a new rate is entered. Except for volume mode, the flow rate can be changed while the pump is running. As soon as the ENTER key is pressed the pump will change to the new flow rate. To change rates from the keypad, while in volume mode, the pump must be stopped first.

4. *Infuse/Withdraw Switch Operation*

For customer convenience, a two position rocker switch is included in the Genie Plus for changing from infuse to withdraw on the fly. When the pump is infusing, and the switch is toggled, the pump will now be in the withdraw mode. Switch the toggle again, it puts it back into infuse mode. The physical position of the switch does not matter. The pump always powers up in infuse mode.

5. *Maintenance*

Keep the pump clean and dry. Avoid liquid spills that may find their way into the electronics. To clean the exterior surfaces, use a lint-free cloth to remove loose dust. Use care to avoid scratching the display window. For more efficient cleaning, use a soft cloth dampened with water or an aqueous solution of 75% isopropyl alcohol. If the pump does not work properly, contact Kent Scientific for appropriate instructions.

6. *Protecting Small, Fragile Syringes*

The Genie Plus will hold microliter size syringes down to 10 μl size. These small syringes have fine wire plungers that may be damaged if allowed to bottom out. The pump is equipped with limit switches to help in avoiding this problem. (See page 7 for instructions on use.)

7. *Remote Communication*

The Genie Plus is equipped at the factory for remote serial communications. The baud rate and address are set in the CONFIG mode options.

a. Pump Address

To set the pump address, at the RATE VOL CONFIG display, move the underline cursor, using the Δ or ∇ key, to CONFIG. Press the SET key to enter the CONFIG mode options. Use the Δ or ∇ key to scroll the CONFIG options until you reach the SET:ADDRESS. Press the SET key again moving the underline cursor to the right. Use the Δ or ∇ key to scroll the two digit number fields. Use the Δ or ∇ key and the SET key to display a unique pump address from 00 to 99. Press the ENTER key to select the desired pump address. Exit the CONFIG mode by pressing the ENTER key again and save the ADDRESS setting in memory.

b. Baud Rate

To set the pump Baud Rate, at the RATE VOL CONFIG display, move the underline cursor, using the Δ or ∇ key, to CONFIG. Press the SET key to enter the CONFIG mode options. Use the Δ or ∇ key to scroll the CONFIG options until you reach the SET:BAUD. Press the SET key again moving the underline cursor to the right. Use the Δ or ∇ key to scroll the SET:BAUD choices; '300', '1200', '2400' or '9600'. Press the ENTER key to select the desired baud rate. Exit the CONFIG mode by pressing the ENTER key again and save the BAUD setting in memory.

Appendix A

Genie Plus Specifications

Type	Microprocessor single syringe
Syringe/Size for Genie Plus:	
Type	Plastic or glass syringes
Size	From 0.5 µl to 50/60 ml
Flow Rate Range:	
Minimum / Maximum	0.0028 µl/hr with 0.5 µl syringe / 53.11 ml/min with 50/60 ml syringe
Flow Rate Accuracy	Typically ±1%
Calibration	Automatic, enter syringe size up to 35 mm Inside Diameter
Display	2 line, 16 character LCD display with back light and green run LED
Nonvolatile Memory	Stores diameter, rate and configuration settings
Maximum Force	25 pounds
Maximum Pressure	8 p.s.i. with 50/60 cc syringe; 100 p.s.i. with 1 ml syringe
Drive Motor	1.8° step angle motor
Step Rate:	
Minimum / Maximum	1 pulse in 27.6 sec / 200 steps/sec
Pusher Advance/Step	1.6 µm pusher advance per motor step
Pusher Travel Rate:	
Minimum / Maximum	1.4 µm/min / 30 mm/min
Dynamic Range	1 to 16,384
Leakage to Ground	Typically < 150 µA
Ground Resistance	Typically < 0.05 ohms
Input Power	12 VDC 1.5Amps
Input Power Connection	2.5 mm ID x 5.5 mm OD male plug
Power Supply	100/250 VAC, 50/60 Hz, 18 Watts Universal Power Supply, Use Only Kent Scientific Approved Power Supply and Line Cord, see page 3.
Size, H x W x D	11.4 x 22.9 x 11.4 cm (4.5 x 9 x 4.5 in)
Weight	2.2 kg (4.8 lb)

Appendix B: Syringe Inside Diameter

14

Kent Scientific Genie Plus Syringe Pump

<i>Terumo</i>		<i>Stainless Steel</i>		<i>SGE</i>	
<u>Size</u>	<u>Diameter</u>	<u>Size</u>	<u>Diameter</u>	<i>Scientific Glass Engineering</i>	
3 cc	8.95 mm	8 cc	9.525 mm	<u>Size</u>	<u>Diameter</u>
5	13.00	20 cc	19.130	25 µl	0.73 mm
10	15.80	50 cc	28.600	50	1.03
20	20.15	<i>Becton Dickinson</i>		100	1.46
30	23.10	<i>Plastic "Plasticpak"</i>		250	2.30
60	29.10	<u>Size</u>	<u>Diameter</u>	500	3.26
<i>Sherwood Monoject</i>		1 cc	4.78 mm	1.0 ml	4.61 mm
<i>Plastic</i>		3	8.66	2.5	7.28
<u>Size</u>	<u>Diameter</u>	5	12.06	5	10.30
1 cc	4.65 mm	10	14.50	10	14.57
3	8.94	20	19.13	<i>Hamilton Microliter</i>	
6	12.70	30	21.70	<i>Series Gastight</i>	
12	15.90	50/60	26.70	<u>Size</u>	<u>Diameter</u>
20	20.40	<i>Air Tite "All Plastic"</i>		0.5 µl	0.103 mm
35	23.80	<u>Size</u>	<u>Diameter</u>	1	0.1457
60	26.60	2.5 cc	9.60 mm	2	0.206
<i>Popper & Sons, Inc.</i>		5.0	12.45	5	0.3257
<i>"Perfektum" Glass</i>		10	15.90	10	0.460
<u>Size</u>	<u>Diameter</u>	20	20.05	25	0.729
0.25 cc	3.45 mm	30	22.50	50	1.031
0.5	3.45	50	29.00	100	1.46
1	4.50	<i>Unimetrics</i>		250	2.3
2	8.92	<i>Series 4000 & 5000</i>		500	3.26
3	8.99	<u>Size</u>	<u>Diameter</u>	1.0 ml	4.61 mm
5	11.70	10 µl	0.460 mm	2.5	7.28
10	14.70	25	0.729	5	10.3
20	19.58	50	1.031	10	14.57
30	22.70	100	1.460	25	23.0
50	29.00	250	2.300	50	32.6
		500	3.260		
		1000	4.610		

Appendix C: Flow Rates

nominal syringe size	nominal diameter (mm)	µl/hr		µl/min		ml/hr		ml/min	
		min	max	min	max	min	max	min	max
Min	0.10	0.0028	44.70	0.0002	0.7450	0.0002	0.0446	0.0002	0.0006
1 µl	0.15	0.0062	100.58	0.0002	1.6766	0.0002	0.1004	0.0002	0.0016
2 µl	0.21	0.0122	197.16	0.0004	3.2860	0.0002	0.1970	0.0002	0.0032
5 µl	0.33	0.0298	486.8	0.0006	8.114	0.0002	0.4868	0.0002	0.0080
10 µl	0.46	0.0578	946.0	0.0010	15.766	0.0002	0.9460	0.0002	0.0156
25 µl	0.73	0.1456	2,382	0.0026	39.70	0.0002	2.382	0.0002	0.0396
50 µl	1.03	0.2896	4,742	0.0050	79.04	0.0004	4.742	0.0002	0.0790
100 µl	1.46	0.5818	9,530	0.0098	158.82	0.0006	9.530	0.0002	0.1588
250 µl	2.30	1.4436	19,998	0.0242	394.0	0.0016	23.64	0.0002	0.3940
1,000 µl	3.26	2.902	19,998	0.0484	791.4	0.0030	47.50	0.0002	0.7918
1 ml	4.61	5.800	19,998	0.0968	1583.6	0.0058	95.00	0.0002	1.5836
2.5 ml	7.28	14.464	19,998	0.2412	3,948	0.0146	236.8	0.0004	3.948
3 ml	8.66	20.48	19,998	0.3412	5,588	0.0206	335.2	0.0004	5.588
5 ml	10.30	29.00	19,998	0.4826	7,904	0.029	474.2	0.0006	7.904
10 ml	14.57	57.94	19,998	0.9656	15,818	0.0580	949.0	0.0010	15.818
20 ml	20.05	109.72	19,998	1.8284	19,998	0.1098	1797.2	0.0020	29.94
30 ml	23.10	145.62	19,998	2.428	19,998	0.1458	2,384	0.0026	39.76
50 ml	53.40	194.54	19,998	3.244	19,998	0.1946	3,152	0.0034	53.12
Max	35.00	334.4	19,998	5.572	19,998	0.3344	5,476	0.0056	91.28

Commands, Queries and Responses

After each transmission to the pump terminating with a CR character (ASCII 13), the pump enters remote mode and responds with the three character sequence:

CR LF *prompt*

The prompt character indicates the status of the pump as follows:

<u><i>prompt</i></u>	<u>meaning</u>	<u>ASCII code</u>
:	When stopped	(ASCII 58 decimal)
>	When running forward	(ASCII 62 decimal)
*	When stalled	(ASCII 42 decimal)
<	When in Reverse	Genie Plus does not include
stall		detection

Serial commands and their meanings:

Commands:

KEY	Return to keyboard control. Exit remote mode
RUN	Start infuse (forward direction)
STP	Stop motor
CLV	Clears volume accumulator to zero
CLT	Clears target volume to zero, dispense disabled
REV	Start (Reverse Direction)

Commands with numbers:

MMD	number	Set syringe diameter, units are mm. Rate is set to zero after MMD command.
ULM	number	Set flow rate and range, units are microliters per minute
MLM	number	Set flow rate and range, units are milliliters per minute
ULH	number	Set flow rate and range, units are microliters per hour
MLH	number	Set flow rate and range, units are milliliters per hour
MLT	number	Set target infusion volume, units are ml or µl depending on range

Numbers can be between 0 and 1999.

Leading zeros and trailing decimal point are optional. Any number of digits to the right of the decimal point may be transmitted. The number will be rounded.

Queries:

DIA	Returns diameter value units in mm
RAT	Returns rate value set in current range units
VOL	Returns current accumulated infused volume, units in ml or µl depending on range
VER	Returns model and version number of firmware
TAR	Returns target volume, units in ml or µl depending on range

value format: nnnn.nnn

The returned value is an 8 character string with leading zeros converted to SP characters (ASCII 32 decimal). The fifth character is a decimal point (ASCII 46 decimal)

Queries with string response:


RNG	Returns range message (character string either: ML/H ML/M UL/H UL/M)
------------	----------------------------------------------------------------------

Error responses:

CR LF ? CR LF prompt	Unrecognized command
CR LF OOR CR LF prompt	Entered value in out of range

Pump Chain


Pump Port 1 (in)	- Computer control side
Pump Port 2 (out)	- Connection for remainder of pump chain
Baud Rate	- 300, 1200, 2400 or 9600
Word Size	- 8
Parity	- none
Stop Bits	- 2

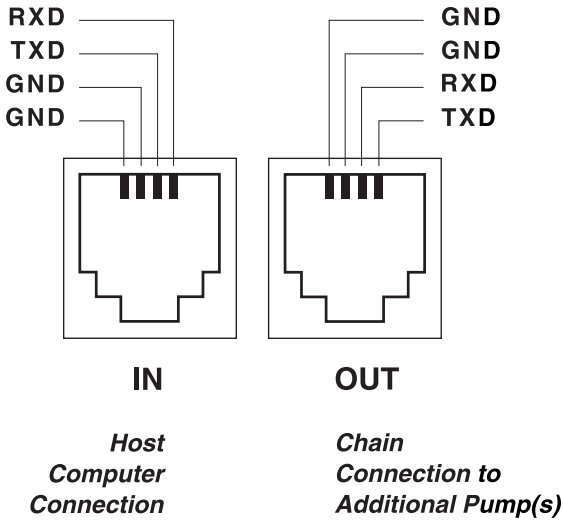


Daisy-Chain Connector & Cables

Part No.	Description
GN-PC7	Primary 7' network PC to pump cable
GN-PC25	Primary 25' network PC to pump cable
GN-NET7	Secondary 7' network cable
GN-NET25	Secondary 25' network cable

Appendix F: PC Connection

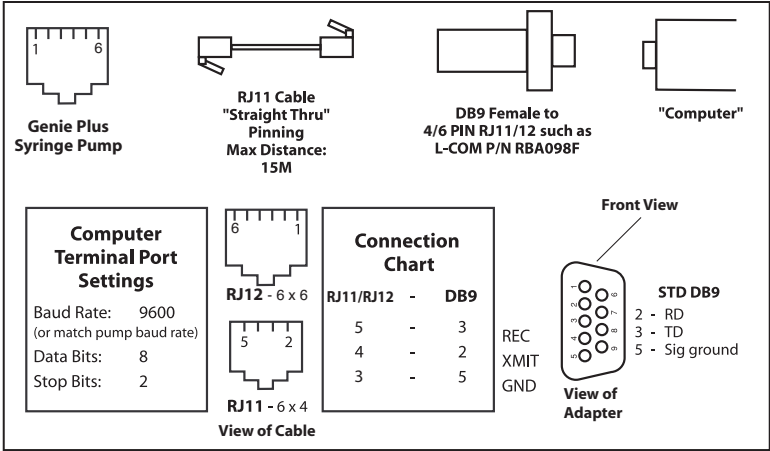



Kent Scientific
C O R P O R A T I O N

Declaration of Conformity

Application of

Council Directive(s):

72/23/EEC, 89/336/EEC

Standard(s) to which

Conformity is declared:

EN61010-1 (1993) + A2 (1995)

EN 61326: 1997 + A1: 1998

Class A Emissions, Class B Immunity

Manufacturer's Name:

Kent Scientific

Manufacturer's Address:

1116 Litchfield St.

Torrington, CT 06790

USA

Type of Equipment:

Syringe Pump

Model No:

Genie Plus