



**AssayMax™**

# **Human Lysozyme ELISA Kit**

Assaypro LLC  
3400 Harry S Truman Blvd  
St. Charles, MO 63301  
T (636) 447-9175  
F (636) 395-7419  
[www.assaypro.com](http://www.assaypro.com)

For any questions regarding troubleshooting or performing the assay, please contact our support team at [support@assaypro.com](mailto:support@assaypro.com).

Thank you for choosing Assaypro.

## Assay Summary

**Step 1.** Add 25  $\mu\text{l}$  of Standard or Sample and 25  $\mu\text{l}$  of Biotinylated Protein per well.  
Incubate 2 hours.

**Step 2.** Wash, then add 50  $\mu\text{l}$  of SP Conjugate per well.  
Incubate 30 minutes.

**Step 3.** Wash, then add 50  $\mu\text{l}$  of Chromogen Substrate per well.  
Incubate 10 minutes.

**Step 4.** Add 50  $\mu\text{l}$  of Stop Solution per well.  
Read at 450 nm immediately.

## Symbol Key



Consult instructions for use.





# Human Lysozyme ELISA Kit

Catalog No. EL3020-1

*Sample insert for reference use only*

## Introduction

Lysozyme is one of the anti-microbial agents found in human milk and is also present in spleen, lung, kidney, white blood cells, plasma, saliva, and tears. Lysozyme has 130 amino acids, is synthesized by granulocytes and macrophages, and its natural substrate is the bacterial cell wall peptidoglycan (1, 2).

## Principle of the Assay

The AssayMax Human Lysozyme ELISA (Enzyme-Linked Immunosorbent Assay) kit is designed for detection of lysozyme in human **milk**. This assay employs a quantitative **competitive enzyme immunoassay** technique that measures lysozyme in less than 3 hours. A polyclonal antibody specific for lysozyme has been pre-coated onto a 96-well microplate with removable strips. Lysozyme in standards and samples is competed with a biotinylated lysozyme sandwiched by the immobilized antibody and streptavidin-peroxidase conjugate. All unbound material is washed away and a peroxidase enzyme substrate is added. The color development is stopped and the intensity of the color is measured

## Caution and Warning

- This product is for **Research Use Only** and is Not For Use In Diagnostic Procedures.
- Prepare all reagents (working diluent buffer, wash buffer, standard, biotinylated protein, and SP conjugate) as instructed, prior to running the assay.
- Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this insert. However, the user should determine the optimal dilution factor.
- Spin down the SP conjugate vial before opening and using contents.
- The Stop Solution is an acidic solution.
- The kit should not be used beyond the expiration date.

## Reagents

- **Human Lysozyme Microplate:** A 96-well polystyrene microplate (12 strips of 8 wells) coated with a polyclonal antibody against human lysozyme.
- **Sealing Tapes:** Each kit contains 3 pre-cut, pressure sensitive sealing tapes, which can be cut to fit the format of the individual assay.
- **Human Lysozyme Standard:** Human lysozyme in a buffered protein base (12 µg, lyophilized).
- **Biotinylated Human Lysozyme:** 1 vial, lyophilized.
- **EIA Diluent Concentrate (10x):** A 10-fold concentrated buffered protein base (30 ml).
- **Wash Buffer Concentrate (20x):** A 20-fold concentrated buffered surfactant (30 ml).
- **Streptavidin-Peroxidase Conjugate (SP Conjugate):** A 100-fold concentrate (80 µl).
- **Chromogen Substrate:** A ready-to-use stabilized peroxidase chromogen substrate tetramethylbenzidine (8 ml).
- **Stop Solution:** A 0.5 N hydrochloric acid to stop the chromogen substrate reaction (12 ml).

## Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store SP Conjugate at -20°C.
- Store Microplate, Diluent Concentrate (10x), Wash Buffer, Stop Solution, and Chromogen Substrate at 2-8°C.
- Unused microplate wells may be returned to the foil pouch with the desiccant packs and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Diluent (1x) may be stored for up to 30 days at 2-8°C.
- Store Standard and Biotinylated Protein at 2-8°C before reconstituting with Diluent and at -20°C after reconstituting with Diluent.

## Other Supplies Required

- Microplate reader capable of measuring absorbance at 450 nm.
- Pipettes (1-20 µl, 20-200 µl, 200-1000 µl, and multiple channel).
- Deionized or distilled reagent grade water.

## Sample Collection, Preparation, and Storage

- Milk:** Collect milk using sample tube. Centrifuge samples at 800 x g for 10 minutes. Dilute samples 1:200 into EIA Diluent or within the range of 1:20 to 1:2000, and assay. The undiluted samples can be stored at -20°C or below for up to 30 days. Avoid repeated freeze-thaw cycles.

*Refer to Sample Dilution Guidelines below for further instruction.*

<b>Guidelines for Dilutions of 1:100 or Greater</b> <i>(for reference only; please follow the insert for specific dilution suggested)</i>	
<b>1:100</b>	<b>1:10000</b>
A) 4 $\mu$ l sample: 396 $\mu$ l buffer (100x) = 100 fold dilution  <i>Assuming the needed volume is less than or equal to 400 <math>\mu</math>l.</i>	A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 4 $\mu$ l of A : 396 $\mu$ l buffer (100x) = 10000 fold dilution  <i>Assuming the needed volume is less than or equal to 400 <math>\mu</math>l.</i>
<b>1:1000</b>	<b>1:100000</b>
A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 24 $\mu$ l of A : 216 $\mu$ l buffer (10x) = 1000 fold dilution  <i>Assuming the needed volume is less than or equal to 240 <math>\mu</math>l.</i>	A) 4 $\mu$ l sample : 396 $\mu$ l buffer (100x) B) 4 $\mu$ l of A : 396 $\mu$ l buffer (100x) C) 24 $\mu$ l of B : 216 $\mu$ l buffer (10x) = 100000 fold dilution  <i>Assuming the needed volume is less than or equal to 240 <math>\mu</math>l.</i>

## Reagent Preparation

- Freshly dilute all reagents and bring all reagents to room temperature before use.
- EIA Diluent Concentrate (10x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the EIA Diluent Concentrate 1:10 with reagent grade water. Store for up to 30 days at 2-8°C.
- Human Lysozyme Standard:** Reconstitute the 12  $\mu$ g of Human Lysozyme Standard with 4 ml of EIA Diluent to generate a 3  $\mu$ g/ml standard stock solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the standard stock solution (3  $\mu$ g/ml) 1:2 with equal volume of EIA Diluent to produce 1.5, 0.75, 0.375, 0.188, 0.094, and 0.047  $\mu$ g/ml solutions. EIA Diluent serves as the zero standard (0  $\mu$ g/ml). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[Lysozyme] ( $\mu\text{g/ml}$ )
P1	1 part Standard (3 $\mu\text{g/ml}$ )	3.000
P2	1 part P1 + 1 part EIA Diluent	1.500
P3	1 part P2 + 1 part EIA Diluent	0.750
P4	1 part P3 + 1 part EIA Diluent	0.375
P5	1 part P4 + 1 part EIA Diluent	0.188
P6	1 part P5 + 1 part EIA Diluent	0.094
P7	1 part P6 + 1 part EIA Diluent	0.047
P8	EIA Diluent	0.000

- **Biotinylated Human Lysozyme (1x):** Reconstitute Biotinylated Human Lysozyme with 4 ml EIA Diluent to produce a stock solution. Allow the biotin to sit for 10 minutes with gentle agitation prior to use. Any remaining solution should be frozen at  $-20^{\circ}\text{C}$  and used within 30 days.
- **Wash Buffer Concentrate (20x):** If crystals have formed in the concentrate, mix gently until the crystals have completely dissolved. Dilute the Wash Buffer Concentrate 1:20 with reagent grade water.
- **SP Conjugate (100x):** Spin down the SP Conjugate briefly and dilute the desired amount of the conjugate 1:100 with EIA Diluent. Any remaining solution should be frozen at  $-20^{\circ}\text{C}$ .

## Assay Procedure

- Prepare all reagents, standard solutions, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at room temperature ( $20-25^{\circ}\text{C}$ ).
- Remove excess microplate strips from the plate frame and return them immediately to the foil pouch with desiccants inside. Reseal the pouch securely to minimize exposure to water vapor and store in a vacuum desiccator.
- Add 25  $\mu\text{l}$  of Human Lysozyme Standard and/or sample per well, and immediately add 25  $\mu\text{l}$  of Biotinylated Human Lysozyme to each well (on top of the standard or sample) and tap plate to mix gently. Cover wells with a sealing tape and incubate for 2 hours at room temperature. Start the timer after the last addition.
- Wash five times with 200  $\mu\text{l}$  of Wash Buffer manually. Invert the plate each time and decant the contents; hit 4-5 times on absorbent material to completely remove the liquid. If using a machine, wash six times with 300  $\mu\text{l}$  of Wash Buffer and then invert the plate, decanting the contents; hit 4-5 times on absorbent material to completely remove the liquid.
- Add 50  $\mu\text{l}$  of Streptavidin-Peroxidase Conjugate per well and incubate for 30 minutes. Turn on the microplate reader and set up the program in advance.
- Wash the microplate as described above.



- Add 50  $\mu$ l of Chromogen Substrate per well and incubate for 10 minutes or till the optimal blue color density develops. Gently tap plate to ensure thorough mixing and break the bubbles in the well with pipette tip.
- Add 50  $\mu$ l of Stop Solution to each well. The color will change from blue to yellow.
- Read the absorbance on a microplate reader at a wavelength of 450 nm **immediately**. If wavelength correction is available, subtract readings at 570 nm from those at 450 nm to correct optical imperfections. Otherwise, read the plate at 450 nm only. Please note that some unstable black particles may be generated at low concentration points after stopping the reaction for about 10 minutes, which will reduce the readings.


## Data Analysis

- Calculate the mean value of the duplicate or triplicate readings for each standard and sample.
- To generate a standard curve, plot the graph using the standard concentrations on the x-axis and the corresponding mean 450 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis using log-log or four-parameter logistic curve-fit.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

## Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

Human Lysozyme Standard Curve

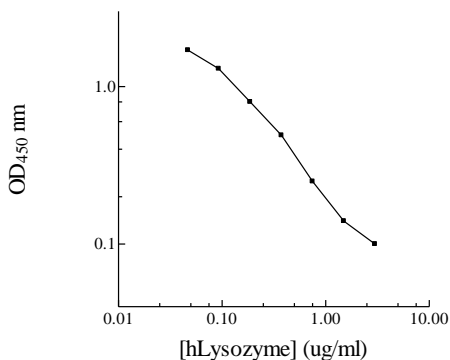

## Performance Characteristics

- The minimum detectable dose of lysozyme is typically ~ 0.04 µg/ml.
- Intra-assay and inter-assay coefficients of variation were 4.9% and 7.0% respectively.
- This assay recognizes both natural and recombinant human lysozyme.

## Linearity

Average Percentage of Expected Value (%)	
Sample Dilution	Milk
1:100	106%
1:200	98%
1:400	94%

## Recovery

Standard Added Value	0.09 – 1.5 µg/ml
Recovery %	86 – 114%
Average Recovery %	98%

## Cross-Reactivity

Species	Cross Reactivity (%)
Canine	None
Bovine	None
Monkey	None
Mouse	None
Rat	None
Swine	<10%
Human	100%

## Troubleshooting

Issue	Causes	Course of Action
Low Precision	Use of expired components	<ul style="list-style-type: none"> <li>• Check the expiration date listed before use.</li> <li>• Do not interchange components from different lots.</li> </ul>
	Improper wash step	<ul style="list-style-type: none"> <li>• Check that the correct wash buffer is being used.</li> <li>• Check that all wells are dry after aspiration.</li> <li>• Check that the microplate washer is dispensing properly.</li> <li>• If washing by pipette, check for proper pipetting technique.</li> </ul>
	Splashing of reagents while loading wells	<ul style="list-style-type: none"> <li>• Pipette properly in a controlled and careful manner.</li> </ul>

	Inconsistent volumes loaded into wells	<ul style="list-style-type: none"> <li>• Pipette properly in a controlled and careful manner.</li> <li>• Check pipette calibration.</li> <li>• Check pipette for proper performance.</li> </ul>
	Insufficient mixing of reagent dilutions	<ul style="list-style-type: none"> <li>• Thoroughly agitate the lyophilized components after reconstitution.</li> <li>• Thoroughly mix dilutions.</li> </ul>
	Improperly sealed microplate	<ul style="list-style-type: none"> <li>• Check the microplate pouch for proper sealing.</li> <li>• Check that the microplate pouch has no punctures.</li> <li>• Check that three desiccants are inside the microplate pouch prior to sealing.</li> </ul>
<b>Unexpectedly Low or High Signal Intensity</b>	Microplate was left unattended between steps	<ul style="list-style-type: none"> <li>• Each step of the procedure should be performed uninterrupted.</li> </ul>
	Omission of step	<ul style="list-style-type: none"> <li>• Consult the provided procedure for complete list of steps.</li> </ul>
	Steps performed in incorrect order	<ul style="list-style-type: none"> <li>• Consult the provided procedure for the correct order.</li> </ul>
	Insufficient amount of reagents added to wells	<ul style="list-style-type: none"> <li>• Check pipette calibration.</li> <li>• Check pipette for proper performance.</li> </ul>
	Wash step was skipped	<ul style="list-style-type: none"> <li>• Consult the provided procedure for all wash steps.</li> </ul>
	Improper wash buffer	<ul style="list-style-type: none"> <li>• Check that the correct wash buffer is being used.</li> </ul>
	Improper reagent preparation	<ul style="list-style-type: none"> <li>• Consult reagent preparation section for the correct dilutions of all reagents.</li> </ul>
Insufficient or prolonged incubation periods	<ul style="list-style-type: none"> <li>• Consult the provided procedure for correct incubation time.</li> </ul>	
<b>Deficient Standard Curve Fit</b>	Non-optimal sample dilution	<ul style="list-style-type: none"> <li>• Sandwich ELISA: If samples generate OD values higher than the highest standard point (P1), dilute samples further and repeat the assay.</li> <li>• Competitive ELISA: If samples generate OD values lower than the highest standard point (P1), dilute samples further and repeat the assay.</li> <li>• User should determine the optimal dilution factor for samples.</li> </ul>
	Contamination of reagents	<ul style="list-style-type: none"> <li>• A new tip must be used for each addition of different samples or reagents during the assay procedure.</li> </ul>
	Contents of wells evaporate	<ul style="list-style-type: none"> <li>• Verify that the sealing film is firmly in place before placing the assay in the incubator or at room temperature.</li> </ul>
	Improper pipetting	<ul style="list-style-type: none"> <li>• Pipette properly in a controlled and careful manner.</li> <li>• Check pipette calibration.</li> <li>• Check pipette for proper performance.</li> </ul>
	Insufficient mixing of reagent dilutions	<ul style="list-style-type: none"> <li>• Thoroughly agitate the lyophilized components after reconstitution.</li> <li>• Thoroughly mix dilutions.</li> </ul>

## References

- (1) Chung LP *et al.* (1988) Proc. Natl. Acad. Sci. USA 85:6227-6231
- (2) Lollike K *et al.* (1995) Leukemia 9:159-164

Version 2.5R

## Related Products

- EL3010-1 AssayMax Human Lysozyme ELISA Kit (Plasma, Serum, Saliva, Urine, and Cell Culture samples)