

Laser Methane mini
SA3C32A

LaserMethane mini

Operation Manual

Read this manual before using the equipment.

Keep this manual with the equipment.




Tokyo Gas Engineering Co., Ltd.

For Safety






Prior to using this product, please read the “For Safety” section to ensure safe and appropriate usage

- In this operation manual and product labels, the methods for safely using this product, methods for avoiding danger by users and others, and various cautions are indicated by picture symbols.
- The degree of danger, potential harm, and urgency in case of incorrect operation are indicated by DANGER, WARNING, and CAUTION. Each of these indicates denotes important safety-related items. Be sure to observe these items. Their markings and meanings are as follows.

Degree of Injury/Damage and Corresponding Safety Symbol

 DANGER	This indicates dangerous contents that are very likely to result in serious injury or death for the user if this symbol is ignored and operation is not performed properly.
 WARNING	This indicates contents that could result in serious injury or death for the user if this Symbol is ignored and operation is not performed properly.
 CAUTION	This indicates contents that could result in injury for the user or physical damage of the product if this symbol is ignored and operation is not performed properly.

Safety Symbols Used on This Product and in This Manual

	This indicates a prohibited operation. The prohibited operation is indicated symbolically in or near the barred circle.
	This indicates an obligatory safety precaution. The obligatory operation is indicated symbolically in or near the circle.
	This indicates warning or caution. The contents are indicated symbolically in or near the triangle.
	This indicates a note. The contents are described in the box.
	This indicates that the marked part should be recycled.

For Safety

SA3C32A
LaserMethane mini
Operation Manual

31 May 2010 (First Edition)
13 August 2010 (Second Edition)

All rights reserved. No part of this manual may be reproduced without the prior written permission of the publisher.

The contents of this manual may be changed without prior notice.

Copyright© 2010, Tokyo Gas Engineering Co., Ltd.

Printed in Japan

For Safety



DANGER

-
- ⊘ Do not use this product in case of anomaly such as smoke or strange smell. Continuing to use the product under such conditions may cause fire or electric shock. In case of an anomaly, immediately take the **Actions** indicated below.
 - ⊘ Do not use the product if its outer body (case) is broken, as this may cause fire or electric shock. Immediately take the **Actions** indicated below.
 - ⊘ Do not use the product if water or foreign objects have gotten inside. Continuing to use the product under such conditions may cause fire or electric shock. Immediately take the **Actions** indicated below.

[Actions]

- Switch off the power of the product.
 - Remove the battery pack from the main unit.
 - Disconnect the power plug of the battery charger from the power outlet.
 - Contact Customer Service.
-

For Safety

⊘ **Incorrect handling of the battery pack may cause fire, electric shock, or an explosion. Be sure to observe the following points.**

- Do not use a battery pack other than the dedicated battery pack for this product.
 - When inserting the battery pack in the main unit (or battery charger), do so by observing the specified direction.
 - Do not charge the battery pack with a method other than that described in the Operation Manual.
 - Do not store or carry the battery pack together with metal objects such as coins, keys, or chain.
 - Do not dismantle, damage, or heat the outer body (chassis) of the battery pack.
 - Do not throw the battery pack into fire.
 - Do not use, store, or discard the battery pack in a place with high temperature (near a fire, a place exposed to direct sunlight, in a car under the blazing sun, etc.).
 - Do not expose the battery pack to water, oil, or other liquids, and do not use it in locations with high humidity.
 - Do not use the battery pack if it leaks.
 - When not using the product for a long time, remove the battery pack from the main unit.
-

For Safety



WARNING

⊘ Do not disassemble the main unit.

This may cause electric shock leading to death, burns, or injury. For internal inspections, adjustments, or repairs, be sure to contact Customer Service.

⊘ Incorrect use of the battery charger may cause fire or electric shock.

Be sure to observe the following points.

- Do not expose the battery charger to water, oil, or other liquids, and do not use it in locations with high humidity.
 - Do not use the battery charger while its outer body (chassis) is broken.
 - Do not use a damaged AC cord (exposed wires, broken wires, etc.)
 - Do not damage the AC cord, break it, process it, bend it forcefully, pull on it, twist it, roll it up, cover it with heavy objects, fix it with nails or wire, or heat it up.
 - Do not connect the AC cord to a multi-outlet such as a cable tap or current tap socket.
 - When inserting the power plug of the AC cord to a power outlet or the battery charger, be sure to insert it securely.
-

⊘ Do not look at the laser light or direct it toward people while the product is powered, as this may cause harmful exposure and injury.

Be sure to observe the following points.

- Do not cast laser light directly into the eyes.
 - Absolutely never look directly into the laser light.
 - Do not let children handle the product.
-

⊘ Never charge the battery pack in locations that contain explosive gas.

⊘ The battery charger does not feature an intrinsically safe design.

For Safety



CAUTION

-
- ⊘ Do not subject the main unit, battery charger, and battery pack to strong shocks or vibrations, because this may cause failure.
-
- ⊘ Do not forcefully push the display or subject it to strong shocks, because this may cause the display screen to break.
-
- ⊘ Do not use the product and battery charger in locations where heat builds up, because this may cause fire. Be sure to observe the following points.
 - Do not charge the unit on soft furnishings (cushions, bedding, furniture etc).
 - Do not cover the product and battery charger with a tablecloth, etc.
 - Do not use the product and battery charger in a location with poor air circulation such as inside a box.
-

For Safety

Improper use of the battery charger may cause fire or electric shock.

Be sure to observe the following points.

- If lightning occurs nearby, remove the power plug of the AC adapter from the power outlet and do not use it before the lightning has ceased.
- Once charging of the battery pack has been completed, remove the battery pack from the battery charger.
- When removing the power plug of the AC adapter from the power outlet or the battery charger, be sure to grasp the power plug instead of the AC cord.
- Do not let the AC cord near thermal appliances.

The battery pack becomes hot during charging. Be careful when handling it.

Do not keep looking at the detection lamp for a long time. This may cause dazzling, which can possibly cause a secondary accident.

In case the detection lamp is unnecessary, this function can be disabled by changing the setting. (See 6. Detection Lamp of 5.3 Changing Settings)

☐ **When using this product, be careful with electrostatic discharge.**

It is necessary for this product to restart because of the electrostatic discharge.

When using the product, be sure to use the strap.

Breakage, failure, and foot injury caused by dropping of the product can be prevented by using the strap.

☐ **Accurate gas measurement may not be possible in the vicinity of electric devices or industrial equipment that produces electrical noise. In this case, perform gas measurement a little farther away.**

☐ **Do not use the product in locations where hydrogen sulfide occurs (such as hot springs), or locations with a lot of salt (such as the seacoast), because this may shorten the life of the product.**

For Safety

When storing the product, be sure to observe the following points.

- Do not store the product in extremely hot locations such as inside a car, or in cold locations directly exposed to outside air.
- Avoid storing the product in locations where it will be exposed to strong vibrations.
- Storing the battery pack in high temperatures may shorten its life, so store it at 30°C or lower.

☐ **When transporting the main unit and battery charger, be sure to observe the following points.**

- When transporting the main unit and battery charger in a car, etc., be sure to protect the product from direct vibration and shocks.
 - When shipping the main unit, battery pack, or battery charger for repair, etc., place shock absorbing material in the shipping box.
-

For Safety



WARNING

Laser Safety

The Measurement light beam radiation in this product is classified as Class 1 according to the IEC 60825-1 specifications.

The guide light beam radiation is classified as Class 2 according to the IEC 60825-1 specifications.

Classes are indicated on the label attached to the top of the product (Refer to “Laser Radiation Markings”).

The laser safety is assured by correct operation of the product. Before starting operation, if you cannot confirm an indication of [LASER] on the display, which is an indication of laser beam output, upon switching on the power or pressing the Start/Stop button, there may be a laser beam output failure. Without using the product, please call customer service to request repair.

Do not view laser radiation from Class 2 laser products directly with optical instruments, because the laser radiation might harm your eyes.

Class 1 and 2 indicate the danger degree of the laser beam specified below according to IEC 60825-1.

Class 1: Laser radiation that is safe under reasonably foreseeable conditions of operation, including the use of optical instruments for intrabeam viewing.

Class 2: Laser radiation that emits visible radiation in the wavelength range from 400 to 700 nm where eye protection is normally afforded by aversion response, including the blink reflex. This reaction may be expected to provide adequate protection under reasonably foreseeable conditions of operation including the use of optical instruments for intrabeam viewing.

For Safety

Laser Radiation Markings



Specification concerning laser radiation

1. Laser Safety Classifications Based on IEC 60825-1:2007

■ Measurement light beam radiation (Class 1 Laser)

- Maximum output power : 10mW or less
- Pulse width : CW
- Wavelength : 1653nm
- Beam extension in collimated beam : 8.5mrad or less

■ Guide light beam radiation (Class 2 Laser)

- Maximum output power : 1mW or less
- Pulse width : CW
- Wavelength : 650nm
- Beam extension in collimated beam : 6mrad or less

2. Incorporated laser Specification

■ Measurement light beam radiation

- Maximum output power : 10mW or less
- Pulse width : CW
- Wavelength : 1653nm
- Beam extension in collimated beam : 8.5mrad or less
- Embedded laser output level : 60mW or less

■ Guide light beam radiation

- Maximum output power : 1mW or less
- Pulse width : CW
- Wavelength : 650nm
- Beam extension in collimated beam : 6mrad or less
- Embedded laser output level : 7mW or less

CAUTION

Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous radiation exposure.

For Safety



WARNING

Employment of an Explosion-Protected Equipment

If the customer conducts repair or modification to an intrinsically safe or explosionproof equipment and the equipment is not restored to its original condition, its intrinsically safe or explosionproof construction may be compromised and the equipment may be hazardous to operate. Please contact Customer Service before making any repair or modifications to an equipment.



CAUTION

This equipment, including SA0Z40A Battery Pack, has been tested and certified as being intrinsically safe or explosionproof. Please note that severe restrictions apply to this equipment's construction, maintenance and repair. A failure to abide by these restrictions could make equipment hazardous to operate.



WARNING

DO NOT disassemble this equipment. Disassembling it is strictly prohibited in order to maintain the safety level of an explosionproof equipment. This equipment cannot be repaired by the user.

For Safety



DANGER

DO NOT use this equipment at explosive atmospheres except the approved category.

Using this equipment at the *Zone 0* for city gas, etc. is strictly prohibited.



DANGER

DO NOT charge the Battery Pack in explosive atmospheres. The Battery Charger is not an explosionproof equipment.


For Safety

CENELEC ATEX (KEMA) Intrinsically Safe Type

Caution for CENELEC ATEX (KEMA) Intrinsically Safe Type.

Note 1. Intrinsically Safe Type

- ATEX intrinsically Safe Type : Type "i"
- Certificate Number : KEMA 08ATEX0005
- Product : SA3C32A Laser Methane mini
- Manufacturer : ANRITSU CORPORATION
- Address : 5-1-1 Onna, Atsugi-shi, Kanagawa, 243-8555 Japan
- Applicable Standard : EN 60079-0:2006, EN 60079-11:2007, EN60079-28:2007
- Type of Protection and Marking code

: CE 0344  I M2
II 2G Ex ib op-pr/op-is I
IIA T1

- Group :I and II
- Category : M2 and 2G
- Ambient Temperature : -17 to +50 °C
- Applicable detection hazardous areas:
 - Zones 1 and 2 for city gas, etc.
 - Zone 1 for coal mines

Note 2. Battery

- Ensure using only the following battery.
SA0Z40A Battery Pack

Note 3. Maintenance and Repair

- Disassembling and modifying this equipment, including SA0Z40A Battery Pack, by other than authorized representative of Anritsu Corporation is prohibited and will void KEMA Intrinsically safe Certification.

For Safety



WARNING



Thank you for cooperating with recycling of the nickel-hydride battery.

This product uses a nickel-hydride battery pack. This battery pack includes rare materials such as nickel oxide and hydrogen storage alloys that can be recycled as precious resources. After implementing the safety measures listed below for the used battery pack, contact Customer Service.



For the sake of safety, recycle battery packs that are no longer used after discharging them as follows.

- Insert the battery pack in the main unit.
- Switch on the power of the main unit.
- Until the empty screen is indicated, leave the main unit (indicating that the battery pack is discharged).
- Remove the battery pack from the main unit.
- Tape insulating tape such as vinyl tape on the contact part of the battery pack (to prevent short-circuit accidents caused by the residual electricity in the battery pack).
- Contact Customer Service and ask for instructions regarding the recycling method.

Warranty

Tokyo Gas Engineering Co., Ltd. offers a 12-month warranty from date of purchase providing free repair of any faults arising from manufacturing defects. However, the following cases are not covered by the warranty.

- Faults that do not fall within the scope of the warranty listed in the Operation Manual
- Faults caused by improper operation, use, unauthorized modifications, dismantling, or repairs on the part of the customer
- Faults caused by heavy use that clearly exceeds normal use
- Faults caused by improper or insufficient maintenance on the part of the customer
- Unavoidable faults arising from fires, floods, earthquakes, other acts of God, etc.
- Faults caused by connecting any other products, parts, or consumables other than the specified ones
- Faults caused by a power supply, usage location, etc., other than the specified ones

Among damages that arise from defects in this product, Tokyo Gas Engineering Co., Ltd. shall not be liable for damages and loss of business of the customer that arise from unforeseeable and special circumstances.

Inquiries to Tokyo Gas Engineering Co., Ltd.

In the case of faults in the product, promptly contact Customer Service listed at the end of this manual.

Electromagnetic Interference

This product complies with the EC Directive on CE Marking and is targeted for use in industrial environments.

Note, however, that if this product is used near a radio or television receiver, reception interference may occur. Also note that the product may be unable to detect gas properly if used near an electrical product or industrial product that generates a strong magnetic field or electrical noise.

Notes In Regard To Use

Ensure the following points.

- Upon handling this product, please take sufficient precautions against static electricity. Please use this product in an environment where sufficient measures are implemented against static electricity.
- This product is an intrinsically safe product. Please use this product in an environment which conforms to the intrinsically safety standards of this product.

Crossed-out Wheeled Bin Symbol

Equipment marked with the Crossed-out Wheeled Bin Symbol complies with the Council Directive 2002/96/EC (the “WEEE Directive”) in the European Union.



For products deployed in the EU market after August 13, 2005, please contact **Tokyo Gas Engineering Co., Ltd.** at the end of the product's useful life to arrange disposal in accordance with your initial contract and local law.

CE Conformity marking

Tokyo Gas Engineering Co., Ltd. affixes the CE Conformity marking on the following product (s) in accordance with the Council Directive 93/68/EEC to indicate that they conform to the EMC, LVD and ATEX Directive of the European Union (EU).



1. Product Model

Model: SA3C32A LaserMethane mini
and

Accessories: SA0Z40A BATTERY PACK
SA0Z41A PROTECT COVER
SA0Z42A BATTERY CHARGER
SA0Z43A AC ADAPTER
SA0Z44B STRAP (Long type)
and

Software: SA0C07A LaserMethane mini Software

2. Applied Directive

EMC: Council Directive 89/336/EEC

LVD: Council Directive 73/23/EEC

ATEX: Council Directive 94/9/EC

3. Applied Standards

EMC: Emission: EN61326-1: 2006

Immunity: EN61326-1: 2006

	SA3C32A	SA0Z42A	Performance Criteria*
IEC61000-4-2 (ESD)	–	√	B
IEC61000-4-3 (EMF)	√	√	A
IEC61000-4-4 (Burst)	–	√	B
IEC61000-4-5 (Surge)	–	–	B
IEC61000-4-6 (CRF)	–	–	A
IEC61000-4-8 (RPFMF)	–	–	A
IEC61000-4-11 (V dip/short)	–	–	C

***: Performance Criteria**

A: Normal performance within the specification limits during testing.

B: Temporary degradation, or functional loss, which self-recovers during testing

C: Temporary functional loss is allowed, provided that the function is self-recoverable or the operational control can be restored.

No limits apply for this equipment with an active input power under 75 W.

- LVD: EN60950-1: 2001 +A11

ATEX: EN60079-0: 2006

EN60079-11: 2007

EN60079-28: 2007

C-tick Conformity marking

Tokyo Gas Engineering Co., Ltd. affixes the C-tick marking on the following product (s) in accordance with the regulation to indicate that they conform to the EMC framework of Australia/New Zealand.

C-tick marking



1. Product Model

Model: SA3C32A LaserMethane mini
and
Accessories: SA0Z40A BATTERY PACK
SA0Z41A PROTECT COVER
SA0Z42A BATTERY CHARGER
SA0Z43A AC ADAPTER
SA0Z44B STRAP (Long type)
and
Software: SA0C07A LaserMethane mini Software

2. Applied Standards

EMC: Emission:
AS/NZS 2064.1/2 (ISM, Group 1, Class A equipment)

The following are the provisions of “Measures for Administration of the Pollution Control of Electronic Information Product” of the People’s Republic of China.

They are applicable only in the People’s Republic of China.

关于符合中国《电子信息产品污染控制管理办法》的声明

产品中有毒有害物质或元素的名称及含量

部件名称	有毒有害物质或元素					
	铅 (Pb)	汞 (Hg)	镉 (Cd)	六价铬 [Cr (VI)]	多溴联苯 (PBB)	多溴二苯醚 (PBDE)
印刷线路板 (PCA)	×	○	×	×	○	○
机壳、支架 (Chassis)	×	○	×	×	○	○
其他（电缆、风扇、 连接器等） (Appended goods)	×	○	×	×	○	○
○：表示该有毒有害物质在该部件所有均质材料中的含量均在 SJ/T 11363-2006 标准规定的限量要求以下。						
×：表示该有毒有害物质至少在该部件的某一均质材料中的含量超出 SJ/T 11363-2006 标准规定的限量要求。						

环保使用期限



这个标记是根据 2006/2/28 公布的「电子信息产品污染控制管理办法」以及 SJ/T 11364-2006「电子信息产品污染控制标识要求」的规定，适用于在中国销售的电子信息产品的环保使用期限。仅限于在遵守该产品的安全规范及使用注意事项的基础上，从生产日起算的该年限内，不会因产品所含有害物质的泄漏或突发性变异，而对环境污染，人身及财产产生深刻地影响。

注) 电池的环保使用期限是 5 年。

About This Manual

This operation manual describes how to use and maintain the SA3C32A LaserMethane mini (hereinafter, this product). Chapter 1 describes “Outline and Principle” and the following sections provide more detailed explanations.

Table of Contents

1. Outline and Principle	1
1.1 Outline	1
1.2 Principle	1
2. Introduction	3
2.1 Checking Package Contents	3
3. Nomenclature	4
3.1 Main unit	4
3.2 Display	5
4. Preparations Before Use	6
4.1 Charging Battery Pack	6
4.2 Attaching Strap	8
4.3 Attaching Battery Pack	9
5. Operation Method	10
5.1 Starting Up and Ending	10
5.2 Measurement	11
5.3 Changing Settings	14
5.4 Automatic Calibration	17
5.5 Indicating Residual Power of Battery Pack	18

6. Error Messages	19
6.1 Explanation of Errors and Measures	19
7. IN CASE OF TROUBLE	22
7.1 Problems and Solutions.....	22
8. Daily Maintenance	24
8.1 Maintenance Method	24
9. Main Specifications.....	25
9.1 Main Specifications of Main Unit.....	25
9.2 Main Specifications of Battery Charger	26
and AC Adapter	26
10. Ordering Information	27
10.1 Main Unit and Standard Accessories	27
11. Inquiries.....	28
11.1 Customer Service	28
12. Distributor and Manufacture	29
12.1 Distributor	29
12.2 Manufacture	29

1. Outline and Principle

1.1 Outline


This product is a handheld gas detector for remote detection of methane and methane-containing gases (natural gas or similar). Gas leakage and accumulation within approximately 30 meters can be detected quickly by directing a laser beam at the area to be inspected.

The measured point is illuminated by a red guide light clearly visible, and then measured value of methane is displayed on the display in real time.

1.2 Principle

This product is based on Infrared Absorption Spectroscopy using a semiconductor laser for methane detection. The integrated concentration of methane between this product and the target point is measured by transmitting a detection laser beam towards the target point (gas piping, ceiling, wall, floor, ground, etc.) then detecting a fraction of the diffusely reflected beam from that target point. The measured value is expressed by a methane column density (ppm·m): the methane concentration (ppm) multiplied by the thickness (m).

1. Outline and Principle

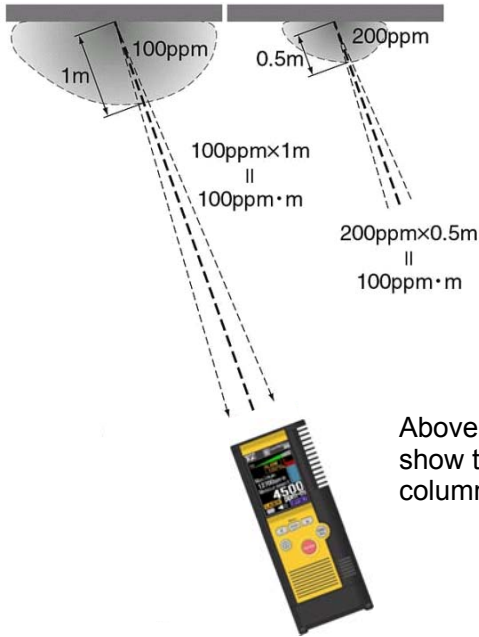

Above two examples show the same methane column density.

In addition, this product does not respond in principle to gases other than methane (butane, propane, etc.). This product cannot perform detection in places where detection laser beam cannot reach, such as the opposite side of a wall or underground.

2. Introduction

2.1 Checking Package Contents

Remove the main unit and the supplied accessories from the package and make sure that you have received all the items listed below. If there are any missing or damaged items, immediately contact Customer Service.

Main unit

Main unit: 1 unit



Battery pack: 1 pc.



Standard Accessories

Battery charger: 1 unit



AC adapter: 1 unit
(AC cord: 1 pc.)



Strap: 1 pc.



Protector: 1 pc.





Operation manual
(this manual): 1 vol.




3. Nomenclature

3.1 Main unit

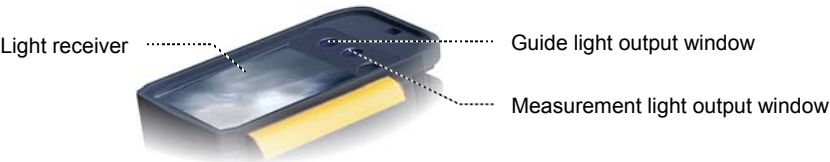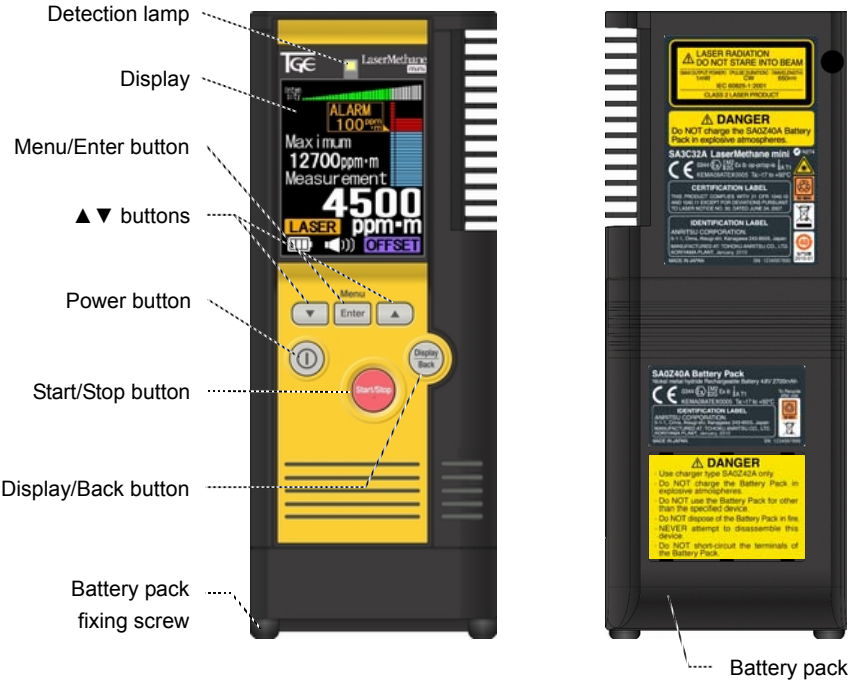


3.2 Display

Numeric Mode

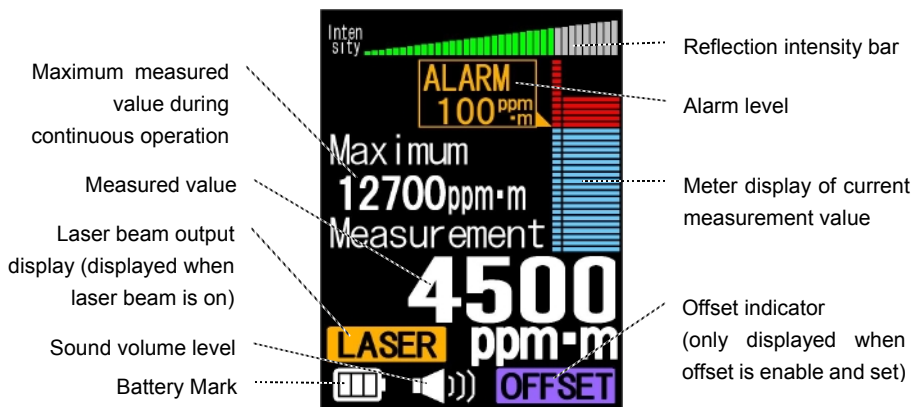

Graph Mode

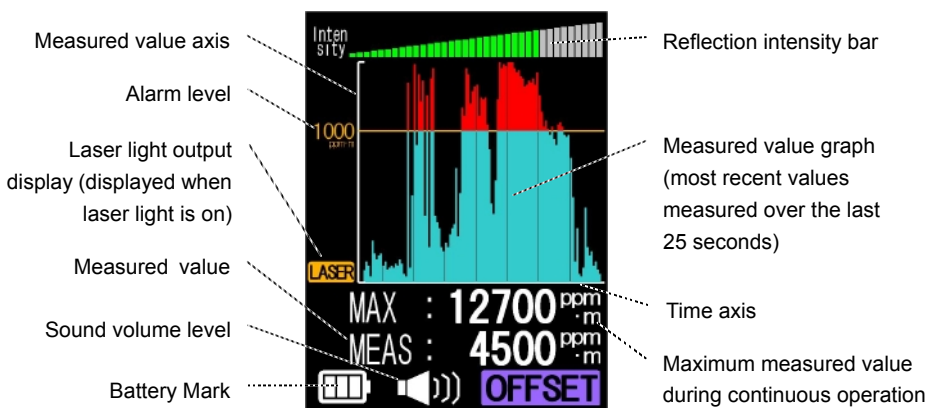

- ❖ When the remaining battery level is shown in the figure on the right, the power will switch off in approx.15 min. If this symbol appears, recharge the battery pack. (See "4.1 Charging Battery Pack.")




4. Preparations Before Use

4.1 Charging Battery Pack

Charging Method

1. Connect the battery charger, AC adapter, AC cord, and power outlet in the sequence shown below, (1-2-3).

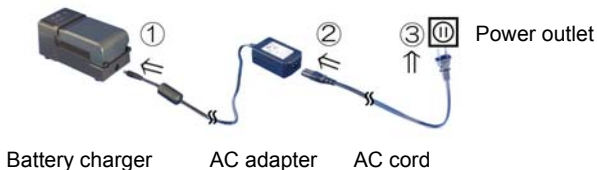

2. Attach the battery pack so that the corner of the battery pack coincides with the Δ mark on the battery charger (slide the battery pack securely all the way to the end).



- ❖ Explanation of LED display of battery charger
 - The orange LED, when lit, indicates that charging is in progress.
 - The green LED, when lit, indicates that charging has been completed.
 - The red LED, when lit, indicates an anomaly.

DANGER

When the red LED of the battery charger lights up, immediately disconnect the power plug of the battery charger from the power outlet, remove the battery pack from the battery charger, and contact Customer Service.

3. When charging is completed, remove the battery pack from the battery charger by sliding it out.



- ❖ Disconnect the power plug of the battery charger from the power outlet after charging is completed.

CAUTION

The battery pack and the battery charger may become hot during charging.

WARNING

Use the dedicated battery pack (SA0Z40A) only with the dedicated battery charger (SA0Z42A).

Do not use an AC adapter such as a car charger other than the dedicated one (SA0Z43A).

WARNING

Never charge the battery pack in a location with flammable gas.

WARNING

The battery charger does not feature an intrinsically safe design.

Replacement Schedule

The battery pack has a service life of approximately 500 cycles*. If the operating time of the product becomes extremely short even though it has been fully charged, this indicates that the battery pack has reached the end of its service life. Replace the battery pack with a new one.

* This figure is a guideline based on JIS C8708 test conditions. (The actual number of cycles may differ according to the product and the usage conditions.)

4.2 Attaching Strap

Attach the strap

See the figure on the right.



CAUTION

To prevent breaking of the product due to dropping, be sure to use it with your hand through the strap.

4.3 Attaching Battery Pack

Attaching the battery pack to the main unit

1. Attach the battery pack so that the corner of the battery pack coincides with the Δ mark on the main unit.
2. Tighten the two battery pack fixing screws at the base of the battery pack.



Removing the battery pack

1. Loosen the two battery pack fixing screws at the base of the battery pack.
2. Remove the battery pack by pulling it sideways to the Δ mark on the main unit and then pull it up.



CAUTION

Two months or more, when you do not use it, please remove a battery pack from a main unit. If a battery pack is kept while connecting with a main unit two months or more, there is a case where a battery pack serves as fault electric discharge, and it becomes impossible to use it.

5. Operation Method

5.1 Starting Up and Ending

Switching on the power

1. Press the Power button for approximately 2 seconds. (The product will emit a beeping sound.)



2. The startup screen appears for a few seconds, followed by the self-test screen, which is also displayed for a few seconds.

- ❖ The startup time may be longer depending on the temperature.
- ❖ The self-test is a self-diagnostic test for accurate measurement.




Startup screen



Self-test screen

3. Once the measurement preparations have been completed, the numeric mode screen shown on the right is displayed, and the product becomes stand-by state of measurement.

- ❖ The screen can be switched to the graph mode by pressing the Display/Back button.



Numeric mode

Switching off the power

1. Press the Power button for approximately 2 seconds. (The product will emit a beeping sound.)
2. The screen will switch off.



5.2 Measurement

1. Press the Start/Stop button (red button at the center) and direct the guide light toward the area to be measured.




2. The measured value is displayed as shown in the screen on the right.

- ❖ If the measured value is displayed in white, the measurement was done accurately.



Numeric mode



Graph mode

- ❖ If the measured value is displayed in gray, it is a reference value (this is a value with low measurement accuracy due to insufficient received light intensity).
- ❖ To toggle the screen, press the Display/Back button (numeric mode ↔ graph mode)

3. To end measurement, press the Start/Stop button again.

- ❖ During measurement, the measured and maximum values are displayed every 0.5 seconds, and when measurement ends, the data is kept.
- ❖ The measurement values displayed in the graph mode are the most recent values measured over the last 25 seconds.
- ❖ If the reflection intensity bars are not indicated in green, try to increase the sensitivity for example by reducing the measuring distance (until four or more bars are lit).
- ❖ The unit is provided with functions that give an acoustic alarm and a flashing detection lamp when it detects a column density exceeding a preset threshold.

(See "5.3 Changing Settings.")



WARNING

Laser beam is on while the "LASER" laser beam output display is lit, so do not direct the laser beam toward people or look into the laser beam output windows.



WARNING


When not using this product, be sure to switch it off.

Notes in methane detection


1. Upon measuring highly reflective material such as metallic material, please be careful with situations as shown in Figure A, where two guide lights (red) are visible caused by reflection, which may cause false alarms by indicating high values regardless of the presence of methane.

In such case, please point as shown in Figure B, where only a single guide light (red) can be seen.

【Figure-A : Possibility of a false alarm with high values】

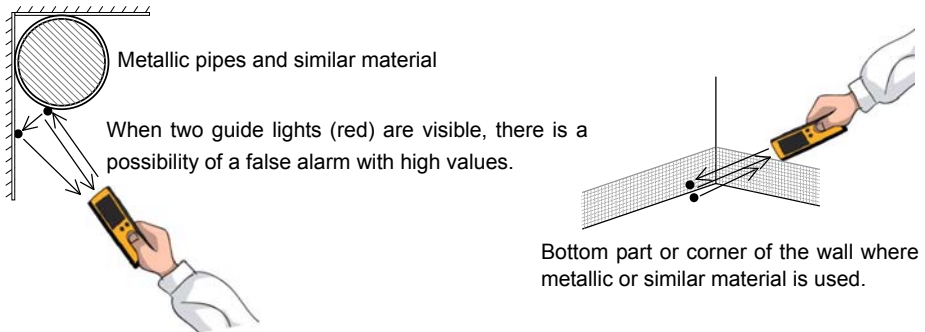

【Figure-B : To get correct value】

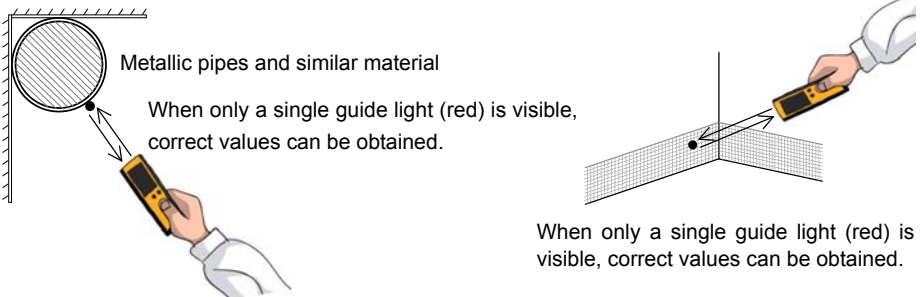


2. For a PE (polyethylene) pipe with a wall thickness of less than 10mm, please note that you may get wrong measurements if you keep pointing the laser directly at the PE pipe, because laser light penetrates through depending on its thickness.

5.3 Changing Settings

Common operations for changing settings

1. Press the Menu/Enter button from the measurement standby state.
2. The [SETTINGS] screen shown on the right will be displayed.
3. Select the item (1 to 5) to be set with the ▲▼ buttons, and then press the Menu/Enter button.
 - ❖ To return to the measurement standby screen, press the Display/Back button.




1. Alarm Level

- The methane column density level at which an alarm threshold can be set.

In the main menu select "1. Alarm level."

1. The [ALARM LEVEL] screen shown on the right will be displayed.

(The default setting value is 100 ppm-m.)
2. Select a value with the ▲▼ buttons for the 1000's digit, and then press the Menu/Enter button.
 - ❖ To leave the value as indicated just press the Menu/Enter button as is.
3. Likewise, select a value for the 100's digit, 10's digit, and 1's digit.
4. Once the setting for the 1's digit is completed, the buzzer sounds twice to indicate that the setting has been accepted.
 - ❖ The setting values are not reset even when the power is switched off.



2. Offset Value


- The measured value is displayed in the screen when it exceeds the offset value.

In the main menu select “2. Offset value.”

1. The [OFFSET VAL.] screen shown on the right will be displayed.

(The default setting value is 0 ppm·m).

2. Select a value with the ▲▼ buttons for the 1000's digit, and then press the Menu/Enter button.



- ❖ To leave the value as indicated just press the Menu/Enter button as is.
3. Likewise, select a value for the 100's digit, 10's digit, and 1's digit.
 4. Once the setting for the 1's digit is completed, the buzzer sounds twice to indicate that the setting has been accepted.
- ❖ The set value will not be reset when the power is switched off.

3. Sound Volume Level

In the main menu select “3. Sound level.”

1. The [SOUND LEVEL] screen shown on the right will be displayed.
2. Adjust the sound volume level with the ▲▼ buttons.
3. Press the Menu/Enter button.



- ❖ The set value will not be reset even when the power is switched off.

4. Screen Brightness

In the main menu select “4. Display.”


1. The [DISPLAY] screen shown on the right will be displayed.
2. Adjust the brightness with the ▲ ▼ buttons.
3. Press the Menu/Enter button.
 - ❖ The set value will not be reset even when the power is switched off.



5. Display Language

In the main menu select “5. Language.”

1. The [LANGUAGE] screen shown on the right will be displayed.
2. Select the language with the ▲ ▼ buttons.
3. Press the Menu/Enter button.
 - ❖ The set value will not be reset even when the power is switched off.



6. Detection lamp

In the main menu select “6. Detect lamp.”

1. The [DETECT LAMP] screen shown on the right will be displayed.
2. Select the enable / disable with the ▲ ▼ buttons.
3. Press the Menu/Enter button.
 - ❖ The set value will not be reset even when the power is switched off.



5.4 Automatic Calibration

- If “SELF TEST FAILURE” is displayed at startup, perform an automatic calibration using the procedure below.

1. After making sure that the power of the product is off, press the Power button for approx. 2 seconds while pressing the Menu/Enter button.




2. Automatic calibration will start, and for 2 to 3 minutes, the [AUTO CALIBRATION] screen shown on the right will be displayed.

(The progress status can be checked with the count-down counter at the center of the screen.)



3. Upon completion of automatic calibration, the self-test is executed. The numeric mode screen shown to the right will be displayed, and the product will enter stand-by state of measurement.




Numeric mode

- ❖ If automatic calibration does not complete successfully, it is performed again a second time.
(Time until completion will be approx. 4 to 5 minutes.)

5.5 Indicating Residual Power of Battery Pack

The battery mark shown on the display indicates the battery pack residual power.

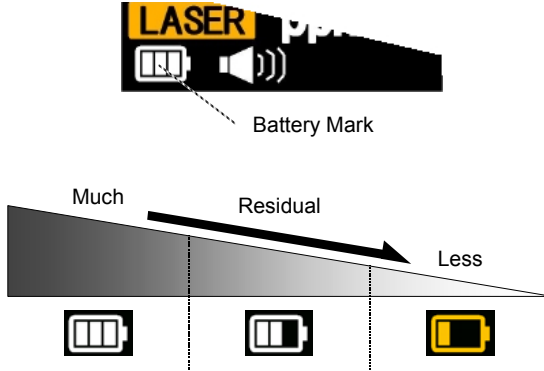

When the battery power of the battery pack is lost until this product doesn't operate, the empty screen shown on the right will be displayed, and there will be an alarm.




6. Error Messages

6.1 Explanation of Errors and Measures

When “OPERATION ERROR” is displayed

1. Switch off the power of the product.
2. (After checking that the power is switched off), switch on the power.
3. If the same error reoccurs, perform automatic calibration after making sure that the power of the product is off. (See “5.4 Automatic Calibration.”)
 - ❖ If the same error message is displayed repeatedly, request repair.




CAUSE The product is not in a measurement-enabled state.


When “SELF TEST FAILURE” is displayed

1. Switch off the power of the product.
2. (After checking that the power is switched off), switch on the power.
 - ❖ If the same error message is displayed repeatedly, perform steps 3 and 4 below.
3. Switch off the power.
4. Perform automatic calibration.

(See “5.4 Automatic Calibration.”)




CAUSE The product does not meet the prescribed measurement capability.



When “AUTO CALIBRATION FAILURE” is displayed

1. Switch off the power of the product.
2. (After checking that the power is switched off), perform automatic calibration.
(See “5.4 Automatic Calibration”).

- ❖ If the same error message is displayed repeatedly, request repair.



CAUSE Automatic calibration is not performed correctly.

When “PARAMETER ERROR” is displayed

1. Switch off the power of the product.
2. (After checking that the power is switched off), switch on the power.
 - ❖ If the same error message is displayed repeatedly, request repair.



CAUSE Abnormal operation parameters

When “SYSTEM ERROR” is displayed

1. Switch off the power of the product.
2. (After checking that the power is switched off), switch on the power.
 - ❖ If the same error message is displayed repeatedly, request repair.




CAUSE Anomaly in control block

When “Not enough reflection” is displayed

- Shorten the distance to the detection point.
- Perform measurement from a perpendicular angle rather than a slanting angle against a reflecting object at the detection point.

CAUSE Insufficient received light




When “Too much reflection” is displayed

- Change the detection direction or the angle of the product so that external light such as sunlight does not get in the unit.
- Change the detection point so that strong light does not get in the unit.


CAUSE Strong light such as sunlight is getting inside the light receiver.

This may be caused by an object with extremely high reflection such as a mirror.



When “High density gas” is displayed

- The unit is detecting methane thicker than the concentration that can be correctly measured.



7. IN CASE OF TROUBLE

7.1 Problems and Solutions

The product does not operate even when the Power button is pressed.

- Did you continue pressing until you hear a beep sound? (approx. 2 seconds)
(See “5.1. Starting Up and Ending.”)
- Is the battery pack sufficiently charged?
Use a fully charged battery pack.
(See “4.1 Charging Battery Pack.”)

No measurement beep sound is emitted

- Has the [SOUND LEVEL] setting been set to off?
(See “5.3 Changing Settings.”)

No alarm of alarm

- Has the [ALARM LEVEL] setting been set to a high value?
(See “5.3 Changing Settings.”)
- Has the [SOUND LEVEL] setting been set to off?
(See “5.3 Changing Settings.”)

The battery pack cannot be charged

- Is the battery pack correctly attached to the battery charger?
(See “4.1 Charging Battery Pack.”)
- Are the battery charger, AC adapter, AC cord, and power outlet correctly connected?
(See “4.1 Charging Battery Pack.”)
- Is the red LED of the battery charger lit?
(See “4.1 Charging Battery Pack.”)



8. Daily Maintenance

8.1 Maintenance Method

If the laser beam output window and the light receiver of the product are soiled, gently wipe them clean with a dry soft cloth being careful not to scratch them.

9. Main Specifications

9.1 Main Specifications of Main Unit

Items	Specifications
Target Gas	Methane (CH ₄) and methane-containing gases (natural gas and similar)
Detection limits	1 ~ 50,000 ppm·m
Accuracy of detection	±10 % note)
Detection speed	0.1 seconds
Detection distance	0.5 m ~ 30 m 0.5 m ~ 100 m (using a reflect sheet)
Battery	Rechargeable nickel metal hydride
Operating time	Approx. 6 hours (at 25°C, Display level: 5)
Laser Safety	IEC60825-1 (JIS C6802)
Guide light	Output wavelength: 650nm Output level: 1mW (Class 2) or less
Measurement light	Output wavelength: 1653nm Output level: 10mW (Class 1) or less NEVER LOOK INTO THE LASER BEAM
Intrinsic safety	Main Unit:  I M2 Ex ib op-pr/op-is I IIA T1 Battery Pack:  I M2 Ex ib I IIA T1
Electromagnetic Compatibility	CE Marking EMC Directive
Operating temperature	-17 ~ 50 °C
Operating humidity	30 ~ 90 % (No dew condensation)
Storage temperature	-20 ~ 60 °C
Storage humidity	90 % or less
Dimensions	70 (W) x 179 (D) x 42 (H) mm
Weight	600 g or less (Including Battery Pack)

note) The Accuracy of detection at 100ppm·m and 1,000ppm·m on the special measurement system.

9.2 Main Specifications of Battery Charger and AC Adapter

Items	Specifications
Specified battery	Dedicated Battery Pack
Charging Time	Approx. 4 hrs
Operating temperature	5 ~ 35 °C
Operating humidity	30 ~ 90 % (No dew condensation)
Storage temperature	-10 ~ 60 °C
Storage humidity	90 % or less
AC adapter input voltage	100 ~ 240VAC
AC adapter output voltage	12VDC



WARNING

Never charge the battery pack in a location with flammable gas.



WARNING

The battery charger does not feature an intrinsically safe design.

10. Ordering Information

10.1 Main Unit and Standard Accessories

Model Type	Product Name	Remarks
SA3C32A	LaserMethane mini	Set in there is one following SA0Z43A AC Adapter SA0Z45A Power Cable(EU)
SA0Z40A	Battery pack: 1 pc.	
SA0Z42A	Battery charger: 1 unit	
SA0Z47A	AC Adapter Set(EU): 1 unit	
SA0Z44B	Strap (Long type): 1 pc.	
SA0Z41A	Protector: 1 pc.	
—	Operation manual: 1 vol.	
		AD-L0009CZ013

11. Inquiries

Direct any questions about the product or reports about problems to Customer Service or to your local sales agent.

11.1 Customer Service

Overseas Sales Department

Tokyo Gas Engineering Co., Ltd.

4F, Nissei Aroma Square,

5-37-1 Kamata, Ota-ku, Tokyo 144-8721 Japan

TEL: +81-3-5480-6831

FAX: +81-3-5480-6838

URL: <http://www.tge.co.jp/>

12. Distributor and Manufacture

12.1 Distributor

Overseas Sales Department

Tokyo Gas Engineering Co., Ltd.

4F, Nissei Aroma Square

5-37-1 Kamata, Ota-ku, Tokyo 144-8721 Japan

TEL: +81-3-5480-6831

FAX: +81-3-5480-6838

URL: <http://www.tge.co.jp/>

12.2 Manufacture

Anrisu Corporation

5-1-1 Onna, Atsugi-shi, Kanagawa, 243-8555 Japan

TEL: +81-46-223-1111

URL: <http://www.anritsu.co.jp/>

Service & Support Section

Tokyo Gas Engineering Co., Ltd.

Overseas Sales Department

4F, Nissei Aroma Square,

5-37-1 Kamata, Ota-ku, Tokyo 144-8721

TEL : +81-3-5480-6831

FAX : +81-3-5480-6838

