

Telescopio Nazionale Galileo

HARPS-N Operation Guide

Draft Manual version 2.2.4 TNG-MAN-HARPN-0003 Date: 22-05-2013

Prepared

R. Cosentino

Change Record

Issue/Rev.	Date	Section/Page affected	Reason/Remarks
V1.0	14-12-2012	First version	
V1.1	14-01-2013		Autoguider added
V1.2	04-02-2013		
V2.0	12-02-2013		New sequencer and Labview SW
V2.1			
V2.2.3	22-05-2013	All document	Paragraph 3.5 added
V2.2.4	19-11-2013	All document	

Contents

1	Ι	ntrodu	iction	4
	1.1	Sco	pe	4
	1.2	Ado	litional information	4
	1.3	Со	ntact information	4
2	E	Before	the observations	5
	2.1	The	e Observation blocks preparation	5
	2.2	The	e Sequencer GUI (initialization and operation)	6
	2	2.2.1	Initialization	7
	2	2.2.2	Sequence Control buttons	8
	2	2.2.3	Instrument control buttons	8
	2	2.2.4	Other changes	8
	2	2.2.5	Before the calibration	9
	2	2.2.6	The standard calibration (daily calibration)	
3	(Observ	ations	11
	3.1	The	e start night	11
	3.2		e focus procedure	
	3.3	The	e pointing model procedure	
	3.4		e science OB execution	
	3.5	The	e Observing Control Software (OBS)	
	3	3.5.1	Common situation: The pointing sends the telescope to the limit switch	
	3.6	The	e Autoguide	
	3	3.6.1	The HARPS-N AutoGuider windows	16
	3	3.6.2	The Integrated Image window	
A	ppe	ndix A	- Useful Harps-N webpages	19
	Ар	pendix	B - Actions of multi task commands	
	Ap	pendix	C	

1 Introduction

1.1 Scope

This User Manual is intended to give all necessary information to potential users of the HARPS-N instrument, to help them to use the instrument and manages the observation at the TNG telescope.

The following documents are closely related to this manual and should be consulted as well:

- The HARPS-N User Manual (TNG-MAN-HARPN-0002)
- The HARPS-N Startup Manual (TNG-MAN-HARPN-0001)
- The New Short Term Scheduler User Manual (NSTS)
- The DRS User Manual (OG-MAN-HAN-13-0004)

Both are available through the TNG web page

http://www.tng.iac.es/instruments/harps/

1.2 Additional information

The latest information updates about the HARPS-N instrument can be found on the HARPS-N web pages

http://www.tng.iac.es/instruments/harps/

1.3 Contact information

Feedback on this User Manual from users is encouraged. Please email to <u>cosentino@tng.iac.es</u>

2 Before the observations

Starts up the system following the instructions of the "HARPS-N Quick Start Guide" and take care to read all the advices reported at the beginning of the manual.

2.1 The Observation blocks preparation

From the NSTS the observer can prepare the sequence of observation blocks of the night (Figure 1).

The target can be inserted directly in the NSTS or by using a catalog file that contains the objects information. The format of the catalog file is an ascii file and the fields separator is a TAB (ascii code = 9).

The fields of the catalog are shown in Table 1, the mandatory fields are shown in bold format.

An example of catalog file is shown in the HARPS-N webpage:

(http://www.tng.iac.es/instruments/harps/data/SpStdHARPSN.cat)

Table 1- Catalog file entries

name	object code
alpha	right ascension (nn:nn:nn.nn)
delta	Declination (nn:nn:nn.nn)
mualpha	proper motion alpha(arcsec/year)
mudelta	proper motion delta (arcsec/year)
mv	magnitude V
bv	Bv
ТурЅр	spectral type
radvel	mean radial velocity (KM/sec) or -99999
snr	Signal/Noise (550nm)
spectr	spectral type for the mask(two chars only)
remarks	Remarks
acquisition	Acquisition template (es. HARPN_ech_acq_objA)
equinox	Equinox
progid	program identificator (es. TAC_xx)
piname	PI name
exptime	Exposure time

Plac Zon Offs		D: 5607		UT: 01:54 LT: 02:54 ST: 16:46	:00	UT: LT: ST:	21:57:27	05:18:27 06:18:27 20:11:50	TCP : 2000 a: Alpha: 05h37m Delta: 21d32m Vel: No Targ	i.
ID	Name	Tornel	Alpha	Deita	MV St., TExp Ai., Nr.,	1	Template Obs	and the second se		
	HARPN ech obs all	Target	Арпа	Deita	01:12 1 1	- 1			Kara Kara Kara	1
21 1	OB TECHNICAL				0 0.0 0		MAIN PARAMETE	RS DET DPR	IS OCS TPL TEL	
	HARPN instr Icu init				01:		INS.MIRR.POS			
	HARPN instr ag init				01:		INS.PIIN.POS			
	HARPN tec set lamp				01:					
22 1	OB TECHNICAL				0 0.0 0		INS.OPTI1.POS	- A.		
22.	HARPN instr ag init			* * *	01:					
	OB TECHNICAL				0 0.0 0		INS.OPTI2.POS			
23 1	HARPN_tec_startnight				01:		indition that ou			
24	OB SCIENCE	HD127334	14h29	41:47:4	6 0 1 1					
254	OB SCIENCE	HD127334	14h29	41:47:4	6 0 6 5		INS.ROT1.DST			
26 1	OB SCIENCE	HD127334	14h29	41:47:4	6 0 1 10					
27 1	OB SCIENCE	HD127334	14h29	41:47:4	6 0 1 1.110		INS.ROT2.DST			
28 /	OB SCIENCE	HD127334	14h29		6 0 1 10					
29 /	OB SCIENCE	HD127334	14h29		6 0 1 10		INS.LAMP1.ST	0 -	Tun	
30 /	OB SCIENCE	HD185144	19h32		4 0 6 10			- 1000		
	OB CALIBRATION	NONE			0 8 2					
	HARPN ech cal waveAB				02:40.0 1		INS.LAMP2.ST	0 -	Thar1	
	HARPN ech cal waveAB				02:40.0 1					
	OB CALIBRATION	NONE			0 8 2		INS.LAMP3.ST	1 -	Thar2	
	OB SCIENCE	K00141	19h12		81 0 3 3					
	HARPN ech acg objAB				13 02:	-				
in com M mil Time Of	23/05/20	00m 20h 00 12 10h 00m	22h ••• 12h 00m	00m 00 56070 14h,00m	· · · · ·	04 00m	+b 00m 06h 20ñ 00m	44/ U	DAY on born 12 5/2012 oh pom / 02h pom	in on

2.2 The Sequencer GUI (initialization and operation)

After the startup of HARPS-N the instrument is ready to the initialization of the subsystems and the start of operation.

The sequencer GUI (Figure 2) is divided into several sections:

- The sequence control buttons, for the interaction with the observing blocks
- The Instrument control buttons, for the interaction with the HARPS-N's subsystems
- *The observation Execution logs* window, where the commands execution and the errors are shown
- *The acquisition control* buttons, (expose, repoint, etc), allows to do actions related with the autoguider's image visualized by the DS9 application.

The DS9 application shows the autoguider's image and interacts with the sequencer.

During the command execution the status is visualized into the observing status window and, at the end of execution, a bell sound confirms the correct execution of the command (if the sound is a horn noise, this means that something goes wrong and an error should be shown in the *observing status* window).

2.2.1 Initialization

From the *instrument control* section, click on the *LCU Init* button and wait until the command ends.

Then click on the *AG Init* button and wait until the command ends.

The system now is ready to calibrations (but not for the observations).

😣 🗐 🗊 HARPS-N NSequencer And Observatio	ons Control System	ı						
Sequence & Instrument Control Commands Simula								
Observations Execution logs	Sequence Control				Instrument Control			
18:25:09: START HARPN_instr_ag_init	N 🔶 N	lext OB	Terminat	e Exposure	Start/End Night			
18:25:24: Execute AG_Init	Single OB	● Single OB			Start	Night	End Night	
18:26:25: OK	Current OB Status							
18:28:29: Finished! 18:30:05: START HARPN_instr_Icu_init	Exposure:		00:00:00		-Start/End Telescop	e		
18:30:07: Execute FEU_LcuUsbInit 18:30:47: OK	OB Block ID:	-1			Start Tel	End Tel	0	UNDEFINED
18:30:47: Execute FEU_Init								
18:32:22: OK 18:32:22: Execute CU_Init	OB Block name	Technical 1			-Start/End Instrume	nt		
18:33:03: OK	Template ID: Template name:	HARPN_instr_lc	u init		Start Ins	End Ins	0	UNDEFINED
18:33:03: Execute EXPM_Init 18:33:03: OK	NEXP:	1						
18:33:03: Execute EXPM_MonitorStart					Auto Guiding	1		
18:33:04: OK 18:34:06: Finished!	Status:	FINISHED			AG Init			READY
					LCU	1		
					LCU Init		۲	READY
					Dust Cover			
	Acquisition Contro	1			Open	Close	\bigcirc	UNDEFINED
	Add Magnitu				This is a second			
			-		TUN Lamp			
		Expose	X Coordinate:	0.0	Turn ON	Turn OFF	\bigcirc	UNDEFINED
	🔎 🔎 Get in	fos from DS9	Y Coordinate:	0.0	THAR1 Lamp			
	Get D	SS field in DS9	FWHM X:	0.0	That Lamp			
			FWHM Y:	0.0	Turn ON	Turn OFF	\bigcirc	UNDEFINED
	•	Repoint	Peak:	0.0	THAR2 Lamp			
	 	Go	Background:	0.0				
	Automatic Acqu	isition	1		Turn ON	Turn OFF	<i>—</i>	UNDEFINED

Figure 2 - The Sequencer GUI

Note-1: The red log "Failed to fetch data from telemetry!" is not an error and can be ignored as error if appears during calibrations or in acquisition with exposure time less than 5 seconds.

Note-2: The yellow log "[...] Warning Final AG guide FITS file not found!" is a warning that don't affect the observation (we are working to fix this bug)

Add magnitude	Increases/decreases the value of the magnitude of the selected star
Expose	Take a new image with the AG camera
Get infos from DS9	Take coordinates and FWHM from the point clicked in the DS9 image
Get DSS fields in	Visualize the compass in the DS9
DS9	
Repoint	put the point clicked in the DS9 image into the fiber position and acquire a
	new image
Go	put the point clicked in the DS9 image into the fiber position and start the
	autoguider
Automatic	Selects , put in the fibre and start the acquisition of the brightest star of the
acquisition	field

Table 2 - Acquisition Control buttons

2.2.2 Sequence Control buttons

Next OB \rightarrow executes the next block available of the NSTS Single OB \rightarrow if checked executes one block when the user click on **Next OB** button Queue Mode \rightarrow if checked executes a series of NSTS blocks (according with the NSTS rules) when the user clicks on **Next OB** button Terminate exposure \rightarrow ends the current exposure and save the scientific frame Abort block \rightarrow aborts the current block

2.2.3 Instrument control buttons

Start night button→ executes the Telescope Start night and the Instrument start nightStart Tel button→ executes the Telescope Start night

Start Ins button → executes the **Instrument start night**

Dust Cover buttons → **Open** and **Close** the dust cover

Note: The *Start Night* button includes the preparation to observation of the telescope and of the instrument.

With the new two buttons the user can do this operation separately by using the **Start Tel** and the **Start Ins** Buttons.

2.2.4 Other changes

The sequencer now has a feedback with the NSTS. If the NSTS is not in execution the sequencer visualizes a warning.

😣 Warning						
	Problem while trying to send Block feedback to STS!					
	OK					

Note: When the sequencer is restarted after an error, the status buttons are not refreshed to the correct status (except the lamps buttons, which are refreshed after a while). The undefined (yellow) status of the other buttons is not real and can be ignored (if the user is sure that the instrument is initialized and ready to work) see Figure 2.

·ile E	dit Vie	w Frame	Bin Zoo	m Scale	Color	Region	WCS	Analysis	Help
ile bject alue K5 mage rame 1	a X Zoom	130402T00 1069 135.32767 237.791 0.505		15,256 497,1				N	
file	edit	view	frame	bin	zoom	scale	colo	r region wc	s help
linear	log	powe	r squ	are root	squ	ared	histog		zscale

Figure 3 - DS9 terminal with a binary star in the field

The compass is represented by the yellow axis, with the orientation shown in Figure 3.

2.2.5 Before the calibration

Few minute before the start of calibration (about 10 minutes), the observer has to turn on the thorium lamps. If the elapsed time is less then 10 minutes a warning windows appears; in this case the observer has to wait the time indicated in the popup window. The observer can ignore this warning but can compromise the quality of observation.

In the *Instrument control* section:

- 1. Click on the Turn ON button of THO1 lamp
- 2. Click on the Turn ON button of THO2 lamp
- 3. On the *LCU Device Monitor* verify the lamps status (Figure 4)

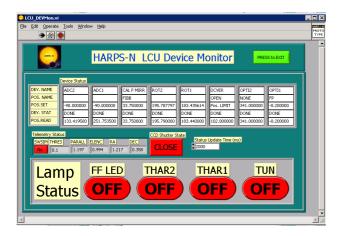


Figure 4 - LCU Device Monitor

A bell sound confirms the correct execution of the command

2.2.6 The standard calibration (daily calibration)

The daily calibration is very important to do in the afternoon (about 1 hour before the start of observation).

- 1. From the NSTS selects the 'standard calibration' OB
- 2. From the sequencer GUI, click in the '*Next OB*' button.
- 3. Verify in the DRS if the calibration goes without errors



Figure 5 - Thorium1 lamp warm warning



Figure 6 - Thorium lamp1 turn off warning

During the command execution the status is visualized into the *observation Execution logs* window and, at the end of execution, a bell sound confirms the correct execution of the command (if the sound is a horn noise, this means that something goes wrong and an error should be shown in the *observation Execution logs* window).

The standard calibration procedure is about 11 minutes long.

Very important: When the calibration ends, turn off the thorium 1 lamp:

- 1. Click on the **Turn OFF** button of THO1 lamp
- 2. Click on the **Turn OFF** button of THO2 lamp (if you will **not observes** in thorium simultaneous mode)
- 3. On the *LCU Device Monitor* verify the lamps status (Figure 4)

Note: If the TH1 lamp remains in the on state, after a while a warning window appears. The observer can decide if maintain the lamp in on (only if he is using it) or turn off it.

3 Observations

3.1 The start night

Before the start of observation the system needs that some processes starts and then the telescope is ready to work in HARPS-N mode.

- 1. Be sure that the system is initialized and ready to work (Start-up procedures, in the HARPS-N Quick Start Guide)
- 2. In the sequencer GUI, click in the *Start Night* button in the *Instrument Control* section and wait the end of execution of the command.

Now HARPS-N is ready for observations.

Note: The *Start Night* button includes the preparation to observation of the telescope and of the instrument.

The user can do that operation separately by using the **Start Tel** and the **Start Ins** Buttons (recommended Action)

3.2 The focus procedure

At the beginning of the night, may be suitable do a focus procedure doing the following actions:

1. In the NSTS selects a star from the catalogue and delete the **HARPN_ech_obs_all** template

ID	Name	Target	Alpha	Delta
9 9 🗸	HAM OB SCIENCE	9596	03h52m54.000	00:00:19.000
9 🗸	HARPN_ech_acq_objAB		03h52m54.000	00:00:19.000

2. Add the HARPN_focus template

ID	Name	Target	Alpha	Delta
9 🗸	HAM OB SCIENCE	9596	03h52m54.000	00:00:19.000
9 🖌	HARPN_ech_acq_objAB		03h52m54.000	00:00:19.000
9 🖋	HARPN_focus	1000		

- From the sequencer execute this OB by clicking the *Next OB* button. (The sequencer sends the commands to: move the telescope, acquire an image from the autoguider camera and shows the image in the *DS9*.)
- 4. Click on the star and then click on the *Go* button in the *Acquisition* Image window. (The sequencer sends an offset to the telescope, puts the star in the fiber position, starts the autoguide, executes the focus procedure and moves the M2 mirror at the best position)

The focus procedure is about 10 minutes long.

3.3 The pointing model procedure

Sometimes the pointing precision can be poor and the telescope could need the execution of a pointing procedure. The pointing procedure must be done in collaboration with the telescope operator (TO) and the TO has to know some information during the procedure.

The sequences of actions to manage the pointing procedure are:

- 1. In the NSTS select a star from the catalog *HARPSN-PointingModel.cat* located in /home/guest/GAPS/CATALOGS
- 2. Delete the HARPN_ech_obs_all template

ID	Name	Target	Alpha	Delta	
γ 1 √	HAM_OB_SCIENCE	HR4554	00h00m00.000	53:41:41.100	
1 🖋	HARPN_ech_acq_objA	67.7.75	00h00m00.000	53:41:41.100	ananan ana ang ang ang ang ang ang ang a

- 3. From the sequencer execute this OB by clicking the **Next OB** button and tell to the TO when the AG image starts, (this is the critical point of this procedure) : Sequencer: Thu Dec 27 23:12:29 UTC 2012 -> launch AG expose
- 4. When the image of the star appears, clicks on the star, then clicks on the *Repoint* button in the *Acquisition* Image window and tell to the TO that the offset has been applied.
- 5. The TO takes note in the VME of the offset applied, the paralactic angle and uses these data in the pointing procedure.
- 6. Repeat the cycle with another star (from point 1.) until the pointing procedure reaches the precision expected.

3.4 The science OB execution

In the execution of a scientific OB the object has to be pointed and centred in the fiber with the intervention of the observer.

1. In the NSTS select a star from the catalog

ID	Name	Target	Alpha	Delta	
γ 1 √	HAM_OB_SCIENCE	HR4554	00h00m00.000	53:41:41.100	
1 🖋	HARPN ech acq objA		00h00m00.000	53:41:41.100	
1 🖋	HARPN ech obs all	1222			

- From the sequencer execute this OB by clicking the *Next OB* button. (The sequencer sends the commands to: move the telescope, acquire an image from the autoguider camera and shows the image in the *DS9*.)
- 3. Click on the star and then click on the *Repoint* button in the *Acquisition* Image window.

(The sequencer sends an offset to the telescope, puts the star in the fiber position, acquires another image from the auto-guider camera and shows the image in the *Acquisition* Image window)

4. When the image appears, if the star is in the fiber position (red circle), click in the *Go* button in the *Acquisition* Image window.

After that the sequencer starts the auto-guide and the spectroscopic acquisition. When the OB ends, a bell sound confirms the correct execution of the command and the Next Acquisition button turns in active mode.

3.5 The Observing Control Software (OBS)

The OCS is the interface to the Telescope Control System (TCS). The interface enables the instrument to send commands to the telescope via the TNG library. Currently HARPS-N is able to send three commands; Pointing, AG offsets and M2 offsets to calculate and correct the focus via an automatic procedure. The connections between both systems are completely asynchronous but when the command finishes successfully the TCS returns an Ok status. When an error condition has arisen, the TCS also returns a message back to the sequencer flagging that condition.

In the Observing manager webpage is possible to monitoring the actions and the results. The operator can also interrupt the action when the condition needs it.

3.5.1 Common situation: The pointing sends the telescope to the limit switch

When one of these conditions will occurs:

- a pointing-command moves the telescope to the limit switch position
- the telescope operator thinks that the telescope can reach the limit switch during the observation

The telescope operator has to stop the command by clicking the cross button in the 'option' section in the "tng observing manager" webpage.

On the sequencer, the astronomer has to wait doing nothing, until the sequencer ends the OB with an abort.

At this point the telescope operator can move the telescope to an appropriate position and the astronomer can repeat the aborted OB.

When the tracking moves the telescope close to the limit switch, and the telescope operator must to stop the telescope during the science exposure. The procedure to stop the processes is the following:

- 1) from the sequencer terminate the exposure of the current OB (click on **terminate exposure** button)
- 2) from the tracking system stop the telescope

Note: if the executing OB consists of more than one exposure, the astronomer has to terminate all the exposure or click on the **abort block** button at the end of the first "**terminate exposure**".

TNG Observing Manager

Main Panel

OCS Systems



OCS Execution Table History


Date	Time (UT)	UT) Command		Status	Options P ×	
18/03/2013	18:40:49	OS_TEL_StartNi	OS_TEL_StartNightHARPS FINISHED			
18/03/2013	16:04: OC	CS Command Summary X			P	×
18/03/2013	16:03:	Name:	OS_TEL_StartNightHARPS		P	×
18/03/2013	15:50:	Parameters			P	×
18/03/2013	15:40:	Status: Sequence:	FINISHED HARPS-BBE7702E		P	×
18/03/2013	14:44:	Source:	HARPS_SEQ		P	×
18/03/2013	14:39:	Started at:	18/03/2013 18:40:49		٩	×
18/03/2013	14:37:		18/03/2013 18:43:28 Command executed successfully		٩	×

Figure 7 - TNG Observing Manager webpage

3.6 The Autoguide

The autoguider starts when the observer clicks on the accept button of the sequencer GUI and two windows opens (Figure 8 and Figure 9):

- 1. The HARPS-N AutoGuider windows
- 2. The Integrated Image window

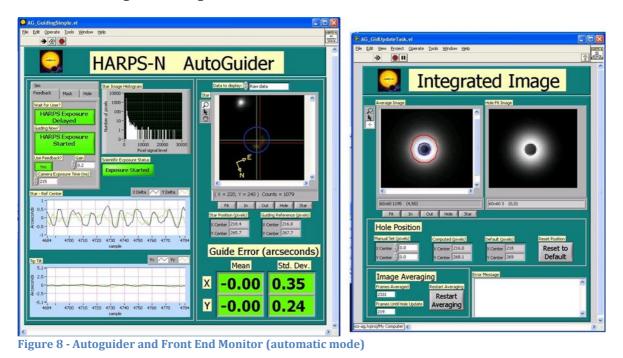

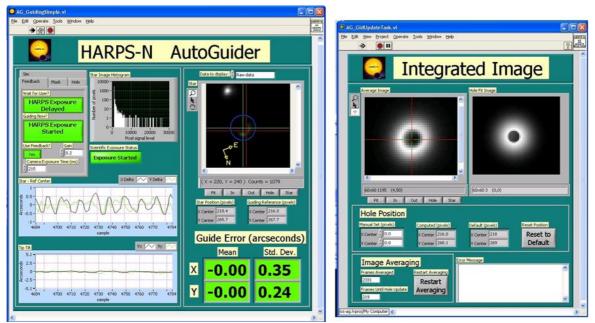


Figure 9 - Autoguider and Front End Monitor (manual mode)

3.6.1 The HARPS-N AutoGuider windows

This window shows the autoguider images, some information about the guide settings and status and allows changing the guide mode:

3.6.1.1 Feedback (offload) tab

The *feedback* tab opens a menu where the user can change the parameter of the tip-tilt correction and can postpone the start of scientific exposure

- Use Feedback \rightarrow enable/disable the tip tilt correction (the offload remain active)
- The gain and delay value change the behavior of tip-tilt
- Wait for user \rightarrow freeze the starting of autoguider (and scientific exposure)
- Guiding now \rightarrow unfreeze the starting of autoguider (start autoguide)




Figure 10 - Feedback panel

The *Wait for user* button remains active few seconds before the automatic starting of autoguide. If the user sets this button on *Yes* the autoguide get stuck until the *Guiding Now* button is selected.

3.6.1.2 Mask tab

To avoid the contamination of others star close to the guide-star during the guide, a mask around the guide star can be selected.

The observer can select the mask's radius around the guide star, all the object out the mask will be ignored by the guiding algorithm.




Figure 11 - Mask window

3.6.1.3 Hole tab

With this panel is possible to select the hole- find method, the centering algorithm, and the hole's dimension (optional)

- *Manual Hole Find* \rightarrow selects the manual or automatic method
- The *auto hole method* → select the algorithm for guiding end for the hole-center calculation
- *Hole shift Limit* → changes the maximum variation permitted (in pixels) in hole position calculation
- **Update Period** → number of frames used in hole position calculation

Feedback Mask H	lole
Manual Hole Find?	
No	
Auto Hole Method	
2D Curve Fit	
Hole Shift Limit (pixels)	
<u>/</u> 7	
Update Period (frames)	
25	

Figure 12 – Hole tab window

In the The HARPS-N AutoGuider windows (Figure 8) the white cross represent the center of the star and the Red Cross is the center of the fiber.

3.6.1.4 Simulation tab

This panel was used in engineer tests. It is no useful in normal observations.




Figure 13 – Shutter simulation panel

3.6.2 The Integrated Image window

This window shows the integrated images, some information of the guide's execution and allows to change the reference point (fiber position) when the manual mode is stetted. The information shown depends by the hole's find method selected:

Manual mode: the fiber's reference position is based on a table and can be modified by the user dragging with the mouse the green cross pointer.

Automatic mode: the fiber's reference position is calculated by the selected algorithm. The red circle represents the contour of the star, the blue circle the shape of the hole.

3.6.2.1 Main frame image

- Average image
- Hole fit image
- Fit
- In
- Out
- Hole
- Star

3.6.2.2 Hole Position

- Manual set
- Computed
- Default
- Reset position

3.6.2.3 Image Averaging

- Frames avaraged
- Frame until frame updated
- Restart averaging
- Error message

	Contraction Programmer Contraction Contraction
HARPS-N TNG webpage	http://www.tng.iac.es/instruments/harps/
TNG Observing Manager	http://ntcs-glassfish1.tng.iac.es:7080/ntcs-ocsservice/manager/ui/observingmanager.jsf
HARPS-N Sensors	http://tngweb.tng.iac.es/harps/
Instrument status	http://ntcs-glassfish2.tng.iac.es:7080/webcontrolpanel/ui/instrumentstatuspanel.jsf

Appendix A - Useful Harps-N webpages

Appendix B - Actions of multi task commands

Telescope start night:

- Open the HARPSN derotator cover
- Power on the Dolores electronics
- Initialize the Dolores movements
- Move the 'entrance slider' (M4) to the HARPS position
- Power on the M3 control
- Move M3 to Nasmyth-B (the TO had to set the telescope in Nasmyth-B mode)
- Power off the M3 control

Telescope end night:

• Close the HARPSN derotator cover

Instrument start night (HARPN_tec_startharps):

- FE_adczero
- FE_startadc
- FE_gettelemetry
- VC_startexp
- VC_useshutter

Instrument end night(HARPN_tec_startharps):

- AG_stopguide
- FE_stopgettelemetry
- FE_stopadc
- VC_stopexp

LCU init:

- Execute USB init
- Execute FEU init
- Execute CU init
- Execute EXPM init
- Execute EXPM monitor start

Appendix C

List of acronyms

ADC	Atmospheric Dispersion Compensator			
AG	Auto-Guider			
CCD	Charge Coupled Device			
CCF	Cross Correlation Function			
CFC	Continuous Flow Cryostat			
CU	Calibration Unit			
DFS	Data Flow System			
DRS	Data Reduction Software			
E2DS	Extracted 2-Dimensional Spectrum			
ETC	Exposure Time Calculator			
FEU	Front End Unit			
FITS	Flexible Image Transport System			
FWHM	Full Width at Half Maximum			
HARPS-N	High Accuracy Radial velocity Planet Searcher in the North hemisphere			
ND	Neutral Density			
NSTS	New Short Time Scheduler			
OB	Observing Block			
RV	Radial Velocity			
SA	Support Astronomer			
SNR	Signal to Noise Ratio			
TBC	To Be Confirmed			
TBD	To Be defined			
ΤBF	To be fixex			
ThAr	Thorium Argon			
TNG	Telescopio Nazionale Galileo			
ТО	Telescope Operator			
VA	Visiting Astronomer			