I.R. thermography camera



C.A 1886 C.A 1888



ENGLISH

User's manual



English

Thank you for buying a RayCAm I.R. thermography camera.

For best results from your device:

- read this user manual attentively,
- **observe** the precautions for its use

MEANING OF THE SYMBOLS USED

<u> </u>	Selective sorting of wastes for the recycling of electrical and electronic equipment within the European Union. In conformity with directive DEEE 2002/96/EC: this equipment must not be treated as household waste.		
	Risk of danger. See explanations in this user manual Problems that may affect the operation of the I.R. camera.		
	Notes completing the essential operating procedures.		
	Laser radiation, do not look directly into the LASER beam.		
CE	This marking certifies compliance with the European "Low Voltage" and "Electromagnetic Compatibility" directives (2006/95/CE and 2004/108/CE).		



Characteristics of the laser: Class 2, < 1 mW, wavelength 635nm



WARNING
LASER RADIATION
DO NOT LOOK DIRECTLY INTO THE
BEAM
CLASS 2 LASER DEVICE

CONTENTS

1. PRECAUTIONS OF USE	6
2. DESCRIPTION	7
2.1 Front panel	7
2.2 Keypad	
2.3 VIEW OF BACK AND BOTTOM	8
3. STARTING UP	9
3.1 Charging the battery	9
3.2 Installing the battery	10
3.3 SWITCHING ON AND OFF	
3.4 CHECKING THE INFORMATION ON THE LCD SCREEN	12
3.5 SETTING THE DATE AND TIME	
3.6 Local settings	13
4. BASIC FUNCTIONS	15
4.1 Using the LCD screen	15
4.2 SELECTION OF MENUS AND PARAMETERS	
4.3 RESTORING THE DEFAULT SETTINGS	16
5. TAKING SHOTS	16
5.1 ADJUSTING THE CAMERA	16
5.1.1 Manual focusing	
5.1.2 I.R., Real, and Real + Mix Display	
5.2 PARALLAX ADJUSTMENT	
5.3 Adjusting the image	
5.3.1 Automatic adjustment	
5.3.2 Manual adjustment	18
5.3.3 Adjusting the image	19
5.4 Measurement range	
5.5 Freeze/Activate an image	21
6. ANALYSIS FUNCTION	22
6.1 ADJUSTMENT OF THE ANALYSIS PARAMETERS	22
6.2 ADJUSTMENT OF THE ANALYSIS PARAMETERS	
6.3 PARAMETERIZING THE ANALYSIS TOOLS	
6.3.1 Analysis by point	25
6.3.2 Isothermal analysis	25
6.4 DEACTIVATING THE ANALYSIS TOOLS	
6.4.1 Deactivation of the analysis tools	
6.5 RECORDING THE IMAGE	
6.6 ASSOCIATING VOICE REMARKS WITH THE IMAGES (OPTION)	27

6.6.1	Voice recording	27
	STMENT OF THE TRIGGER	
6.7.1	Adjustment of the release	27
7. READING	G AND ERASING	29
7.1 Openii	NG THE IMAGES	29
7.2 Playin	NG THE REMARKS (OPTION)	30
7.3 Erasin	NG THE IMAGES	31
8. TRANSF	TERRING IMAGES	32
8.1 Trans	SFER BY MINI SD CARD	32
9. CONNEC	CTIONS AND DOWNLOADING	33
9.1 Conne	ECTION TO A MONITOR	33
9.2 Using	THE BLUETOOTH HEADSET (OPTION)	33
10. TROUB	LESHOOTING	35
11. MAINT	ENANCE	36
11.1 CLEA	ANING AND MAINTAINING THE CAMERA	36
-	g of the device	
	reenROLOGICAL CHECK	
	AIR	
12. WARRA	ANTY	37
13. APPENI	DIX	38
13.1 TABL	LE OF EMISSIVITIES	38
14. TECHN	TICAL CHARACTERISTICS	40
15. DELIVE	ERY CONDITION	42


1. PRECAUTIONS OF USE

Before using the camera, make sure that you have read and understood the safety precautions described below. Make sure that the camera is used correctly.

Please refer to this manual each time you encounter a hazard symbol. To avoid exposure to laser radiation, injury, or damage to the device, and be sure that you use the camera in a risk-free way, observe the safety recommendations given below:



Do not look directly into the laser beam. Do not point the laser beam at





Do not aim the device towards the sun or other source of intense heat.

Use only the recommended batteries and accessories. Do not leave the device connected to mains when not necessary.



Avoid problems due to condensation.


Moving the I.R. camera rapidly from a cold to a warm place can cause condensation (droplets of water) to form on its outside and inside surfaces.

You can avoid this problem by placing the camera in the plastic case and letting it warm slowly to the ambient temperature before withdrawing it from the case.


- When you switch on the camera, wait 10 to 15 minutes before recording your first thermograms, to be certain that the camera's temperature has stabilized and that your measurements are correct.
- Focus the objective correctly according to the distance to the target to be inspected.
- Device that may, but only under special conditions, be sensitive to electrostatic discharges (ESD).

2. DESCRIPTION


2.1 FRONT PANEL

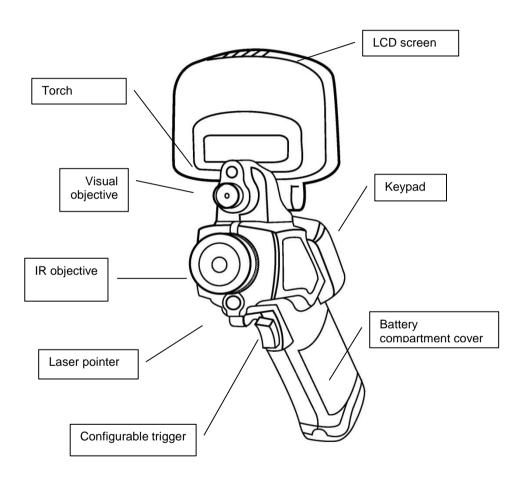

2.2 KEYPAD

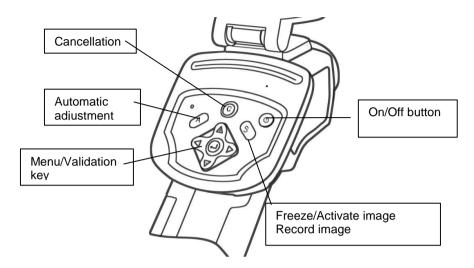


2.3 VIEW OF BACK AND BOTTOM

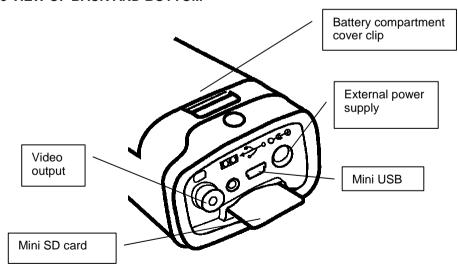

3. STARTING UP

3.1 CHARGING THE BATTERY

1. Align the edge of the charger on the line marked on the battery and push the battery in until it locks.



- 2. Connect the power cord to the charger and plug into a power outlet.
 - The charging indicator lights red during recharging and green when charging is over.
 - After recharging, disconnect the charger and withdraw the battery



- It is a lithium ion battery. It does not have to be fully discharged before
 recharging (no memory effect). The number of complete
 charging/discharging cycles is approximately 500; beyond this number,
 the battery loses its capacity and has to be recharged more often.
- The charging time varies with the ambient temperature and the initial charge condition.

C.A1886 - C.A1888


3.2 INSTALLING THE BATTERY



- The battery must be fully charged before it is used for the first time (the battery reaches its full capacity only after 5 complete charging/discharging cycles).
- Switch off the camera. Push the clip of the battery compartment cover toward the front, then lift the cover.



2. Install the battery in its compartment, then push it in until it locks.



3. Close the battery compartment cover.

Withdraw the battery when you expect to leave the camera unused for an extended period (in order to avoid discharging too deeply): even when the camera is off, there is some consumption (C.A 1886: 8 mA; C.A 1888: 6,6 mA).

The Mini SD card must be formatted to FAT16 or FAT32, since otherwise the camera may fail to recognize it.


Symbols representing the battery charge condition

4 1111 4 1111 4 111.	Battery adequately charged	
(-1)	Battery low	
1	Battery needs to be replaced or recharged	

3.3 SWITCHING ON AND OFF


The power check light remains on for as long as the camera is on.

1. Place your thumb above the keypad and your index finger in front of the configurable trigger.



2. Press the On/Off button and hold it down for three seconds.

The power check light lights green.

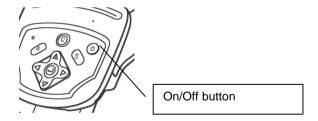

3. After a few seconds, the start-up screen is displayed.

4. Power down


Press the On/Off button for three seconds.

The power supply indicator goes off.

C.A1886 – C.A1888

3.4 CHECKING THE INFORMATION ON THE LCD SCREEN

The LCD screen provides a field of view corresponding to 100% of the actual shot

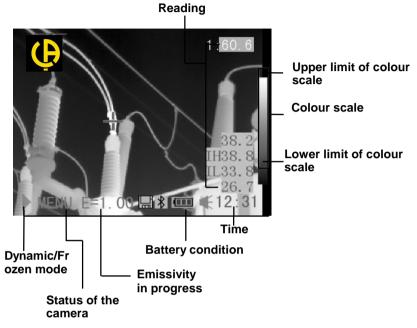



About the status of the camera

	Menu	The device is in Menu mode		
	Null	The device is not in Menu mode and no analysis tool has been selected.		
	1 3	The analysis tool selected is cursor 1, 2, or 3.		
Status of the camera	Сар	The analysis tool selected is the auto Max/Min detection cursor.		
	Isot	The analysis tool selected is isothermal analysis		
	Е	Emissivity in progress.		
		A Mini SD card has been inserted		
	*	The Bluetooth headset has been installed		

3.5 SETTING THE DATE AND TIME

You must set the date and time when you switch the camera on for the first time.

- 1. Check that the camera is in Null mode.
- 2. Press the MENU key and select the [Setup] menu.




- 3. Select the [Date and Time] sub-menu.
- 4. Set the date and time
 - Press the UP or DOWN arrow to select the field to be modified.
 - Press the LEFT or RIGHT arrow to define the values.
- After completing the parameterizing, press the MENU/VALIDATION key to close the window and save the modifications, or the C key to exit without saving.

3.6 LOCAL SETTINGS

This menu is used to display the local parameters of your geographical zone.


- 1. Check that the camera is in Null mode.
- 2. Press the MENU/VALIDATION key, then the UP or DOWN arrow to select the [Setup] menu.



C.A1886 – C.A1888

English

3. Press the UP or DOWN arrow to select [Local], then press the MENU/VALIDATION key.



4. Local parameters

- Press the UP or DOWN arrow to select the field to be modified.
- Press the LEFT or RIGHT arrow to define the values.
- After completing the settings, press the Menu/Validation key to close the window and save the modifications, or the C key to exit without saving.



About the local settings

Language	Selects the language of the menus and messages.		
Temp unit	Selects the temperature format of the camera: ℃ or ℉.		
Distance unit	Selects the unit of distance of the camera: Metres or Feet.		
Video output	Selects the video output format of the camera: PAL or NTSC.		

4. BASIC FUNCTIONS

4.1 USING THE LCD SCREEN

- 1. Open the LCD screen in the direction
- 2. Aim the I.R. camera at the target.



- For a better temperature measurement, frame the subject in the centre of the LCD screen.
- The screen is switched to standby when you close it.


4.2 SELECTION OF MENUS AND PARAMETERS



Press the MENU/VALIDATION key to view the menus.

2. Select the desired menu using the UP and DOWN arrows.

Setup





Enter the menu by pressing the MENU/VALIDATION key.



Modify the desired values/modes using the up, down, right, and left arrows.



Validate the modifications using the MENU/VALIDATION key or exit without saving by pressing the C key.

C.A1886 – C.A1888

4.3 RESTORING THE DEFAULT SETTINGS

- Switch the I.R. camera off.
- Press the On/Off and C buttons simultaneously.
 Hold them down a few seconds.
 The camera reboots with the default parameters.




The stored data are not deleted when you reset the camera.

5. TAKING SHOTS

5.1 ADJUSTING THE CAMERA

5.1.1 Manual focusing

- 1. Check that the camera is in Null mode.
- 2. Aim the I.R. camera towards the target
- 3. Turn the focusing ring to focus on the target.



4. Continue turning until the image is sharp

5.1.2 I.R., Real, and Real + Mix Display.

This I.R. camera records visual images with its built-in digital device. This lets you record a real image and compare it to the thermal image.

 Press the "Menu/Validation" key to display the menu, then select "I.R./CCD".



2. Press the "left" or "right" arrow to select the percentage of infrared (possible only in "Vision + mix" mode).

This percentage is the percentage of thermal image in the display (100% means pure I.R. image, 0% means real image only).

The various modes available:

I.R.

In this mode, only the I.R. image is displayed on screen. All of the analysis tools are available in this mode. 6 sorts of palettes can be selected.

Vision

In this mode, only the visual image is displayed on screen. The analysis tools are not all available in this mode.

Vision + Mix

In this mode, the visual image appears in the background and the central window is the fusion zone. You can apply all of the analysis tools to this zone. You can also set the proportions of visual and thermal image using the "Percentage I.R." option.

5.2 PARALLAX ADJUSTMENT

Since the infrared and visual objectives are offset, the two images may be misaligned in the "Vision + Mix" mode.

C.A1886 - C.A1888

English

To align the two images:

- 1. Make sure that you are in NULL mode
- 2. Hold the C key down and press; the left arrow to shift the image to the left; the right arrow to shift the image to the right; the up arrow to shift the image upward; the down arrow to shift the image downward.

5.3 ADJUSTING THE IMAGE

You can set the brightness (Level) and contrast (Span) of the image captured by the I.R. camera manually or automatically.

5.3.1 Automatic adjustment

The I.R. camera adjusts the brightness and/or the contrast automatically when you press the A key.

5.3.2 Manual adjustment

You can adjust the image brightness and contrast in the menu or by pressing the arrows in NULL mode: press the UP or DOWN arrow to modify the contrast, the LEFT or RIGHT arrow to modify the brightness.

Manual adjustment in the menu:

- 1. Press the MENU/VALIDATION key
- 2. Press the UP or DOWN arrow to select the [Manual Adjust] menu. Validate by pressing the MENU/VALIDATION key.



3. Adjusting the brightness and contrast

- Press the LEFT or RIGHT arrow to select the field to be modified.
- Press the UP or DOWN arrow to define the values.


4. After this operation, press the MENU/VALIDATION key to save the modifications or the C key to close the menu window without saving.




 To activate manual adjustment, make sure that continuous adjustment (Menu -> Other) is deactivated.

5.3.3 Adjusting the image

- 1. Press the MENU/VALIDATION key.
- 2. Press the UP or DOWN arrow to select the [Setup] menu, then press the MENU/VALIDATION key.





3. Press the UP or DOWN arrow to select [Other], then press the MENU/VALIDATION key.

C.A1886 – C.A1888

English

- 4. Define the adjustments of the image.
 - Press the UP or DOWN arrow to select the field to be modified.
 - Press the LEFT or RIGHT arrow to define the values.
- 5. After this operation, press the MENU/VALIDATION key to save the modifications or the C key to close the menu window without saving.




About the adjustments of the image

	Assigns the pseudo-colours of the thermal image. 6		
Palette	palettes are provided: Metal, Reversed metal, Rainbow,		
	Natural, Grey, and Reversed grey.		
	Assigns the function of the A key. You may choose		
	among three option	ns: Level and contrast, level, or	
	contrast.		
		The device automatically	
	Level and	adjusts the brightness and	
	span	contrast of the image to their	
Auto Adjust.		optimum levels.	
, tato , tajaoti		The device automatically	
	Level	adjusts the brightness of the	
		image.	
		The device automatically	
	Sman	,	
	Span	adjusts the contrast of the	
		image.	
	Determines whether the brightness and contrast of the		
	image displayed on	screen are adjusted automatically	
	or not, continuously	with no press.	
Continuous	Level and	Automatic adjustment of the	
	span	brightness and contrast.	
Adjust.	Level	Automatic adjustment of the	
	Level	brightness.	
	N	No automatic adjustment of the	
	None	brightness or contrast.	

5.4 MEASUREMENT RANGE

You can switch from one temperature range to another, depending on the model of camera you have.

- 1. Press the MENU/VALIDATION key.
- 2. Press the UP or DOWN arrow to select [Adjust Manual], then press the MENU/VALIDATION key.
- 3. Adjustment of measurement range.
 - Press the LEFT or RIGHT arrow to select the range.
 - Press the UP or DOWN arrow to define the measurement range.
 - This option is not available when the image is frozen.



 When you have finished, press the MENU/VALIDATION key to close the menu window.

5.5 FREEZE/ACTIVATE AN IMAGE

You can activate/freeze a thermal image by pressing the S key of the selector.

- 1. Check that the camera is in NULL mode.
- 2. Press the S key to freeze the image.
- Press the S key again to activate the image and return to continuous measurements.

C.A1886 - C.A1888

6. ANALYSIS FUNCTION

6.1 ADJUSTMENT OF THE ANALYSIS PARAMETERS

- 1. Press the MENU/VALIDATION key.
- Press the UP or DOWN arrow to select [Obj Par], then the MENU/VALIDATION key.
- 3. Press the UP or DOWN arrow to select the field to be modified. Press the LEFT or RIGHT arrow to define the values.

 Emiss
 : 0.95

 Distance
 : 5m

 Amb Temp
 : 25.0℃

 Humidity
 : 50%

4. When you have finished, press the MENU/VALIDATION key to save the modifications or the C key to close the menu window without saving.



About the analysis parameters

	Different objects have different emissivities;	
Emiss	use different emissivities to measure different	
	objects.	
	The distance between an object and the I.R.	
Distance	camera is not a constant. Set this value	
	according to the distance to the target.	
Amb Temp	Entry of the ambient temperature.	
Humidity	Entry of the ambient relative humidity.	


6.2 ADJUSTMENT OF THE ANALYSIS PARAMETERS

- 1. Press the MENU/VALIDATION key.
- 2. Press the UP or DOWN arrow to select the [Setup] menu, then press the MENU/VALIDATION key.

3. Press the UP or DOWN arrow to select [Analysis], then the MENU/VALIDATION key.



- 4. Adjustment of an analysis parameter.
 - Press the UP or DOWN arrow to select the field to be modified.
 - Press the LEFT or RIGHT arrow to define the values.



5. When you have finished, press the MENU/VALIDATION key to save the modifications or the C key to close the window without saving.



About the analysis adjustments.


	Adjusts spot4 for au	utomatic tracking of the	
	hottest/coldest point on the screen.		
		Assigns spot4 to	
	Maximum	tracking the hottest	
Capture spot		point on the screen.	
		Assigns spot4 to	
	Minimum	tracking the coldest	
		point on the screen.	
	Activates or deactivat	es the temperature alert.	
	When the parameter i	s set to "On":	
	- if the [Captu	re Spot] parameter is	
	"Maximum", the a	alert is triggered as soon	
Alert	as the threshold set is exceeded.		
	- If the [Capture Spot] parameter is		
	"Minimum", the alert is triggered as soon		
	as there are temperatures below the		
	threshold set.		
Temp Alert	To set the temperature alert threshold.		
Corrects temperature measured by the can		measured by the camera	
Correct Temp	so as to ensure the accuracy of the		
Correct Temp	measurement in the event of drift of the		
	camera.		
Isotherm width	Assigns the width of the interval. This width		
isotherm width	can be as little as 0.1°	C.	
	Assigns the colour of the interval. The colours		
Isotherm colour	available are Transparent, Green, Black, and		
	White.		
Isotherm Alert	Assigns the isotherm alert temperature.		
Moves the image of the laser pointer on t		the laser pointer on the	
Adjust Laser	LCD display unit.		

6.3 PARAMETERIZING THE ANALYSIS TOOLS

This item describes how to adjust the thermal image analysis tools.

6.3.1 Analysis by point

- 1. Press the MENU/VALIDATION key.
- Press the UP or DOWN arrow to select the [Analysis] menu, then validate.
- 3. Adjustment of the point to be analyzed
 - Press the UP or DOWN arrow to select a point (cursor 1 to 3), then the MENU/VALIDATE key. One or more reticles appear on screen.
 - Max Sp automatically tracks the hottest or coldest point on the screen.



4. Moving the analysis point.

 Once the cursor has been selected (SP1 to SP3 is displayed in the bottom left corner), press the UP, DOWN, LEFT, and RIGHT arrows to move the active point.



The temperature of the active point is displayed in the top right corner.

6.3.2 Isothermal analysis

- 1. Press the MENU/VALIDATION key.
- 2. Press the UP or DOWN arrow to select the [Analysis] menu.
- Press the UP or DOWN key to select [Isotherm], then press the MENU/VALIDATION key. Zones where the temperature is between IL and IH (the max and min values of the isotherm) are displayed in the same colour on screen.
- 4. Adjustment of the isothermal page
 - Activate the isotherm (ISO is displayed in the bottom left corner).
 - Press the UP or DOWN arrow to shift the whole range of the isotherm.
 - Press the right or left arrow to diminish/expand the isothermal range.

C.A1886 – C.A1888 25

English



To change the type of isotherm, its width, its alert, and its colour, refer to the previous section.

6.4 DEACTIVATING THE ANALYSIS TOOLS

This section describes how to remove the analysis tools used from the screen.


6.4.1 Deactivation of the analysis tools

- 1. Press the MENU/VALIDATION key
- 2. Press the UP or DOWN arrow to select the [Analysis] menu.
- 3. Select the analysis tool you want to remove.
- 4. Press the C key to remove it.
- 5. To remove all of the analysis tools:
 - Press the UP or DOWN key to select [Remove All], then the MENU/VALIDATION key.
 - All of the analysis tools are removed.

6.5 RECORDING THE IMAGE

You can record an image after freezing it or record it directly by holding the S key down for 3 seconds with the device in NULL mode.

- 1. Press the MENU/VALIDATION key.
- 2. Press the UP or DOWN arrow to select the [File] menu.



- 3. Press the UP or DOWN arrow to select [Save], then the MENU/VALIDATION key to record the image.
- 4. The name of the image recorded is displayed on screen.



The image is recorded in the active directory. To change directories, go to "Menu" => "Other" => "Name of folder".

6.6 ASSOCIATING VOICE REMARKS WITH THE IMAGES (OPTION)

6.6.1 Voice recording

You can associate up to 30 seconds of voice remarks with an image.

- 1. Install the Bluetooth headset (provided as an option).
- 2. Freeze an image and press the MENU/VALIDATION key.
- 3. Press the UP or DOWN arrow to select the [File] menu.
- 4. Press the UP or DOWN arrow to select [Voice REC], then press the MENU/VALIDATION key.
 - The message [Voice Recording] is displayed on the LCD screen.
- 5. Speak into the microphone of the headset. To stop recording, press the C key.
- 6. Recording the image.

6.7 ADJUSTMENT OF THE TRIGGER

6.7.1 Adjustment of the release


1. Press the MENU/VALIDATION key, then the UP or DOWN arrow to select the [Setup] menu, then the MENU/VALIDATION key again.



C.A1886 – C.A1888 27

English

Press the UP or DOWN arrow to select the [Other] menu, then press the MENU/VALIDATION key.



- 3. Press the UP or DOWN arrow to select the [Trigger Button] menu, then the LEFT or RIGHT arrow to select the desired function.
 - About the configurable release function:


None	The function is inactive.		
Save	Makes it possible to record the image by keeping the		
Save	release pre	essed for 3 seconds	
Auto Adjust.	Function identical to that of the A key.		
	Used to activate the Laser pointer.		
Laser on		Do not aim the laser beam towards anyone's eyes, because a laser beam can damage eyesight.	
Used to activate the luminous torch.		tivate the luminous torch.	
Lum on	The luminous torch can be used to obtain sharp real images in darkness.		

7. READING AND ERASING

7.1 OPENING THE IMAGES

You can display recorded images and analyze them on the LCD screen.

- 1. Press the MENU/ENTER key.
- 2. Press the UP or DOWN arrow to select the [File] menu.
- 3. Press the UP or DOWN arrow to select [Open], then press the MENU/VALIDATION key.




4. Select an image and press the MENU/VALIDATION key to open it.



When you open an image, you can analyze it and associate a voice remark with it.



- Selecting an image
- 1. When the [Open] or [Delete] option is selected in the [File] menu, the following message is displayed in the bottom left corner of the screen.



C.A1886 – C.A1888

2. If the image to be opened or deleted is not in the current directory, press the UP arrow until the following message is displayed



3. Press the C key, then the S key, to return to image analysis.



- Select the directory name.
- 1. Press the MENU/VALIDATION key.
- Press the UP or DOWN arrow to select the [Menu] menu, then press the MENU/VALIDATION key.
- 3. Press the UP or DOWN arrow to select the [Other] menu, then press the MENU/VALIDATION key.
- 4. Press the UP or DOWN key to select the [Directory Name] menu, then press the LEFT or RIGHT key to select the desired directory.



You can press the A, C, and S keys simultaneously to reset the directory name to RAYCA000.

7.2 PLAYING THE REMARKS (OPTION)

If a voice remark is associated with an image, you can listen to it on the camera.

- 1. Install the Bluetooth headset (optional).
- 2. Open an image.
- 3. Press the MENU/Validation key, then the UP or DOWN arrow to select the [File] menu.
- 4. Press the UP or DOWN key to select [Voice Play], then press the MENU/VALIDATION key.
 - The message [Playing Record] is displayed on the LCD screen.
- 5. You can stop playing the voice remark by pressing the C key.

7.3 ERASING THE IMAGES

Note that images once erased cannot be recovered. So be very careful before erasing an image.

- 1. Press the MENU/VALIDATION key, then the UP or DOWN arrow to select the [File] menu.
- 2. Press the UP or DOWN arrow to select [Delete], then press the MENU/VALIDATION key.

Open Save Delete Voice rec. Voice Play


- 3. Select an image, then press the MENU/VALIDATION key to delete it.
- 4. Press the C key to exit.

8. TRANSFERRING IMAGES

8.1 TRANSFER BY MINI SD CARD

You can withdraw the Mini SD card from the device and load the images into your computer using the Mini SD card reader provided.

- 1. Open the flap on the Mini SD card slot.
- 2. Press lightly on the card, then let it exit. It ejects automatically.



3. You can load the IR images directly from the Mini SD card or via a card reader.

9. CONNECTIONS AND DOWNLOADING

9.1 CONNECTION TO A MONITOR

It is possible to use a video screen connected by a video cable (provided) to display and analyze the images you have taken.

- 1. Switch the LR camera off.
- Connect the video cable to the video output jack on the bottom of the device.



- Connect the other end of the video cable to the video input jack of the screen.
- 4. Switch on the screen and the I.R. camera.


9.2 USING THE BLUETOOTH HEADSET (OPTION)

The device has a module that lets you use the Bluetooth headset (optional) to record voice remarks. To install the headset the first time, proceed as follows:


- 1. Switch off the camera and the Bluetooth headset.
- Start by powering up the Bluetooth headset. Press the On/Off button and hold it down for approximately 10 seconds. You will then see the power indicator start to flash, first red, then blue. The headset is in the coupling mode at the end of 120 seconds.

C.A1886 – C.A1888 33

Switch on the camera. The power indicator of the camera lights green while flashing blue. In this mode, the camera is getting ready to search for the Bluetooth headset.



- 4. Hold the On/Off button of the headset down for approximately 2 seconds to couple the headset and the camera. When the coupling has been performed, the power indicator of the headset flashes blue and that of the camera lights in green. You then see at bottom centre on the screen.
- Switch off the camera and the Bluetooth headset after completing step 4.
- 5. After this first coupling between the camera and the headset, you can simply power up the headset (the power indicator flashes blue), then the camera, and the coupling takes place.





- Press the C and Enter keys simultaneously to clear the Bluetooth headset.
- 6. When you are wearing the headset, you can record voice remarks or listen to those already recorded.

10. TROUBLESHOOTING

Problem	Cause	Solution
The camera fails to operate	The device is off	 Switch the camera on. See "Switching On and Off"
	Battery voltage too low	 Fully charge the battery.
	Poor contact between the camera and the terminals of the battery	Wipe the terminals with a clean, dry cloth.
The camera fails to record	Internal memory full	 If necessary, load the images into a computer and erase them in the camera to make room.
	Internal memory incorrectly formatted	 Format the internal memory to FAT16 format.
The battery unit discharges rapidly	Battery capacity reduced because left unused for a year or more after its last full charge.	Replace the battery unit with a new one.
	Battery has reached end of life	 Replace the battery unit with a new one.
The battery fails to charge	Poor contact between the camera and the terminals of the battery	 Wipe the terminals with a clean cloth. Connect the power cord to the battery charger and insert the other end firmly into a power outlet.
	Battery has reached end of life	 Replace the battery unit with a new one.

C.A1886 - C.A1888

11. MAINTENANCE

For maintenance, use only the spare parts specified. The manufacturer cannot be held liable for any accident following a repair not done by its own customer service department or an approved repairer.

11.1 CLEANING AND MAINTAINING THE CAMERA

Proceed as follows to clean the housing of the camera, the lens, the LCD screen, and the other parts.

Housing of the device

Wipe with a soft cloth or a lens cleaning cloth

Lens

Eliminate dust and dirt using a blow brush, then eliminate any remaining dirt by wiping the lens gently with a soft cloth.

Never use synthetic cleansers on the housing or on the lens.

LCD screen

Use a blow brush to eliminate dust and dirt. If necessary, wipe the screen gently with a soft cloth or a lens cleaning cloth to remove any adherent dirt.

Never rub the LCD screen and never press firmly on its surface. These
actions could damage it or cause other problems.

Never use thinners, benzene, synthetic cleansers, or water to clean the camera. These products could damage the equipment or alter its performance.

11.2 METROLOGICAL CHECK

Like all measuring or testing devices, the instrument must be checked regularly.

We recommend checking this instrument yearly. For checks and calibrations, contact one of our accredited metrology laboratories (information and contact details available on request), at our Chauvin Arnoux subsidiary or the branch in your country.

11.3 REPAIR

For all repairs before or after expiry of warranty, please return the device to your distributor.

12. WARRANTY

Except as otherwise stated, our warranty is valid for twelve months starting from the date on which the equipment was sold. Extract from our General Conditions of Sale provided on request.

The warranty does not apply in the following cases:

- Inappropriate use of the equipment or use with incompatible equipment,
- Modifications made to the equipment without the explicit permission of the manufacturer's technical staff.
- Work done on the device by a person not approved by the manufacturer,
- Adaptation to a particular application not anticipated in the definition of the equipment or not indicated in the user's manual,
- Damage caused by shocks, falls, or floods.

C.A1886 – C.A1888 37

13. APPENDIX

13.1 TABLE OF EMISSIVITIES

Material	Temperature (℃)	Approximate emissivity		
Metals				
Aluminium				
Polished aluminium	100	0.09		
Commercial aluminium sheet	100	0.09		
Oxidized chrome- anodised aluminium	25 ~ 600	0.55		
Slightly oxidized aluminium	25 ~ 600	0.10~0.20		
Highly oxidized aluminium	25~600	0.30 ~ 0.40		
Brass				
Shiny brass (extreme polishing)	28	0.03		
Oxidized brass	200 ~ 600	0.61 ~ 0.59		
Chromium				
Polished chromium	40~1090	0.08 ~ 0.36		
Copper				
Shiny copper	100	0.05		
Highly oxidized copper	25	0.078		
Copper oxide	800 ~ 1100	0.66 ~ 0.54		
Molten copper	1080 ~ 1280	0.16 ~ 0.13		
Gold				
Shiny gold	230 ~ 630	0.02		
Lead				
Pure lead (no oxidation)	125 ~ 225	0.06 ~ 0.08		
Slightly oxidized	25~300	0.20 ~ 0.45		
Magnesium				
Magnesia	275 ~ 825	0.55 ~ 0.20		
Magnesia	900 ~ 1670	0.20		
Mercury	0~100	0.09 ~ 0.12		

English

Nickel		English
Polished by anodising	25	0.05
Electrolysed	20	0.01
Unpolished	1 20	0.01
Nickel wire	185 ~ 1010	0.09~0.19
Nickel sheet (oxidized)	198 ~ 600	0.37 ~ 0.48
Nickel oxide	650 ~ 1255	0.59 ~ 0.86
Nickel alloy		
Nickel-chromium alloy wire (shiny) (refractory)	50 ~ 1000	0.65 ~ 0.79
Nickel-chromium alloy	50 ~ 1040	0.64 ~ 0.76
Refractory nickel- chromium	50~500	0.95 ~ 0.98
Nickel-silver alloy	100	0.14
Stainless steel		
18-8	25	0.16
304(8Cr, 18Ni)	215 ~ 490	0.44 ~ 0.36
310(25Cr, 20Ni)	215 ~ 520	0.90 ~ 0.97
Tin		
Commercial tinplate	100	0.07
Highly oxidized	0~200	0.60
Zinc		
Oxidation at 400℃	400	0.01
Shiny galvanized iron plate	28	0.23
Oxidized zinc powder	25	0.28
Non-metallic materials		
Brick	1100	0.75
Refractory brick	1100	0.75
Graphite (carbon black)	96 ~ 225	0.95
Enamel (white)	18	0.90
Asphalt	0~200	0.85
Glass (surface)	23	0.94
Refractory glass	200 ~ 540	0.85 ~ 0.95
Calcimine	20	0.90
Oak	20	0.90

C.A1886 - C.A1888

14. TECHNICAL CHARACTERISTICS

Description	Characteristic	C.A 1886	C.A 1888
Detecter	Туре	UFPA microbolometer	
	Spectral band	8 ~14µm	
	Resolution	160x120	384x288
Imaging performance	NETD	0.1°C@ 30°C	0.08°C@ 30°C
	Objective/focusing	20%15°	24%18°
	IFOV (spatial resolution)	2.2mrad	1.3mrad
	Min. focal distance	0.1m	0.1m
Visual image	Digital video	640x480 pixels, "full colour"	
	Illuminator	Produces sharp, high-quality visual images in dark areas	
	Min. focal distance	0.1m	
Presentation of the images	Display of image	Infrared image, real image, or "Mix vision" function with adjustment of percentage of fusion of I.R. image	
	Video output	PAL/NTSC	
	LCD screen	3.5 inches	
	Display of images	Pseudo-colours, multiple palettes	
Functions	Image freeze	Image moving or frozen	
	Storage of files	Removable Mini SD card, up to 2 GB.	
Measurement	Temperature range	-20°C ~600°C (standard) Up to 1500℃ optional.	
	Precision	±2°C or ±2%	

Description	Characteristic	C.A 1886	C.A 1888
Analysis functions	Points of analysis	4 points: 3 that can be positioned anywhere on the screen and 1 for automatic detection of Max or Min temp.	
	Tracking of temperature	Automatic tracking of the hottest or coldest point in the whole image	
	Temperature alarm	If a temperature alarm threshold is predefined, the camera beeps if it is exceeded.	
	Adjustment	Automatic or manual adjustment of brightness and contrast.	
	Correction	Emissivity, Distance, Ambient temperature, Relative humidity	
	Display of isotherms	Mono-colour display of a user-adjustable temperature interval.	
	Voice remarks	By Bluetooth (option).	
Software	Analysis software	Report generation software	
Laser pointer	Type		
	Туре	Rechargeable lithium battery	
Battery system	Life between charges	at least 3 hours	
Conformity	Electromagnetic compatibility	EN-61236-1:2006	
	Safety	EN-61010-1-Ed.2	
Environmental specification	Operating temperature range	-15℃ to 50℃ (-4℉ to 122℉)	
	Storage temperature range	-40℃ to 70℃ (-40℉ to 158℉)	
	Humidity	10% to 95%	
	Impact resistance	25G	
	Vibration resistance	2G	
	Protection	IP 54	
Physical	Weight	650g (with battery)	
characteristics Dimension		211x80x195mm	

15. DELIVERY CONDITION

C.A 1886 I.R. th	ermography camera	P01651260
C.A 1888 I.R. th	ermography camera	P01651270

Delivered with:

- 1 battery charger
- 2 batteries
- 1 2GB Mini SD card
- 1 card reader
- 1 video cable
- RayCAm standard report on CD ROM
- 1 user manual on CD ROM, in 5 languages
- 1 test report
- 1 Carrying case

ACCESSORIES & SPARES

Battery	P01296041
Sun guard	P01651531
Adapter for photographic tripod	P01651526
Mains power unit	P01651527
Lens cap	P01651522
USB cable	P01295274
Cigar lighter adapter	HX0061
Introduction to thermography	Contact us



07 - 2010 Code 693056A02 - Ed. 2

DEUTSCHLAND - Chauvin Arnoux GmbH

Straßburger Str. 34 - 77694 Kehl/Rhein Tel: (07851) 99 26-0 - Fax: (07851) 99 26-60

ESPAÑA - Chauvin Arnoux Ibérica S.A.

C/ Roger de Flor N°293, Planta 1- 08025 Barcelona Tel: 902 20 22 26 - Fax: 934 59 14 43

ITALIA - Amra SpA

Via Sant'Ambrogio, 23/25 - 20050 Bareggia di Macherio (MI) Tel: 039 245 75 45 - Fax: 039 481 561

ÖSTERREICH - Chauvin Arnoux Ges.m.b.H

Slamastrasse 29/2/4 - 1230 Wien Tel: 01 61 61 961-0 - Fax: 01 61 61 961-61

SCANDINAVIA - CA Mätsystem AB

Box 4501 - SE 18304 TÄBY

Tel: +46 8 50 52 68 00 - Fax: +46 8 50 52 68 10

SCHWEIZ - Chauvin Arnoux AG

Moosacherstrasse 15 - 8804 AU / ZH Tel: 044 727 75 55 - Fax: 044 727 75 56

UNITED KINGDOM - Chauvin Arnoux Ltd

Unit 1 Nelson Court – Flagship Square-Shaw Cross Business Park
DEWSBURY – West Yorkshire – WF12 7TH
Tel: 011628 788 888 – Fax: 01628 628 099

MIDDLE EAST - Chauvin Arnoux Middle East

P.O. BOX 60-154 - 1241 2020 JAL EL DIB (Beirut) - LEBANON Tel: (01) 89 04 25 - Fax: (01) 89 04 24

CHINA - Shanghai Pu-Jiang - Enerdis Instruments Co. Ltd

3 F, 3 rd Building - N°381 Xiang De Road - 200081 SHANGHAI Tel: +86 21 65 21 51 96 - Fax: +86 21 65 21 61 07

USA - Chauvin Arnoux Inc - d.b.a AEMC Instruments

200 Foxborough Blvd. - Foxborough - MA 02035 Tel: (508) 698-2115 - Fax: (508) 698-2118

http://www.chauvin-arnoux.com

190, rue Championnet - 75876 PARIS Cedex 18 - FRANCE

Tél.: +33 1 44 85 44 85 - Fax: +33 1 46 27 73 89 - info@chauvin-arnoux.fr Export: Tél.: +33 1 44 85 44 86 - Fax: +33 1 46 27 95 59 - export@chauvin-arnoux.fr