Pacifier clinical thermometer
Geratherm® daisy color GT-126

Geratherm Medical AG
Germany CE0197


GB

INSTRUCTION FOR USE Please read carefully before using

FEATURES

1. With visual fever alarm.
2. With orthodontic nipple design, made of hard-wearing silicon.
3. Compact, accurate and durable LSI (Large Scale Integration) device.
4. Sensitive temperature sensor for fast results.
5. Automatic power off wihtin 30 seconds.
6. Easy-to-read large LCD (liquid crystal display).
7. The device is waterproof.
8. No mercury inside.

PARTS DESCRIPTION

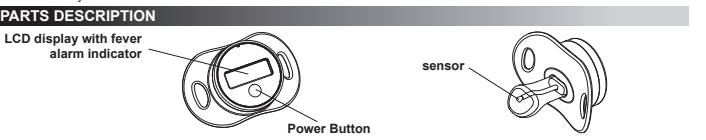

SPECIFICATIONS

Measuring range:	32.0 ~ 43.9 °C; below 32.0 °C, display L °C; above 43.9 °C, display H °C
Intended use:	Measurement of body temperature
Resolution:	0,1 °C (°F)
Accuracy:	±0,1 °C (34.0 °C to 42.0 °C), ±0.2 °C (other range) +0.2 °F (93.2 °F to 107.6 °F) +0.4 °F (other range)
Display:	Liquid crystal display 3 1/2 digits
Battery (included):	CR2032 (3 V)
Energieverbrauch:	0.15 milliwatts in measurement mode
Battery life:	More than 160 hours of continuous operation
IP classification:	IP27 (Protected against solid foreign objects with a diameter of 12.5 mm and protection against temporary immersion)
Dimensions:	60 mm x 50 mm x 42 mm
Weight:	Approx. 23 grams (including battery)
Beeper:	Approx. 5 secs. sound signal when end temperature reached
Memory:	Built-in memory enabling display of the previously measured value
Shut-off:	Automatic shut-off in approx. 30 seconds
Working Conditions:	Temperature: 10 °C to 40 °C; (50 °F to 104 °F) Humidity: 15 % to 95 % R.H. ⚠ It is only is possible to measure temperatures that are above the ambient temperature.
Storage Conditions:	Temperature: -25 °C to 55 °C; (-13 °F to 131 °F) Humidity 15 % to 95 % R.H.
Guarantee of Quality:	EN 12470-3 Clinical thermometers - Part 3: Performance of compact electrical thermometers with maximum device. Geratherm® is certified in accordance with Council Directive 93/42/EWG and EN ISO 13485 and is entitled to affix the CE-mark CE0197 (Notified Body: TÜV Rheinland LGA Products GmbH).
Electromagnetic compatibility (EMC):	The present medical product is a device with extremely high degree of noise immunity. Therefore, the enclosure with the EMC tables was not printed out.

⚠ PRECAUTIONS

1. Use of this instrument is not intended as a substitute for consultation with your physician. Prolonged high fever requires medical attention especially for your children. Please contact your physician.
2. Child's temperature shall be taken under adult's surveillance.
3. Keep out of the reach of unsupervised children. Choking resulting from a child swallowing a small part that has become detached from the thermometer.
4. Do not boil, bite, bend, drop or disassemble this thermometer.
5. Do not attempt to disassemble the unit except to replace the battery.
6. Avoid taking temperature in 30 minutes after physical exercises, bathing or dining.
7. Do not store, use and transport the unit under direct sunlight, at a high temperature, or in high humidity or dust. Performance may be degraded.
8. Stop using the thermometer if it operates erratically or if the display malfunctions.
9. If the thermometer has been stored at below-freezing temperatures, allow the thermometer to warm naturally to room temperature before using.
10. Before every use, check the pacifier thermometer and especially the silicon nipple for signs of damage or wear.
11. Do not use damaged pacifier any more.
12. Always maintain the minimum time required for measurement which is indicated by the acoustic signal.
13. The pacifier thermometer is intended only for oral measurement of body temperature in children up to 3 years of age.
14. It is not suitable for constant sucking.
15. Under specific conditions (crying, breathing through the mouth), the displayed temperature may be too low.
16. In case of doubt and signs of fever (temperature higher than 38.5 °C, flushed appearance, perspiration, unwillingness to drink, restlessness) measure the body temperature rectally.

BATTERY DISPOSAL

For safety reasons, the battery cannot be exchanged.
1. When the symbol „ ⊖ „ appears, the unit should be disposed of. Discard the battery before disposing of the unit.
2. Separate the panel sticker from the unit.
3. Use a screwdriver to do it.
4. Discard the battery.



⚠ **Note:**
Discard old battery carefully, out of reach of young children.
Do not dispose of the battery in a fire. It may explode.

⚠ **Note:**
Replacing the battery may damage the unit.

HOW TO USE

1. Remove the protective cover.
2. Place the pacifier nipple in the child´s mouth like a normal baby pacifier. Be sure the child keeps the thermometer in his mouth during measurement, and keep the child´s mouth closed as much as possible.

⚠ **Note:**
Drinking or eating prior to use may affect the reading.

3. Start with the measurement after abt. 3 - 5 minutes by pressing the ON/OFF button. The display will read 8888 with fever alarm indicator flashing (red -> yellow -> green) for 2 seconds.
4. The display will show L,°C with °C flashing.
5. Once the degree sign °C stops flashing, the measurement is ready and the correct temperature is displayed. An alarm will sound for approximately 5 seconds after measurement.
6. The fever alarm indicator (colored backlight) will light up for 5 seconds, the color depending on the temperature measured. It is recommended to leave the thermometer in the baby`s mouth to allow the nipple to warm up and obtain a more accurate reading.
7. The unit will automatically turn off in approx. 30 seconds. However, to save energy, it is best to turn the thermometer off immediately after the temperature has been noted.

⚠ **Note:**
Oral temperature readings are often 0.5°C lower than actual body temperature readings.

Special Features:
Last-temperature memory recall:
Press and hold the ON/OFF button while turning on the unit for more than 3 seconds. The last measured temperature will appear with the letter "M" under the °C sign.

Visual fever alarm:
If the temperature registers higher than 37.5 °C, the display will have a red background light for 5 seconds.

temperature	fever alarm indicator
35,9 ≙ T	clear
36,0 ≙ T ≙ 37,1	green
37,2 ≙ T ≙ 37,4	yellow
37,5 ≙ T ≙ 43,9	red
44,0 ≙ T	clear

⚠ **NOTE:**
Children should be attended by an adult during the entire temperature recording process. After use, the digital pacifier thermometer should be stored in a safe place, out of reach of young children.

CLEANING INSTRUCTIONS

Disinfect the thermometer by wiping the teat (with the sensor) and the shield with a cloth that has been immersed in a household antiseptic solution, such as rubbing alcohol.

DISPOSAL

Observe the applicable regulations when disposing of the thermometer and batteries. This thermometer must not be disposed of together with domestic waste. All users are obliged to hand in all electrical or electronic devices, regardless of whether or not they contain toxic substances, at a municipal or commercial collection point so that they can be disposed of in an environmentally acceptable manner.
Please remove the batteries before disposing of the thermometer.
Do not dispose of old batteries with your household waste, but at a battery collection station at a recycling site or in a shop.

LIMITED WARRANTY

This thermometer is guaranteed for 2 years from the date of purchase against manufacturer's defect under normal use. The warranty does not cover damage to your unit due to improper handling. Following the directions closely will ensure years of dependable operation.
In case of professional use, the manufacturer recommends to verify the accuracy by an authorized laboratory every 2 years (in Germany this is compulsory).

SYMBOLINDEX

	Follow instructions for use		Type BF applied part		Keep dry
	The device must not be disposed of with household waste.		Caution! Read the instruction manual!		Manufacturer
95 % 15 %	Store between 15 % and 95 % R.H.	+55 °C -25 °C	Store between -25 °C and +55 °C	LOT	Batch code (mm/yyyy; month/ year)

Geratherm Medical AG
Fahrenheitstrasse 1
98716 Geschwenda
Germany
www.geratherm.com

CE0197