

Citrate Colorimetric/Fluorometric Assay Kit

(Catalog #K655-100; 100 assays; Store Kit at -20°C)

I. Introduction:

Citric acid (HOOC-CH₂-C(OH)(-COOH)-CH₂-COOH) is a key intermediate in the TCA cycle which occurs in mitochondria. It is formed by the addition of oxaloacetate to the acetyl group of acetyl-CoA derived from the glycolytic pathway. Citrate can be transported out of mitochondria and converted back to acetyl CoA for fatty acid synthesis. Citrate is an allosteric modulator of both fatty acid synthesis (acetyl-CoA carboxylase) and glycolysis (phosphofructokinase). Citrate is widely used industrially in foods, beverages and pharmaceuticals. Citrate metabolism and disposition can vary widely due to sex, age and a variety of other factors. BioVision's Citrate Assay Kit provides a simple, sensitive and rapid means of quantifying citrate in a variety of samples. In the assay, citrate is converted to pyruvate via oxaloacetate. The pyruvate is quantified by converting a nearly colorless probe to an intensely colored ($\lambda_{max}=570$ nm) and fluorescent (E_x/E_m , 535/587 nm) product. The Citrate Assay Kit can detect 0.1 to 10 nmoles (~2 μ M-10 mM) of citrate in a variety of samples.

II. Kit Contents:

Components	K655-100	Cap Code	Part Number
Citrate Assay Buffer	25 ml	WM	K655-100-1
Citrate Probe	0.2 ml	Red	K655-100-2
Citrate Enzyme Mix	lyophilized	Purple	K655-100-3
Citrate Developer	lyophilized	Green	K655-100-4
Citrate Standard (10 μ mol)	lyophilized	Yellow	K655-100-5

III. Storage and Handling:

Store kit at -20°C, protect from light. Warm Citrate Assay Buffer to room temperature before use. Briefly centrifuge all small vials prior to opening.

IV. Reagent Preparation and Storage Conditions:

Citrate Probe: Ready to use as supplied. Warm to 37°C for 1 – 2 min to completely melt the DMSO solution before use. Store at -20°C, protect from light. Use within two months.

Citrate Developer, Enzyme Mix: Dissolve with 220 μ l Assay Buffer separately. Pipette up and down to dissolve. Aliquot into portions, store at -20°C. Avoid repeated freeze/thaw cycles. Use within 2 months.

Citrate Standard: Dissolve in 100 μ l dH₂O to generate 100 mM (100 nmol/ μ l) Citrate Standard solution. Keep on ice while in use. Store at -20°C.

V. Assay Protocol:

1. Standard Curve Preparations:

Colorimetric Assay: Dilute the Citrate Standard to 1 nmol/ μ l by adding 10 μ l of the Standard to 990 μ l of dH₂O, mix well. Add 0, 2, 4, 6, 8, 10 μ l into a series of standards wells on a 96 well plate. Adjust volume to 50 μ l/well with Assay Buffer to generate 0, 2, 4, 6, 8, 10 nmol/well of the Standard.

Fluorometric Assay: Dilute the Citrate standard to 0.1 nmol/ μ l by adding 10 μ l of the standard to 990 μ l of dH₂O, mix well, then further dilute by adding 10 μ l to 90 μ l of dH₂O. Add 0, 2, 4, 6, 8, 10 μ l into a series of standards wells on a 96-well plate. Adjust the volume to 50 μ l/well to generate 0, 0.2, 0.4, 0.6, 0.8, 1.0 nmol/well.

2. Sample Preparation:

Tissue (20 mg) or cells (2 x 10⁶) should be rapidly homogenized with 100 μ l of Citrate Assay Buffer. Centrifuge at 15,000 g for 10 min to remove cell debris. Enzymes in samples may interfere with the assay. We suggest deproteinizing samples using a perchloric acid/KOH protocol (BioVision, Cat. #K808-200) or 10 kDa molecular weight cut off spin columns (BioVision, Cat # 1997-25). Add 1-50 μ l sample into duplicate wells of a 96-well plate and bring volume to 50 μ l with Assay Buffer. We suggest testing several doses of your samples to ensure readings are within the standard curve range.

3. **Develop:** Mix enough reagent for the number of samples and standards to be performed: For each well, prepare a total 50 μ l Reaction Mix containing:

	Colorimetric Assay		Fluorometric Assay	
	Sample	Bkgd Control*	Sample	Bkgd Control*
Citrate Assay Buffer	44 μ l	46 μ l	44 μ l	46 μ l
Citrate Enzyme Mix	2 μ l	----	2 μ l	----
Developer	2 μ l	2 μ l	2 μ l	2 μ l
Citrate Probe**	2 μ l	2 μ l	2 μ l	2 μ l


*Samples may contain oxaloacetate or pyruvate which can generate a background and need to be subtracted from the sample background signal.

**For the fluorometric assay, dilute 10X with DMSO to reduce fluorescent background.

4. Add 50 μ l of the Reaction Mix to each well containing the Citrate Standard and test samples. Add 50 μ l of the sample background control mix to background control wells.
5. Incubate for 30 min at room temperature, protect from light.
6. Measure OD at 570 nm or fluorescence at E_x/E_m 535/587 nm.
7. **Calculation:** Correct background by subtracting the value of the 0 Citrate Standard from all readings. Next subtract the value of the Sample Background Control from the test sample. Plot the standard curve. Apply corrected sample readings to the standard curve to get Citrate amount in the sample wells. The Citrate concentration in the test samples equals:

$$C = Ay/Sv \text{ (nmol/}\mu\text{l; or } \mu\text{mol/ml; or mM)}$$

Where: Ay is the amount of citrate (nmol) in your sample from the standard curve.
Sv is the sample volume (μ l) added to the sample well.
Citric acid molecular weight: 191 g/mol.

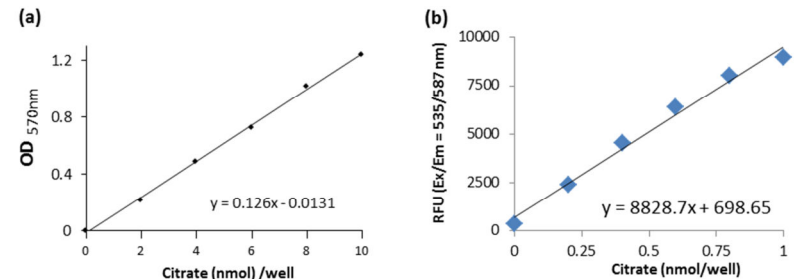

Citrate standard curve generated using this kit protocol

VI. RELATED PRODUCTS:

ADP/ATP Kit
CoA/Acetyl CoA Assay Kits
Malic Acid Assay Kit
 α -Ketoglutarate Assay Kit
Malic Acid Assay Kit
Isocitrate Assay Kit
Starch Assay Kit
Pyruvate Assay Kit

NAD/NADH and NADP/NADPH Assay Kits
Pyruvate Assay Kit
Glutamate Assay Kit
Lactate Assay Kits
Oxaloacetate Assay Kit
Glycogen Assay Kit
Glucose Assay Kit
Maltose Assay Kit

GENERAL TROUBLESHOOTING GUIDE:

Problems	Cause	Solution
Assay not working	<ul style="list-style-type: none"> • Use of ice-cold assay buffer • Omission of a step in the protocol • Plate read at incorrect wavelength • Use of a different 96-well plate 	<ul style="list-style-type: none"> • Assay buffer must be at room temperature • Refer and follow the data sheet precisely • Check the wavelength in the data sheet and the filter settings of the instrument • Fluorescence: Black plates (clear bottoms) ; Luminescence: White plates ; Colorimeters: Clear plates
Samples with erratic readings	<ul style="list-style-type: none"> • Use of an incompatible sample type • Samples prepared in a different buffer • Samples were not deproteinized (if indicated in datasheet) • Cell/ tissue samples were not completely homogenized • Samples used after multiple free-thaw cycles • Presence of interfering substance in the sample • Use of old or inappropriately stored samples 	<ul style="list-style-type: none"> • Refer data sheet for details about incompatible samples • Use the assay buffer provided in the kit or refer data sheet for instructions • Use the 10 kDa spin cut-off filter or PCA precipitation as indicated • Use Dounce homogenizer (increase the number of strokes); observe for lysis under microscope • Aliquot and freeze samples if needed to use multiple times • Troubleshoot if needed, deproteinize samples • Use fresh samples or store at correct temperatures till use
Lower/ Higher readings in Samples and Standards	<ul style="list-style-type: none"> • Improperly thawed components • Use of expired kit or improperly stored reagents • Allowing the reagents to sit for extended times on ice • Incorrect incubation times or temperatures • Incorrect volumes used 	<ul style="list-style-type: none"> • Thaw all components completely and mix gently before use • Always check the expiry date and store the components appropriately • Always thaw and prepare fresh reaction mix before use • Refer datasheet & verify correct incubation times and temperatures • Use calibrated pipettes and aliquot correctly
Readings do not follow a linear pattern for Standard curve	<ul style="list-style-type: none"> • Use of partially thawed components • Pipetting errors in the standard • Pipetting errors in the reaction mix • Air bubbles formed in well • Standard stock is at an incorrect concentration • Calculation errors • Substituting reagents from older kits/ lots 	<ul style="list-style-type: none"> • Thaw and resuspend all components before preparing the reaction mix • Avoid pipetting small volumes • Prepare a master reaction mix whenever possible • Pipette gently against the wall of the tubes • Always refer the dilutions in the data sheet • Recheck calculations after referring the data sheet • Use fresh components from the same kit
Unanticipated results	<ul style="list-style-type: none"> • Measured at incorrect wavelength • Samples contain interfering substances • Use of incompatible sample type • Sample readings above/below the linear range 	<ul style="list-style-type: none"> • Check the equipment and the filter setting • Troubleshoot if it interferes with the kit • Refer data sheet to check if sample is compatible with the kit or optimization is needed • Concentrate/ Dilute sample so as to be in the linear range

Note# The most probable list of causes is under each problem section. Causes/ Solutions may overlap with other problems.