

Invacare® **APM™ Model CG9900** Mattress



## User Manual

EN

For more information regarding bed rail safety, refer to the Bed Rail Entrapment Risk Notification Guide at [www.invacare.com](http://www.invacare.com).

This manual **MUST** be given to the user of the product.

Before using this product, read this manual and save for future reference.



**Yes, you can.®**

© 2011 Invacare Corporation. All rights reserved. Reproduction, duplication or modification in whole or in part is prohibited without prior written permission from Invacare. Trademarks are identified by ™ and ®. All trademarks are owned by or licensed to Invacare Corporation or its subsidiaries unless otherwise noted.

<b>1</b>	<b>GENERAL</b>	<b>4</b>
	Symbols .....	4
	Limited Warranty .....	5
<b>2</b>	<b>OVERVIEW</b>	<b>6</b>
	Label Location.....	6
	Typical Product Parameters .....	7
<b>3</b>	<b>SAFETY</b>	<b>9</b>
	General Guidelines .....	9
<b>4</b>	<b>OPERATION</b>	<b>13</b>
	Mattress Replacement System .....	13
	Installing the Side Rails.....	14
	Installing the Power Unit.....	14
	Connecting the Hose.....	15
	Connecting the Power Cord.....	16
	Using the Front Panel.....	17
	Failure Modes.....	20
	Powering Up the System.....	20
	Placing the Patient on the Mattress .....	20
	Transferring Patient From/To a Gurney.....	21
	Transferring Patient From/To a Wheelchair .....	22
	Preparing for CPR Procedure.....	22
	About Power Outage and Transportation.....	23
<b>5</b>	<b>MAINTENANCE AND TROUBLESHOOTING</b>	<b>24</b>
	Cleaning the System .....	24
	Troubleshooting.....	27

### I General

---

#### I.1 Symbols

##### Warnings

Signal words are used in this manual and apply to hazards or unsafe practices which could result in personal injury or property damage. See the information below for definitions of the signal words.



#### **DANGER**

Danger indicates an imminently hazardous situation which, if not avoided, will result in death or serious injury.



#### **WARNING**

Warning indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.



#### **CAUTION**

Caution indicates a potentially hazardous situation which, if not avoided, may result in property damage or minor injury or both.



#### **IMPORTANT**

Indicates a hazardous situation that could result in damage to property if it is not avoided.



Gives useful tips, recommendations and information for efficient, trouble-free use.

## 1.2 Limited Warranty

**PLEASE NOTE: THE WARRANTY BELOW HAS BEEN DRAFTED TO COMPLY WITH FEDERAL LAW APPLICABLE TO PRODUCTS MANUFACTURED AFTER JULY 4, 1975.**

This warranty is extended only to the original purchaser who purchases this product when new and unused from Invacare or a dealer. This warranty is not extended to any other person or entity and is not transferable or assignable to any subsequent purchaser or owner. Coverage under this warranty will end upon any such subsequent sale or other transfer of title to any other person.

This warranty gives you specific legal rights and you may also have other legal rights which vary from state to state.

Invacare warrants the mattress and cover when purchased new and unused to be free from defects in materials and workmanship for a period of one year from the date of purchase from Invacare or a dealer, with a copy of the seller's invoice required for coverage under this warranty. Invacare warrants the control unit when purchased new and unused to be free from defects in materials and workmanship for a period of one year from the date of purchase from Invacare or a dealer, with a copy of the seller's invoice required for coverage under this warranty. If within such warranty period any such product shall be proven to be defective, such product shall be repaired or replaced, at Invacare's option, with refurbished or new parts. This warranty does not include any labor or shipping charges incurred in replacement part installation or repair of any such product. Product repairs shall not extend this warranty - coverage for repaired product shall end when this limited warranty terminates. Invacare's sole obligation and your exclusive remedy under this warranty shall be limited to such repair and/or replacement.

For warranty service, please contact the dealer from whom you purchased your Invacare product. In the event you do not receive satisfactory warranty service, please write directly to Invacare at the address on the back cover. Provide dealer's name, address, model number, and the date of purchase, indicate nature of the defect and, if the product is serialized, indicate the serial number.

Invacare Corporation will issue a return authorization. The defective unit or parts must be returned for warranty inspection using the serial number, when applicable, as identification within thirty days of return authorization date. **DO NOT** return products to our factory without our prior consent. C.O.D. shipments will be refused; please prepay shipping charges.

**LIMITATIONS AND EXCLUSIONS: THE WARRANTY SHALL NOT APPLY TO PROBLEMS ARISING FROM NORMAL WEAR OR FAILURE TO ADHERE TO THE ENCLOSED INSTRUCTIONS. IN ADDITION, THE FOREGOING WARRANTY SHALL NOT APPLY TO SERIAL NUMBERED PRODUCTS IF THE SERIAL NUMBER HAS BEEN REMOVED OR DEFACED; PRODUCTS SUBJECTED TO NEGLIGENCE, ACCIDENT, IMPROPER OPERATION, MAINTENANCE OR STORAGE; OR PRODUCTS MODIFIED WITHOUT INVACARE'S EXPRESS WRITTEN CONSENT INCLUDING, BUT NOT LIMITED TO: MODIFICATION THROUGH THE USE OF UNAUTHORIZED PARTS OR ATTACHMENTS; PRODUCTS DAMAGED BY REASON OF REPAIRS MADE TO ANY COMPONENT WITHOUT THE SPECIFIC CONSENT OF INVACARE; PRODUCTS DAMAGED BY CIRCUMSTANCES BEYOND INVACARE'S CONTROL; PRODUCTS REPAIRED BY ANYONE OTHER THAN AN INVACARE DEALER, SUCH EVALUATION SHALL BE SOLELY DETERMINED BY INVACARE.**

**THE FOREGOING EXPRESS WARRANTY IS EXCLUSIVE AND IN LIEU OF ALL OTHER EXPRESS WARRANTIES WHATSOEVER, WHETHER EXPRESS OR IMPLIED, INCLUDING THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE AND THE SOLE REMEDY FOR VIOLATIONS OF ANY WARRANTY WHATSOEVER, SHALL BE LIMITED TO REPAIR OR REPLACEMENT OF THE DEFECTIVE PRODUCT PURSUANT TO THE TERMS CONTAINED HEREIN. THE APPLICATION OF ANY IMPLIED WARRANTY WHATSOEVER SHALL NOT EXTEND BEYOND THE DURATION OF THE EXPRESS WARRANTY PROVIDED HEREIN. INVACARE SHALL NOT BE LIABLE FOR ANY CONSEQUENTIAL OR INCIDENTAL DAMAGES WHATSOEVER.**

**THIS WARRANTY SHALL BE EXTENDED TO COMPLY WITH STATE/PROVINCIAL LAWS AND REQUIREMENTS.**

## 2 OVERVIEW

### 2 Overview

#### 2.1 Label Location

**DANGER-EXPLOSION HAZARD:** DO NOT use in the presence of flammable anesthetics.

**CAUTION:** Equipment should be connected to a properly grounded receptacle (3-prong). Risk of Electrical shock. DO NOT remove back. Disconnect air hose before administering CPR.

#### **WARNING**

Patient entrapment with bed side rails may cause injury or death. Mattress MUST fit bed frame and side rails snugly to prevent patient entrapment. Follow the manufacturer's instructions. Monitor patient frequently. Read and understand the Owner's/Operator's Manual prior to using this equipment. Invacare product manuals are available at [www.invacare.com](http://www.invacare.com) or your dealer. P/N 1150708 Rev A



## 2.2 Typical Product Parameters

## Electrical Parameters

	CG9900
<b>INPUT VOLTAGE AC:</b>	90 V
<b>INPUT FREQUENCY:</b>	60 Hz
<b>CURRENT:</b>	1 A
<b>MAXIMUM POWER CONSUMPTION:</b>	5 ± 3 W
<b>CIRCUIT PROTECTION:</b>	Dual fused, 250 V, 1 A fast blow fuses
<b>MODE OF OPERATION:</b>	Continuous

## Performance Parameters

	CG9900
<b>WEIGHT CAPACITY:</b>	350 lbs
<b>PRESSURE ZONE:</b>	2
<b>MAXIMUM FLOW:</b>	12 ± 4 LPM
<b>MAXIMUM FLOW PRESSURE:</b>	35 ± 5 mmHg
<b>MAXIMUM FLOW TIMER:</b>	45 minutes
<b>SUPPORT SURFACE INFLATION TIME:</b>	20 - 45 minutes

	CG9900
<b>PATIENT COMFORT CONTROL PRESSURES</b>	
SOFT PRESSURE:	8 ± 4 mmHg
FIRM PRESSURE:	32 ± 4 mmHg
CYCLE TIME:	10 minutes
<b>PATIENT CONTACT:</b>	Control unit and mattress have Latex-Free components

## 2 OVERVIEW

### Mechanical Parameters

<b>CONTROL UNIT</b>	CG9900
<b>DIMENSIONS (L X W X H):</b>	9" x 4.5" x 5"
<b>WEIGHT:</b>	5 lbs
<b>POWER CORD:</b>	10 - 14 Feet Long, Hospital Grade
<b>CONNECTION:</b>	Two ¼" Flow Couplings
<b>PACKAGING:</b>	1 piece/box
<b>AIR FILTER:</b>	None

### Environmental Parameters

	CG9900
<b>OPERATING CONDITIONS</b> AMBIENT TEMPERATURE: RELATIVE HUMIDITY: ATMOSPHERIC PRESSURE:	50° - 104° F 30% - 75% Non-Condensing 70 - 106 kPa
<b>STORAGE AND SHIPPING CONDITIONS</b> AMBIENT TEMPERATURE: RELATIVE HUMIDITY: ATMOSPHERIC PRESSURE:	-40° - 158° F 10% - 100% Non-Condensing 50 - 106 kPa



## 3 Safety

### 3.1 General Guidelines

#### **!** NOTICE

THE INFORMATION CONTAINED IN THIS DOCUMENT IS SUBJECT TO CHANGE WITHOUT NOTICE.

Check all parts for shipping damage and test before using. In case of damage, DO NOT use. Contact Invacare/Carrier for further instruction.

### Contraindications



#### **WARNING**

ALWAYS consult the patient's physician before using the CG9900 system.

### Electrical



#### **DANGER**

Electrical shock hazard. DO NOT remove cover. Refer to qualified service personnel.

#### **WARNING**

Before performing any maintenance to the power unit, disconnect the power cord from the wall outlet.

DO NOT insert items into any openings of the control unit. Doing so may cause fire or electric shock by shorting the internal components.

The control unit MUST be kept away from all heat sources and radiators during operation.

Connect the equipment to properly grounded three prong wall outlet using 10-14 ft hospital grade power cord provided with the product.

Grounding reliability depends upon a properly grounded receptacle (3-prong).

## 3 SAFETY

### Installation



#### **WARNING**

The CG9900 system is recommended to be installed on medical bed frames with bed side or assist rails. It is preferred that the rails be in the raised position whenever a patient is on the bed. Health care professionals assigned to each case should make the final determination whether side or assist rails are warranted after assessing patient risks of entrapment and falls in accordance with State patient restraint legislation or facility interpretation of such legislation.

Controls on the footboard may be obstructed by the power unit on a few bed frames. It may be necessary to relocate the power unit. Refer to [Installing the Power Unit](#) on page 14.

Check that air hoses and power cord are clear of moving bed components before placing a patient on the bed. Operate all bed frame motorized functions through their full range of motion to be certain that there is no pulling, interference or pinching.

DO NOT strap the mattress to the **bed frame** at the head and foot ends. Secure ALL mattress straps. Secure the straps to the **bed deck** at the head and foot ends and to the frame at the center of the bed. Otherwise damage to the mattress will occur when the head and foot ends are raised. Refer to [Mattress Replacement System](#) on page 13.

**Entrapment May Occur****DANGER**

Patient entrapment with bed side rails may cause injury or death. Mattress **MUST** fit bed frame and side rails snugly to prevent patient entrapment. Follow the manufacturer's instructions. Monitor patient frequently. Read and understand the Owner's/Operator's Manual prior to using this equipment. Invacare product manuals are available at [www.invacare.com](http://www.invacare.com) or your dealer.

Proper patient assessment and monitoring, and proper maintenance and use of equipment is required to reduce the risk of entrapment. Variations in bed rail dimensions, and mattress thickness, size or density could increase the risk of entrapment. Visit the FDA website at <http://www.fda.gov> to learn about the risks of entrapment. Review "A Guide to Bed Safety", published by the Hospital Bed Safety Workgroup, located at [www.invacare.com](http://www.invacare.com). Use the link located under each bed rail product entry to access this bed safety guide.

Refer to the owner's manuals for beds and rails for additional product and safety information.

After any adjustments, repair or service and before use, make sure all attaching hardware is tightened securely. Assist rails with dimensions different from the original equipment supplied or specified by the bed manufacturer may not be interchangeable and may result in entrapment or other injury.

**Fire Hazard- Smoking****DANGER**

**DO NOT SMOKE** while using this device. A cigarette can burn a hole in the bed surface and cause damage to the mattress. Also, patient clothing, bed sheets, etc. may be combustible and cause a fire. Failure to observe this warning can result in severe fire, property damage and cause physical injury or death.

Smoking by visitors in the room will contaminate the system. Therefore, visitor smoking is **NOT** permitted.

### 3 SAFETY

#### Fire Hazard - Anesthesia Equipment



#### **DANGER**

There is an explosion risk if used with flammable anesthetics.

#### Fire Hazard - Oxygen



#### **DANGER**

There is a possible fire hazard when used with oxygen administering equipment other than nasal mask or half bed tent type. The oxygen tent should NOT extend below mattress support level.

## 4 Operation



### CAUTION

DO NOT strap the mattress to the **bed frame** at the head and foot ends. Secure ALL mattress straps. Secure the straps to the **bed deck** at the head and foot ends and to the frame at the center of the bed. Otherwise damage to the mattress will occur when the head and foot ends are raised.

### 4.1 Mattress Replacement System




The powered mattress comes with eight nylon buckle straps.

1. Remove the original mattress from the bed.
2. If necessary, lower the side rails to facilitate installation of the mattress.
3. Unroll the powered mattress and place it on the bed frame.



Ensure that the hose is towards the foot end of the bed.

4. Use the buckle straps to secure the powered mattress to the bed deck in the following locations:
  - Head End - Head End Bed Deck
  - Foot End - Foot End Bed Deck
  - Center - Center of the Bed Frame

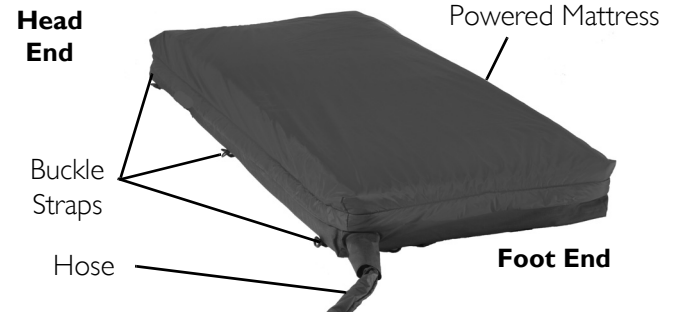

**FIGURE I** Mattress Replacement System - Mattress Replacement System

## 4 OPERATION

### 4.2 Installing the Side Rails



#### **WARNING**

Patient entrapment with bed side rails may cause injury or death. Mattress **MUST** fit bed frame and side rails snugly to prevent patient entrapment. Follow the manufacturer's instructions. Monitor patient frequently. Read and understand the Owner's/Operator's Manual prior to using this equipment. Invacare product manuals are available at [www.invacare.com](http://www.invacare.com) or your dealer.




Refer to the instructions provided with the side rails for the installation procedure.

### **Installing the Power Unit**

1. Swing out the bed hooks on the back of the control unit.
2. Place the control unit on the footboard.



If the bed does not have a footboard, place the control unit on a flat surface, leaving room for the hose to hang down.

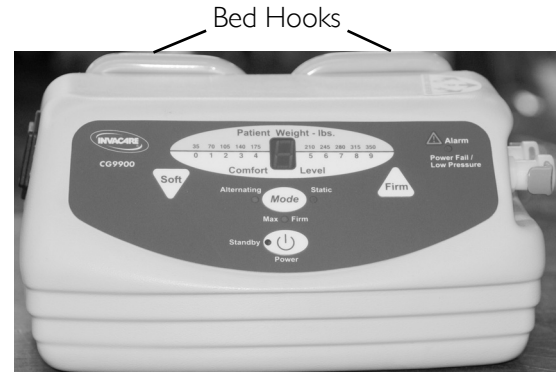

**FIGURE 2** Installing the Power Unit

### 4.3 Connecting the Hose




#### CAUTION

Ensure that the hose connecting the control unit to the mattress is routed such that it cannot be stepped on, kinked, squeezed or otherwise damaged.

1. Locate the hose at the foot end of the mattress.
2. Locate the control unit connectors on the right side of the control unit.
3. Squeeze and hold the tabs on the hose connectors.
4. Push the hose connectors onto the control connectors until an audible click is heard.



The audible click indicates that the hose connectors are properly engaged with the control connectors.

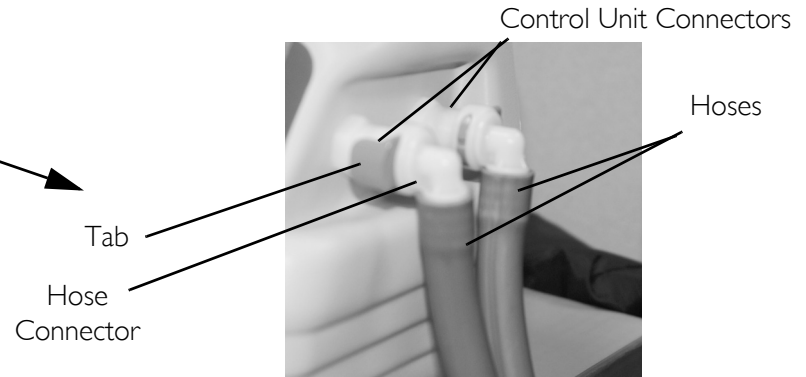

**FIGURE 3** Connecting the Hose

## 4 OPERATION

### 4.4 Connecting the Power Cord



#### **WARNING**

DO NOT alter plug to fit a non-conforming outlet. Instead, have an electrician install a properly grounded 3-prong outlet. Failure to use the correct plug and outlet can result in a potential safety hazard.

#### **CAUTION**

Ensure that the power cord of the control unit is not pinched, or has any objects placed on it, and also ensure it is not located where it can be stepped on or tripped over.

1. Examine the hospital grade power cord supplied with the control unit.
2. Perform one of the following:
  - If the cord is damaged - Call your supplier for a replacement hospital grade cord.
  - If the cord is not damaged - Plug the end of the supplied hospital grade power cord into the power outlet on the side of the control unit.
3. Plug the other end of the plug into a properly grounded outlet on the wall.



Once the unit is plugged in, an amber LED on the control unit is lit indicating that the system is in STAND BY mode.



## 4.5 Using the Front Panel

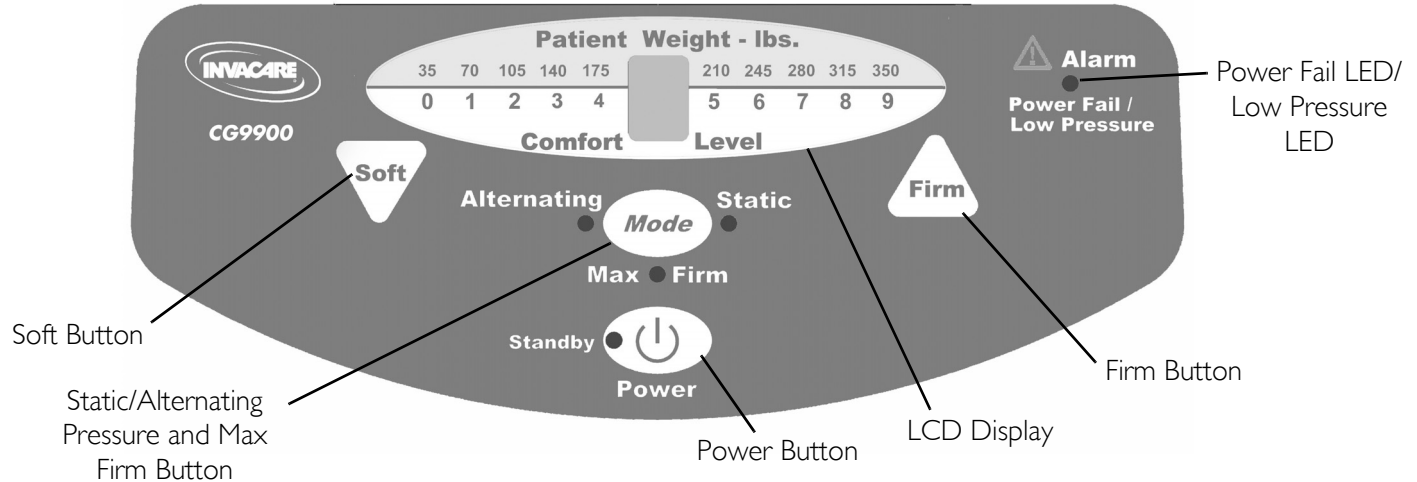


FIGURE 4 Using the Front Panel

**Power Button**

- I. To turn the control unit on or off, press and release the Power button.





Once the unit is plugged in, an amber LED on the control unit is lit indicating that the system is in stand by mode. Once the Power button is pressed and released, a green LED on either AP or Static or Max Firm illuminates indicating that the control unit is on.

If the power comes on after a power outage, the control unit will go through its system initialization routine for a few seconds and then resume the desired function.

## 4 OPERATION

### Firm/Soft Buttons

1. Select comfort pressure settings by pressing Firm (  ) or Soft (  ) button.
  - Soft Button - Pressing this button reduces the pressure setting in the mattress.
  - Firm Button - Pressing this button increases the pressure setting in the mattress.




The patient comfort pressure ranges from Soft (level 0 =  $8\pm 4$  mmHg) to Firm (level 9 =  $32\pm 4$  mmHg). The Comfort Control LED displays the patient comfort pressure levels from 0 to 9 and provides a guide to the caregiver to set approximate comfort pressure level depending on the patient weight. If the patient's weight to height ratio is above average, increase the pressure setting by approximately 20% or raising the control setting by 1 or 2 above the expected setting for that weight.

### Recommended Pressure Settings

1. For rapid inflation of the mattress, activate "Max Firm" (by following the "Max Firm" instructions).
2. For extra firm support during patient ingress/egress, patient wound care, patient turning or patient cleaning, it is recommended to set the mattress pressure to Max Firm.

### Max Firm

1. Activate Max Firm by pressing mode key: (  ). Max Firm LED will light up this mode. The Max Firm is used to rapidly inflate the mattress. Max Firm Mode will deactivate after 44 minutes, at which point the LED will turn off and the unit will default to its previous setting. In this mode the entire mattress will be pressurized to  $35\pm 5$  mm Hg.



It takes 40-60 minutes for the mattress to inflate fully (inflation time depends on size of mattress).

It is recommended that Max Firm setting be used during patient ingress/egress, patient wound care, patient turning or patient cleaning.

### Static

1. To set static mode, press the "Mode" key until the "Static" LED is lit. In static mode, all the air cushions in the mattress will be maintained at constant pressure.

### Alternating Pressure

1. To set alternating pressure (A/P) mode, press the "Mode" key until the "A/P" alternating pressure LED is lit.
2. In the A/P mode, the even numbered air cushions in the mattress will deflate, while the odd numbered cushions remain at constant pressure. When 10 minutes has elapsed, the even numbered air cushions will inflate while the odd numbered cushions remain at constant pressure. When 10 minutes has elapsed again, the odd numbered air cushions deflate while the even numbered cushions remain at constant pressure. The air cushions continue to inflate or deflate like this as long as the alternating pressure mode is selected.

### Adjusting the Minimum Pressure Setting (A/P Low)

The minimum pressure setting during alternating pressure is set to 0 (3mm Hg) at the factory. This means the mattress will deflate as much as possible during the deflation time when using the "A/P" mode. The setting can be changed so the mattress will only deflate to 50% of the selected pressure setting.

1. Ensure the standby LED is lit.
2. Perform the following:
  - Press and hold the "Firm" and "Mode" keys while in standby.
3. Read the LCD display. The LCD display will flash:
  - UNIT WILL DISPLAY "0" FOR LOW A/P SET TO 0 (3 mmHg)
  - UNIT WILL DISPLAY "5" FOR LOW A/P SET TO 50% OF High
4. Perform one of the following to toggle between the two settings
  - PRESS MODE KEY TO TOGGLE LOW SIDE A/P PRESSURE
  - PRESS ON/STANDBY KEY TO END ROUTINE

## 4 OPERATION

### 4.6 Failure Modes

#### Power Fail LED

In the event of power outage, Power Fail LED flashes AMBER. The control unit has internal memory and retains the previous settings during the power outage.



During a power outage, the mattress retains the air as long as the mattress is connected to the control unit.

#### Low Pressure LED

In the event that the mattress hose disconnects, or low pressure is detected, an alarm sounds and Low Pressure LED flashes AMBER. Once the low pressure problem is fixed, the control unit resumes operation in the previously set mode.

1. The mattress will hold air during transportation or power failure as long as the mattress is connected to the control unit.

### 4.7 Powering Up the System



For this procedure, refer to FIGURE 4 on page 17.

1. Turn on the power to the system by pressing the Power button on the control unit.



Once the button is released, a green LED illuminates when the unit is on.

### 4.8 Placing the Patient on the Mattress

1. Press the Mode button to select Max Firm Mode.



In this mode, the Max Firm LED lights up.

2. After the mattress is fully inflated, place the patient on the mattress.
3. Ensure that the patient's feet are towards the foot end of the mattress (the end with the hose).

4. Center the patient on the bed from side-to-side and head-to-foot.



Special positioning may be required with contracted patients to provide comfortable positions.

5. After placing the patient, make certain no objects will fall under the patient, such as feeding tubes, IV's etc.
6. Wait five minutes for the mattress pressure to stabilize.
7. Once the mattress inflates to its normal size, set the comfort pressure to the desired comfort level.
8. Wait five minutes for the mattress pressure to stabilize.
9. Verify that the patient has not bottomed out by performing the following steps:
  - A. Ensure that the patient is lying flat on his/her back in the middle of the mattress.
  - B. Place four fingers between the air cushions directly underneath the sacral region of the patient's body.
  - C. Ensure that there is 3 to 4-finger width clearance between the bottom of the patient and the bed frame.
  - D. Adjust the comfort setting, if needed.
  - E. Wait five minutes for the mattress pressure to stabilize.
  - F. Repeat STEPS A-E until patient has not bottomed out and patient comfort is achieved.
10. If the patient feels that the bed is too soft/hard, press the Soft or Firm button to adjust the comfort settings.
11. Use a regular pillow to help support and stabilize the patient's head.

#### 4.9 Transferring Patient From/To a Gurney



### **WARNING**

ALWAYS engage the wheel locks of the bed and the wheel locks of the gurney before transferring the patient between the bed and the gurney.

1. Engage the wheel locks of the bed. Refer to the owner's manual provided with the bed.
2. Engage the wheel locks of the gurney. Refer to the owner's manual provided with the gurney.
3. Press the Max Firm or Mode button to achieve maximum mattress pressure.

## 4 OPERATION

4. Raise or lower the bed to match the gurney height. Refer to the owner's manual provided with the bed.
5. When the mattress has reached maximum firmness, perform one of the following:
  - Bed to Gurney Transfer - Slide the patient onto the gurney.
  - Gurney to Bed Transfer - Slide the patient onto the bed.

### 4.10 Transferring Patient From/To a Wheelchair



#### **WARNING**

ALWAYS engage the wheel locks of the bed and the wheel locks of the wheelchair before transferring the patient between the bed and the wheelchair.


1. Engage the wheel locks of the bed. Refer to the owner's manual provided with the bed.
2. Engage the wheel locks of the wheelchair, if applicable. Refer to the owner's manual provided with the wheelchair.
3. Press the Max Firm or Mode button to achieve maximum mattress pressure.
4. Raise or lower the bed to match the wheelchair height. Refer to the owner's manual provided with the bed.
5. When the mattress has reached maximum firmness, perform one of the following:
  - Bed to Wheelchair Transfer - Slide the patient onto the wheelchair.
  - Wheelchair to Bed Transfer - Slide the patient onto the bed.

### 4.11 Preparing for CPR Procedure



For this procedure, refer to FIGURE 5.

1. Press and hold the tabs on hose connector while pulling the hose from the control unit.

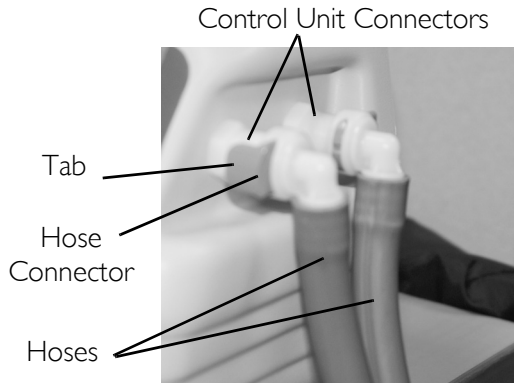

**FIGURE 5** Preparing for CPR Procedure

#### 4.12 About Power Outage and Transportation

If the hoses remain connected to the control unit, the mattress retains air during a power outage, during transportation, when the control unit is unplugged or when the control unit is turned Off.

### 5 Maintenance and Troubleshooting

---

#### 5.1 Cleaning the System



#### **WARNING**

Before cleaning or disassembling the CG9900 mattress, check the underside of the mattress folds for sharp objects such as scissors, needles, etc. These objects should be removed and discarded before proceeding with further cleaning or disassembly; otherwise injury or damage to the product may occur.

Because of potential risk of infectious exposure, cleaning with the patient on the bed is not recommended.

All equipment should be inspected. Any item that is visibly soiled with the patient's blood or other body fluids should be properly cleaned or removed.

Laundry workers should treat all soiled bedding as if it were contaminated with pathogenic microorganisms.

1. Remove the bedding.
2. If necessary, inflate the mattress.
3. Ensure that the control unit is off.
4. Unplug the power cord from the wall outlet.
5. Ensure that the underside of the mattress is clear of all sharp objects.
6. Examine the surface of the control unit and mattress assembly components for visible blood or body fluids.
7. Perform one of the following:
  - If blood is present, decontaminate the product.
    - i. Remove all visible soil with disposable paper towels.
    - ii. Scrub the area with freshly prepared effective phenolic detergent disinfectant solution.



## 5 MAINTENANCE AND TROUBLESHOOTING

- If blood is not present, remove any soil from the cover with paper towels.



If soiled, the cover should be removed, cleaned and decontaminated.

8. Perform the following steps to clean the mattress cover:

- A. Using a clean sponge or paper towel, Scrub the area with freshly prepared effective phenolic detergent disinfectant solution.
- B. Remove the cover and launder it using the following method:



### **CAUTION**

Laundry workers should always wash their hands before working with clean bedding.

**DO NOT** overload the machine.

**DO NOT** use chlorine bleach because it may damage the fabric coating.

High air temperatures will damage the fabrics and void the Invacare warranty.

- i. Place the cover in a washing machine.
  - ii. Wash with warm water (below 120°F).
  - iii. Add detergent and disinfectant according to the manufacturer's instructions.
  - iv. Remove excess water.
  - v. Set the dryer to the lowest setting (below 120°F).
  - vi. Dry the cover until it is completely dry.
9. Perform the following steps to clean the control unit and hose fittings:
- A. Wipe all controls, chassis and hose fittings with a quaternary disinfectant solution.
  - B. Using a nylon brush, gently clean all crevices as they can harbor microorganisms.
  - C. Air dry all treated surfaces.

## 5 MAINTENANCE AND TROUBLESHOOTING

10. Perform the following steps to clean the mattress components (air cushions, mattress base, etc.):
  - A. Using a clean sponge or paper towel, wipe down the mattress components with a dilute detergent solution of quaternary cleaner disinfectant or other germicidal detergent solution.
  - B. Wipe the mattress components with a clean dry cloth.

### Storing the System

1. Ensure that the control unit is off and disconnect the power cord from the wall outlet.
2. Clean the system. Refer to [Cleaning the System](#) on page 24.
3. Disconnect the air hose connector(s) from the control unit and allow air to vent from the mattress.
4. Gently roll up the mattress with minimal handling and agitation.
5. Ensure the cover surface is inside the roll.
6. Store the unit, keeping the mattress with the control unit.

### Replacing Bladders

To replace an individual bladder:

1. Unsnap the buttons for the bladder on both sides.
2. Cut a small slit on the red female connector.
3. Pull apart the cut female end of the connector and bladder from the male end of the manifold.
4. Take the new bladder and dampen the inside of the female end of the connector.
5. Push the new female end of the connector and bladder onto the male end of the manifold securely.

### 5.2 Troubleshooting

PROBLEM	CAUSE	SOLUTION
Mattress not inflating Not alternating properly	Mattress hose disconnected	Connect hose connectors and lock them in place
	Air hose kinked or split	Unkink hose or replace split hose
	Major leak in the air cushions	Replace leaking air cushions
	Kinked or split manifold	Unkink manifold or replace split manifold
	Has power and fuse is good, control unit does not come on	Send control unit back to factory for repair
	Not alternating, solenoid malfunction	Send control unit back to factory for repair
	No air, pump malfunction	Send unit for repair
No power	Control unit off	Check power source and turn on unit
	Power cord disconnected	Connect power cord to the power source
	No power in the power source	Check power source has power and turn it On
	Power outage	Wait till the power source has power
	Blown fuse	Replace blown fuse with an equivalent fuse

Part No 1171739

Rev A - 2/11



**Invacare Corporation**

**USA**

One Invacare Way  
Elyria, Ohio USA  
44036-2125  
800-333-6900

[www.invacare.com](http://www.invacare.com)

**Canada**

570 Matheson Blvd E  
Unit 8  
Mississauga Ontario  
L4Z 4G4 Canada  
800-668-5324



*Yes, you can.®*