



ExoQuick™ Exosome Precipitation Solution

Cat. # EXOQ5A-1

Cat. # EXOQ20A-1

User Manual

Store kit at 4°C on receipt

A limited-use label license covers this product. By use of this product, you accept the terms and conditions outlined in the Licensing and Warranty Statement contained in this user manual.

ver. 4-2011-07-11

Contents

I.	Overview	2
II.	Exosome Isolation Protocol	3
III.	Exosome analysis	
	A. RNA analysis	4
	B. Protein analysis	4
IV.	Example Data and Applications	6
V.	Appendix	10
VI.	References	10
VII.	Technical Support	11
VIII.	Licensing and Warranty	12

List of Components

Item	Catalog #	Reactions
ExoQuick exosome precipitation solution (20 ml)	EXOQ20A-1	300 reactions
ExoQuick exosome precipitation solution (5 ml)	EXOQ5A-1	75 reactions

The ExoQuick™ kits are shipped at room temperature or on blue ice and should be stored at +4°C upon receipt. Properly stored kits are stable for 1 year from the date received. The reaction size is based on using 250 µl serum for exosome isolation. Examples of precipitating exosomes from various biofluids can be seen in the Table below.

Bio-fluid	Sample volume	ExoQuick volume
Serum	250 µl	63 µl
Ascites fluid	250 µl	63 µl


To isolate exosomes from tissue culture media or urine, we recommend using the ExoQuick-TC reagent (cat# EXOTC50A-1) which is a distinct formulation from the original ExoQuick reagent detailed in this manual.

ExoQuick Exosome Precipitation


I. Overview

Exosomes are 40 –150 nm membrane vesicles secreted by most cell types in vivo and in vitro. Exosomes are found in blood, urine, amniotic fluid, malignant ascite fluids and contain distinct subsets of microRNAs depending upon the tumor from which they are secreted. SBI's ExoQuick exosome precipitation reagent makes microRNA and protein biomarker discoveries simple, reliable and quantitative. Enrich for circulating exosomal microRNAs with ExoQuick™ and accurately profile them using SBI's QuantiMir™ qPCR arrays.

- * No time-consuming ultracentrifugation
- * Less expensive than costly antibodies and beads
- * More effective than any other method
- * Use as little as 100 µl of serum or bio-fluid

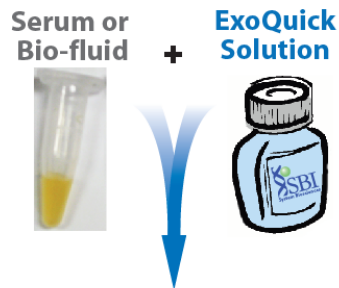


Simple one-step precipitation

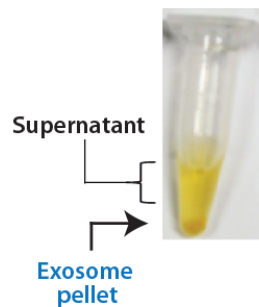


Exosome precipitation from 250 µl human serum samples was verified by Western blot using antibodies against two commonly found exosome biomarker proteins, CD63 and CD9 and small RNAs analyzed on RNA gels after Trizol extraction.

Exosome Protein Marker Analysis



Exosome RNA Analysis



II. Exosome Precipitation Protocol

Isolate exosomes with ExoQuick


1. Collect biofluid and centrifuge at $3000 \times g$ for 15 minutes to remove cells and cell debris.
2. Transfer supernatant to a sterile vessel and add the appropriate volume of ExoQuick Exosome Precipitation Solution to the bio-fluid. Some examples are shown in the Table below. Mix well by inverting or flicking the tube.

Incubation Time	Bio-fluid	Sample volume	ExoQuick volume
30 minutes	Serum*	250 μ l	63 μ l
Overnight	Ascites fluid	250 μ l	63 μ l

*Note when precipitating exosomes from plasma, the resulting pellet may be difficult to resuspend due to precipitated fibrin and other fibrinogens. For plasma, please refer to the Appendix for additional preparation steps.

3. Refrigerate overnight (at least 12 hours). The tubes do not need to be rotated during the incubation period.
4. Centrifuge ExoQuick/biofluid mixture at $1500 \times g$ for 30 minutes. Centrifugation may be performed at either room temperature or 4°C with similar results. After centrifugation, the exosomes may appear as a beige or white pellet at the bottom of the vessel.

Exosome pellets obtained from 10 ml of cerebral spinal fluid using ExoQuick.

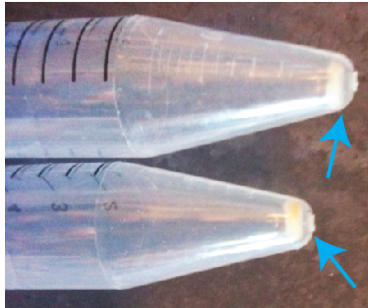

5. Aspirate supernatant. Spin down residual ExoQuick solution by centrifugation at $1500 \times g$ for 5 minutes. Remove all traces of fluid by aspiration, taking great care not to disturb the precipitated exosomes in pellet.
6. Resuspend exosome pellet in 1/10 of original volume using sterile or nuclease-free water. If the pellet is difficult to resuspend, add slightly more water to the pellet to further dilute the salt.

III.

A. Using Precipitated Exosomes for RNA Extraction

For RNA extraction, we recommend following the protocol outlined in the SeraMir Kit user manual as shown here (Catalog #: RA800A-1, RA805A-1, RA806A-1, RA810A-1, and RA820A-1).

1. Thaw serum sample on ice
2. Combine 500µl serum + 120 µl **ExoQuick**
3. Mix well by inversion three times
4. Place at 4°C for 30 minutes
5. Centrifuge at 13,000 rpm for 2 minutes
6. Remove supernatant, keep exosome pellet
7. Add 350 µl **LYSIS Buffer** to exosome pellet and vortex 15 seconds
8. Place at room temperature for 5 minutes (to allow complete lysis)
--- optional--- add 5µl of SeraMir control RNA spike-in
(cat#RA805A-1)
9. Add 200µl of 100% **Ethanol**, vortex 10 seconds
10. Assemble spin column and collection tube
11. Transfer all (600µl) to spin column
12. Centrifuge at 13,000 rpm for 1 minute
(check to see that all flowed through,
otherwise spin longer)
13. Discard flow-through and place spin column back into collection tube
14. Add 400µl **WASH Buffer**
15. Centrifuge at 13,000 rpm for 1 minute
16. Repeat steps 13 to 15 once again (total of 2 Washes)
17. Discard flow-through and centrifuge at 13,000 rpm for 2 minutes to dry (IMPORTANT !)

Exosome
Isolation
and Lysis

exoRNA
Purification

18. Discard collection tube and assemble spin column with a fresh, RNase-free 1.5ml elution tube (not provided)
19. Add 30µl **ELUTION Buffer** directly to membrane in spin column
20. Centrifuge at 2,000 rpm for 2 minutes (loads buffer in membrane)
21. Increase speed to 13,000 rpm and centrifuge for 1 minute (elutes exoRNAs)
22. You should have recovered 30-40µl exosome RNA

exoRNA
Elution

The yield of RNA from isolated exosomes is different depending on the starting biofluid or the type of cells that were grown in culture. Different cell types secrete varying levels of exosomes. For serum, the level of RNA isolated from 500 µl is usually in the 500ng range and can be measured using a Agilent Bioanalyzer or a NanoDrop Spectrophotometer.

B. Using Precipitated Exosomes for Protein Extraction**ELISA analysis**

SBI offers three ELISA kits (Catalog#: ExoELISA-63, ExoELISA-9, ExoELISA-81) for fast and quantitative analysis of well-characterized exosomal protein markers: **CD63**, **CD9** and **CD81**.

1. If frozen, thaw culture media or urine sample on ice
2. Combine 10ml sample + 2ml **ExoQuick-TC**
3. Mix well by inversion three times
4. Place at 4°C for overnight (at least 12 hours)
5. Centrifuge at 1500 × g for 30 minutes
6. Remove supernatant, keep exosome pellet
7. Centrifuge at 1500 × g for 5 minutes to remove all traces of fluid (take great care not to disturb the pellet)
8. Add 200 µl **Exosome Binding buffer** to exosome pellet and vortex 15 seconds
9. Place at room temperature for 5 minutes (to allow complete lysis)
10. Exosome protein is now ready for immobilization onto micro-titer plate.

Please refer to the ExoELISA manual for the complete protocol.

Western blot analysis

For Western blotting analysis, we recommend resuspending the exosome pellet in **1XRIPA buffer**¹ with the appropriate protease inhibitor cocktail.

SBI offers a Western blot antibody detection kit (Catalog# ExoAB4-1) which includes four exosomal marker antibodies: **CD63, CD9, CD81, HSP70** and a Goat anti-Rabbit IgG HRP conjugated secondary antibody specifically tested for use in exosomal protein analysis.

1. If frozen, thaw culture media or urine sample on ice
2. Combine 10 ml sample + 2 ml **ExoQuick-TC**
3. Mix well by inversion three times
4. Place at 4°C for overnight (at least 12 hours)
5. Centrifuge at 1500 × *g* for 30 minutes
6. Remove supernatant, keep exosome pellet
7. Centrifuge at 1500 × *g* for 5 minutes to remove all traces of fluid (take great care not to disturb the pellet)
8. Add 200 µl **RIPA buffer**¹ to exosome pellet and vortex 15 seconds
9. Place at room temperature for 5 minutes (to allow complete lysis)
10. Add **Laemmli buffer**² (with Beta-mercaptoethanol) and heat at 95°C for 5 minutes.
11. Chilled on ice for 5 minutes before loading onto gel
12. Perform standard SDS-PAGE electrophoresis and Western transfer onto PVDF membrane
13. Block with 5% dry milk in Tris Buffered Saline + 0.05% Tween (TBS-T) for 1 hour
14. Incubate blot overnight at 4°C with SBI's exosome specific antibody (e.g. CD9) at 1:1000 dilution (5% dry milk in TBS-T)
15. Wash 3X with TBS-T
16. Incubate one hour at room temperature with SBI's Goat anti-Rabbit-HRP antibody at 1:20,000 dilution (5% dry milk in TBS-T)
17. Wash 3X with TBS-T
18. Incubate blot with chemi-luminescence substrate and visualize on film or other imaging equipment



Exosome
Isolation and
lysis

- ¹ 1X **RIPA buffer** contains:
- 25mM Tris-HCl pH 7.6
 - 150mM NaCl
 - 1% NP-40
 - 1% sodium deoxycholate
 - 0.1% SDS

- ² 2X **Laemmli buffer** contains:
- 4% SDS
 - 20% glycerol
 - 10% 2-mercaptoethanol
 - 0.004% bromphenol blue
 - 0.125 M Tris-HCl pH 6.8

IV. Example Data and Applications

1. Protein Yield from Exosomes precipitated with ExoQuick versus other Extraction Methods

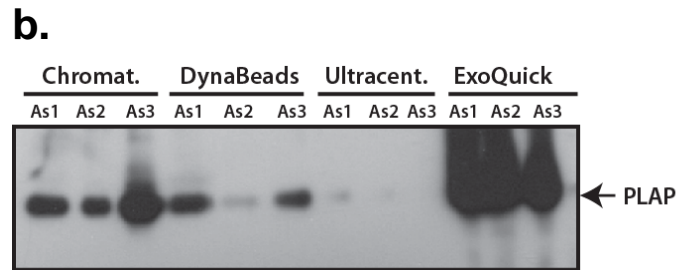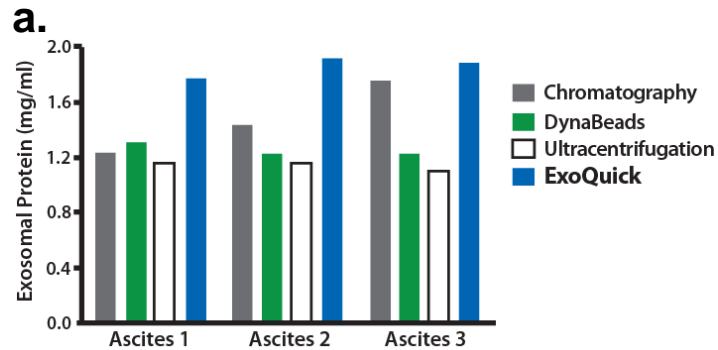


Data courtesy of Dr. Douglas Taylor, Univ. Louisville, KY.

a. The quantity of protein was determined by the Bradford microassay method (Bio-Rad Laboratories) using BSA as a standard.

b. Proteins from each exosome isolate were standardized to the original sample volume and equal volumes were applied per lane of a 12.5% SDS-PAGE gel. Western immunoblotting was performed to analyze the presence of the specific marker protein, placental alkaline phosphatase (PLAP). The SDS-PAGE gel was transferred to a nitrocellulose membrane, the membrane blocked for 1 hour at room temperature with non-fat dried milk, and probed overnight at 4°C with primary antibody. The bound immune complexes were visualized by enhanced chemiluminescence (ECL, Amersham Life Sciences) and quantitated by densitometry (Un-Scan-it Software, Silk Scientific Corp).

2. MicroRNA Yield from Exosomes precipitated with ExoQuick versus other Extraction Methods

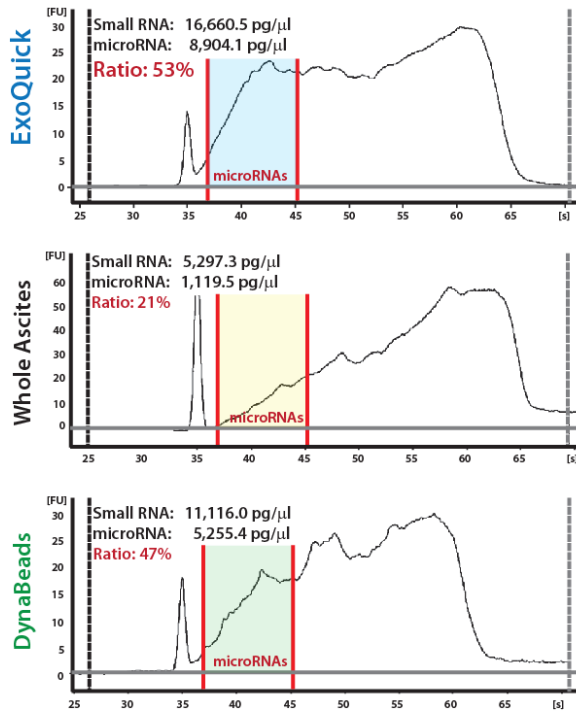


Agilent Bioanalyzer data courtesy of Dr. Douglas Taylor, Univ. Louisville, KY.

The RNA quality and yield was assessed using a GeneQuant II. Small RNAs were analyzed with the Agilent 2100 Bioanalyzer Lab-on-a-Chip instrument system (Agilent Technologies), using the Agilent Small RNA chip and reagent kit. Approximately 100ng of isolated total RNA in 1μl was applied to each run. The manufacturer’s recommended protocol was strictly followed to obtain Bioanalyzer profiles for the size range 6 to 150 nucleotides (nt). The profiles were calibrated for size (nt) using the small RNA ladder supplied with the kit, containing markers of 20, 40, 60, 80, and 150 nt in size, as reference. The instrument software quantitated the peak area between 0 and 150 nt as small RNA region, the area within 10 to 40 nt as microRNA region, and provides percentages of miRNA detected for each sample.

4. Activity Assays: Track Exosomes using Cyto-Tracers

SBI has created a line of lentivector-based Cyto-Tracers™ that utilize GFP-fusion proteins to mark cellular compartments, organelles, vesicles and structures to enable more long-term and more in-depth experimentation. The Cyto-Tracers can be used in transfections as well as packaged into virus to create stable GFP tracer cell lines in primary cells, tumor cell lines and stem cells.

The Tetraspanin CD63 protein is a common biomarker for exosomes. With the pCT-CD63-GFP construct you can make your cells of interest secrete exosomes that glow green for downstream functional delivery studies (Cat. # CYTO120-PA-1).

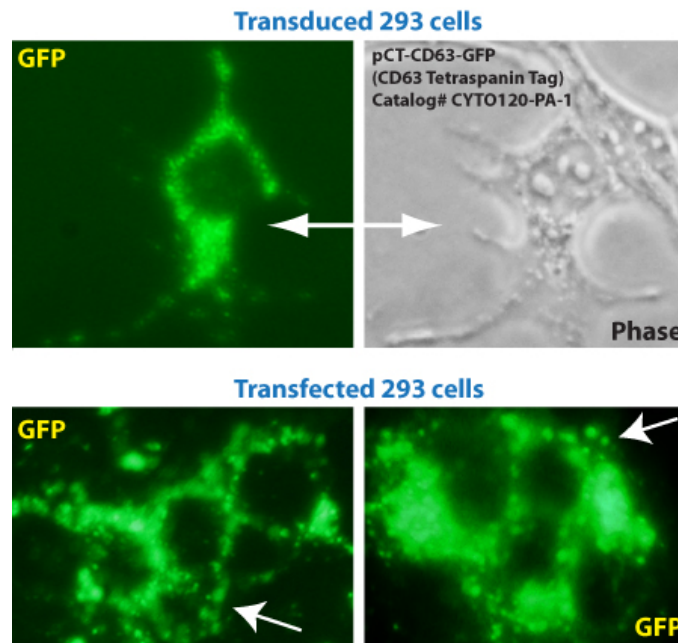


1. NanoSight

The NanoSight LM10 instrument is based on a conventional optical microscope and uses a laser light source to illuminate nano-scale particles within a 0.3 ml sample introduced to the viewing unit with a disposable syringe. Enhanced by a near perfect black background, particles appear individually as point-scatterers moving under Brownian motion.

The image analysis Nanoparticle Tracking Analysis (NTA) software suite allows users to automatically track and size nanoparticles on an individual basis. Results are displayed as a frequency size distribution graph and output to spreadsheet.

ExoQuick serum exosome analysis

Normal human serum from 50 pooled samples was used. Only 250ul serum was combined with 63ul ExoQuick to pellet the exosomes in 30 minutes. The exosome pellet was resuspended in 100ul PBS, diluted 1:10,000 and visualized on the NanoSight LM10 instrument. The analysis shows that ExoQuick isolated 90nm exosomes with a recovery of 2.74×10^{12} particles/ml.

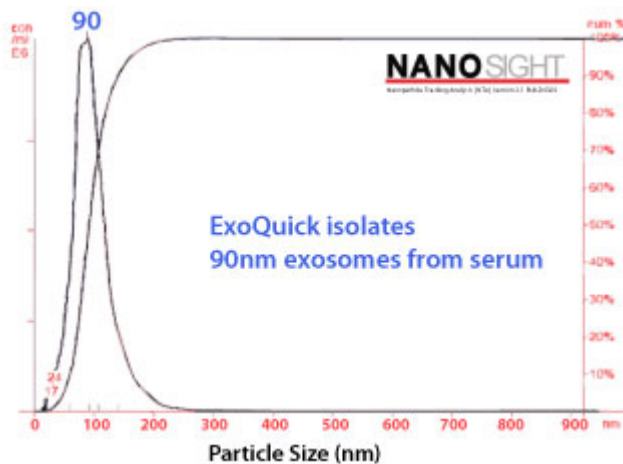

Data acquisition and analysis

These experiments were done in collaboration with Particle Characterization Laboratories, Inc (PCL).

V. Appendix

1. Use ½ amount of Thromboplastin D in attached protocol.
2. Squirt in Thromboplastin D reagent rapidly into plasma sample to mix thoroughly
3. Incubate at 37°C for 15 minutes.
4. Spin at 10,000 rpm at RT for 5 minutes (microfuge)
5. Save supernatant = “serum-like” sample, discard coagulated pellet
6. Use “serum-like” supernatant with ExoQuick to isolate exosomes as stated in ExoQuick protocol (use 25ul ExoQuick per 100ul coagulated plasma supernatant).

VI. References

As featured in: **Exosome Isolation for Proteomic Analyses and RNA Profiling** Douglas D. Taylor, Wolfgang Zacharias and Cicek Gercel-Taylor, [Serum/Plasma Proteomics. Methods in Molecular Biology. 2011, Volume 728, Part 4, 235-246, \(PDF\) »](#)

Tae Hoon Lee, Esterina D'Asti, Nathalie Magnus, Khalid Al-Nedawi, Brian Meehan and Janusz Rak. [Review: Microvesicles as mediators of intercellular communication in cancer—the emerging science of cellular 'debris'. Seminars in Immunopathology DOI: 10.1007/s00281-011-0250-3. \(PDF\) »](#)

Technical References

Adachi T, Nakanishi M, Otsuka Y, Nishimura K, Hirokawa G, Goto Y, Nonogi H, Iwai N. [Plasma microRNA 499 as a biomarker of acute myocardial infarction. Clin Chem. 2010 Jul;56\(7\):1183-5.](#)

De Smaele E, Ferretti E, Gulino A. [MicroRNAs as biomarkers for CNS cancer and other disorders. Brain Res. 2010 Jun 18;1338:100-11.](#)

Mitchell PS, Parkin RK, Kroh EM, Fritz BR, Wyman SK, Pogosova-Agadjanyan EL, Peterson A, Noteboom J, O'Briant KC, Allen A, Lin DW, Urban N, Drescher CW, Knudsen BS, Stirewalt DL, Gentleman R, Vessella RL, Nelson PS, Martin DB, Tewari M. [Circulating microRNAs as stable blood-based markers for cancer detection. Proc Natl Acad Sci U S A. 2008 Jul 29;105\(30\):10513-8.](#)

Laterza OF, Lim L, Garrett-Engele PW, Vlasakova K, Muniappa N, Tanaka WK, Johnson JM, Sina JF, Fare TL, Sistare FD, Glaab WE. [Plasma MicroRNAs as sensitive and specific biomarkers of tissue injury. Clin Chem. 2009 Nov;55\(11\):1977-83.](#)

Valadi H, Ekström K, Bossios A, Sjöstrand M, Lee JJ, Lötvall JO. [Exosome-mediated transfer of mRNAs and microRNAs is a novel mechanism of genetic exchange between cells. Nat Cell Biol. 2007 Jun;9\(6\):654-9.](#)

Pegtel DM, Cosmopoulos K, Thorley-Lawson DA, van Eijndhoven MA, Hopmans ES, Lindenberg JL, de Gruijl TD, Wordinger T, Middeldorp JM. [Functional delivery of viral miRNAs via exosomes. Proc Natl Acad Sci USA; 2010 Apr 6; 107\(14\):6328-33.](#)

Mathivanan, S. and Simpson, R.J. [ExoCarta: A compendium of exosomal proteins and RNA. Proteomics. 2009.21, 4997-5000.](#)

They C, Ostrowski M, Segura E. [Membrane vesicles as conveyors of immune responses. Nat Rev Immunol. 2009. 8, 581-93.](#)

Michael A, Bajracharya SD, Yuen PS, Zhou H, Star RA, Illei GG, Alevizos I. [Exosomes from human saliva as a source of microRNA biomarkers. Oral Dis; 2010 Jan; 16\(1\):34-8.](#)

Luo SS, Ishibashi O, Ishikawa G, Ishikawa T, Katayama A, Mishima T, Takizawa T, Shigihara T, Goto T, Izumi A, Ohkuchi A, Matsubara S, Takeshita T, Takizawa T. [Human villous trophoblasts express and secrete placenta-specific microRNAs into maternal circulation via exosomes. Biol Reprod; 2009 Oct; 81\(4\):717-29.](#)

Taylor DD, Gercel-Taylor C. [MicroRNA signatures of tumor-derived exosomes as diagnostic biomarkers of ovarian cancer. Gynecol Oncol; 2008 Jul; 110\(1\):13-21.](#)

Simpson RJ, Lim JW, Moritz RL, Mathivanan S. [Exosomes: proteomic insights and diagnostic potential. Expert Rev Proteomics. 2009 Jun;6\(3\):267-83. Review.](#)

VII. Technical Support

For more information about SBI products and to download manuals in PDF format, please visit our web site:

<http://www.systembio.com>

For additional information or technical assistance, please call or email us at:

System Biosciences (SBI)
265 North Whisman Road.
Mountain View, CA 94043

Phone: (650) 968-2200
(888) 266-5066 (Toll Free)

Fax: (650) 968-2277

E-mail:

General Information: info@systembio.com

Technical Support: tech@systembio.com

Ordering Information: orders@systembio.com

II. Licensing and Warranty Statement

Limited Use License

Use of the ExoQuick™ Exosome Precipitation Solution (*i.e.*, the "Product") is subject to the following terms and conditions. If the terms and conditions are not acceptable, return all components of the Product to System Biosciences (SBI) within 7 calendar days. Purchase and use of any part of the Product constitutes acceptance of the above terms.

The purchaser of the Product is granted a limited license to use the Product under the following terms and conditions:

The Product shall be used by the purchaser for internal research purposes only. The Product is expressly not designed, intended, or warranted for use in humans or for therapeutic or diagnostic use.

The Product may not be resold, modified for resale, or used to manufacture commercial products without prior written consent of SBI.

This Product should be used in accordance with the NIH guidelines developed for recombinant DNA and genetic research.

SBI has pending patent applications related to the Product. For information concerning licenses for commercial use, contact SBI.

Purchase of the product does not grant any rights or license for use other than those explicitly listed in this Licensing and Warranty Statement. Use of the Product for any use other than described expressly herein may be covered by patents or subject to rights other than those mentioned. SBI disclaims any and all responsibility for injury or damage which may be caused by the failure of the buyer or any other person to use the Product in accordance with the terms and conditions outlined herein.

Limited Warranty

SBI warrants that the Product meets the specifications described in this manual. If it is proven to the satisfaction of SBI that the Product fails to meet these specifications, SBI will replace the Product or provide the purchaser with a refund. This limited warranty shall not extend to anyone other than the original purchaser of the Product. Notice of nonconforming products must be made to SBI within 30 days of receipt of the Product.

SBI's liability is expressly limited to replacement of Product or a refund limited to the actual purchase price. SBI's liability does not extend to any damages arising from use or improper use of the Product, or losses associated with the use of additional materials or reagents. This limited warranty is the sole and exclusive warranty. SBI does not provide any other warranties of any kind, expressed or implied, including the merchantability or fitness of the Product for a particular purpose.

SBI is committed to providing our customers with high-quality products. If you should have any questions or concerns about any SBI products, please contact us at (888) 266-5066.

© 2011 System Biosciences (SBI), All Rights Reserved