

# Bipolar Temperature Controller

*Model CL-100*



**WARNER**  
INSTRUMENTS

A Harvard Apparatus Company

# WEEE/RoHS Compliance Statement


## EU Directives WEEE and RoHS

To Our Valued Customers:

We are committed to being a good corporate citizen. As part of that commitment, we strive to maintain an environmentally conscious manufacturing operation. The European Union (EU) has enacted two Directives, the first on product recycling (Waste Electrical and Electronic Equipment, WEEE) and the second limiting the use of certain substances (Restriction on the use of Hazardous Substances, RoHS). Over time, these Directives will be implemented in the national laws of each EU Member State.

Once the final national regulations have been put into place, recycling will be offered for our products which are within the scope of the WEEE Directive. Products falling under the scope of the WEEE Directive available for sale after August 13, 2005 will be identified with a "wheelie bin" symbol.

Two Categories of products covered by the WEEE Directive are currently exempt from the RoHS Directive – Category 8, medical devices (with the exception of implanted or infected products) and Category 9, monitoring and control instruments. Most of our products fall into either Category 8 or 9 and are currently exempt from the RoHS Directive. We will continue to monitor the application of the RoHS Directive to its products and will comply with any changes as they apply.

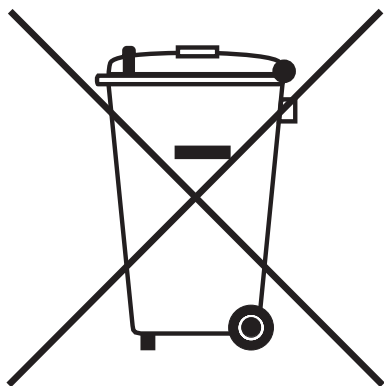

- **Do Not Dispose Product with Municipal Waste**
  - **Special Collection/Disposal Required**

# Table of Contents

1

Bipolar Temperature Controller Model CL-100

Warner Instruments

<b>SUBJECT</b>	<b>PAGE</b>
<b>Introduction .....</b>	<b>3</b>
<b>Nomenclature.....</b>	<b>4</b>
Text Conventions .....	4
<b>Control Description .....</b>	<b>5-8</b>
Front Panel.....	5
<i>Power Switch (Item A) .....</i>	<i>5</i>
<i>Meter Selector Switch and Meter (Item B) .....</i>	<i>5</i>
<i>Cooling Mode Switch (Item C) .....</i>	<i>6</i>
<i>Thermistor Recorder Outputs (Items D, E).....</i>	<i>6</i>
<i>Monitor Temp In BNC (Item F) .....</i>	<i>6</i>
<i>Loop Speed Switch (Item G) .....</i>	<i>6</i>
<i>Set Temperature Control (Item H).....</i>	<i>6</i>
<i>External/Internal Select Control (Item J) .....</i>	<i>6</i>
<i>Manual Voltage Control (Item K).....</i>	<i>7</i>
<i>Peltier Limit LED (Item L) .....</i>	<i>7</i>
<i>Freeze Alert LED (Item M) .....</i>	<i>7</i>
<i>Heat / Cool LED's (Item N) .....</i>	<i>7</i>
Rear panel .....	8
<i>External Volts Set (Item P) .....</i>	<i>8</i>
<i>External Temp Set (Item Q) .....</i>	<i>8</i>
<i>Heater/Cooler input (Item R) .....</i>	<i>8</i>
<i>Power Entry Module (Item S) .....</i>	<i>8</i>
<i>Ground Terminals (Item T) .....</i>	<i>8</i>
<b>Setup.....</b>	<b>9</b>
Warner Peltier Driven Systems .....	9
Operating With Other Equipment.....	9
<i>Warner Resistive Heating Systems .....</i>	<i>9</i>
<i>Third-Party Equipment .....</i>	<i>9</i>
<i>Thermistor Considerations .....</i>	<i>9</i>

# Table of Contents (Cont'd)

SUBJECT	PAGE
Operation .....	10-11
Automatic Mode .....	10
Manual Mode .....	11
Appendix .....	12
Specifications .....	12
Accessories and Replacement Parts .....	12
Warranty & Service .....	13-14
Warranty .....	13
Service Notes .....	13-14

# Introduction

The **CL-100 Bipolar Temperature Controller** from Warner Instruments is a versatile and simple to use thermal control device. This single channel, automatic controller capable of accurately maintaining a Peltier device between 0° and 50°C. The unit will also maintain a resistive heater from ambient to +65°C.

Although primarily designed for use with Warner **In-Line Solution Heater/Coolers**, this instrument can be easily adapted for use with custom-built equipment according to the requirements of the user. When coupled with the **SC-20 Dual In-line Solution Heater/Cooler**, the **CL-100** provides efficient control of perfusion solution temperatures.

The unit is simple to use with a single control for temperature adjustment. Total automatic control is provided in automatic mode, while manual control is available in manual mode. A loop-speed selector is used to optimize the response of the system to accommodate thermal delay characteristics intrinsic to the setup.

## ***Features of the CL-100 Include:***

- Quiet operation
- Automatic and manual modes
- Single control temperature adjustment
- Freeze alert
- Built-in protection for Peltier devices
- Selectable loop speed optimizes system speed and stability
- Simultaneous monitoring of system temperature and a separate point of interest
- Compatible with all Warner Peltier Driven Heater/Coolers



**CAUTION:** This equipment is not designed nor intended for use on human subjects.

## Text Conventions

This manual refers to instrument controls at two functional levels; specific controls and settings of these controls. To increase readability, we employ the following text conventions. Since our goal is to provide clarity rather than complexity, we welcome any feedback you may wish to provide.

- Warner Instrument product numbers are presented using **bold type**.
- References to controls are specified using CAPS.
- References to control settings are specified using *italic type*.
- Special comments and warnings are presented in **highlighted text**.

Any other formatting should be apparent from context.

# Control Description

5

## Front Panel

A schematic of the face panel of the **CL-100** is shown below. Important components are identified by letter (A-H, J-N). Refer to this diagram as an aid in identification of the described components.



### ***Power Switch (Item A)***

Supplies power to the CL-100.

### ***Meter Selector Switch and Meter (Item B)***

THE SELECTOR SWITCH selects the parameter displayed on the associated METER. Included options are *Set Temp*, *Control Temp*, *Monitor Temp*, and *Output Volts* and are described below.

*Set Temp* reports the adjustment from either the SET TEMPERATURE control (Item H) or the EXT TEMP SET BNC (Item Q). Displayed units are °C.

*Control Temp* reports the actual temperature of the feedback thermistor situated within the heater/cooler device being used. The data is informative only and is in units of °C.

*Monitor Temp* reports the temperature of the sensor thermistor which connects via the MONITOR TEMP IN BNC (Item F). This provides a convenient means to determine the temperature of any point of interest within your setup. Displayed units are °C.

*Output Volts* reports the adjustment from either the MANUAL VOLTAGE control (Item K) or the EXT VOLT SET BNC (Item P). Displayed units are V.

The METER also provides an indication that the main POWER is *on*.

## **Cooling Mode Switch (Item C)**

Selects between *Automatic* or *Manual* operational modes, or center select for *off*.

## **Thermistor Recorder Outputs (Items D, E)**

BNC connectors are provided to send thermistor readings to a data acquisition system or chart recorder.

CONTROL TEMP OUT (Item D) reports the actual temperature of the feedback thermistor situated within the heater/cooler device being used. Output is calibrated to 100 mV/°C.

MONITOR TEMP OUT (Item E) reports the temperature of the sensor thermistor which connects via the MONITOR TEMP IN BNC (Item F). Output is calibrated to 100 mV/°C.

## **Monitor Temp In BNC (Item F)**

BNC for connecting a sensor thermistor used to sample the temperature at a point of interest. Designed for use with the TA-29 cable assembly.

## **Loop Speed Switch (Item G)**

Sets the feedback loop speed for the CONTROL TEMP THERMISTOR when the CL-100 is used in *automatic mode*. Feedback options include *fast*, *medium*, and *slow*. Optimally set to fast for most applications but can be set to medium or slow for systems with longer thermal delay characteristics.

## **Set Temperature Control (Item H)**

Used to adjust the set point of the *automatic* temperature control system. The associated GREEN LED is on when the INTERNAL/EXTERNAL SELECT CONTROL (Item J) is set to *internal*, and the COOLING MODE SWITCH (Item C) is set to *auto*. Set value can be read from the METER (Item B) in the *set temp* position.

## **External/Internal Select Control (Item J)**

Used to select between *internal* or *external* control inputs when the instrument is in *Manual* mode (Item C).

When the INTERNAL/EXTERNAL SELECT CONTROL is set to *internal*, and the COOLING MODE SWITCH (Item C) is set to *auto*, the SET TEMPERATURE CONTROL (Item H) will be active. Setting the COOLING MODE SWITCH (Item C) to *manual* disables the SET TEMPERATURE CONTROL (Item H) and activates the MANUAL VOLTAGE CONTROL (Item K).



## **Manual Voltage Control (Item K)**

Used to manually adjust the voltage output to the heater/cooler device. The associated GREEN LED is on when the INTERNAL/EXTERNAL SELECT CONTROL (Item J) is set to *internal*, and the COOLING MODE SWITCH (Item C) is set to *manual*. Set value can be read from the METER (Item B) in the *output volts* position.

## **Peltier Limit LED (Item L)**

This option functions only when the CL-100 is used with an SC-20 Dual In-line Solution Heater/Cooler. The RED LED is *lit* when the temperature of the Peltier device within the SC-20 exceeds its operational limits. Activation of this circuit automatically sets the output voltage of the CL-100 to 0 V.

## **Freeze Alert LED (Item M)**

This option functions only when the CL-100 is used with an SC-20 Dual In-line Solution Heater/Cooler. The BLUE LED is *lit* when the Peltier device within the CL-100 approaches 0°C. Activation of this circuit is informative only and will not alter any instrument setting.

## **Heat / Cool LED's (Item N)**

RED and BLUE LED's indicate *heating* or *cooling* power applied to the Peltier device.

# Control Description (Cont'd)


8

Bipolar Temperature Controller Model CL-100

Warner Instruments

## Rear Panel

A schematic of the rear panel of the **CL-100** is shown below. Important components are identified by letter (P-T). Refer to this diagram as an aid in identification of the described components.

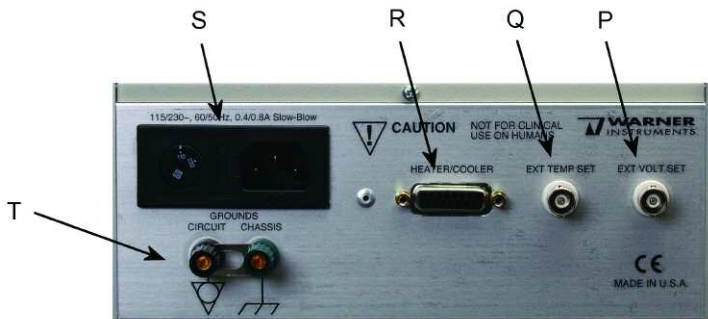

### External Volts Set (Item P)

Input BNC for the application of a specified voltage to be applied to the heater/cooler being controlled. Input functions only when the INTERNAL/EXTERNAL SELECT CONTROL (Item J) is set to *external*, and the COOLING MODE SWITCH (Item C) is set to *manual*. Units are 1 V/V input. Can be used for computer control purposes.

### External Temp Set (Item Q)

Input BNC for adjusting the SET TEMPERATURE of the **CL-100**. Input functions only when the INTERNAL/EXTERNAL SELECT CONTROL (Item J) is set to *external*, and the COOLING MODE SWITCH (Item C) is set to *auto*. Units are 100 mV/°C. Can be used for computer control purposes.

### Heater/Cooler input (Item R)

This is the connection port for Warner Heater/Cooler devices such as the **SC-20** Dual In-line Heater/Cooler.

### Power Entry Module (Item S)

Comprised of the line cord attachment point, line voltage selector and fuse buss. Power entry is selectable between 115 VAC, 60 Hz or 230 VAC, 50 Hz. The replaceable fuse is 0.4 amp slow-blow for 230 V applications, or 0.8 amp slow-blow for 115 V applications.

### Ground Terminals (Item T)

Provides separate connections for *chassis* and *circuit* ground. Banana jacks are bridged when shipped from the factory.

# Control Description

9

Warner Instruments Bipolar Temperature Controller Model CL-100

## AC Conversion

### ATTENTION

**PLEASE READ BEFORE APPLYING POWER TO YOUR UNIT!!**


The unit has been set to be used with 120 VAC.

If the VAC needs to be changed to 220VAC, enclosed you will find a kit (power cord (1) and fuses (2)) to be used to convert the unit from 120VAC to 220 VAC.

The unit uses only one fuse; the second one is sent as spare.

Follow these instructions to change the unit(s) from 120VAC or 220VAC:

### Power Entry Module

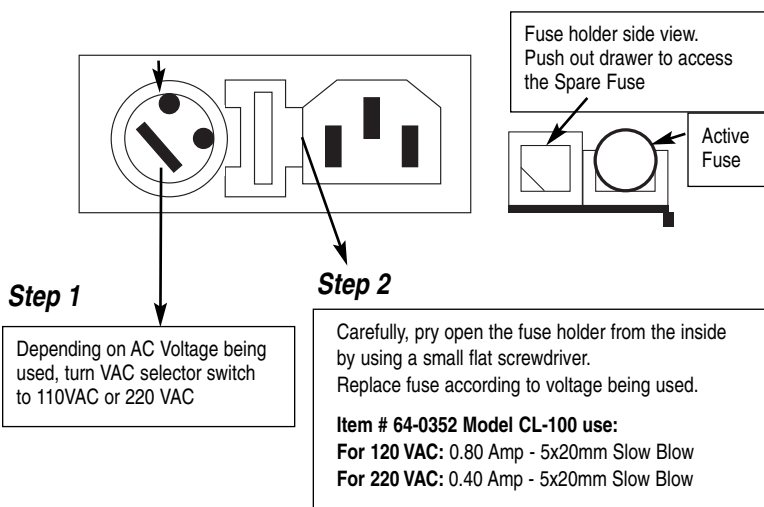

The **CL-100** has been designed primarily to drive Warner's expanding line of Peltier driven Heater/Coolers. However, the device is also capable of supplying power to Warner's full line of resistive heaters (e.g., Series 20 Heater Platforms, In-line Solution Heaters, etc.). The instrument will auto-detect when a resistive heating device has been attached and will disable cooling commands.

## Warner Peltier Driven Systems

The basic set up for the **CL-100** is straightforward when used with Warner's Peltier Driven Heater/Coolers.

First connect the cable from the heater/cooler device into the 15-pin D-connector on the back of the **CL-100**. Then connect the **TA-29** Thermistor (supplied with the heater/cooler device) to the MONITOR TEMP IN BNC (Item F).

If using external control inputs, make connections from your *command output* (e.g., analog out on the A/D board, power supply) to either the EXT TEMP SET (Item Q) or EXT VOLT SET (Item P) BNC's on the rear panel.

## Operating With Other Equipment

The **CL-100** can be used to power other Warner equipment such as the **SH-27B** and **SF-28 Slow-Flow** solution heaters. In addition, the controller can be used as an independent device to power third-party equipment as long as the following considerations are met.

### Warner Resistive Heating Systems

Use of the **CL-100** to power Warner resistive heaters is allowed if used in conjunction with the **AC-100** adapter cable. When the **CL-100** is connected to a resistive device, all command inputs (auto and manual modes for both internal and external commands) are functional with the exception that cooling commands are not executed.

### Third-party Equipment

The **CL-100** heater controller will work with many other heating devices if used in conjunction with the **AC-100** adapter cable. To obtain maximum heating power, the resistance of the third-party heating element should be between 8-12  $\Omega$ . However, any element that works at a maximum of 15 V and 2.4 A will also work with the **CL-100**.

### Thermistor Considerations

The **CL-100** heater controller was designed to accommodate Unical thermistors from Thermometrics (Edison, New Jersey). This family of thermistors can be interchanged without recalibration of the instrument. The nominal resistance of Unical thermistors is 10.0 k $\Omega$  at 25°C.

Other thermistors may be used with the **CL-100** if the nominal resistance also is 10.0 k $\Omega$  at 25°C.

The main use of a heater/cooler control device such as the **CL-100** is to maintain a constant bath temperature with minimum deviation from a set temperature. This is usually achieved by using a thermally controlled chamber/platform or in-line solution heater, or a combination of both.

**NOTE:** Refer to the front and rear panel schematics on pages 6-9 for orientation of the CL-100 controls.

## Automatic Mode

In *Automatic Mode*, the **CL-100** maintains the temperature of the connected heater/cooler at the value set by the user.

Operation is straightforward. Connect your heater/cooler device and sensor thermistor as described on page 10. Set the **CL-100** to *internal commands* by setting the INTERNAL/EXTERNAL SELECT control (Item J) to *internal*. Place the **CL-100** into *auto* mode by switching the COOLING MODE SWITCH (Item C) to *auto*. Switch the METER (Item B) to *Set Temp* and adjust to the desired set-point using the SET TEMPERATURE control (Item H).

Alternatively, the **CL-100** can be commanded using external inputs. Set the **CL-100** to *external commands* by setting the INTERNAL/EXTERNAL SELECT control (Item J) to *external*. In this mode the **CL-100** will accept external temperature settings from the EXT TEMP SET BNC (Item R) on the instrument rear panel. This input is calibrated to 100 mV/°C.

The selectable LOOP SPEED control (Item G) is used to adjust the speed of the feedback loop in the heater/cooler-thermistor system, which controls the rate of change of the **CL-100's** output voltage. Non-Warner heater systems with feedback thermistors can be used in *automatic mode* provided they are compatible with the **CL-100** requirements.

LOOP SPEED is normally set to *fast* to provide the shortest cycle time between the application of power to the heater element and the sensing of temperature at the thermistor. For heater/cooler-thermistor systems with long response times, the *fast* setting will cause the temperature to overshoot the target by a large amount resulting in system oscillation. For this condition, try *medium* or *slow* settings to find the optimum feedback rate.

## Manual Mode

In *manual mode*, the MANUAL VOLTAGE control (Item K) is used to set the output voltage to a fixed value. In *manual mode*, the SET TEMPERATURE control (Item H) is disabled, as is the feedback system of the **CL-100**.

Operation is again straightforward. Set the **CL-100** to accept *internal* commands by setting the INTERNAL/EXTERNAL SELECT control (Item J) to *internal*. Place the **CL-100** into *manual mode* by switching the COOLING MODE SWITCH (Item C) to *manual*. Switch the METER (Item B) to *Output Volts* and adjust to the desired set-point using the MANUAL VOLTAGE control (Item K).

Alternatively, the **CL-100** can be commanded using external inputs. Set the **CL-100** to *external commands* by setting the INTERNAL/EXTERNAL SELECT control (Item J) to *external*. In this mode the **CL-100** will accept external voltage commands at the EXT VOLT SET BNC (Item P) located on the instrument rear panel.

In this mode, the instrument operates as a **0-12 VDC** power supply that can provide up to **1.5 A** of current to a device. Use this mode with heater systems that will operate properly with a fixed voltage and lack feedback thermistors.

# Appendix

Specifications	
Maximum Output Voltage	±15 VDC
Maximum Output Current	2.4 A
Manual Voltage Range	0 to ±15 VDC
Maximum Output Power	18 W into a 8 W load
Power Requirements	100-130 or 200-260 VAC, 50/60 Hz, 80 VA
Power Fuse (5 x 20 mm)	0.8 A Slow-Blow for 100-130 VAC 0.4 A Slow-Blow for 200-260 VAC
Front Panel Input	External thermistor (BNC, calibrated to 10.0 kW at 25°C )
Front Panel Recorder Outputs	Monitor Temp Out (BNC, 100 mV/°C ) Control Temp Out (BNC, 100 mV/°C )
Rear Panel Inputs	External Temperature Set (BNC, 100 mV/°C ) External Voltage Set (BNC) Heater/Cooler Device (15-pin D connector)
Temperature Range Peltier	0 to 50°C Resistive: Ambient to 65°C
Meter Display	3.5 digit LED display of °C or V
Meter Readouts	Set Temperature (°C ) Control Temperature (°C ) Monitor Temperature (°C ) Output Voltage (V )
Enclosure, H x W x D	20.0 x 8.9 x 25.4 cm
Weight	5.6 kg

## Accessories and Replacement Parts

Catalog No.	Model	Product
64-1427	ACC-1	Adapter cable for heater only components

## Warranty

The model **CL-100** is covered by our Warranty to be free from defects in materials and workmanship for a period of two years from the date of shipment. If a failure occurs within this time, we will either repair or replace the faulty component(s).

This warranty does not extend to damage resulting from misuse, neglect or abuse, normal wear and tear, or accident.

This warranty extends only to the original customer purchaser.

**IN NO EVENT SHALL HARVARD APPARATUS BE LIABLE FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES.** Some states do not allow exclusion or limitation of incidental or consequential damages so the above limitation or exclusion may not apply to you. **THERE ARE NO IMPLIED WARRANTIES OF MERCHANTABILITY, OR FITNESS FOR A PARTICULAR USE, OR OF ANY OTHER NATURE.** Some states do not allow this limitation on an implied warranty, so the above limitation may not apply to you.

If a defect arises within the one-year warranty period, promptly contact your local distributor or ***Harvard Apparatus, Inc. 84 October Hill Road Holliston, Massachusetts 01746-1388*** using our toll free number 1-800-272-2775 (valid only in the U.S., outside U.S. call 508-893-8999). Goods will not be accepted for return unless an RMA (returned materials authorization) number has been issued by our customer service department. The customer is responsible for shipping charges. Please allow a reasonable period of time for completion of repairs, replacement and return. If the unit is replaced, the replacement unit is covered only for the remainder of the original warranty period dating from the purchase of the original device.

This warranty gives you specific rights, and you may also have other rights which vary from state to state.

In addition, we can be reached by e-mail at **support@warneronline.com** or through the web at **www.warneronline.com**.



## Service Notes

Please refer all questions regarding service to our Engineering Department.

- A) If the instrument POWER light fails to light, check the fuse at the rear panel (located in the black POWER INPUT MODULE). If the fuse is found to be defective replace it with a 5x20 mm, 0.8 A, slow-blow fuse (0.4 A for facilities using 220-240 V line voltages). If the replacement fuse also fails, please call Warner Instruments for assistance.
- B) Occasionally, a knob on the front panel will loosen after long use. These are "collet" style knobs and are tightened with a screw located under the knob cap. To gain access to the adjustment screw, pry the cap off with a thin bladed screwdriver or similar tool.
- C) Should service be required, please contact the factory. The problem may often be corrected by our shipping a replacement part. Factory service, if required will be expedited to minimize the customer inconvenience.
- D) Instruments are inspected immediately upon receipt and the customer is notified if the repair is not covered by the warranty. Repairs can often be completed in 1-2 days from our receipt of the instrument.
- E) If factory service is required, please observe the following instructions:
  - 1) Package the instrument with at least 3 inches of cushioning on all sides. Use the original shipping carton if it is available.
  - 2) Insure the shipment for its full value.
  - 3) Include with the shipment an explanation of the problem experienced.

### ***IMPORTANT for Customers Outside of the U.S.:***

Please contact us before return shipping any goods. We will provide instructions so that the shipment will not be delayed or subject to unnecessary expense in clearing U.S. Customs.