

Agilent 4263B LCR Meter 100 Hz to 100 kHz

Technical Overview



Introduction

The Agilent Technologies LCR meter makes fast measurements on components. It is optimized for applications that require precision and versatility. The instrument's performance ranges from general bench-top impedance measurements to complex transformer, coil and electrolytic capacitor measurements. The LCR meter offers fast, reliable, and versatile testing at a low cost.

Satisfy your needs for...

Fast system test throughput


- Maximize testing with rapid 25 ms measurements
- Minimize user intervention with pass/fail testing
- Communicate results with display and GPIB
- Automate testing with built-in handler interface

Fault-free results

- Test with confidence using contact check function
- Remove parasitics with error correction
- Get the best data with 0.1% basic accuracy
- Eliminate trigger timing errors with trigger delay function

Versatile measurements

- Select from 11 impedance parameters
- Add three complex transformer parameters with Option 4263B-001
- Set signal level with 5 mVrms resolution
- Monitor actual ac voltage and current levels
- Pick from many test fixtures and accessories
- Save and recall up to ten measurement setups

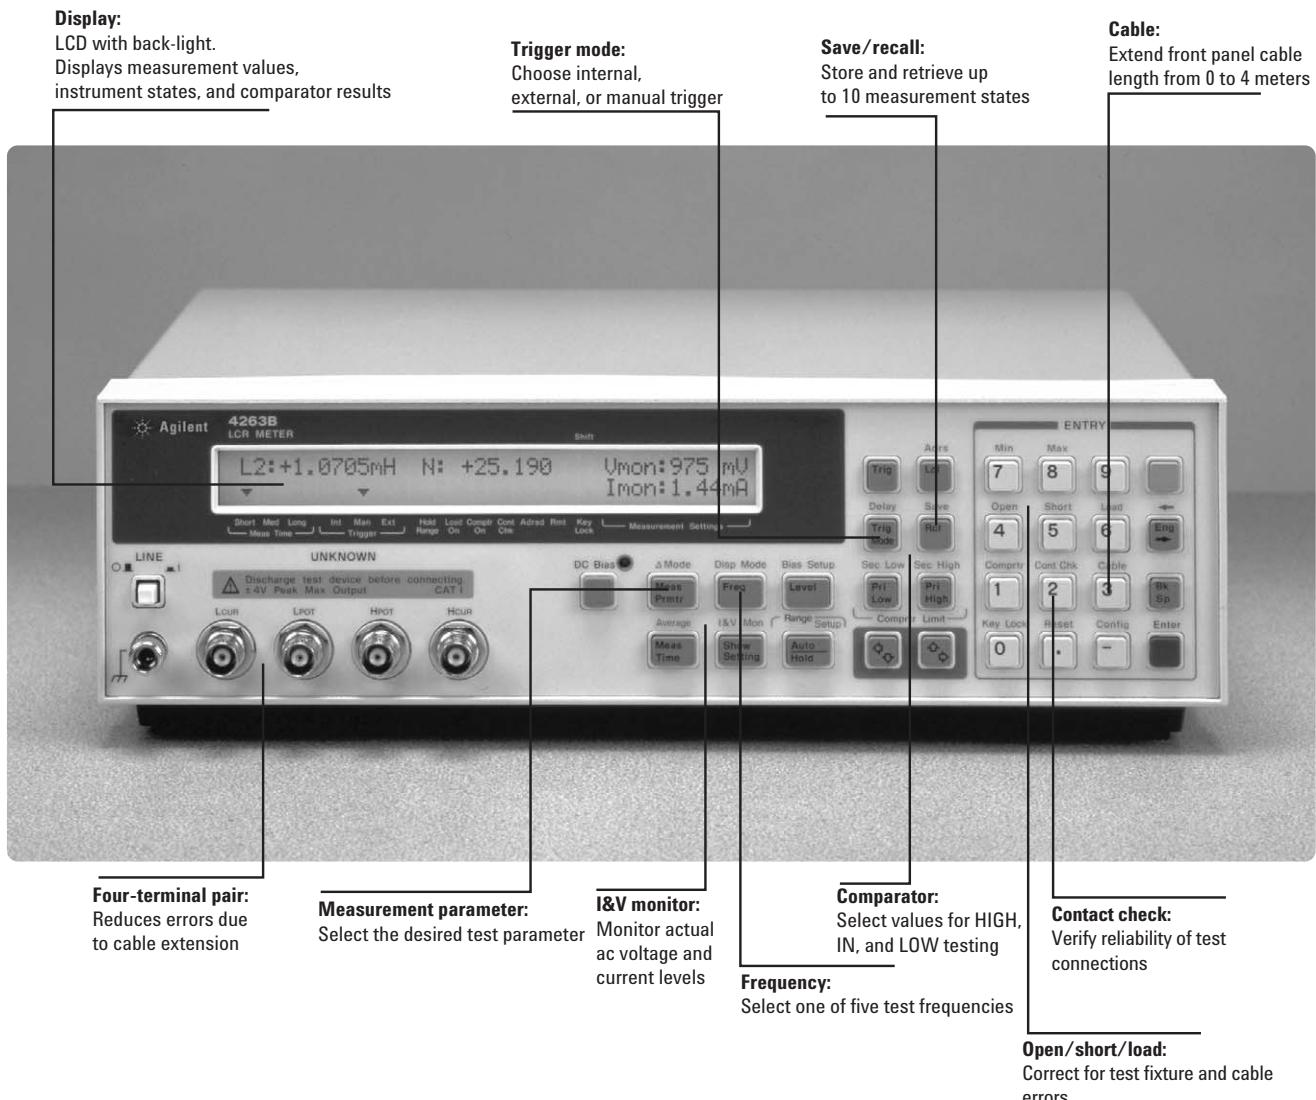

Key Parameters and Specifications

Test frequencies:

100 Hz, 120 Hz, 1 kHz, 10 kHz, 100 kHz

Option 4263B-002 adds 20 kHz

AC test signal levels:

20 m-1 Vrms, 5 mVrms steps

Basic accuracy:

0.1%

Impedance parameters:

|Z|, R, X, |Y|, G, B, C, L, D, Q, U

Option 4263B-001 adds transformer measurement functions: turns-ratio, mutual-inductance and dc-resistance

Cable length settings:

0, 1, 2, 4 meters

Bias:

1.5 and 2.0 Vdc

Error correction:

Open, short, and load

Built-in system features:

GPIB and handler interfaces

Measurement time (typical):


25 ms at best conditions

Contact check time (typical):

5 ms per measurement

High-quality results

- See five digits of data
- Make precise measurements with 0.1% basic accuracy
- Select from 11 impedance parameters
- Verify device performance at simulated operating conditions
- Monitor actual test signal voltage and current levels

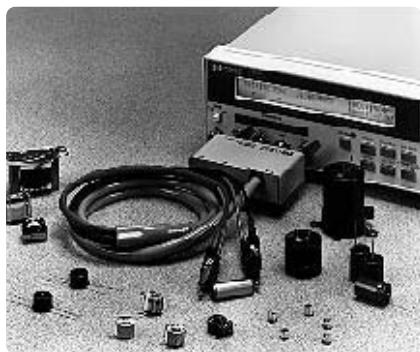

Make reliable impedance measurements.

System features for test automation


- Maximize accuracy with error correction
- Use performance specified with 0, 1, 2, and 4 meter cables
- Test device contact failure with contact check function
- Automate testing with GPIB interface
- Reduce ground-loops with isolated handler interface
- Continue testing after ac power loss with continuous memory
- Perform pass/fail testing with comparator function (High/In/Low)



The 4263B LCR meter is designed for automated applications.

Evaluate transformers and coils with Option 4263B-001

- Measure turns-ratio, mutual inductance and dc-resistance
- Easily make connections with 16060A transformer test fixture
- Measure parameter responses with variable signal levels

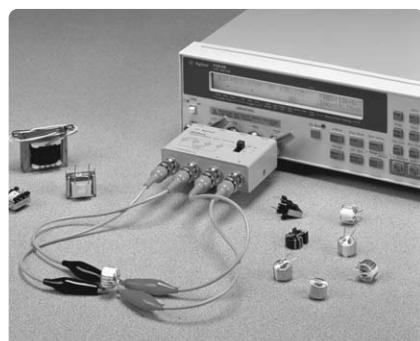

Simplify transformer testing.

Make electrolytic capacitor measurements

- Obtain versatile testing with a large capacitance range
- Keep costs down with built-in dc bias source
- Protect your investment: high energy protection on terminals
- Increase test throughput with fast system measurements
- Make reliable handler measurements with contact check function



Quickly evaluate electrolytic capacitors.

Specifications

Measurement accuracy

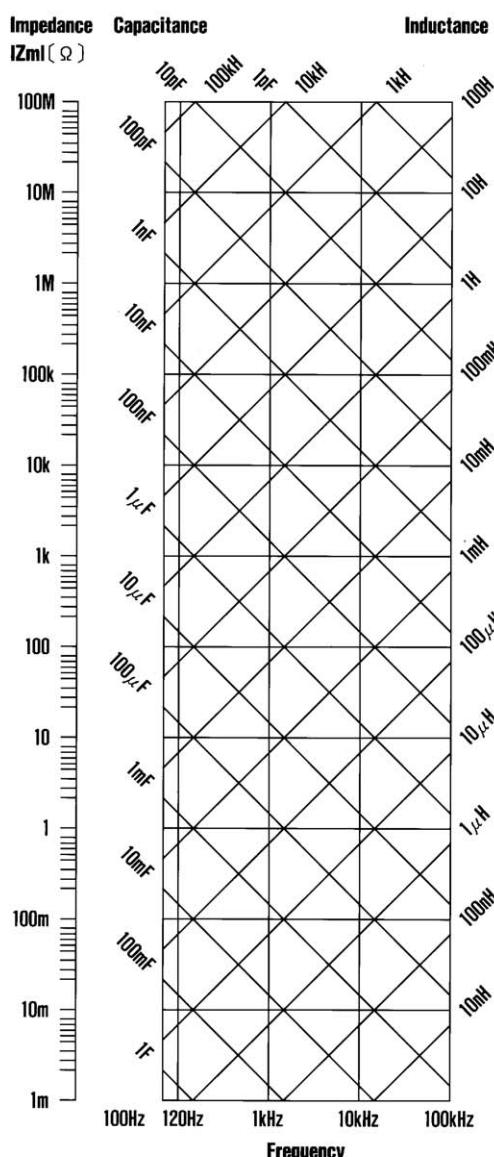


Figure 1. Conversion diagram

Impedance $ Z_{ml} (\Omega)$	Capacitance	Inductance	DC	$100/120$	$1k$	$10k$	$20k$ (Option 002 only)	$100k$	Accuracy not specified
100M	100PF	10H	$0.85 + 2.9 \times 10^{-8} / Z_{ml} $	$0.15 + 2.9 \times 10^{-8} / Z_{ml} $	$0.1 + 5.6 \times 10^{-8} / Z_{ml} $	$0.48 + 3.8 \times 10^{-7} / Z_{ml} $	$1.9 + 7.7 \times 10^{-7} / Z_{ml} $		
10M	1nF	1H	$0.85 + 2 \times 10^{-7} / Z_{ml} $	$0.15 + 2 \times 10^{-7} / Z_{ml} $	$0.095 + 1.4 \times 10^{-7} / Z_{ml} $	$0.36 + 5.1 \times 10^{-7} / Z_{ml} $	$1.4 + 1 \times 10^{-6} / Z_{ml} $		$1.2 + 1.4 \times 10^{-5} / Z_{ml} $
1M	10PF	100mH	$0.85 + 2 \times 10^{-6} / Z_{ml} $	$0.15 + 2 \times 10^{-6} / Z_{ml} $	$0.09 + 1 \times 10^{-6} / Z_{ml} $	$0.16 + 1.9 \times 10^{-6} / Z_{ml} $	$0.8 + 3.7 \times 10^{-6} / Z_{ml} $		
100k	1fF	1mH	$0.85 + 2 \times 10^{-5} / Z_{ml} $	$0.15 + 2 \times 10^{-5} / Z_{ml} $	$0.09 + 1 \times 10^{-5} / Z_{ml} $	$0.16 + 1.5 \times 10^{-5} / Z_{ml} $	$0.7 + 3.1 \times 10^{-5} / Z_{ml} $		$1.1 + 1 \times 10^{-4} / Z_{ml} $
10k	10fF	$100\mu\text{H}$	$0.85 + 2 \times 10^{-4} / Z_{ml} $	$0.15 + 2 \times 10^{-4} / Z_{ml} $	$0.09 + 1 \times 10^{-4} / Z_{ml} $	$0.16 + 1.5 \times 10^{-4} / Z_{ml} $	$0.7 + 3 \times 10^{-4} / Z_{ml} $		$1.1 + 1 \times 10^{-3} / Z_{ml} $
1k	1pF	$1\mu\text{H}$	$0.85 + 2 / Z_{ml} $	$0.15 + 2 / Z_{ml} $	$0.09 + 1 / Z_{ml} $	$0.16 + 1.5 / Z_{ml} $	$0.5 + 3.1 / Z_{ml} $		$0.83 + 10 / Z_{ml} $
100m	100fF	100mH	$0.85 + 0.2 / Z_{ml} $	$0.17 + 0.22 / Z_{ml} $	$0.12 + 0.1 / Z_{ml} $	$0.2 + 0.18 / Z_{ml} $	$0.6 + 0.35 / Z_{ml} $		$0.97 + 1.3 / Z_{ml} $
10m	1pF	1mH	$0.85 + 0.022 / Z_{ml} $	$0.4 + 0.022 / Z_{ml} $	$0.4 + 0.015 / Z_{ml} $	$0.4 + 0.04 / Z_{ml} $	$0.6 + 0.08 / Z_{ml} $		$0.97 + 0.35 / Z_{ml} $
1m	1fF	10mH	$0.85 + 0.012 / Z_{ml} $	$0.4 + 0.012 / Z_{ml} $	$0.4 + 0.0075 / Z_{ml} $	$0.4 + 0.028 / Z_{ml} $	$0.6 + 0.056 / Z_{ml} $		$0.97 + 0.26 / Z_{ml} $

Table 1. Measurement accuracy ($\pm\%$ of reading)

Measurement conditions

1. Warm-up time: \geq 15 min.
2. Ambient temperature: 23 ± 5 °C
3. Test signal voltage: 1 Vrms
4. Test cable length: 0 meter
5. Open and short corrections performed
6. Measurement time: Medium or Long
(Other test condition data is available in the operation manual.)

For $|Z|$, $|Y|$, L, C, R, X, G, and B accuracy (A_e), refer to Table 1. Table 1 equations yield accuracy based on frequency and DUT characteristic impedance (Z_m). Z_m is from Figure 1, Conversion Diagram.

$$D \text{ accuracy}(D_e) = \pm A_e / 100$$

$$Q \text{ accuracy}(Q_e) = \pm \frac{(Q_m) \times D_e}{1 - (Q_m \times D_e)}$$

$$u \text{ accuracy } (u_e) = 0.573 \times A_e$$

A_e = Accuracy of $|Z|$, $|Y|$, L, C, R, X, G, and B

D_e = D accuracy

D_m = Measured value of D

Q_e = Q accuracy

Q_m = Measured value of Q

u_e = u phase angle accuracy

Z_m = DUT impedance at test frequency in Hertz

Other Specifications

Measurement parameters/ranges

Parameter	Range
$ Z $, R, X	1 mΩ to 100 MΩ
$ Y $, G, B	10 nS to 1000 S
C	1 pF to 1 F
L	10 nH to 100 kH
D	0.0001 to 9.9999
Q	0.1 to 9999.9
u	-180° to +180°
Δ	-999.99% to 999.99%

Option 4263B-001: DC resistance 1 mΩ to 100 MΩ

Mutual inductance 1 µH to 100 H
(typical)

Turns-ratio 0.9 to 200 (typical)

Measurement conditions and functions

Test frequency: 100 Hz, 120 Hz,
1 kHz, 10 kHz, 100 kHz. (Option 4263B-002
adds 20 kHz.)

AC test signal level: 20 m - 1 Vrms,
5 mVrms steps

Bias:

Internal: + 1.5 and +2.0 Vdc
External: 0 to + 3.0 Vdc

Ranging: Auto and Hold

Trigger: Internal, Manual, and External

Trigger delay time: 0 to 9999 ms in
1 ms steps

Test cable lengths:

0, 1 meter @ $f \leq 100$ kHz
2 meter @ $f \leq 10$ kHz (20 kHz)
4 meter @ $f \leq 1$ kHz

Measurement time:

SHORT	MEDIUM	LONG
25 ms	65 ms	500 ms

Other instrument functions

Test signal level monitor:

Voltage, current

Error Correction: Open, Short, Load

Comparator: HIGH, IN, and LOW for each displayed parameter

Save/recall: 10 instrument states from non-volatile memory

Front-end Protection:

$V_{max} = \sqrt{8/C}$ @ $V_{max} \leq 250$ V

$V_{max} = \sqrt{2/C}$ @ $V_{max} \leq 1000$ V

C in Farads

Handler interface: Negative logic and isolated.
Signals are HIGH/IN/LOW, No-Contact, EOM, Index, Alarm, Keylock, Ext. Trigger.

GPIB interface: Instrument control, TALK-only mode for LISTEN-only printers using GPIB or Centronics/GPIB converter

Physical characteristics

Power: 90-132 Vac or 198-264 Vac.
47-66 Hz. 45 VA typical.

Operating temperature: 0 to 45 °C


Dimensions: 320 (W) x 100 (H) x 300 (H) mm

Weight: 4.5 kg (typical)


Test Fixtures/Accessories for the Agilent 4263B



16060A transformer test fixture
Allows fast connections to
transformers

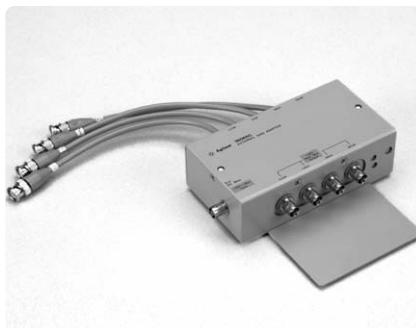

16065C external bias adapter
For external dc bias of DUT. Vmax
 ≤ 40 Vdc.

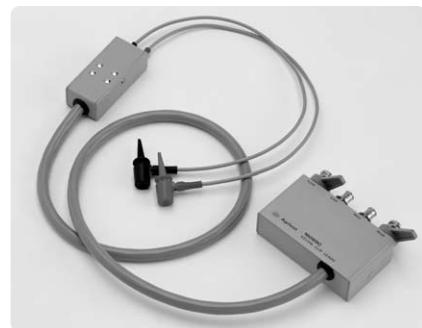

16089C Kelvin IC clip leads
IC package clip. 1 meter length.



16089A Kelvin clip leads
Large clip. 1 meter length.



16034G Test fixture
For SMD components.

Component dimensions (L x W):
0.6 mm x 0.3 mm to 5.0. mm x 1.6 mm

16089B Kelvin clip leads
Medium clip. 1 meter length.

16089D Alligator clip leads
Four clips. 1 meter length.

Ordering information¹

Agilent 4263B LCR Meter

Furnished accessory: power cable

Options

4263B-001 Add N/M/DCR Measurement Function

4263B-002 Add 20 kHz Test Frequency

Test fixtures are not furnished as standard.

Manual options²

4263B-ABA U.S. - English localization

4263B-ABJ Japan - Japanese localization

4263B-0BW Add service manual

Cabinet options

4263B-1CM Rackmount kit

4263B-1CN Handle kit

(Rack flange and handle kit are not compatible.)

Calibration certificate option

4263B-1A7 ISO 17025 compliant calibration

Test fixtures and accessories

16034E/G/H SMD component test fixture

16043-60011/12 3-terminal SMD test fixture

16044A³ Test fixture

Options

16044A-ABA U.S. - English localization

16044A-ABJ Japan - Japanese localization

16047A/E³ Axial and radial test fixture

Options

16047E-ABA U.S. - English localization

16047E-ABJ Japan - Japanese localization

16334A SMD tweezer test fixture

16048A 0.94-meter/BNC test leads

16048-60030 0.94-meter/SMC test leads

16048D 1.89-meter/BNC test leads

16048E 3.8-meter/BNC test leads

16060A Transformer test fixture

16065A 200-Vdc external voltage bias fixture

16065C 40-Vdc external voltage bias adapter

16089A Large Kelvin clip leads

16089B Medium Kelvin clip leads

16089C Kelvin IC clip leads

16089D Alligator clip leads

16089E Kelvin clip leads

¹ Accessories and options are priced individually.

² Manual is not furnished as standard

³ Must specify one of language options (ABA or ABJ) for operation manual of 16047E for shipment with product.

Faxantwort

(Bitte vorher kopieren)

07121 / 51 50 10

An: dataTec Gruppe
 Ferdinand-Lassalle-Str. 52
 72770 Reutlingen

Tel.: 07121 / 51 50 50

Absender:

Firma

Name, Vorname

Abteilung

Straße

PLZ/Ort

Telefon

Telefax

E-Mail

Firmenstempel/Datum/Unterschrift

DATATEC AKADEMIE

Technische Seminare

Vertiefen Sie Ihre theoretischen und praktischen Kenntnisse indem Sie die Seminarangebote von dataTec nutzen. Die dataTec Akademie bietet Ihnen Seminare zu allen Bereichen der Messtechnik an und vermittelt praktisches Wissen rund um Oszilloskope, Messgeräte, Netzgeräte, Thermografie und Prüfgeräte. **Gleich reinklicken und Platz sichern: www.datatec-akademie.de**

DATATEC

Mess- und Prüfgeräte Distribution

Sie und Ihr Unternehmen haben Anforderungen und Ziele, die bestmöglich erfüllt werden wollen. Durch die einzigartig **große Produktvielfalt**, gepaart mit höchster technischer Kompetenz, steht Ihnen mit dataTec ein zuverlässiger Partner zur Seite, der Sie auf diesem Weg begleitet.

Bitte nehmen Sie Kontakt mit mir auf.

Ich interessiere mich für folgendes:

- Oszilloskope, Analysatoren, Messgeräte
- Generatoren, Quellen, Stromversorgungen
- Datenlogger, Multimeter
- Thermografie
- Gerätetyp:

DATATEC ATP

Autorisierter Technologie Partner von Agilent

Ihr Vertriebspartner für höherwertige elektronische Messtechnik (Produkte, die nicht über die Distributionskanäle vertrieben werden) von Agilent Technologies in Deutschland

Unverbindliche Beratung vor Ort

Sie haben anspruchsvolle Messaufgaben – um Sie dabei optimal unterstützen zu können, stehen wir Ihnen bei der Auswahl der geeigneten Messmittel zur Seite. Gerne besucht Sie ein technischer Experte im Außendienst für eine individuelle, persönliche Beratung an Ihrem Arbeitsplatz.

- Ja, ich möchte eine **Beratung vor Ort**
- Mein Wunschtermin:
- Gerätetyp:

www.datatec-gruppe.de



dataTec Ihr Spezialist für Mess- und Prüfgeräte | Agilent Premium Distributor + Autorisierter Technologie Partner von Agilent