



# **Veterinary Patient Warming System Service Manual**

***For information on operating the Hot Dog Patient Warming  
System, refer to the "Instructions for Use"***

## Contents

Definition of Symbols.....	3
Introduction.....	4
Description of the Hot Dog™ Patient Warming System.....	<b>Error! Bookmark not defined.</b>
Precautions .....	5
Proper Use and Maintenance.....	6
Read Before Servicing Equipment.....	6
Initial Setup & Assembly.....	7
Contents.....	7
Assembly Procedure.....	7
Mounting the Hot Dog Controller to an IV Pole.....	8
Overview of Control Panel & Operating Modes .....	9
Maintenance & Testing.....	11
Verification of Start-up Sequence .....	11
Preventive Maintenance .....	13
Cleaning of the Controller Housing .....	17
Cleaning of the Warming Blankets .....	17
Troubleshooting.....	18
Technical Support & Customer Service .....	21
Specifications.....	22
Emissions and Immunity .....	24

## DEFINITION OF SYMBOLS



Attention, consult  
accompanying documents



Reference Number



BF Patient Applied Part



Serial Number



Lot Number



Manufacture Date



Temperature in Range



Storage Temperatures



Temperature Adjustment



Alarm



Main's Power On Indicator



Fuse



Equipotential



Return to Authorized  
Representative

## INTRODUCTION

The Hot Dog Patient Warming System consists of two components: the Hot Dog Controller and the Hot Dog Warming Blanket. The Controller is pre-set to deliver a constant, efficacious temperature to help maintain normothermia in patients before, during, and after surgical procedures and to help prevent unintended hypothermia.

This manual includes maintenance instructions and specifications for the Hot Dog Patient Warming System. For additional information about the Hot Dog Controller and Warming Blankets, refer to the “Instructions for Use” provided with each of these components.

## VETERINARY INSTRUCTIONS FOR USE:

### INDICATIONS FOR USE

The Hot Dog Patient Warming System is intended to prevent or treat hypothermia and to provide warmth to patients. The Hot Dog Patient Warming System should be used in circumstances in which patients may not maintain a state of normothermia.

### CONTRAINDICATIONS

Do not warm patients with ischemic or non-perfused limbs; thermal injury may result.

### WARNINGS

Do not layer multiple warming methods i.e. a hot dog blanket should not be used under a patient in combination with a heated surgical table or a hot water mattress.

**EXPLOSION HAZARD** - Do not use the Controller or Warming Blanket in the presence of flammable anesthetics or highly oxygen-enriched environments such as hyperbaric chambers, oxygen tents, etc.

**Inspect the Warming Blanket prior to use and cleaning** for signs of damage or excessive wear such as cuts, holes, or loose electrical connections. If signs of wear are evident, do not use the Warming Blanket until it is inspected by technical staff. Do not expose the inner heating element to fluids.

Do not continue to use the Hot Dog Patient Warming System if the over temperature indicator and/or alarm continue to sound after reset. See alarm section of this manual.

### Pressure reduction

When a patient remains in a single position for an extended amount of time, ischemia can occur at points of elevated pressure which can lead to tissue necrosis. Warming

ischemic tissue is contraindicated, therefore precautions should be taken when using the Hot Dog blankets under a patient. The Hot Dog warming blanket IS NOT a pressure reduction device.

When using blankets under a patient, ensure that adequate steps are taken to mitigate pressure.

Hard objects should not be placed between the patient and the blanket.

If a rigid cautery ground plate is used, ensure that adequate steps are taken to mitigate pressure. Do not place the cautery plate on the sensor area of the blanket. The cautery plate must not be larger than the patient, i.e. the patient must completely cover the cautery plate.

## **PRECAUTIONS**

Monitor the patient's vital signs regularly during warming according to institutional protocol. If vital sign instability occurs, notify the clinician.

Do not use the highest heat setting on or under patients with poor perfusion.

Use over-body warming instead of under body warming on patients with multiple risk factors such as short hair, poor circulation, severe illness that may impact circulation, or long duration procedures (> 2 hours).

Do not expose the warming blanket to a continuous exchange of cold irrigation fluids.

## **INSTRUCTIONS FOR USE**

### **When using the Hot Dog Blanket over the patient**

Use on warmest setting appropriate to the patient condition and procedure for maximum effectiveness.

Place blanket directly on the patient with the sensor in contact with the patient.

### **When using the Hot Dog Blanket under patient or wrapped around patient**

Do not use the highest heat setting unless you have a towel placed between the patient and the warming blanket.

The sensor should be in contact with the patient. A towel between the sensor and patient is acceptable.

Ensure that adequate steps are taken to mitigate pressure.

## **Proper Use and Maintenance**

Augustine Biomedical + Design assumes no responsibility for the reliability, performance, or safety of the Hot Dog Patient Warming System if the following events occur:

- The Controller is disassembled or serviced by unauthorized personnel.
- The patient warming system components are used in a manner other than described in the Instructions for Use manuals.
- The Controller is installed in an environment that does not meet the appropriate electrical and grounding requirements.

## **Read Before Servicing Equipment**

Repair, preventive maintenance, and servicing of the patient warming system requires the skill of qualified medical equipment service technicians who are familiar with good practice for medical device repair. Do not open the Hot Dog Controller. There are no user serviceable parts. If service is required, contact Technical Support (see page 21). Perform all maintenance activities in accordance with the instructions in this service manual.

## INITIAL SETUP & ASSEMBLY

### Contents

The following components are included in the Hot Dog Patient Warming System box:


- Hot Dog Controller
- Mains power cord
- Warming Blanket power cord
- IFU
- Service Manual

Reusable Hot Dog Warming Blankets are sold separately.

### Assembly Procedure

1. Remove all items from the box and discard packaging per institutional protocol.
2. Loosen and remove the two cord retainer screws and the cord retainer (see Figure 1; the cord retainer is located on the back of the Controller).
3. Firmly insert the mains power cord into the receptacle on the back of the Controller.
4. Place the cord retainer over the strain relief of the mains power cord; replace both screws and tighten to secure the cord retainer (see Figure 1).

**Figure 1: Cord Retainer Assembly**

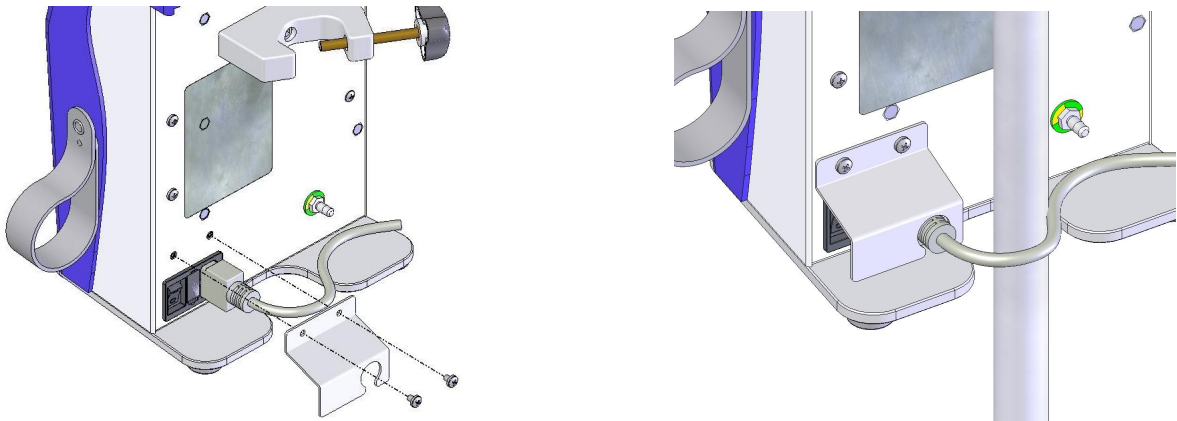


## Mounting the Hot Dog Controller to an IV Pole

To mount the Hot Dog Controller to an IV pole, place the Controller IV pole adapter around the IV pole and turn the clamp handle clockwise until securely tightened. To remove the Controller from the IV pole, turn the clamp handle counterclockwise until the unit releases. (See Figure 3.)

### **Caution**

To prevent the IV pole from tipping, the Controller must be attached at a height that provides stability. It is recommended to use an IV pole with a minimum wheelbase radius of 35.6 cm (14 in.) and to mount the Controller no higher than 112 cm (44 in.) from the floor. Failure to properly mount the Controller may result in IV pole tipping, catheter site trauma, and patient injury.

**Figure 3: Hot Dog Controller Mounted on an IV Pole**


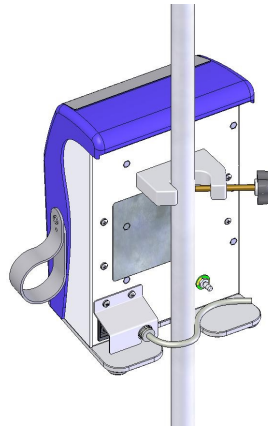




## OVERVIEW OF CONTROL PANEL & OPERATING MODES

Figure 4: Hot Dog Control Panel

- A. ON-OFF Power LED
- B. Temperature In Range LED
- C. Temperature Adjust Button
- D. Temperature Setting Indicator (3)
- E. Alarm Port A LED
- F. Alarm Port B LED
- G. Port A Outlet (Warming Blanket)
- H. Port B Outlet (Accessory Option)
- I. Serial Label
- J. IV Pole Clamp
- K. Mains Power Switch
- L. Power Plug and Inlet (fuses inside)
- M. Cord Retainer (optional)
- N. Cord Strap

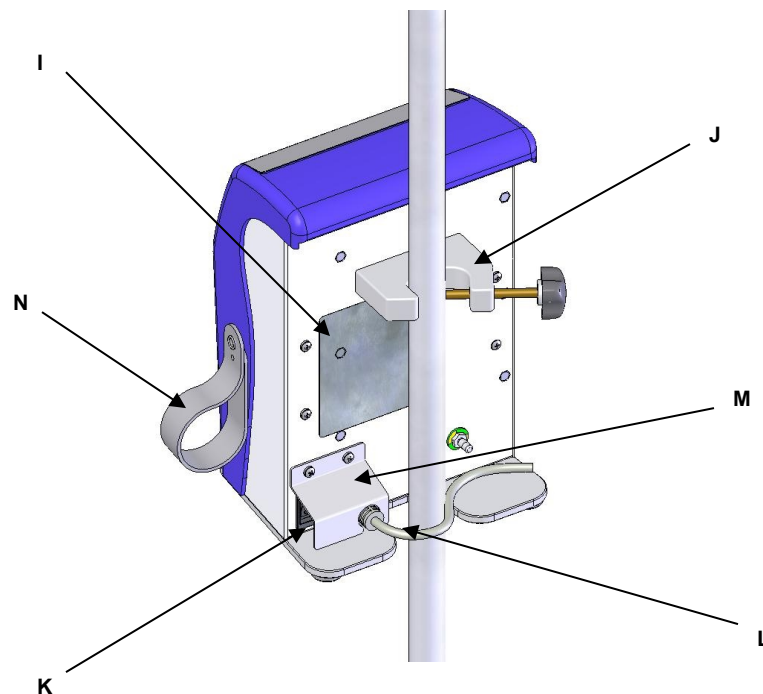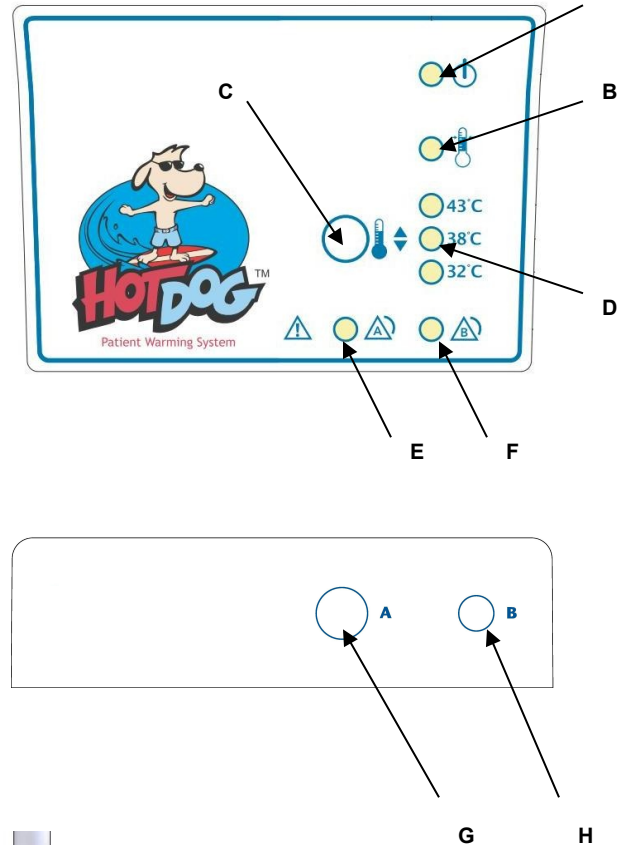

***Mains Power Switch / ON Power Light***

When the Hot Dog Controller is plugged into an electrical outlet and the Mains Power Switch on the back of the Controller is turned ON, the Controller will beep and all lights will illuminate briefly. The Mains Power ON light will illuminate and the Controller will remain idle until a temperature is selected with the Temperature Adjust Button. If there is a loss of power to the Controller, the unit will return to ON when power is returned. When the unit is ON and idle (i.e., no Temperature Setting lights are illuminated), no power is applied to the Warming Blanket and no alarm conditions are indicated.

***Temp Adjust Button / Temp Setting Lights***

Press the Temperature Adjust Button until the desired high (43°C), medium (40°C), or low (37°C) temperature is selected, as indicated by the illuminated Temperature Setting light. The designated warming temperature will be reached within 5 minutes.

***Temp in Range Light***

The green Temperature in Range light will illuminate when the temperature of the Warming Blanket is  $\pm 1^{\circ}\text{C}$  of the selected temperature setting.

***Port A***

Port A is only to be used for Hot Dog Warming Blanket connection. When plugging a Warming Blanket into the Controller, an audible beep indicates that the control and over temperature sensors (safety device) are present and functioning properly.

***Alarm Port A***

If the Warming Blanket exceeds one degree above nominal (including tolerances) or other fault conditions exist, an audible alarm sounds and the Alarm Port A light illuminates red. The Controller will automatically discontinue power to the Warming Blanket. When the operating temperature is regained, the alarm will shut off and normal function will be restored. If the Alarm Port A light illuminates steadily and the alarm continues to sound, turn the Mains Power Switch to the OFF position and disconnect the Warming Blanket from the Controller.

- If Alarm Port A occurs when connecting a Warming Blanket to the Controller, disconnect the Warming Blanket and replace it with another Warming Blanket.

***Port B (Applies to Model V004 Controllers only)***

Port B is a 48V output for Hot Dog accessories.

***Alarm Port B (Applies to Model V004 controllers only)***

If the accessory attached to Port B exceeds the pre-set current threshold, an audible alarm sounds and the Alarm Port B light illuminates red. Power is removed from the port. Disconnect the accessory from Port B to reset alarm.

- If Alarm Port B occurs when connecting an accessory to the Controller, disconnect the accessory and replace it with another accessory.
- If Alarm Port B occurs during use and the Alarm Port B light illuminates steadily, disconnect the accessory from the Controller and replace with another accessory.

## **MAINTENANCE & TESTING**

### **Verification of Start-up Sequence**

#### ***Frequency***

These checks should be completed upon initial equipment check-in and once every 12 months (or more frequently if required by hospital guidelines).

#### ***Tools/Equipment***

- Standard IV pole or vertical pole

#### ***Method***

1. Mount the Controller on a standard IV pole or vertical pole.
2. Do NOT attach a Warming Blanket to the Controller.
3. Insert the Hot Dog Controller power plug into a properly-grounded hospital-grade electrical outlet.
4. Turn the Mains Power Switch to ON and carefully observe for the following proper start-up sequence:
  - a. All lights illuminate briefly.
  - b. The Mains Power ON light remains illuminated while the other lights illuminate one by one in the following order:
    1. Temperature in Range
    2. Alarm A
    3. Alarm B
    4. 43°
    5. 40°

6. 37°

- c. All of the lights will illuminate simultaneously, and then the unit will emit an audible tone.
- d. After the sequence completes, only the Mains Power ON light remains illuminated.

If this sequence varies or is incomplete, contact Technical Support (see page 21).

## Preventive Maintenance

### Frequency

These checks should be completed once every 12 months (or more frequently if required by hospital guidelines).

### Tools/Equipment

- Test fixture (REF A104 or A115)
- Warming Blanket Cable (REF HDPC1, A101 or A102)
- Ground continuity tester
- Leakage current tester
- Calibrated, fast-reacting thermocouple and meter
- Hot Dog Warming Blanket (optional)

### Method

1. Perform “Verification of Start-up Sequence” testing (see page 11).
2. Perform the following tests on the Controller per standard institutional protocol (*note: the equipotential stud on the back of the Hot Dog Controller may be used as a grounding point for these tests*):
  - A. Ground continuity
  - B. Connect a Blanket to the Controller and test leakage current to ensure the maximum leakage current does not exceed the requirements in Table 1.

Table 1: Maximum Allowable Leakage Current		
Polarity	Condition	Current (mA)
Normal / Reversed	Normal	0.1
	Open Ground	0.5
	Open Neutral	0.5
	Open Ground & Open Neutral	0.5

3. Perform Functional Testing using either Method A or Method B, described on the following page.

## **Functional Testing Method A (Preferred)**


Use a Temperature Test Fixture (REF A104 or A115) to perform the steps outlined below. The Test Fixture simulates a Warming Blanket that is operating at 43°C. If a failure is observed during any of these steps, call customer service.

1. Using a standard blanket cable (REF HDPC1, A101 or A102), connect the test fixture to the Controller. *The Controller will emit an audible tone and the Mains Power ON light will illuminate. No other lights should be illuminated on the Controller.*
2. Press the Temperature Adjust button on the Controller to select 43°C. *The 43°C and the Temperature in Range lights should both illuminate. The heater indicator light may flash intermittently or not at all, which is normal.*
3. Press the “Temperature Low” button on the test fixture to simulate a cold warming blanket. *The Temperature in Range light should go off and the light at the top of the test fixture should illuminate to indicate that power is being applied to the test fixture (the alternating on/off shows the duty cycle applied by the Controller). Release the button and the Controller should return to “in range” as described in step 2.*
4. Press the “Temperature High” button on the test fixture to trigger the primary over-temperature alarm. *The “A” alarm light should be illuminated and an audible alarm should sound. Release the button and the Controller should return to “in range” as described in step 2.*
5. Press the “Primary Short” button on the test fixture to simulate a shorted primary sensor. *The “A” alarm light should be illuminated and an audible alarm should sound. Release the button and the Controller should return to “in range” as described in step 2.*
6. Press the “Primary Open” button on the test fixture to simulate an open primary sensor. *The “A” alarm light should be illuminated and an audible alarm should sound. Release the button and the alarm state should be latched. Unplug test fixture cord to clear the alarm. Plug the test fixture cord back in to prepare for the next step.*
7. Press the “Secondary Open” button on the test fixture to simulate an open secondary sensor. *The “A” alarm light should be illuminated and an audible alarm should sound. Release the button and the alarm state should be latched. Unplug test fixture cord to clear the alarm. Plug the test fixture cord back in to prepare for the next step.*
8. Press the “Secondary Short” button on the test fixture to simulate a shorted primary sensor or secondary over temperature. *The “A” alarm light should be illuminated and an audible alarm should sound. Release the button and the alarm state should be latched. Unplug test fixture cord to clear the alarm.*

## **Functional Testing Method B (Alternate)**

Use a Hot Dog Warming Blanket to perform the steps outlined below. If a failure is observed during any of these steps, contact Technical Support (see page 21).

1. Tape a calibrated, fast-reacting thermocouple to the patient-facing (black) surface of the Warming Blanket, directly on the sensor area of the Warming Blanket. The sensor area on the blankets is marked by a series of circles and the word “Sensor”
2. Turn the Mains Power Switch to the ON position. Supply power to the Warming Blanket by connecting the Warming Blanket power cable to the Controller. *The Controller will emit an audible tone and the Mains Power ON light will illuminate. No other lights should be illuminated.*
3. Place the blanket with the black side up on a table or other flat surface. Select the temperature to be verified by pressing the temperature select button on the controller until the desire temperature setpoint light is illuminated. If checking all set-points, start with the low temperature setting. Wait for the blanket to reach the setpoint as indicated by the Temperature-In-Range light on the controller. This should take 3 to 7 minutes at normal room temperature of 20-24° C.
4. Fold the Warming Blanket back on itself (black face to black face) so that the thermocouple is between the two layers of the heated Blanket. Ensure that the Blanket layers are pressed together in the location of the thermocouple. Place a 750 to 1000gm weight (such as a small book or notebook) over the sensor location to ensure that the pad remains folded and that there is good contact between the sensor and the folded blanket. (See figure 6)

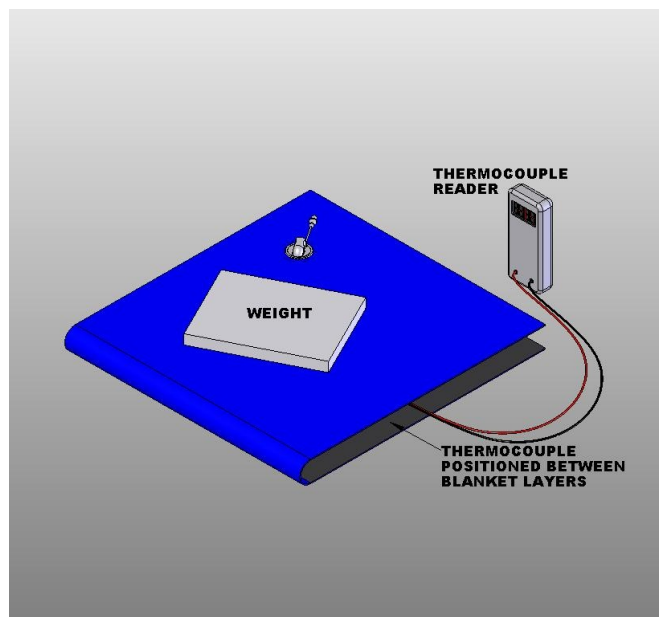

**Figure 6: Warming Blanket Testing configuration**

5. Allow the temperature to stabilize for 3 minutes. *NOTE: a slight temperature overshoot may be noted during this time, which is normal.* After 3 minutes have elapsed, check the reading of the thermocouple. The temperature should be within 1°C of the set-point temperature (including the additional tolerance of the thermocouple meter, which is usually  $\pm 1^\circ\text{C}$ ).
6. Repeat steps 3-6 for the next temperature setting, if required.



## **Cleaning of the Controller Housing**

### ***Frequency***

As needed.

### ***Tools/Equipment***

- Sponge or soft cloth
- Mild detergent or anti-microbial spray
- Dry soft cloth

### ***Warning***

Do not use a dripping wet cloth and do not immerse Hot Dog components in liquid. Moisture will damage the components, and thermal injury may result.

### ***Precautions***

Do not use pure alcohol or other caustic, chloro or flouro solvents (e.g., MEK, acetone, etc.) to clean Hot Dog components. Solvents may damage plastic parts, labeling and product finish.

### ***Method***

1. Disconnect the patient warming controller from the power source before cleaning.
2. Wipe unit with moistened sponge or soft cloth; avoid pushing fluids into any openings.
3. Dry with a separate soft cloth.

## **Cleaning of the Warming Blankets**

Refer to separate cleaning instructions provide with the Warming Blankets.

## Troubleshooting

Alarm Mode	Description
Primary over-temp	<p>When the temperature exceeds one degree above nominal (including tolerances), audible and visual alarms are initiated and power is removed from the output. The alarm will reset when:</p> <ul style="list-style-type: none"><li>• Temperature is within acceptable limits (<math>\pm 1^{\circ}\text{C}</math>)</li><li>• Cable connecting Warming Blanket to Controller is disconnected</li><li>• Power is removed at mains</li></ul>
Secondary over-temp	<p>When the temperature exceeds <math>46^{\circ}\text{C}</math>, audible and visual alarms are initiated. The alarm will reset when:</p> <ul style="list-style-type: none"><li>• Cable connecting Warming Blanket to Controller is disconnected</li><li>• Power is removed at mains</li></ul>
Over-current	<p>When current draw exceeds a predetermined level, audible and visual alarms are initiated. The alarm will reset when:</p> <ul style="list-style-type: none"><li>• Power is removed at mains</li></ul>
Failure to reach temp	<p>When the system does not achieve <math>43^{\circ}\text{C}</math> within 10 minutes, audible and visual alarms are initiated. The alarm will reset when:</p> <ul style="list-style-type: none"><li>• Cable connecting Warming Blanket to Controller is disconnected</li><li>• Power is removed at mains</li></ul>
Sensor failure	<p>When either sensor is opened or shorted, audible and visual alarms are initiated and power is removed from output. If both sensors are opened or shorted, no alarms are initiated, power is removed from output, and the temperature selector switch becomes inactive.</p> <ul style="list-style-type: none"><li>• Replace the Warming Blanket</li></ul>

### Basic Troubleshooting Steps

**If a system alarm occurs, the following steps will help identify which system component is malfunctioning. Once a malfunctioning device has been identified, or for additional troubleshooting support, contact Customer Service at 866-484-3505.**

1. Turn off the controller and unplug all blankets and cables. Let the blanket cool to room temperature. Complete the following steps IN ORDER.
2. Turn the mains power switch on the controller to ON and ensure that the controller successfully completes the brief diagnostic check (all lights illuminate sequentially, followed by a short audible beep).
  - a. If the startup sequence varies or is incomplete, the controller is malfunctioning.
3. Plug one end of the cable into the temperature controller.
  - a. If the controller alarms, the cable is malfunctioning.
4. Plug the other end of the cable into a blanket.
  - a. If the controller alarms immediately upon attaching a blanket, the blanket or the cable may be malfunctioning.
  - b. If a second cable is available, swap cables. If the alarm resolves, the original cable is malfunctioning.
  - c. If a second blanket is available, swap blankets. If the alarm resolves, the original blanket is malfunctioning.
5. Select the highest temperature setpoint.
  - a. If the controller alarms immediately upon selecting a temperature setpoint, the blanket or the cable may be malfunctioning.
  - b. If a second cable is available, swap cables. If the alarm resolves, the original cable is malfunctioning.
  - c. If a second blanket is available, swap blankets. If the alarm resolves, the original blanket is malfunctioning.
6. Place the blanket black (heated) side down on a thermally insulated surface (such as several layers of blankets or towels, or another warming blanket of similar or larger size) and let it run.
  - a. Observe the “Temperature In Range” indicator. If the controller alarms approximately 10 minutes after warming was initiated, but the temperature in range indicator did not indicate that set point temperature had been achieved, the blanket may be malfunctioning.
  - b. If the Temperature In Range indicator indicates that set point has been achieved, and the controller then alarms, the controller or the blanket may be malfunctioning.

**Note:** The controller has a 6-hour shut down alarm indicated by 3 audible beeps after which the alarm LED will flash continuously. This alarm condition occurs if a blanket is left on for 6 hours with no user intervention. Selecting a temperature set point will clear this alarm condition.

**TECHNICAL SUPPORT & CUSTOMER SERVICE**

Please have the serial number of your Hot Dog Controller when you call for technical support. The serial number is located on the back of the Controller. If it is necessary to return the Controller for service or repair, contact your local supplier or sales representative.

**USA and Worldwide:**

Augustine Biomedical + Design  
6581 City West Parkway  
Eden Prairie, MN 55344 USA  
TEL 952.465.3500  
FAX 952.465.3501  
[www.augbiomed.com](http://www.augbiomed.com)

## SPECIFICATIONS

### Physical Characteristics

Dimensions	29.21 cm high x 13.97 cm deep x 19.69 cm wide 11.5" high x 5.5" deep x 7.75" wide
Weight	3.6 kg (8.0 lb)
Mounting	Can be clamped to an IV pole

### Temperature Characteristics

Recommended Operating Environment	15°C to 25°C		
Temperature Control	Micro-processor		
Operating Temperatures	Average temperature at the Warming Blanket:		
	High	43° ± 1.0°C	109.4° ± 1.8°F
	Medium	40° ± 1.0°C	104° ± 1.8°F
	Low	37° ± 1.0°C	98.6° ± 1.8°F

### Safety System

Primary Over-temp Alarm	High-Alarm sounds at 44°C + 1°C
Secondary Over-temp Alarm	Independent electronic circuit shuts the heater off if the Warming Blanket temperature reaches 46°C ± 1°C.
Over-current Monitoring	
- Port A	12 amps max.
- Port B	1.7 amps max.
Over-current Protection	Dual input fused lines.

### Electrical Characteristics

Leakage Current	Meets UL 2601-1 and IEC 60601-1 requirements for Class I, Type BF equipment.
Power Consumption	Peak 580 W
Power Cord	4.6 m (15 ft.)
Device Ratings	Input: 100-240 VAC, 50/60 Hz, 600VA Output A: 48 VDC, 500 VA Max Output B: 48 VDC, 80 VA Max
Fuses	T6.3AL250V (2 x 5x20mm)

---

## SPECIFICATIONS

---

### Certifications

IEC 60601-1; EN 60601-1-2; UL 60601-1; CAN/CSA-C22.2, No. 601.1, EN 55011



### Classification

Classified under IEC 60601-1 Guidelines (and other national versions of the Guidelines) as Class I, Type BF, Ordinary equipment, Continuous operation. Not suitable for use in presence of flammable anesthetic mixtures with air or with oxygen or nitrous oxide. Classified by Intertek Testing Services NA Inc. with respect to electric shock, fire, and mechanical hazards only, in accordance with UL 60601-1. Classified under the Medical Device Directive (93/42/EEC) as a Class IIb device. Classified under Canadian Medical Device Regulation as Class II.

### Diagnostics

A qualified technician can perform general system testing. The Controller has no user serviceable parts.

### Transport/Storage

Temperature: -20°C to 60°C

Humidity: 20% to 80%

Keep Dry

### Important Information

This device complies with the EMC requirements according to IEC 60601-1-2. Radio transmitting equipment, cellular phones, etc. shall not be used in the close proximity of the device since this could influence the performances of the device. Particular precaution must be considered during use of strong emission sources such as High Frequency surgical equipment and similar so that, e.g., the HF-cables are not routed on or near the device. If in doubt, contact a qualified technician or your local representative.

---

## EMISSIONS AND IMMUNITY

The Hot Dog Patient Warming System needs special precautions regarding EMC and needs to be installed and put into service according to the EMC information provided in Table 2 through Table 4 below.

### **Warning**

- Accessories and cables other than those specified may result in increased emissions or decreased immunity of the Hot Dog Patient Warming system.
- The Hot Dog Patient Warming System should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the Hot Dog Patient Warming System should be observed to verify normal operation in the configuration in which it will be used.


<b>Table 2: Guidance and manufacturer's declaration – electromagnetic emissions</b>		
The Hot Dog™ Patient Warming System is intended for use in the electromagnetic environment specified below. The customer or user of the Hot Dog Patient Warming System should assure that it is used in such an environment.		
<b>Emissions test</b>	<b>Compliance</b>	<b>Electromagnetic environment – guidance</b>
RF emissions CISPR 11	Group 1	The Hot Dog Patient Warming System uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A	The Hot Dog Patient Warming System is suitable for use in all establishments other than domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	



<b>Table 3: Guidance and manufacturer's declaration – electromagnetic immunity</b>			
The Hot Dog™ Patient Warming System is intended for use in the electromagnetic environment specified below. The customer or the user of the Hot Dog Patient Warming System should assure that it is used in such an environment.			
<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment – guidance</b>
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line(s) to line(s) ±2 kV line(s) to earth	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5 % $U_T$ (>95 % dip in $U_T$ ) for 0,5 cycle 40 % $U_T$ (60 % dip in $U_T$ ) for 5 cycles 70 % $U_T$ (30 % dip in $U_T$ ) for 25 cycles <5 % $U_T$ (>95 % dip in $U_T$ ) for 5 sec	<5 % $U_T$ (>95 % dip in $U_T$ ) for 0,5 cycle 40 % $U_T$ (60 % dip in $U_T$ ) for 5 cycles 70 % $U_T$ (30 % dip in $U_T$ ) for 25 cycles <5 % $U_T$ (>95 % dip in $U_T$ ) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. If the user of the Hot Dog Patient Warming System requires continued operation during power mains interruptions, it is recommended that the Hot Dog Patient Warming System be powered from an uninterruptible power supply or a battery.
Power frequency 50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.
NOTE $U_T$ is the a.c. mains voltage prior to application of the test level.			

**Table 3 (cont'd): Guidance and manufacturer's declaration – electromagnetic immunity**

The Hot Dog™ Patient Warming System is intended for use in the electromagnetic environment specified below. The customer or the user of the Hot Dog Patient Warming System should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 V	<p>Portable and mobile RF communications equipment should be used no closer to any part of the Hot Dog Patient Warming System, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p><b>Recommended separation distance</b></p> $d = 1,2\sqrt{P}$ $d = 0,35\sqrt{P} \quad 80 \text{ MHz to } 800 \text{ MHz}$ $d = 0,7\sqrt{P} \quad 800 \text{ MHz to } 2,5 \text{ GHz}$ <p>where <math>P</math> is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and <math>d</math> is the recommended separation distance in metres (m).</p> <p>Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,<sup>a</sup> should be less than the compliance level in each frequency range.<sup>b</sup></p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p> 
Radiated RF IEC 61000-4-3	10 V/m 80 MHz to 2,5 GHz	10 V/m	

NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

<sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Hot Dog Patient Warming System is used exceeds the applicable RF compliance level above, the Hot Dog Patient Warming System should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the Hot Dog Patient Warming System.

<sup>b</sup> Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

**Table 4: Recommended separation distances between portable and mobile RF communications equipment and the Hot Dog Patient Warming System**

The Hot Dog Patient Warming System is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Hot Dog Patient Warming System can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Hot Dog Patient Warming System as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of transmitter W	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1,2\sqrt{P}$	80 MHz to 800 MHz $d = 0,35\sqrt{P}$	800 MHz to 2,5 GHz $d = 0,7\sqrt{P}$
0,01	0,12	0,04	0,07
0,1	0,37	0,11	0,22
1	1,2	0,35	0,70
10	3,7	1,1	2,2
100	12	3,5	7,0

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

<p><b><u>Manufactured by:</u></b>  Augustine Biomedical + Design  6581 City West Parkway  Eden Prairie, MN 55344 USA  TEL 952.465.3500  FAX 952.465.3501  <a href="http://www.augbiomed.com">www.augbiomed.com</a></p>	
------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------	--

Hot Dog is a trademark of Augustine Biomedical + Design, registered in the U.S. Patent & Trademark Office. Patents pending.

© 2013 Augustine Biomedical + Design. All rights reserved.

2087 Rev C (6-18-13)